


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG061319\
 Data File : BG041231.D
 Acq On : 13 Jun 2019 20:47
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sun Jun 09 23:08:34 2019

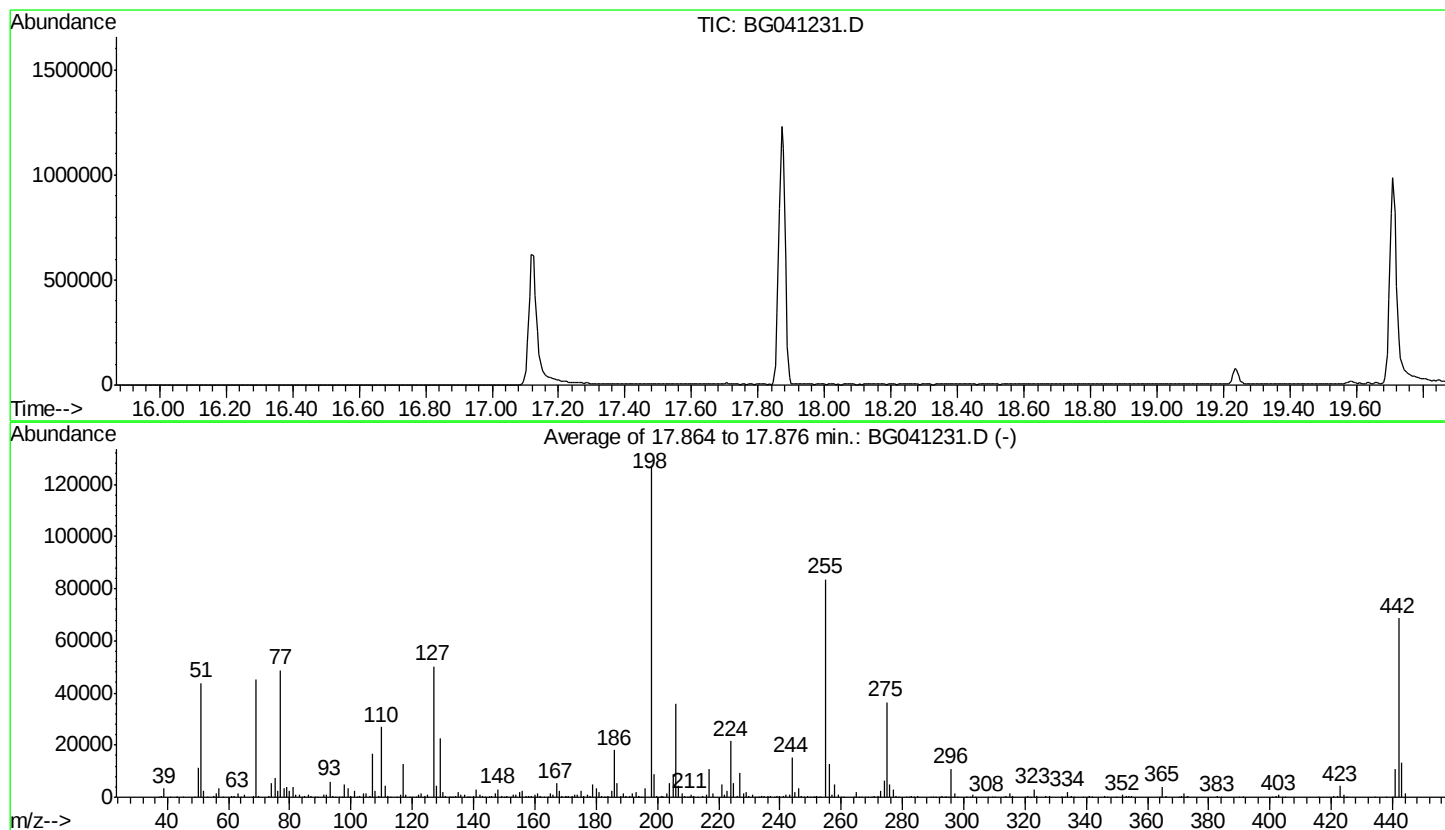

AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2509

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.5	43874	PASS
68	69	0.00	2	0.7	310	PASS
69	198	0.00	100	35.4	44976	PASS
70	69	0.00	2	0.7	316	PASS
127	198	10	80	39.6	50314	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	127181	PASS
199	198	5	9	6.8	8687	PASS
275	198	10	60	28.6	36368	PASS
365	198	1	100	3.2	4061	PASS
441	198	0.01	100	8.4	10630	PASS
442	198	50	100	53.9	68573	PASS
443	442	15	24	19.0	13039	PASS