
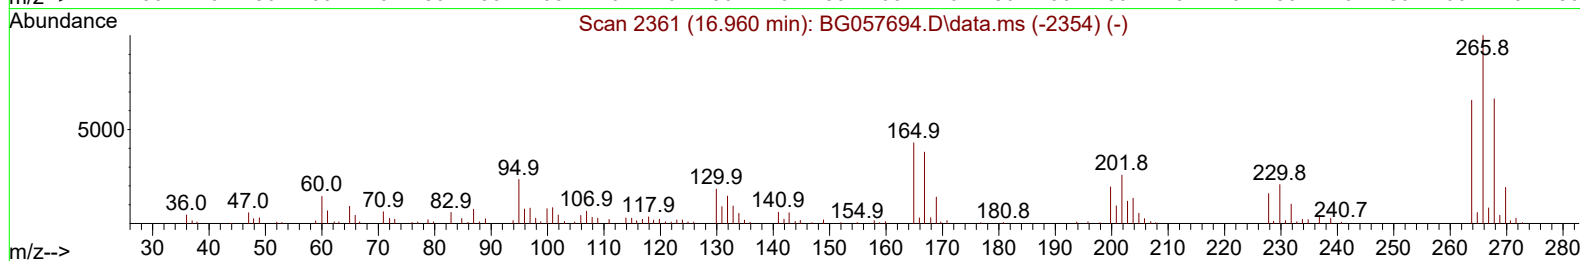
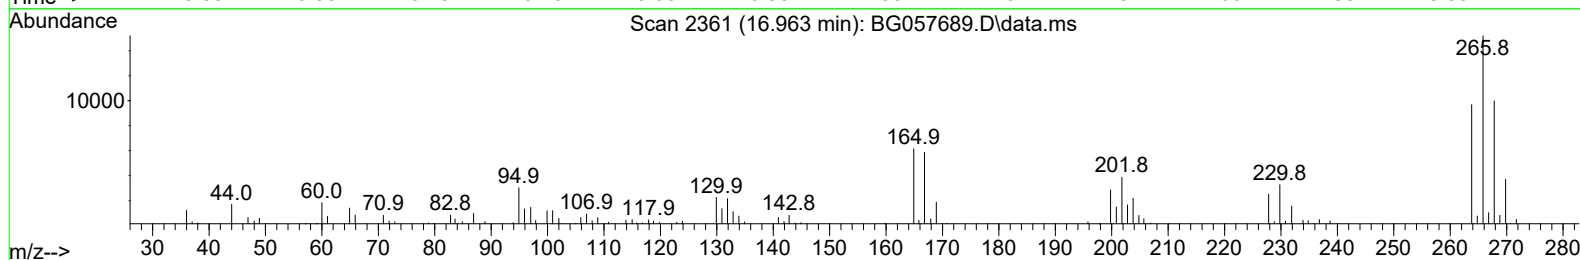


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061323\
Data File : BG057689.D
Acq On : 13 Jun 2023 15:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 14 06:03:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 14 03:52:08 2023
Response via : Initial Calibration

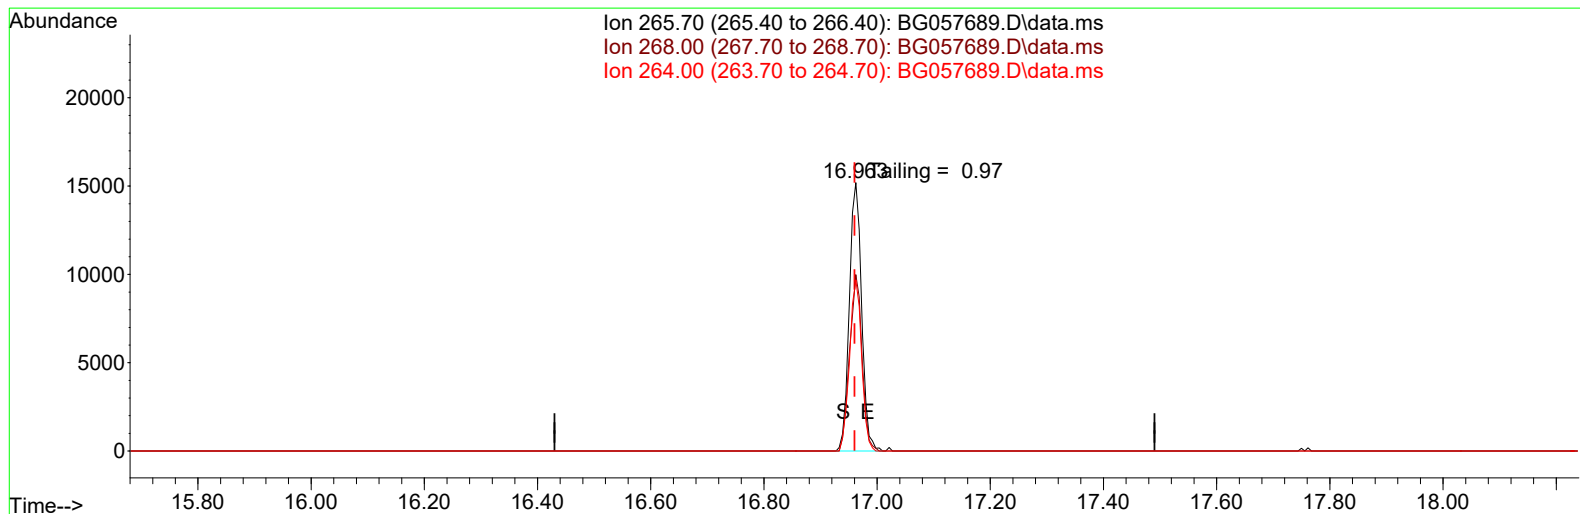

TIC: BG057689.D\data.ms

(70) Pentachlorophenol (C)




16.963min (+ 0.003) 16220.31 ng

response 22901

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	65.73
264.00	65.50	63.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061323\
Data File : BG057689.D
Acq On : 13 Jun 2023 15:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 14 06:03:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 14 03:52:08 2023
Response via : Initial Calibration

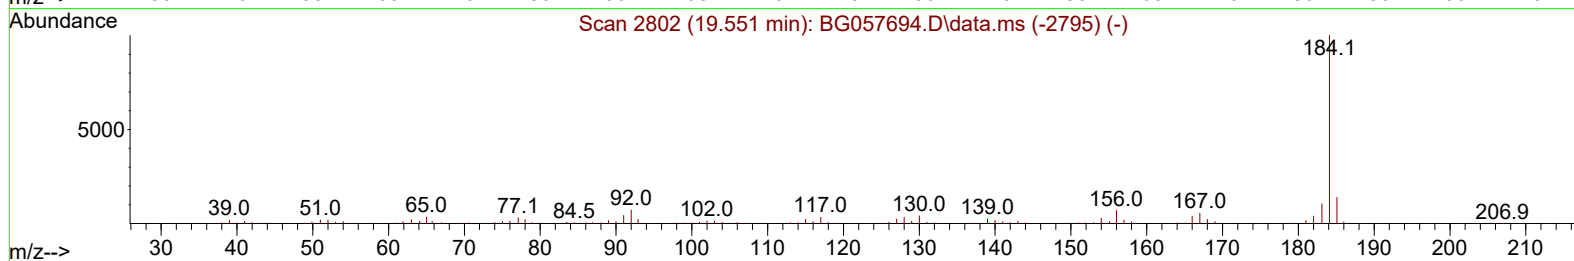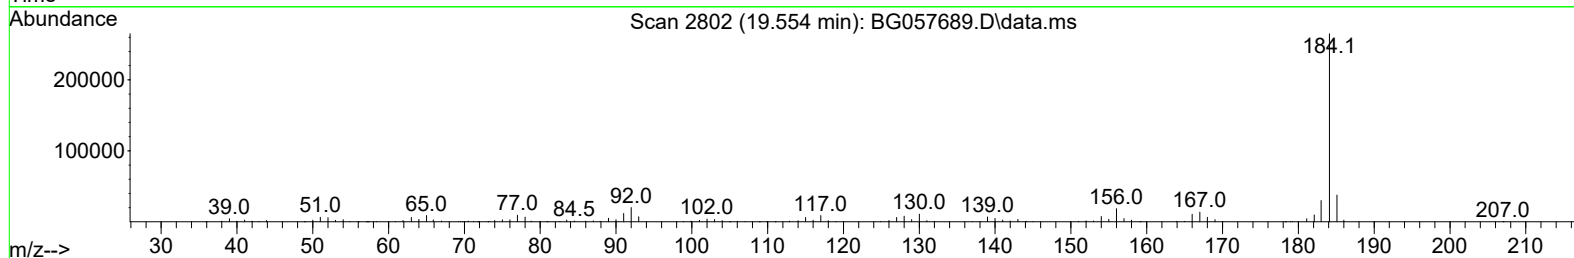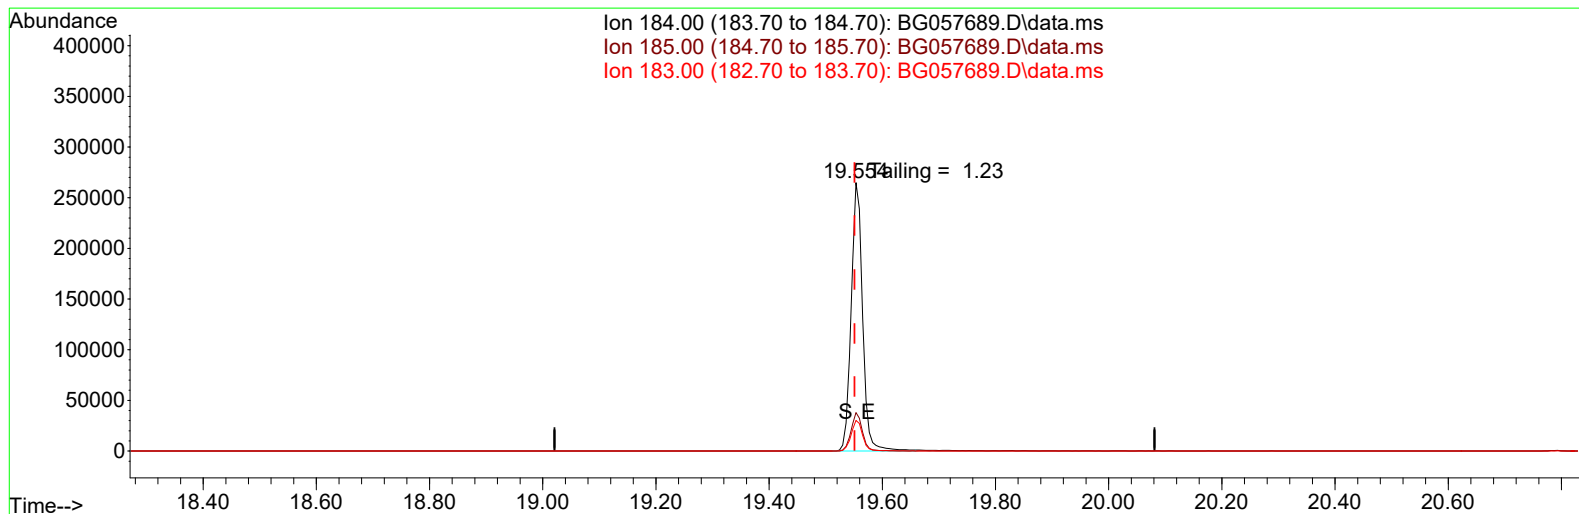

TIC: BG057689.D\data.ms

(77) Benzidine

19.554min (+ 0.003) 0.00 ng

response 373729

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.29
183.00	10.50	11.39
0.00	0.00	0.00