
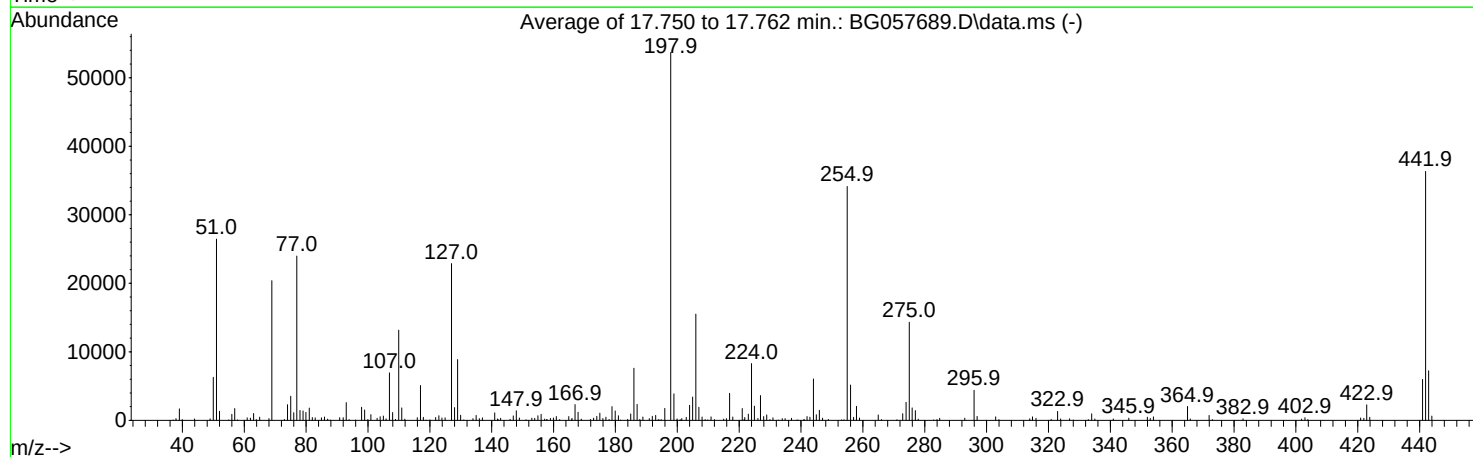


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061323\
 Data File : BG057689.D
 Acq On : 13 Jun 2023 15:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061323.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 14 03:52:08 2023

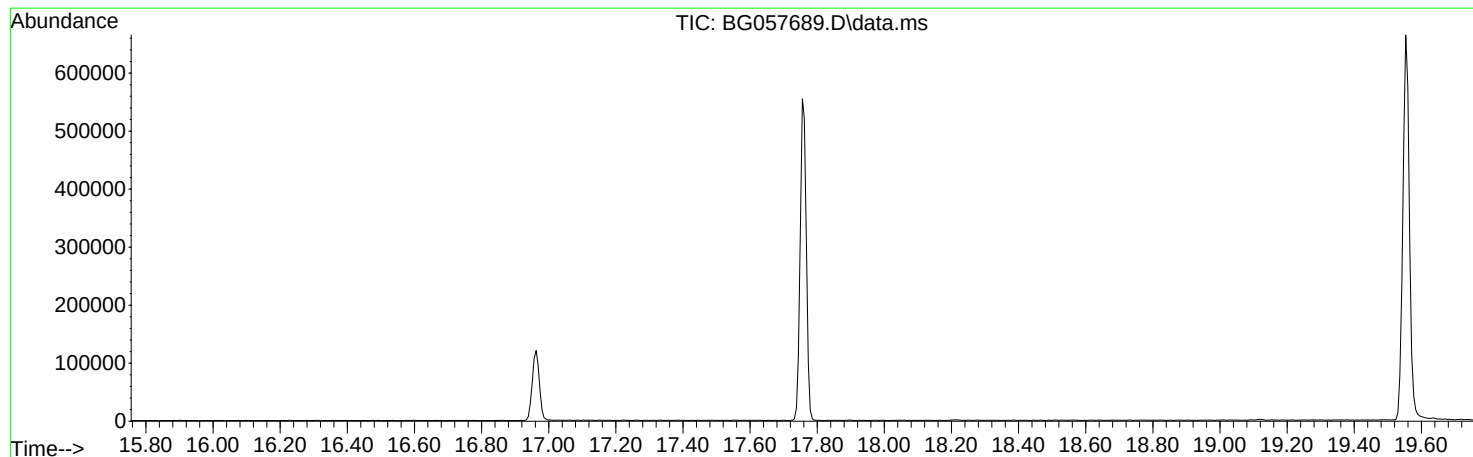

AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.3	26464	PASS
68	69	0.00	2	1.3	264	PASS
69	198	0.00	100	38.0	20390	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.6	22880	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	53680	PASS
199	198	5	9	7.2	3888	PASS
275	198	10	60	26.7	14313	PASS
365	198	1	100	3.8	2025	PASS
441	198	0.01	100	11.2	5987	PASS
442	442	50	100	100.0	36341	PASS
443	442	15	24	19.9	7234	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/13/2023	BNA_G	<u>BG057689.D</u>
Compound Name	Response	Retention Time
DDT	72660	20.787
DDD	647	20.4
DDE	0	20.162
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
647	73307	0.88

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061323\
Data File : BG057689.D
Acq On : 13 Jun 2023 15:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 14 06:03:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 14 03:52:08 2023
Response via : Initial Calibration

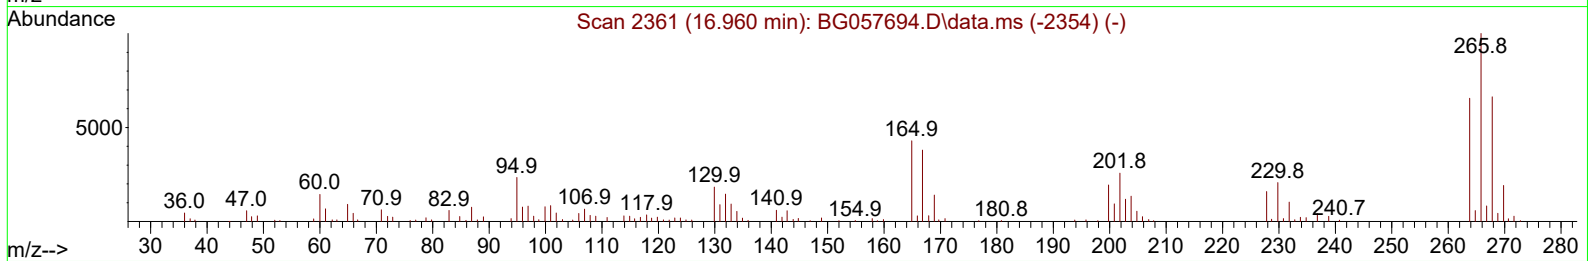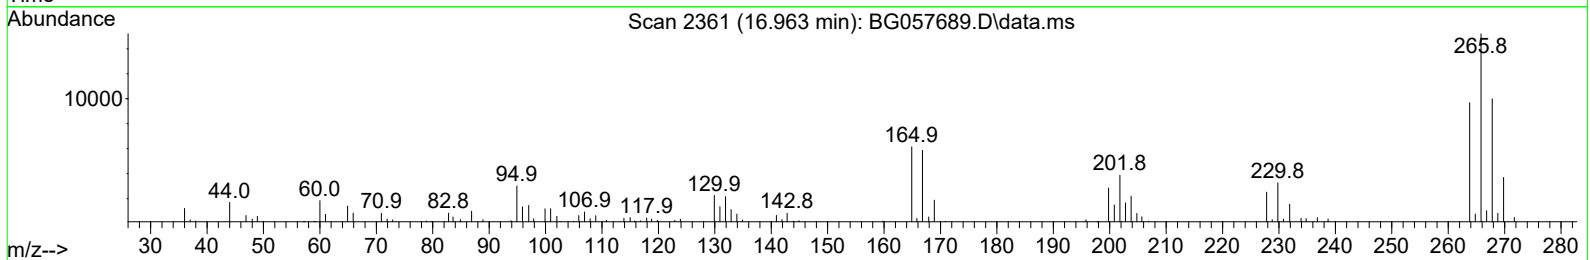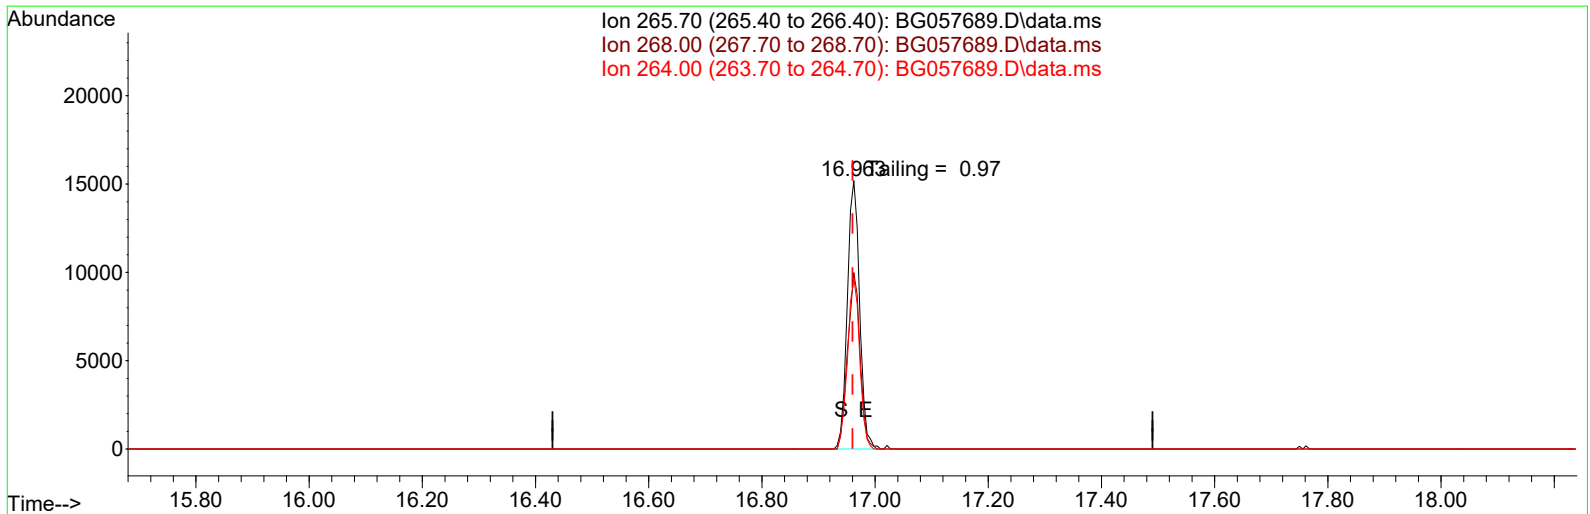

TIC: BG057689.D\data.ms

(70) Pentachlorophenol (C)

16.963min (+ 0.003) 16220.31 ng




response 22901

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	65.73
264.00	65.50	63.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061323\
Data File : BG057689.D
Acq On : 13 Jun 2023 15:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 14 06:03:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 14 03:52:08 2023
Response via : Initial Calibration

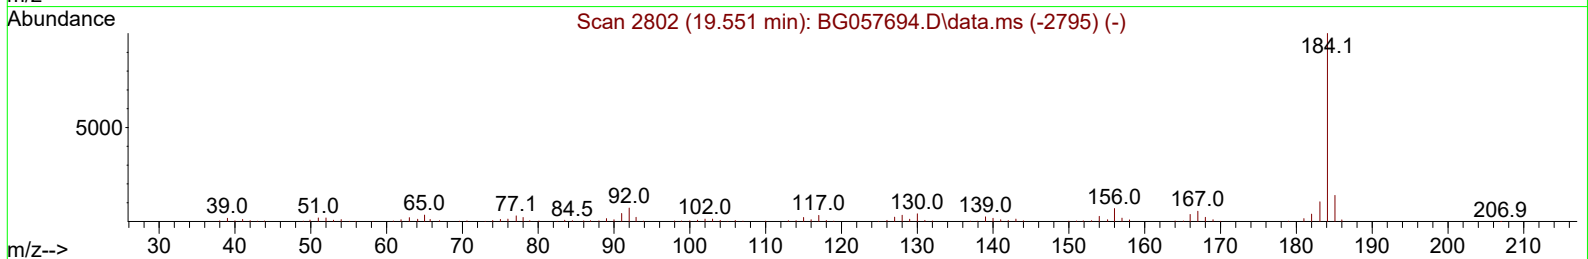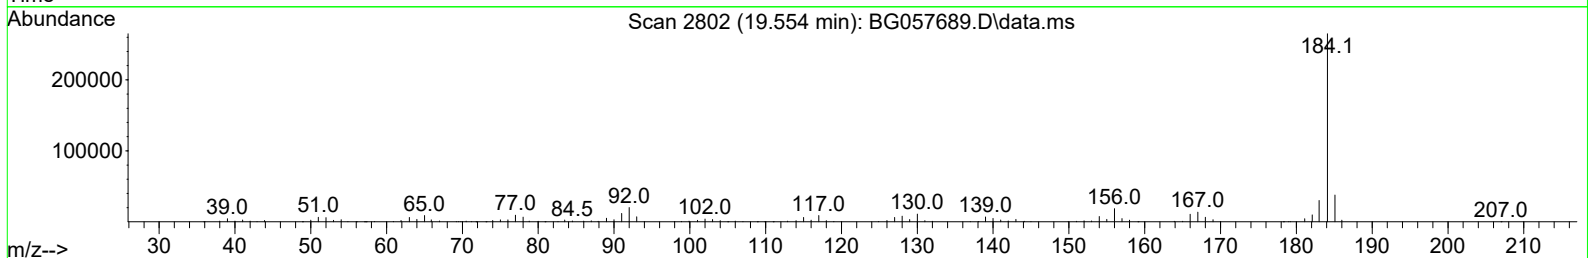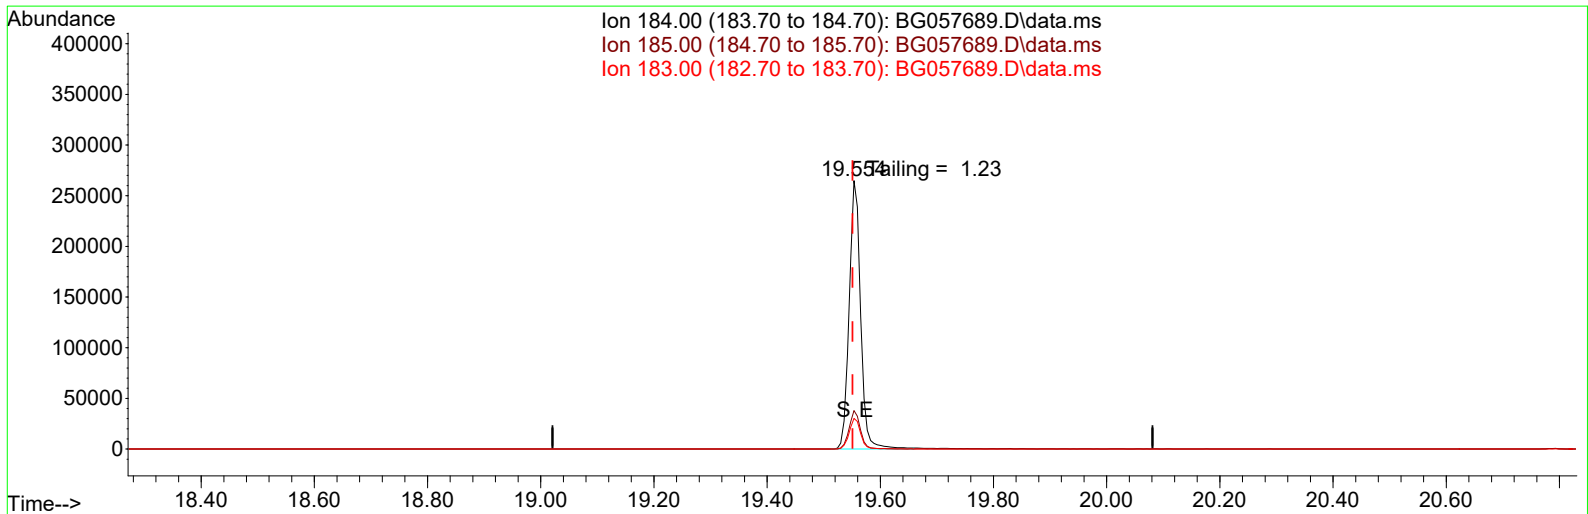

TIC: BG057689.D\data.ms

(77) Benzidine

19.554min (+ 0.003) 0.00 ng

response 373729

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.29
183.00	10.50	11.39
0.00	0.00	0.00