
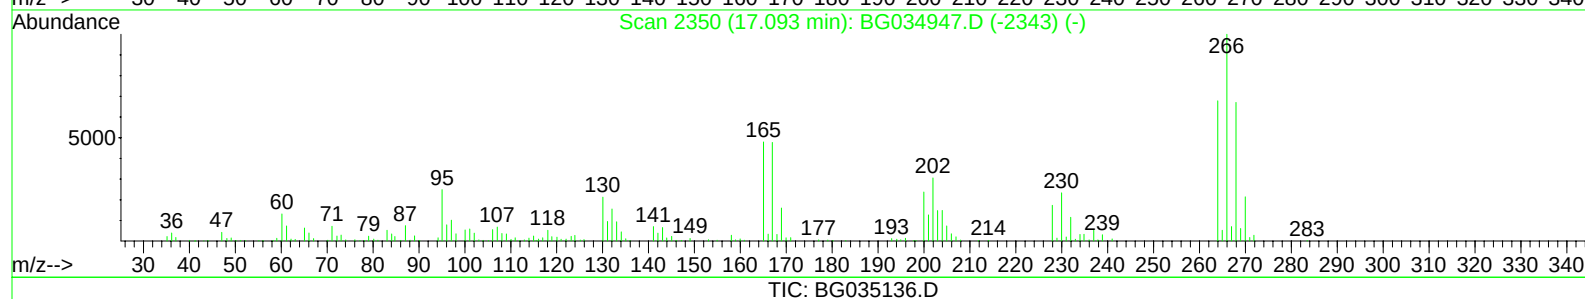
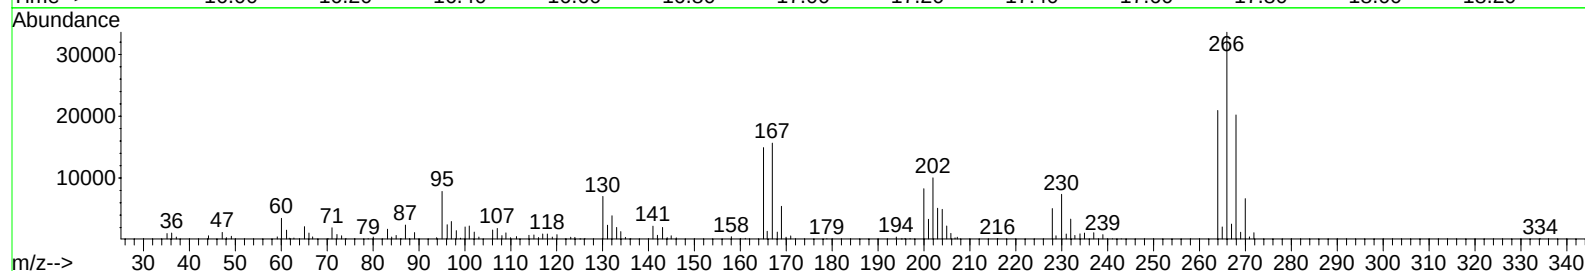


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG061418\
Data File : BG035136.D
Acq On : 14 Jun 2018 14:00
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 14 18:05:18 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

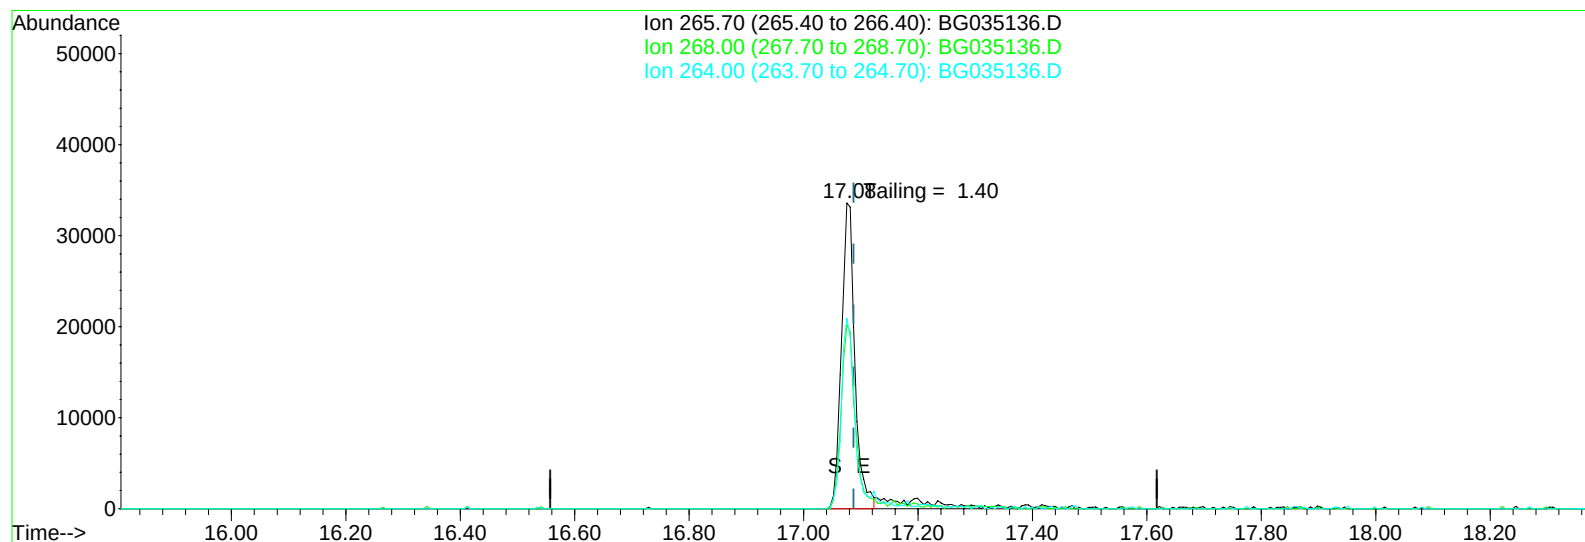

(69) Pentachlorophenol (C)




17.076min (-0.012) 0.00ng

response 57288

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.13
264.00	62.00	62.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG061418\
Data File : BG035136.D
Acq On : 14 Jun 2018 14:00
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 14 18:05:18 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

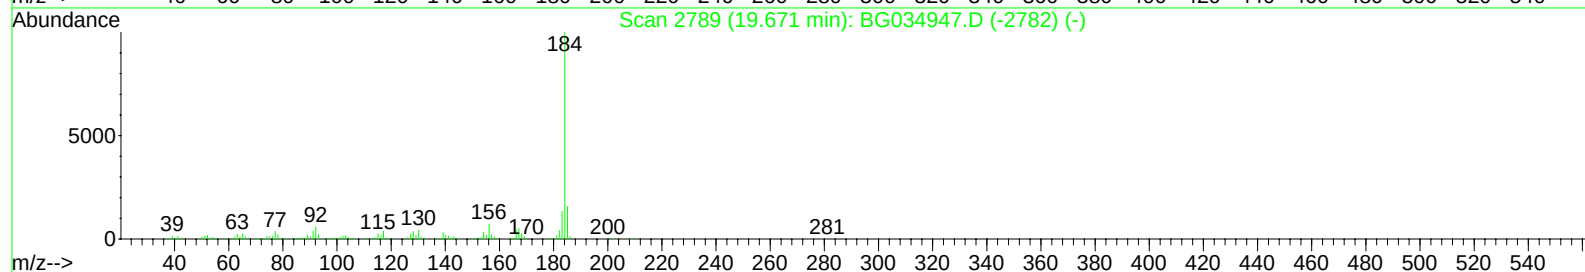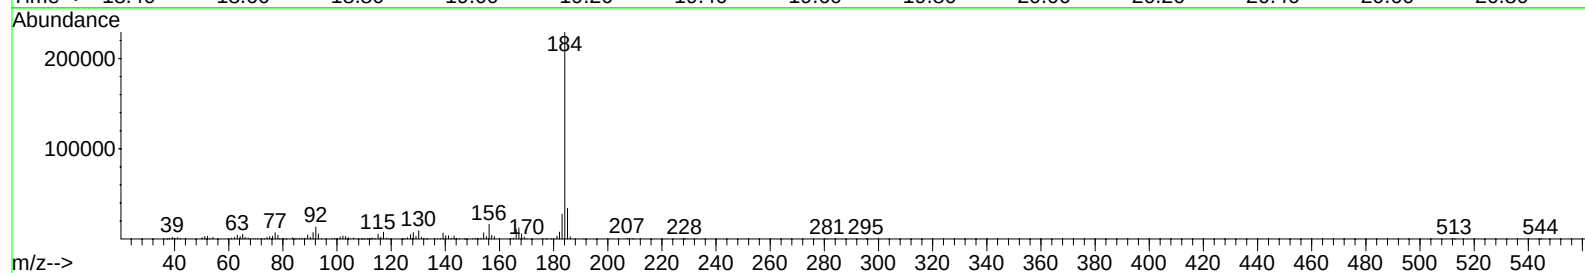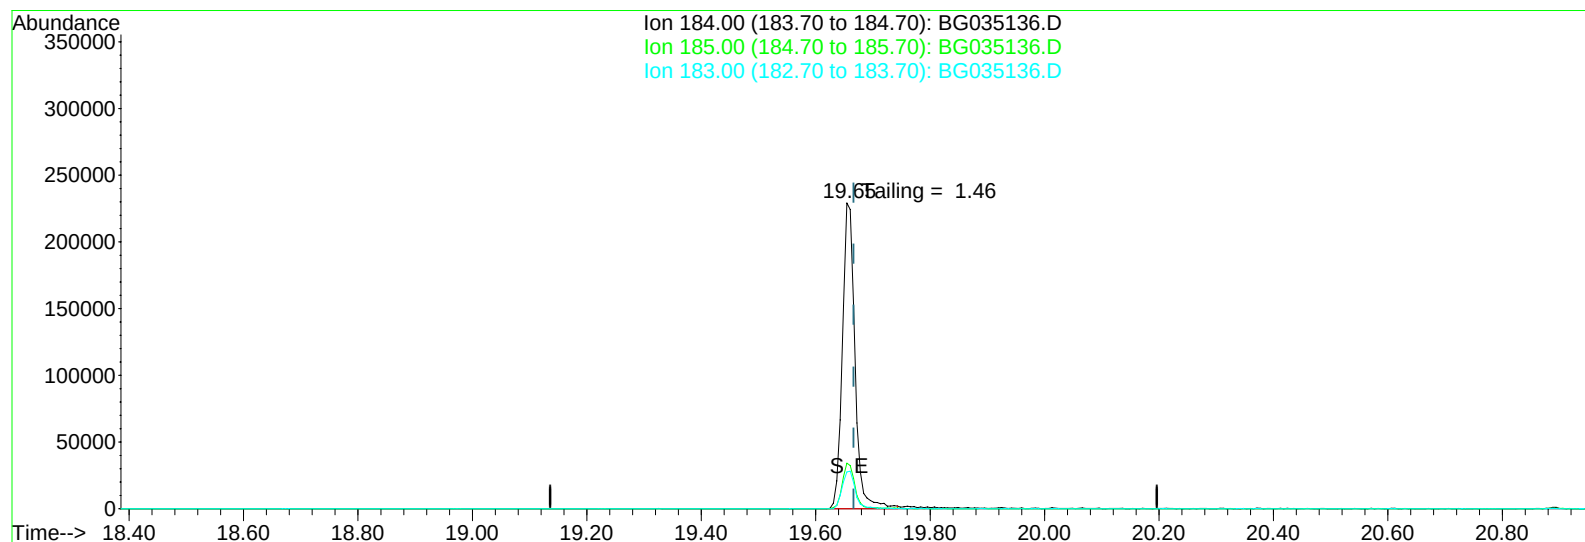

TIC: BG035136.D

(76) Benzidine

19.655min (-0.012) 149520.29ng

response 350450

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.92
183.00	13.30	12.05
0.00	0.00	0.00