
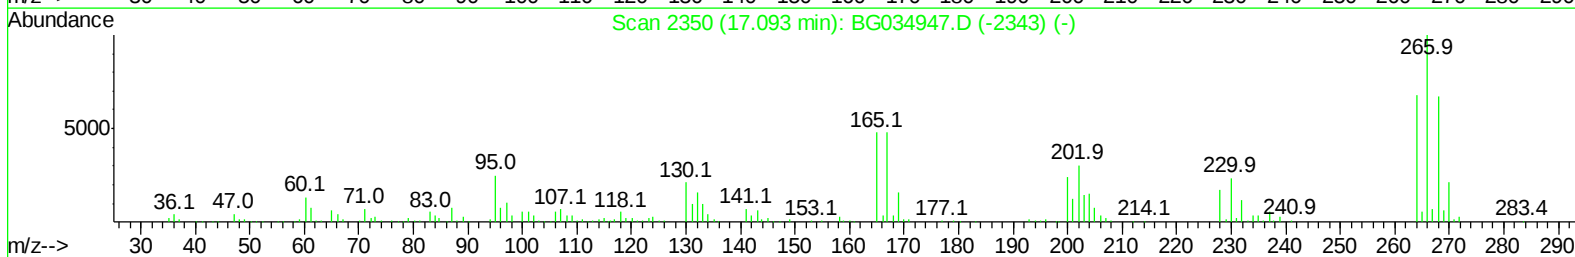
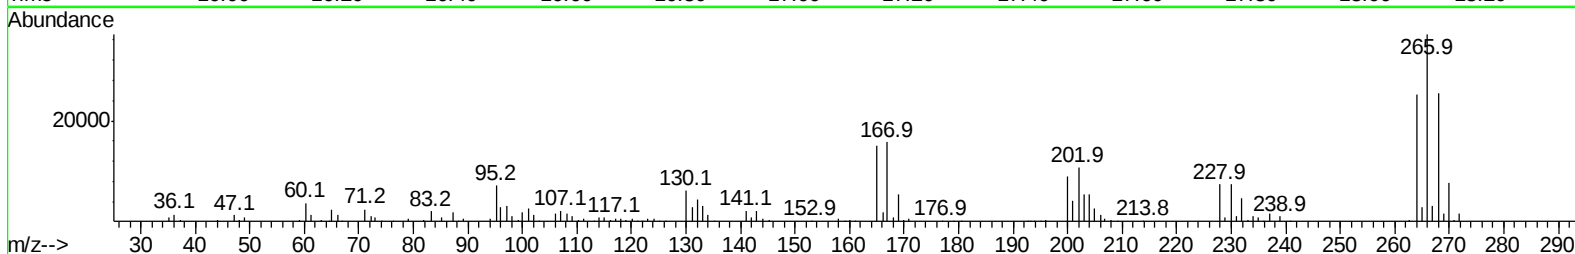


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061418\
Data File : BG035155.D
Acq On : 15 Jun 2018 2:56
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 15 07:26:34 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

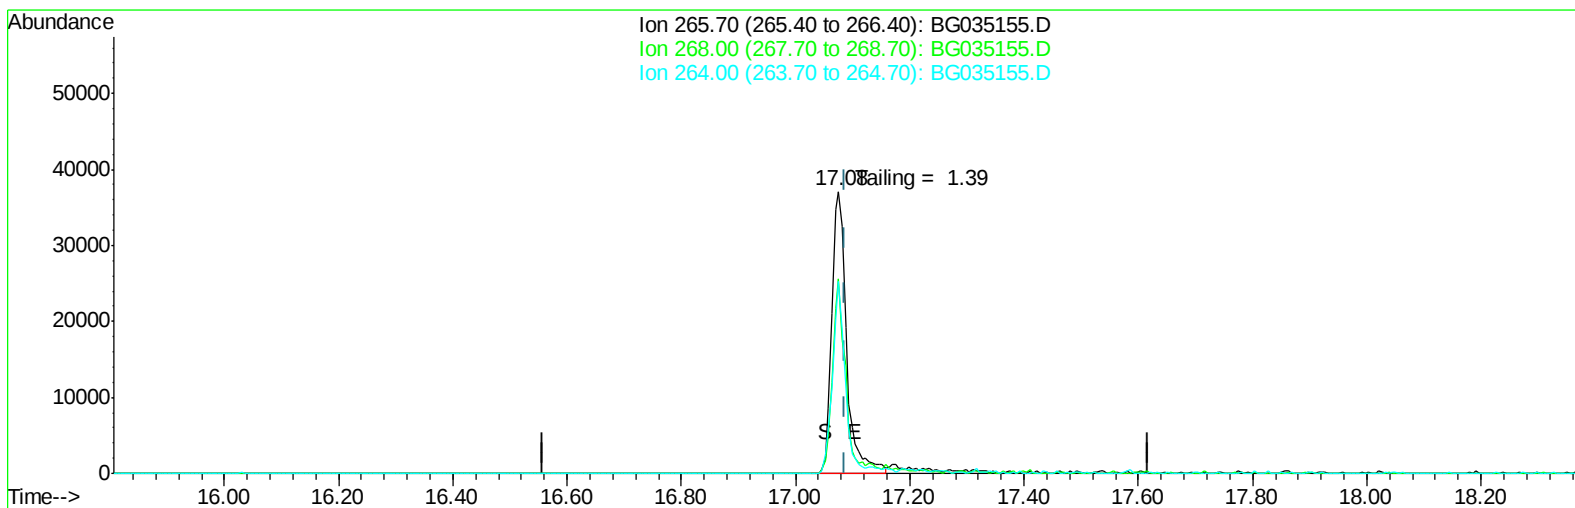

TIC: BG035155.D

(69) Pentachlorophenol (C)




17.075min (-0.012) 149449.76ng

response 66516

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	68.96
264.00	62.00	68.22
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061418\
 Data File : BG035155.D
 Acq On : 15 Jun 2018 2:56
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 15 07:26:34 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 08 17:16:28 2018
 Response via : Initial Calibration

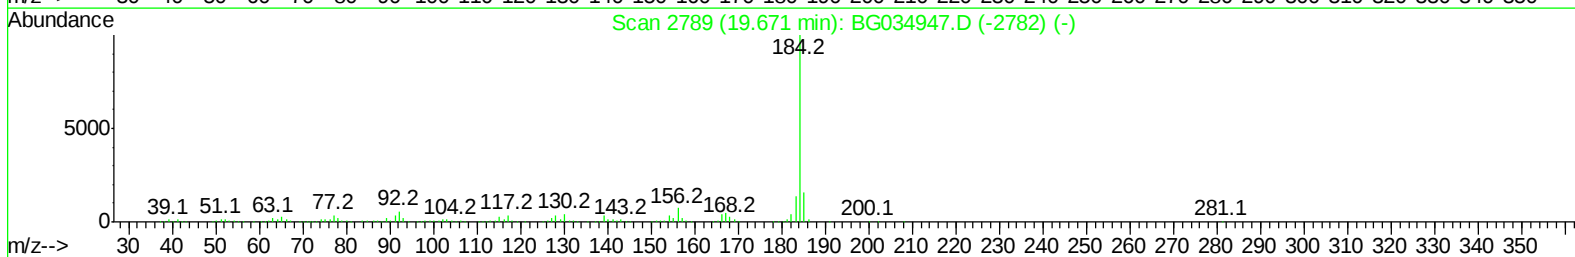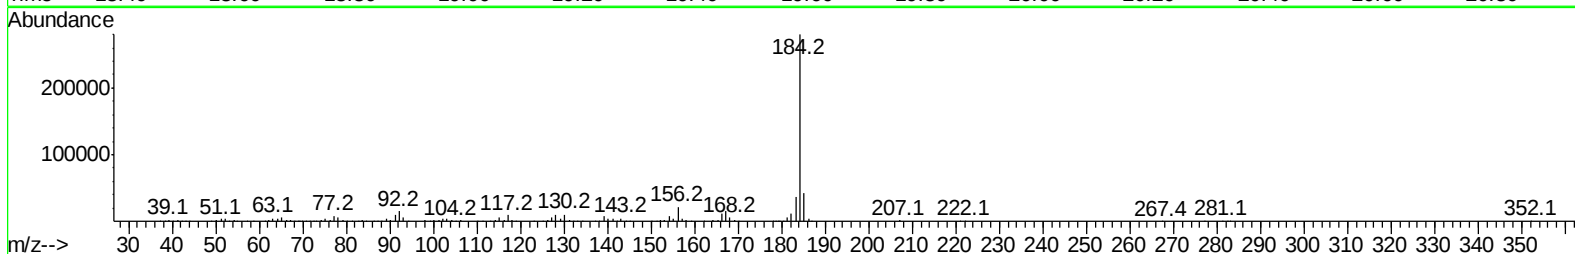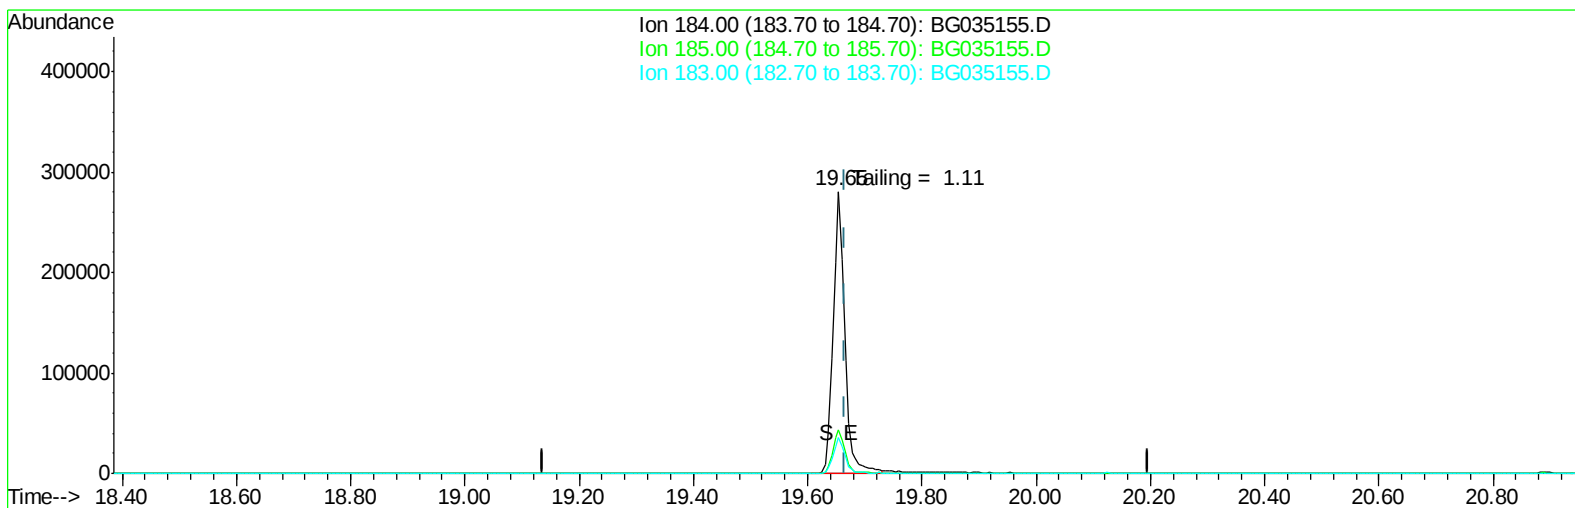

TIC: BG035155.D

(76) Benzidine

19.654min (-0.012) 169407.84ng

response 397063

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.41
183.00	13.30	12.80
0.00	0.00	0.00