

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061418\
 Data File : BG035171.D
 Acq On : 15 Jun 2018 13:15
 Operator : SJ/JU
 Sample : J3442-02
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CAS1-WC-S-01-1-57

Quant Time: Jun 15 14:21:30 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 08 17:16:28 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.07	152	44125	20.00	ng	0.00
21) Naphthalene-d8	10.87	136	175823	20.00	ng	-0.02
38) Acenaphthene-d10	14.69	164	133385	20.00	ng	0.00
63) Phenanthrene-d10	17.42	188	376206	20.00	ng	-0.02
75) Chrysene-d12	21.70	240	410299	20.00	ng	-0.02
86) Perylene-d12	24.93	264	342902	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.63	112	307243	117.51	ng	0.00
7) Phenol-d6	7.21	99	415847	107.76	ng	0.00
23) Nitrobenzene-d5	9.22	82	344914	93.25	ng	-0.02
41) 2,4,6-Tribromophenol	16.17	330	238416	139.63	ng	-0.02
44) 2-Fluorobiphenyl	13.31	172	824039	80.31	ng	-0.02
78) Terphenyl-d14	20.03	244	1648721	84.17	ng	-0.02


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061418\
Data File : BG035171.D
Acq On : 15 Jun 2018 13:15
Operator : SJ/JU
Sample : J3442-02
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CAS1-WC-S-01-1-57

Quant Time: Jun 15 14:21:30 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

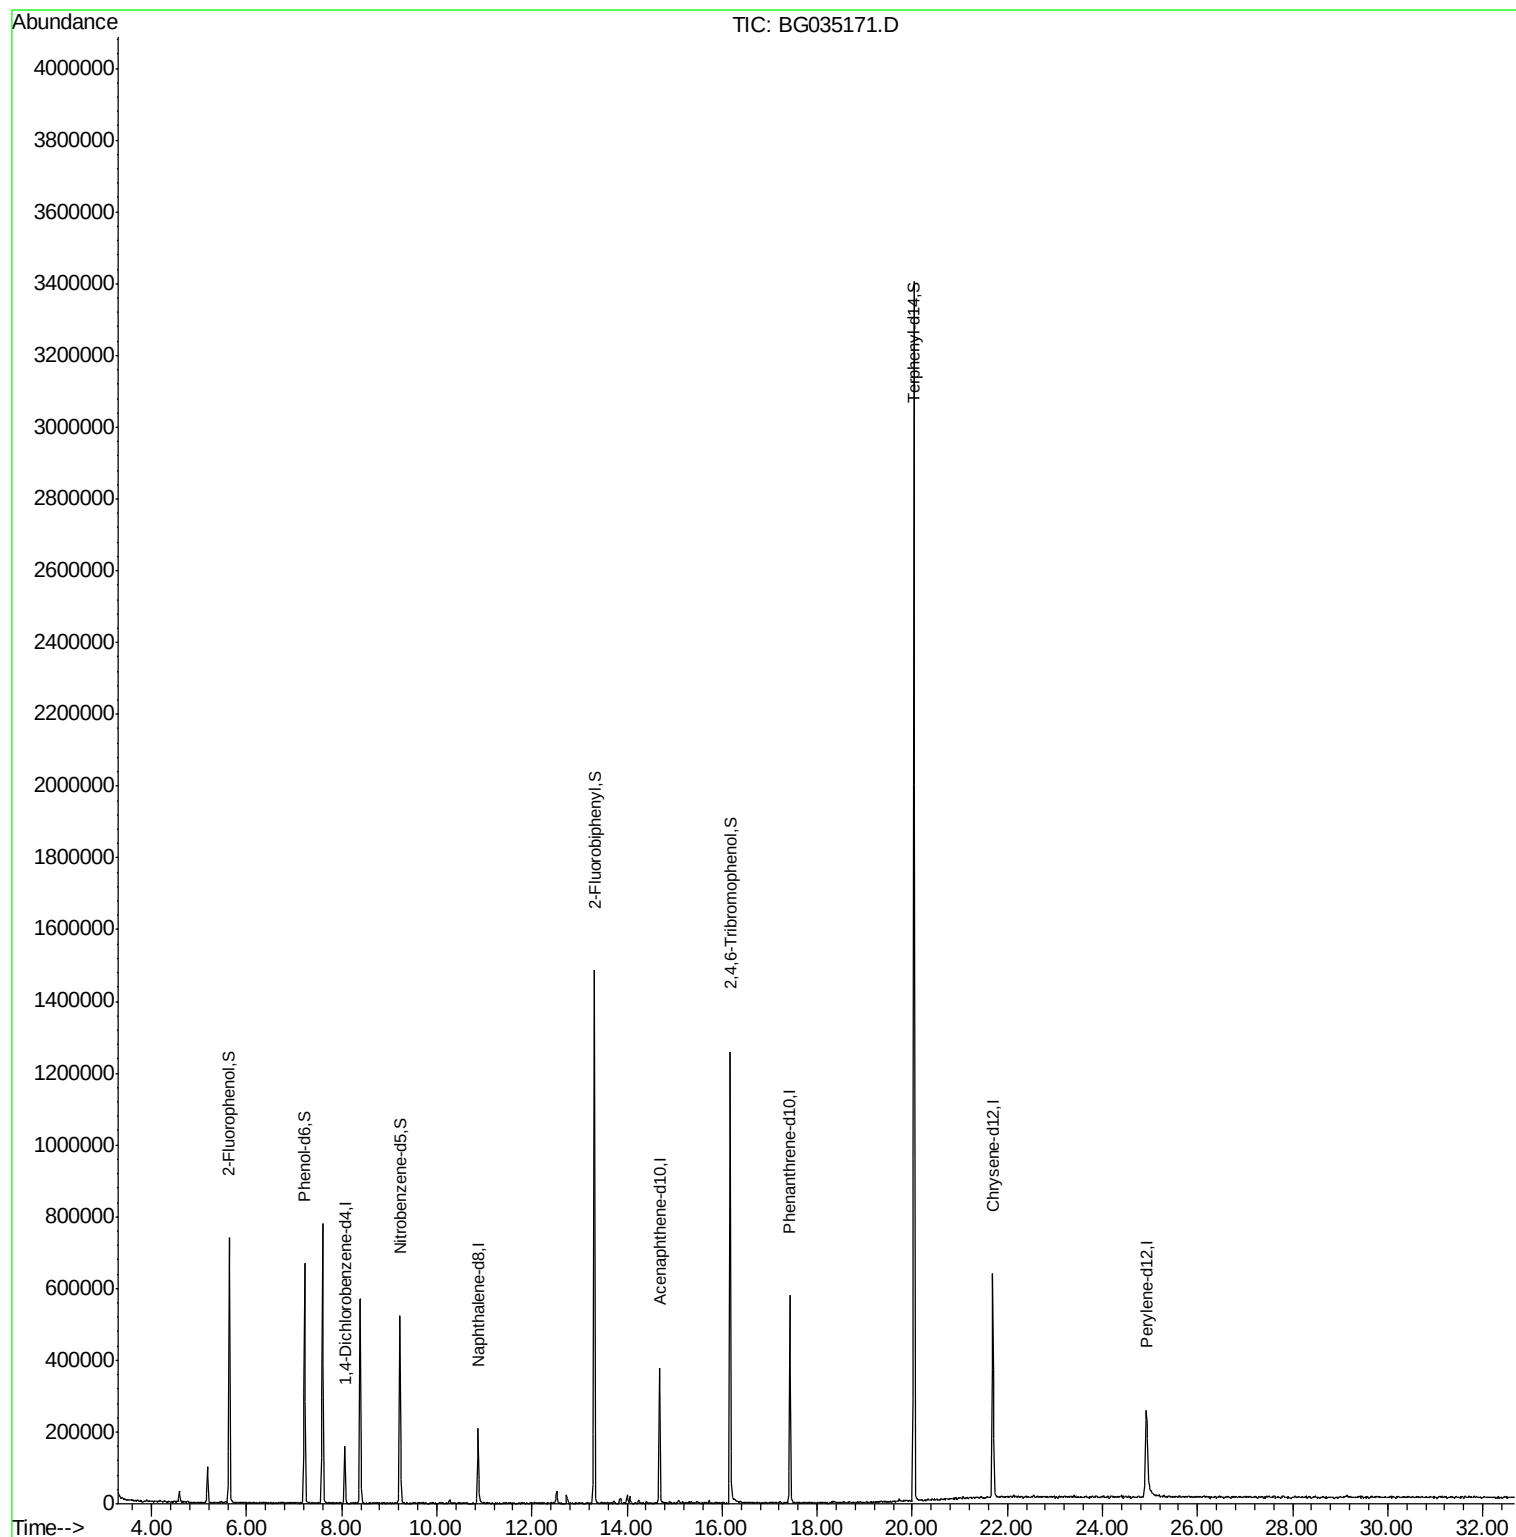

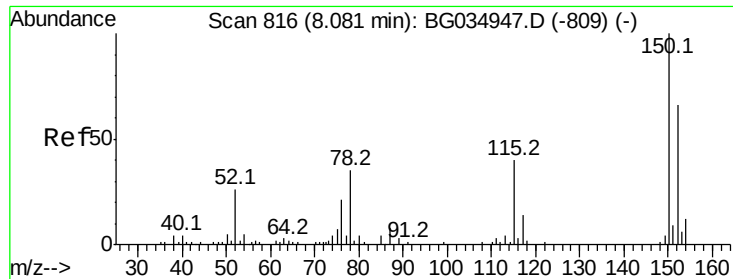


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.07 min Scan# 813
Delta R.T. -0.01 min
Lab File: BG035171.D
Acq: 15 Jun 2018 13:15

Instrument :
BNA_G
ClientSampleId :
CAS1-WC-S-01-1-57

Tot Ion:152 Resp: 44125
Ion Ratio Lower Upper
152 100
150 148.1 126.6 189.8
115 61.6 53.0 79.4

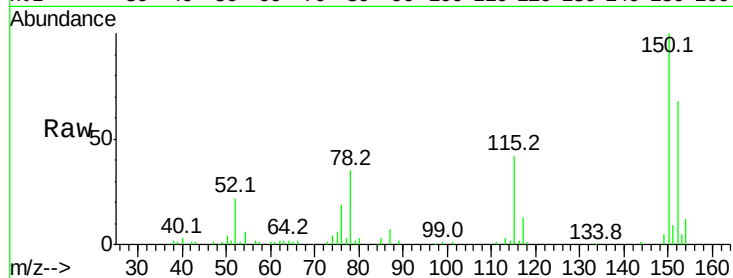


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

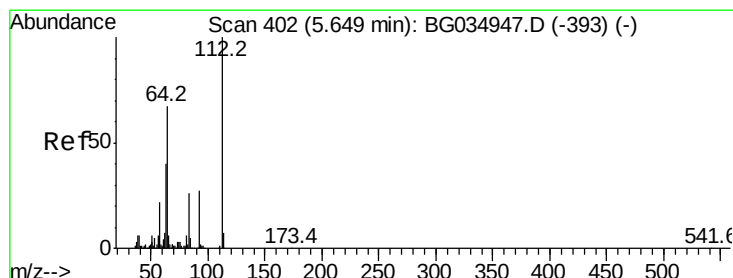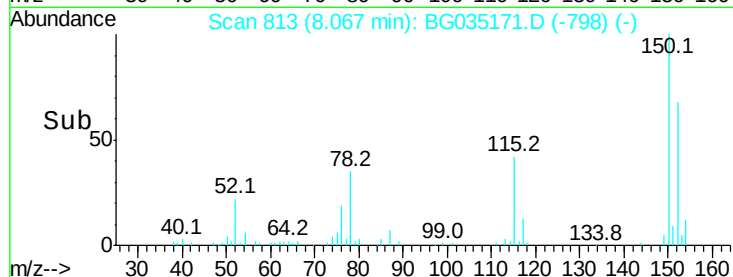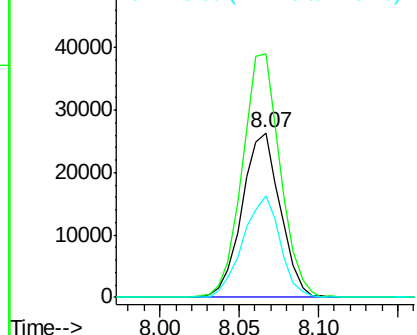



#5


2-Fluorophenol
Concen: 117.508 ng
RT: 5.63 min Scan# 399
Delta R.T. -0.01 min
Lab File: BG035171.D
Acq: 15 Jun 2018 13:15

Tgt Ion:112 Resp: 307243
Ion Ratio Lower Upper
112 100
64 62.9 56.3 84.5
63 33.8 30.1 45.1

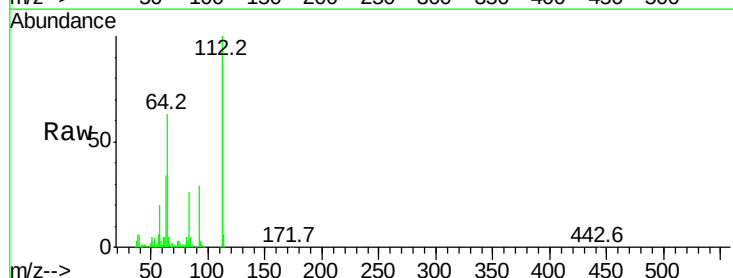

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

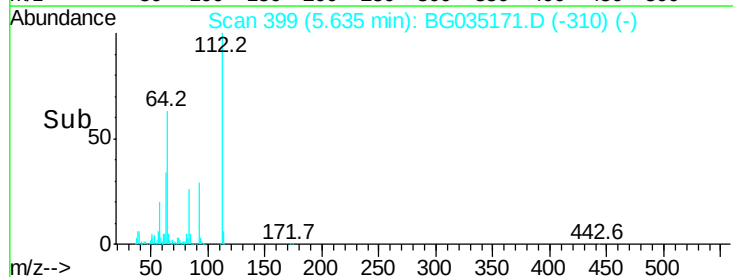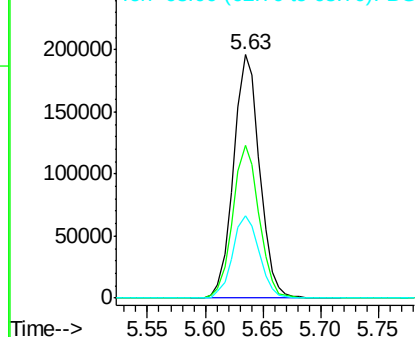

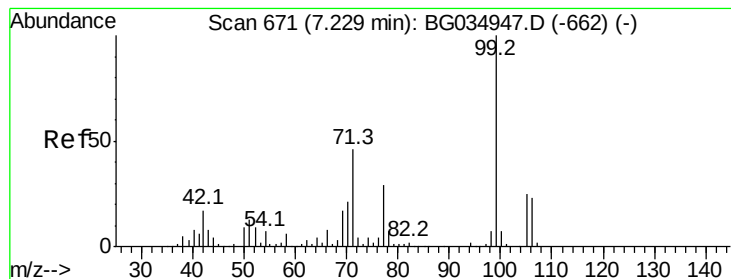

#7

Phenol-d6

Concen: 107.758 ng

RT: 7.21 min Scan# 668

Delta R.T. -0.01 min

Lab File: BG035171.D

Acq: 15 Jun 2018 13:15

Instrument :

BNA_G

ClientSampleId :

CAS1-WC-S-01-1-57


Tot Ion: 99 Resp: 415847

Ion Ratio Lower Upper




99 100

42 14.6 14.1 21.1

71 41.7 26.1 39.1#

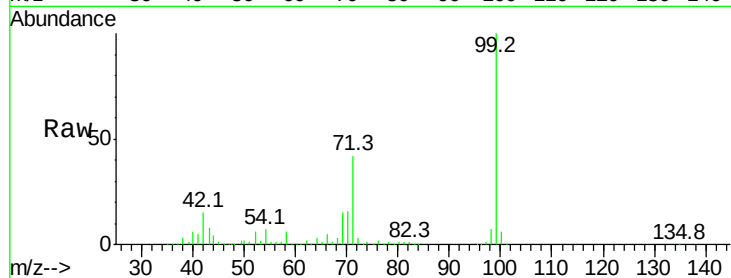

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

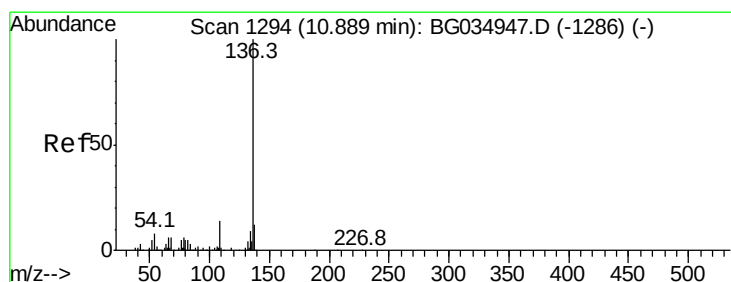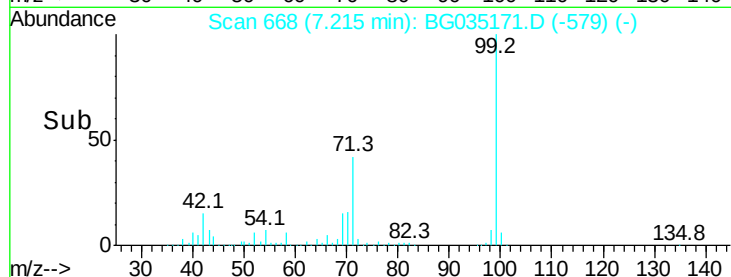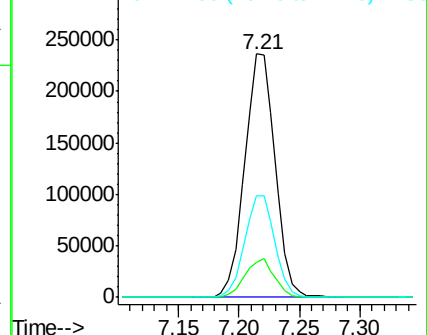

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.87 min Scan# 1290

Delta R.T. -0.02 min

Lab File: BG035171.D

Acq: 15 Jun 2018 13:15

Tgt Ion: 136 Resp: 175823


Ion Ratio Lower Upper

136 100



137 10.9 9.2 13.8


54 7.5 10.3 15.5#

68 5.5 4.5 6.7

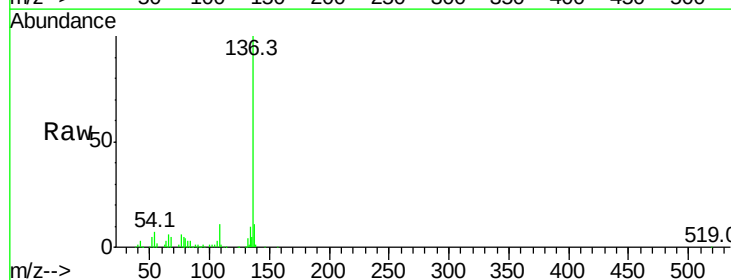

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



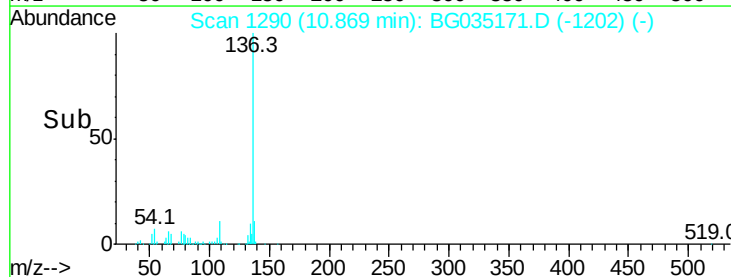
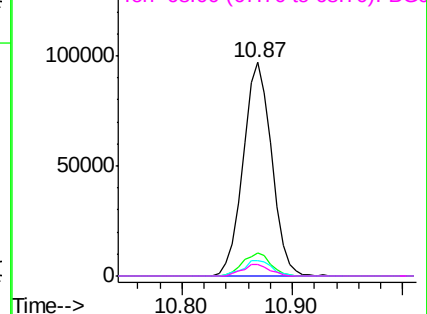


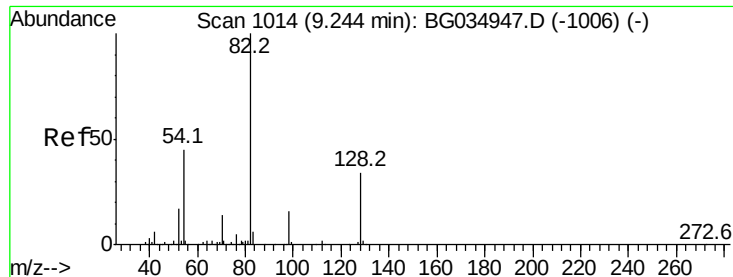

#23
Nitrobenzene-d5
Concen: 93.249 ng
RT: 9.22 min Scan# 1010
Delta R.T. -0.02 min
Lab File: BG035171.D
Acq: 15 Jun 2018 13:15




Instrument :
BNA_G
ClientSampleId :
CAS1-WC-S-01-1-57


Tot Ion	82	Resp	344914
Ion Ratio	100	Lower	Upper
128	37.2	29.7	44.5
54	45.1	43.1	64.7

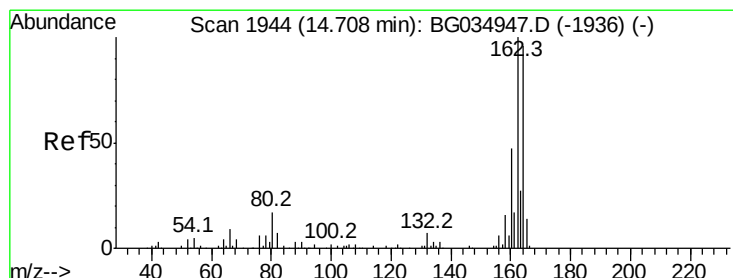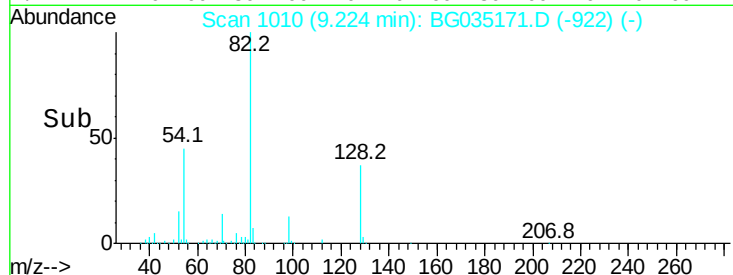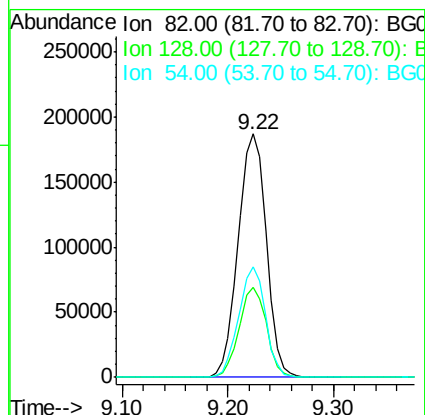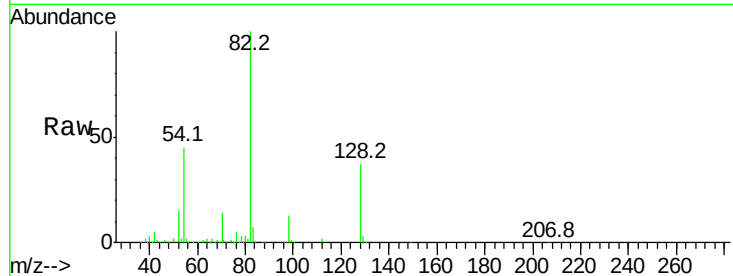

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.69 min Scan# 1940
Delta R.T. -0.01 min
Lab File: BG035171.D
Acq: 15 Jun 2018 13:15

Tgt Ion	164	Resp	133385
Ion Ratio	100	Lower	Upper
162	107.6	78.8	118.2
160	47.7	35.4	53.0

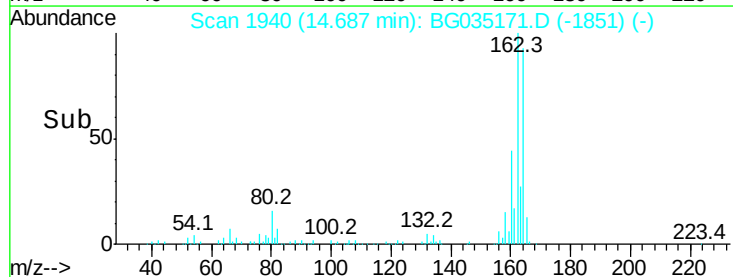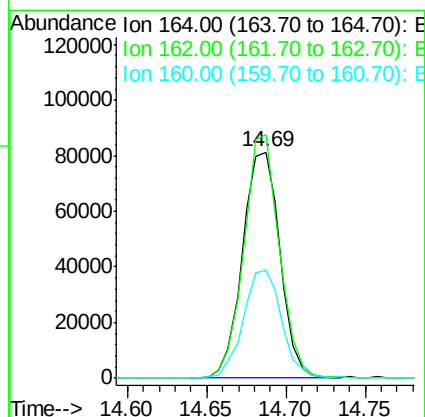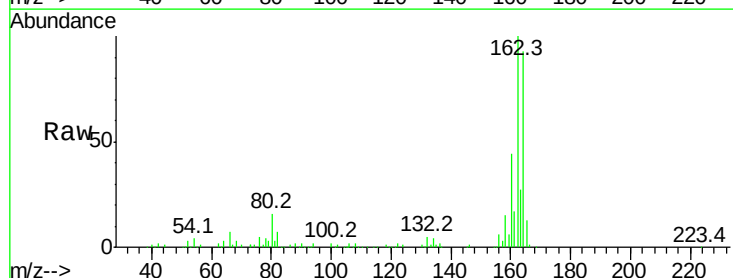


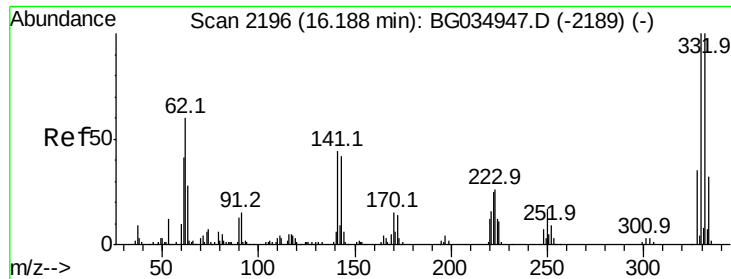




#41
 2,4,6-Tribromophenol
 Concen: 139.629 ng
 RT: 16.17 min Scan# 2192
 Delta R.T. -0.02 min
 Lab File: BG035171.D
 Acq: 15 Jun 2018 13:15

Instrument :
 BNA_G
 ClientSampleId :
 CAS1-WC-S-01-1-57

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.9	77.0	115.6
141	38.0	25.2	37.8#

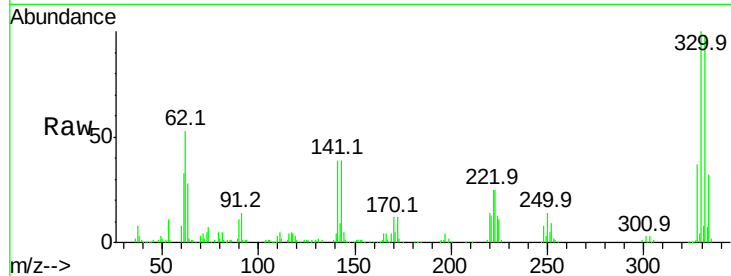


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

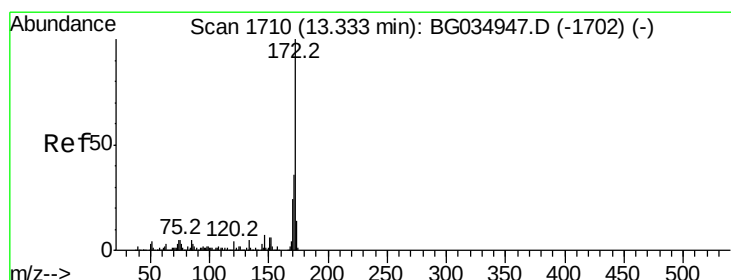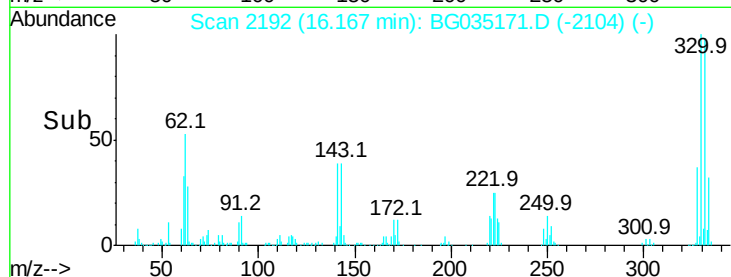
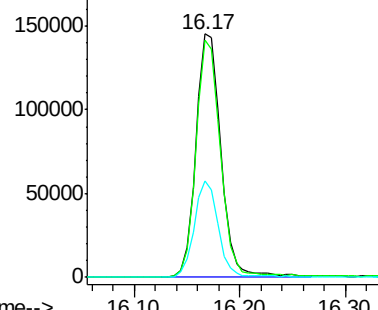



#44
 2-Fluorobiphenyl
 Concen: 80.312 ng
 RT: 13.31 min Scan# 1706
 Delta R.T. -0.02 min
 Lab File: BG035171.D
 Acq: 15 Jun 2018 13:15

Tgt Ion	Ratio	Lower	Upper
172	100		
171	34.0	30.0	45.0
170	23.7	19.5	29.3

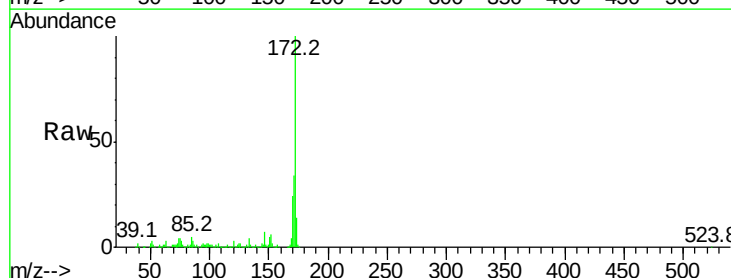

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

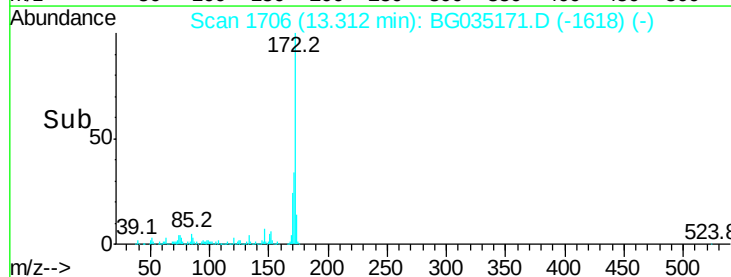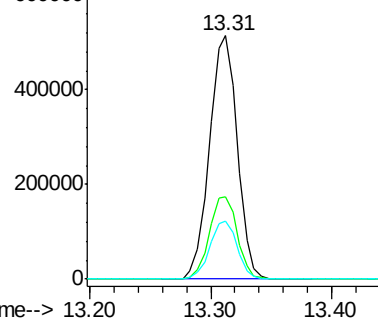

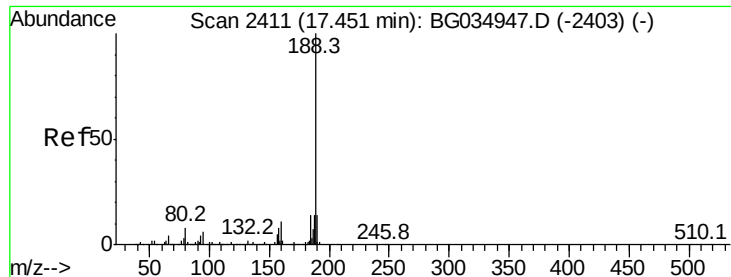

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.42 min Scan# 2406

Delta R.T. -0.02 min

Lab File: BG035171.D

Acq: 15 Jun 2018 13:15

Instrument :

BNA_G

ClientSampleId :

CAS1-WC-S-01-1-57


Tot Ion:188 Resp: 376206

Ion Ratio Lower Upper

188 100

94 6.5 6.9 10.3#




80 8.4 7.7 11.5

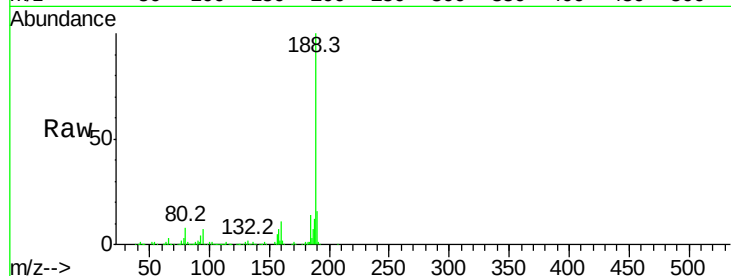

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

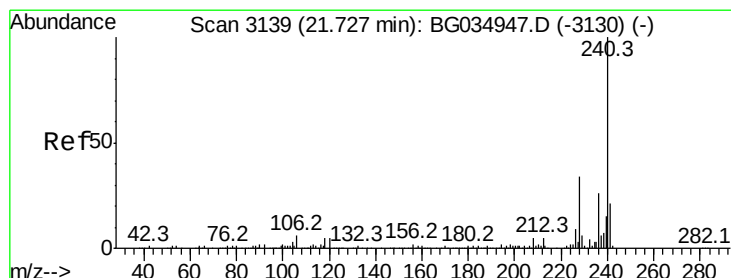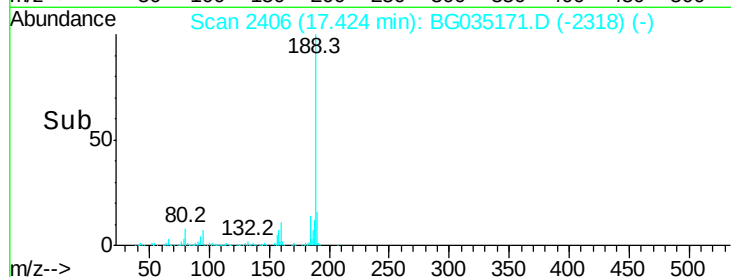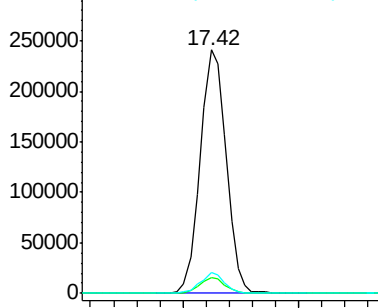

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.70 min Scan# 3133

Delta R.T. -0.02 min

Lab File: BG035171.D

Acq: 15 Jun 2018 13:15


Tgt Ion:240 Resp: 410299

Ion Ratio Lower Upper

240 100

120 5.6 6.8 10.2#



236 27.5 20.9 31.3

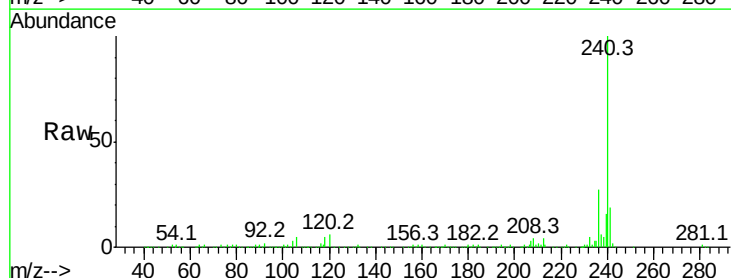


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

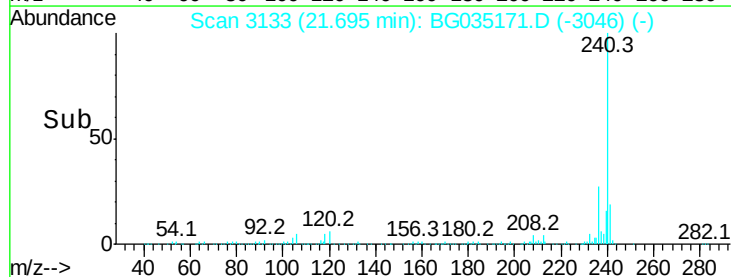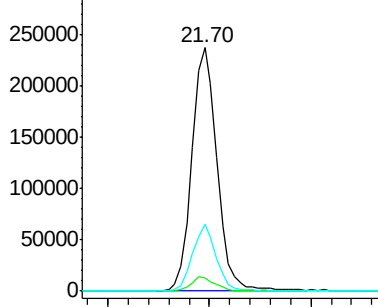

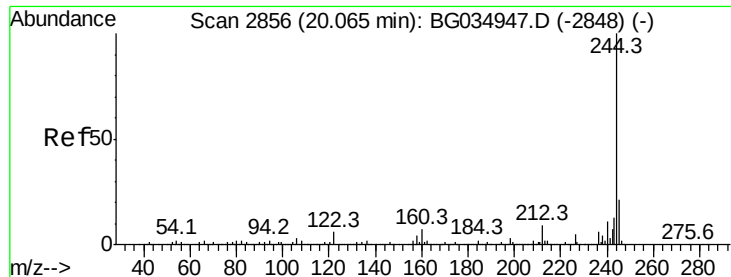

#78

Terphenyl-d14

Concen: 84.171 ng

RT: 20.03 min Scan# 2850

Delta R.T. -0.02 min

Lab File: BG035171.D

Acq: 15 Jun 2018 13:15

Instrument :

BNA_G

ClientSampleId :

CAS1-WC-S-01-1-57


Tot Ion:244 Resp: 1648721

Ion Ratio Lower Upper

244 100

212 9.6 5.8 8.8#




122 7.4 7.0 10.4

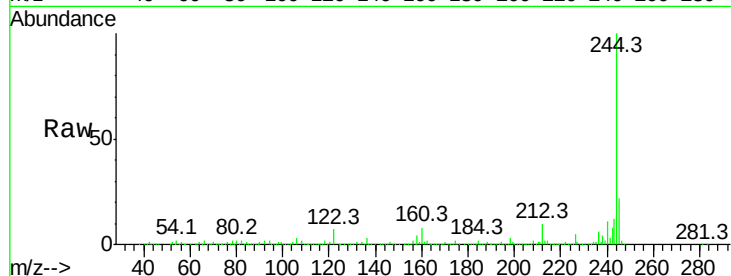

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

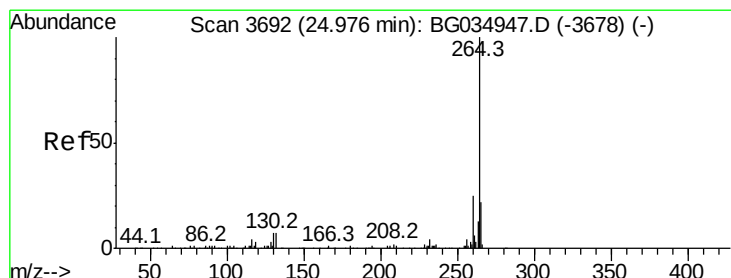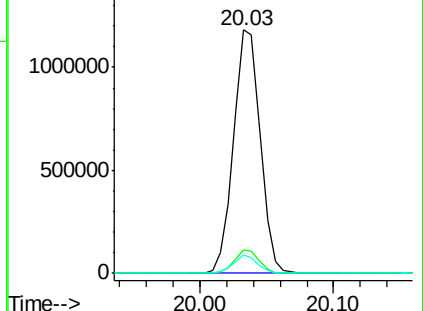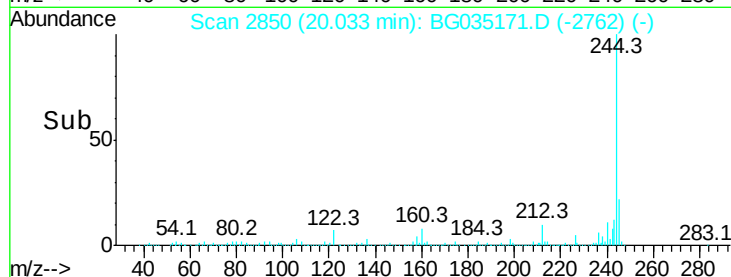

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.93 min Scan# 3683

Delta R.T. -0.03 min

Lab File: BG035171.D

Acq: 15 Jun 2018 13:15


Tgt Ion:264 Resp: 342902

Ion Ratio Lower Upper

264 100

260 22.8 17.4 26.0

265 23.5 17.7 26.5

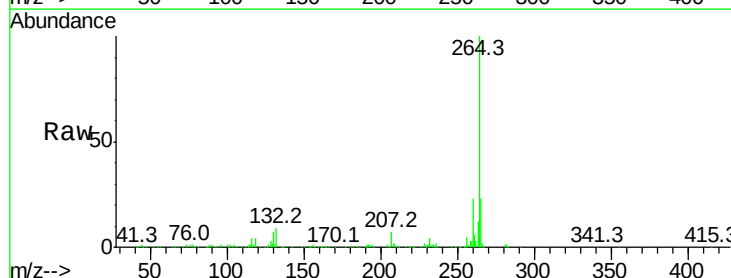

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

