

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061418\
Data File : BG035141.D
Acq On : 14 Jun 2018 17:14
Operator : SJ/JU
Sample : J3467-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FB-061118

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG060718.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.632	393	399	409	rVB	352666	582605	12.24%	3.284%
2	7.212	660	668	681	rBV	244330	428192	8.99%	2.414%
3	7.594	725	733	745	rBV	668556	1160860	24.38%	6.544%
4	8.064	806	813	822	rBV	147044	255398	5.36%	1.440%
5	8.387	859	868	877	rBV	605542	1045303	21.96%	5.893%
6	9.227	1001	1011	1020	rBV	541002	979722	20.58%	5.523%
7	10.872	1281	1291	1298	rBV	207396	367017	7.71%	2.069%
8	13.310	1699	1706	1720	rBV	1591956	2512069	52.77%	14.161%
9	14.685	1933	1940	1948	rBV2	364282	598510	12.57%	3.374%
10	16.171	2186	2193	2203	rBV	1450221	2213041	46.49%	12.476%
11	17.428	2401	2407	2417	rVB2	561559	853784	17.93%	4.813%
12	20.042	2845	2852	2860	rBV	3443378	4760610	100.00%	26.837%
13	21.699	3125	3134	3146	rBV2	634187	1047524	22.00%	5.905%
14	24.930	3671	3684	3704	rBV2	287638	934429	19.63%	5.268%


Sum of corrected areas: 17739064

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061418\
Data File : BG035141.D
Acq On : 14 Jun 2018 17:14
Operator : SJ/JU
Sample : J3467-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FB-061118

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

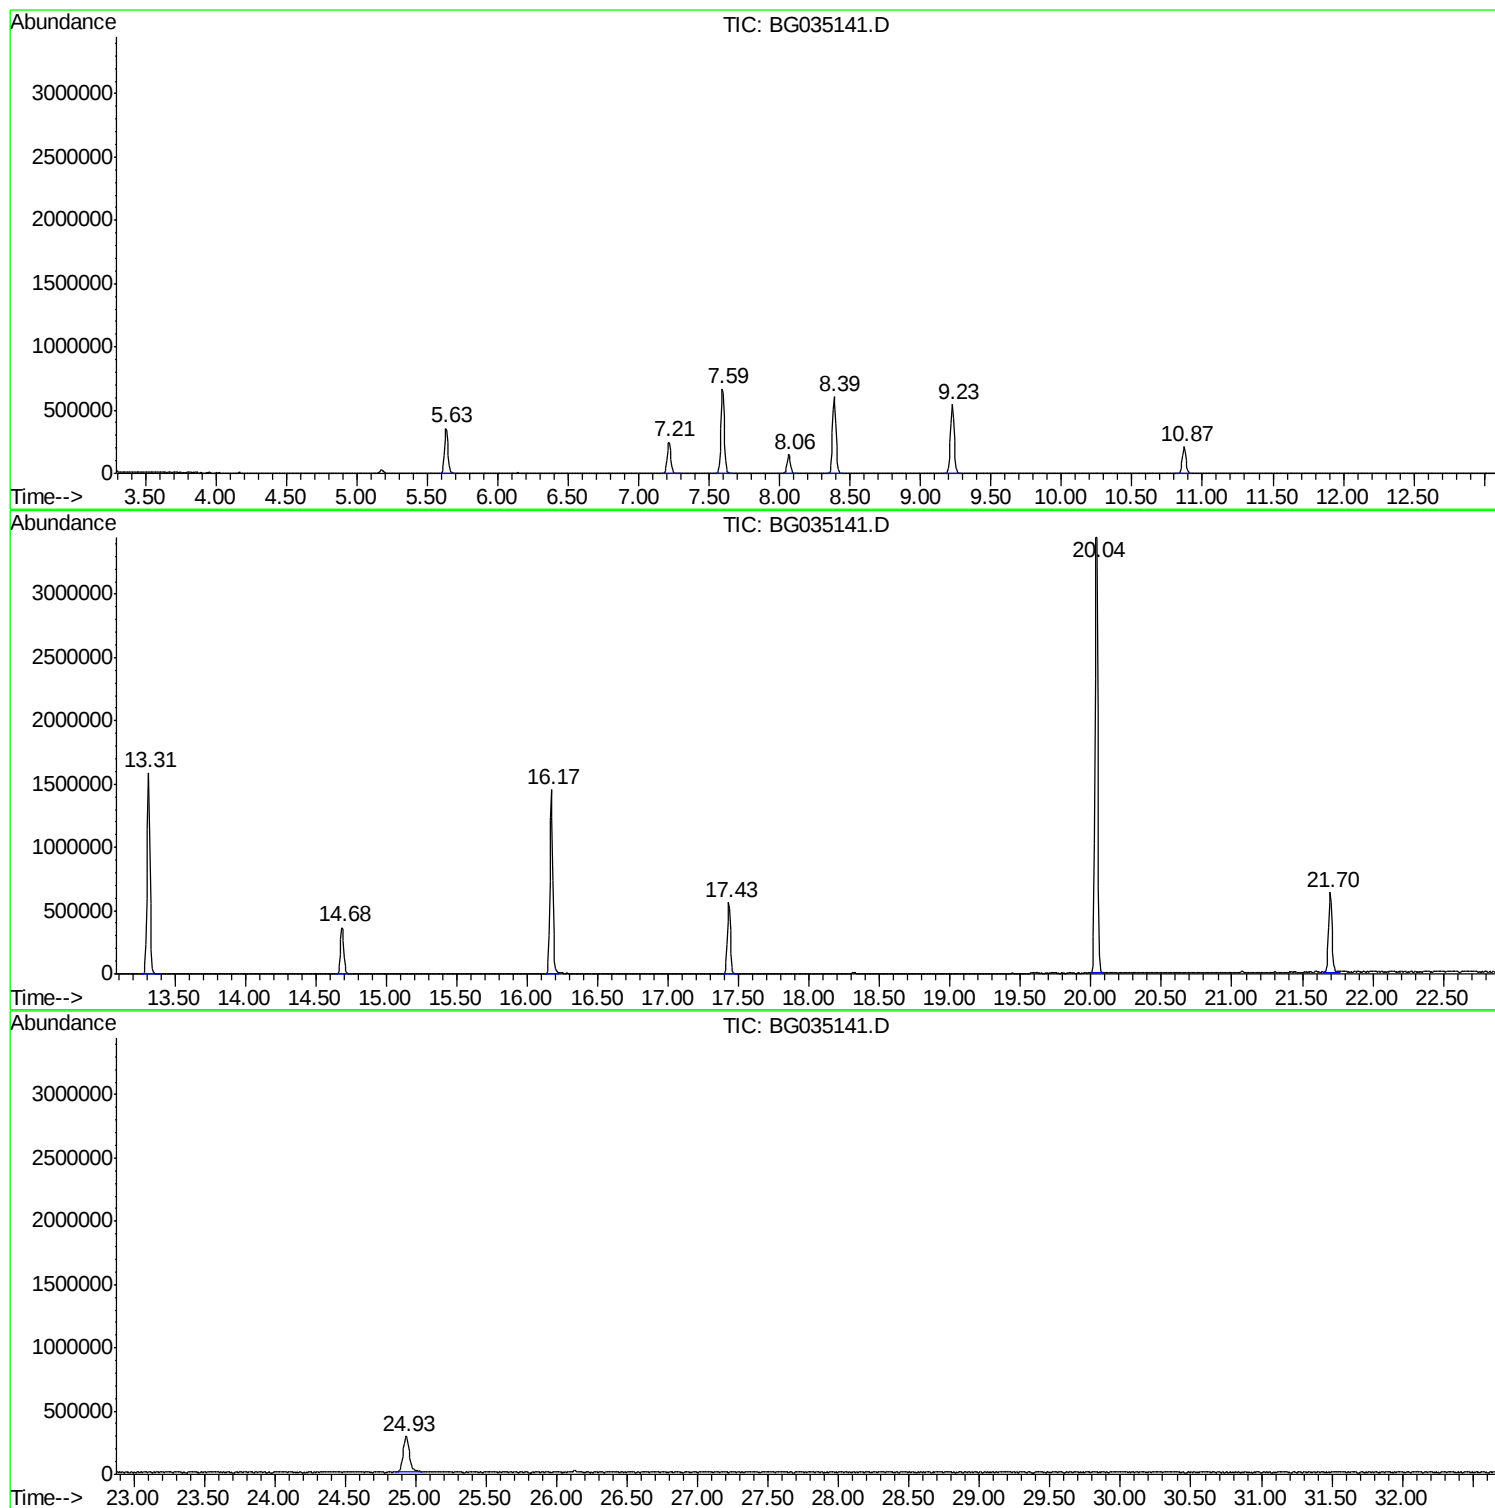

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061418\
Data File : BG035141.D
Acq On : 14 Jun 2018 17:14
Operator : SJ/JU
Sample : J3467-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FB-061118










Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.59 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.59	90.91 ng	1160860	1,4-Dichlorobenzene-d4	8.06

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2		1H-Indazole, 3-methyl-	132	C8H8N2	1000316-00-2	12
3		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
4		5-Aminoindole	132	C8H8N2	005192-03-0	12
5		N-(-3,4-Methylenedioxyphenylisop...	267	C17H17NO2	1000378-96-6	10

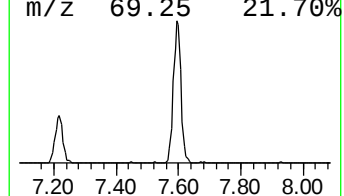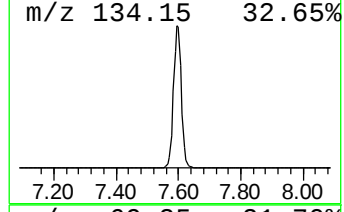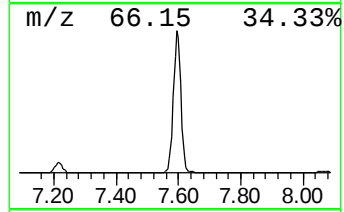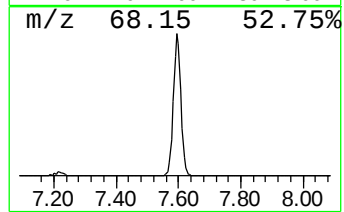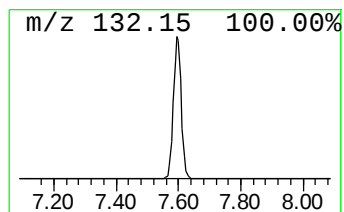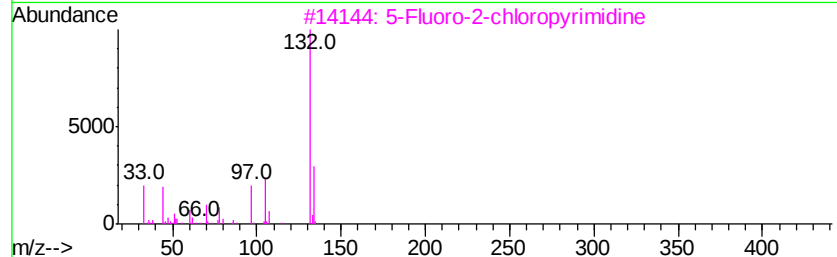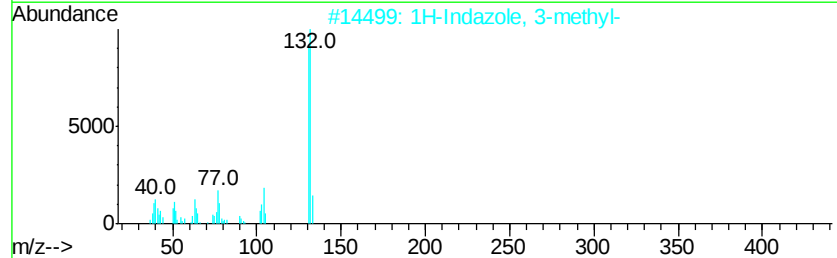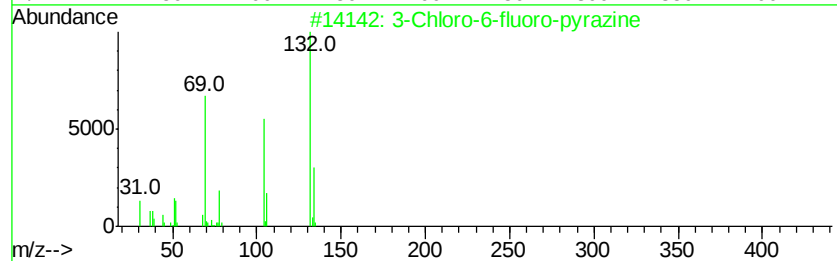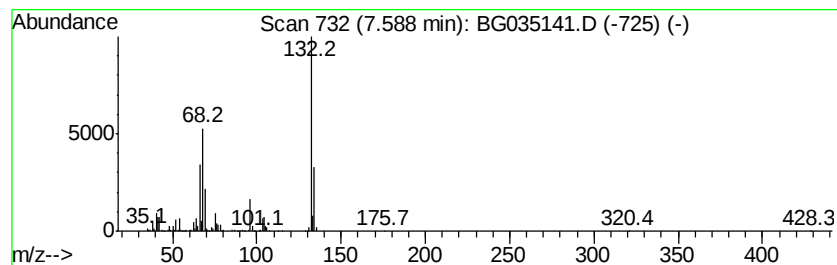

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG061418\
Data File : BG035141.D
Acq On : 14 Jun 2018 17:14
Operator : SJ/JU
Sample : J3467-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FB-061118

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.59	7.59	90.9	ng	1160860	1	8.06	255398	20.0