


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG061418\
 Data File : BG035136.D
 Acq On : 14 Jun 2018 14:00
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG060718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 08 17:16:28 2018

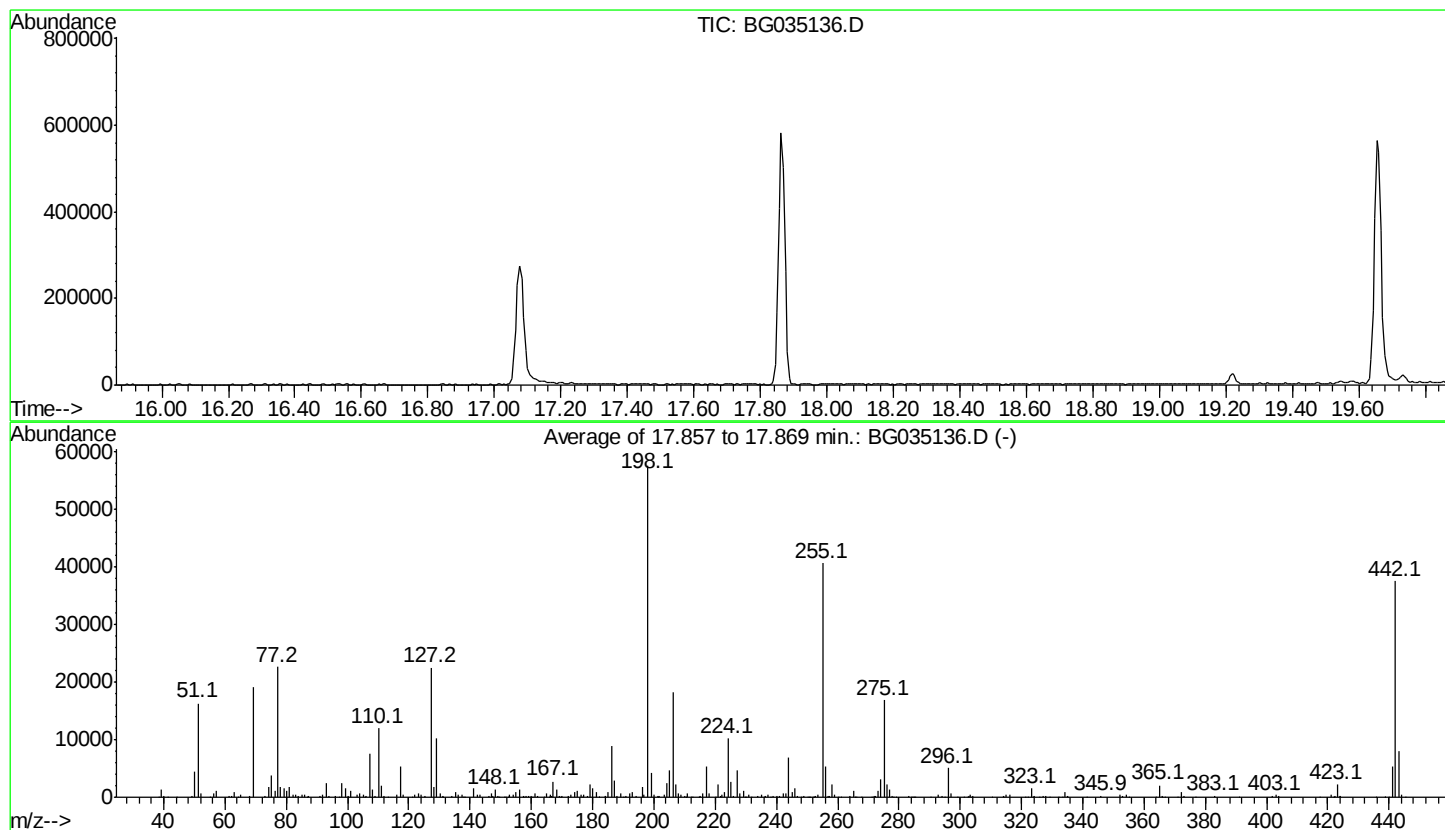

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.3	16245	PASS
68	69	0.00	2	0.9	168	PASS
69	198	0.00	100	33.4	19170	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	39.0	22424	PASS
197	198	0.00	2	0.9	542	PASS
198	198	100	100	100.0	57464	PASS
199	198	5	9	7.3	4183	PASS
275	198	10	60	29.3	16815	PASS
365	198	1	100	3.6	2096	PASS
441	443	0.01	100	65.6	5274	PASS
442	198	50	100	65.1	37432	PASS
443	442	15	24	21.5	8042	PASS