


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG061418\  
 Data File : BG035155.D  
 Acq On : 15 Jun 2018 2:56  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG060718.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Jun 08 17:16:28 2018

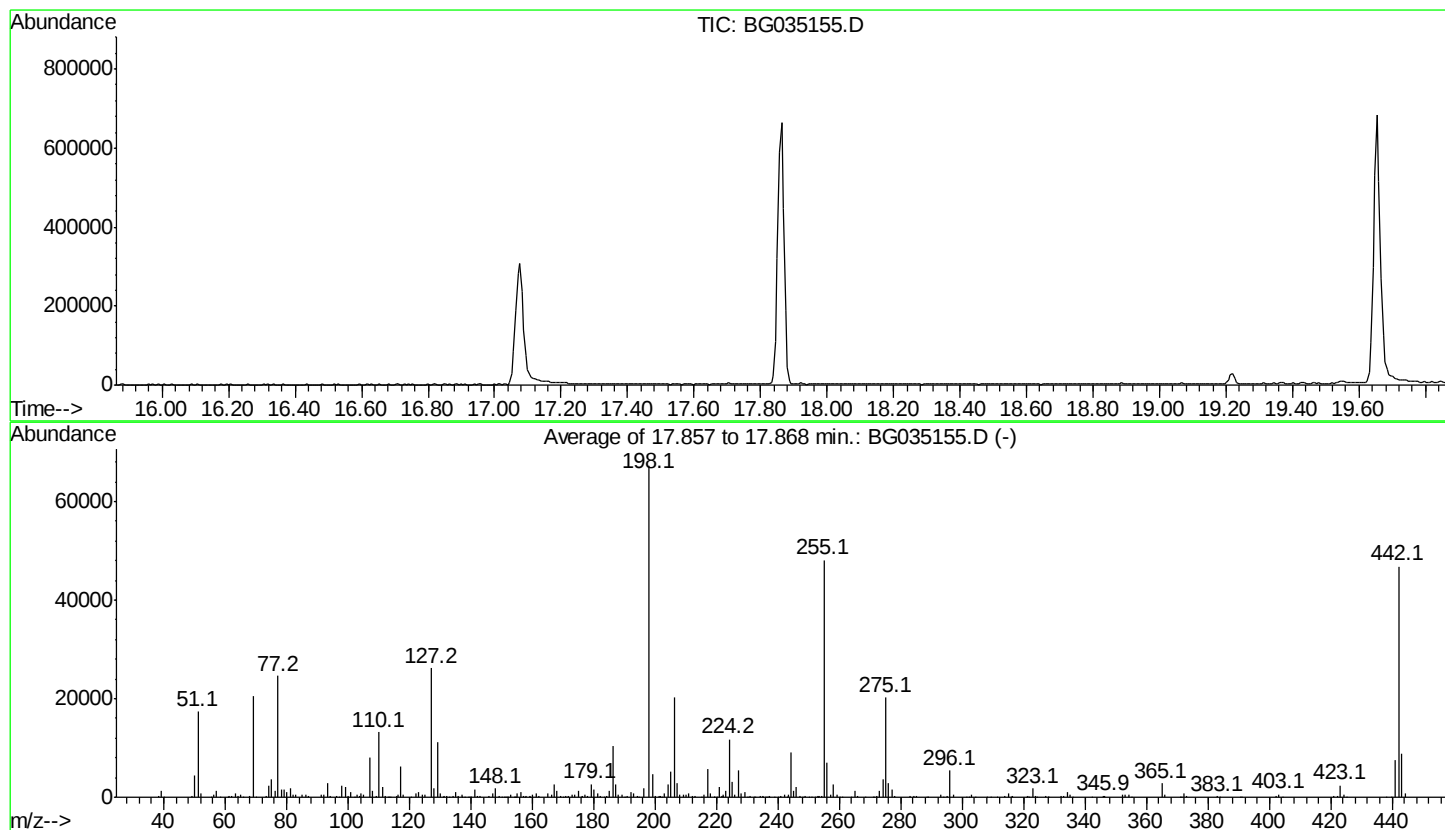

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 25.8      | 17384   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.1       | 221     | PASS             |
| 69          | 198          | 0.00         | 100          | 30.4      | 20473   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.6       | 125     | PASS             |
| 127         | 198          | 10           | 80           | 38.9      | 26146   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 67261   | PASS             |
| 199         | 198          | 5            | 9            | 6.9       | 4651    | PASS             |
| 275         | 198          | 10           | 60           | 30.1      | 20255   | PASS             |
| 365         | 198          | 1            | 100          | 4.1       | 2738    | PASS             |
| 441         | 443          | 0.01         | 100          | 86.1      | 7567    | PASS             |
| 442         | 198          | 50           | 100          | 69.7      | 46861   | PASS             |
| 443         | 442          | 15           | 24           | 18.8      | 8792    | PASS             |