



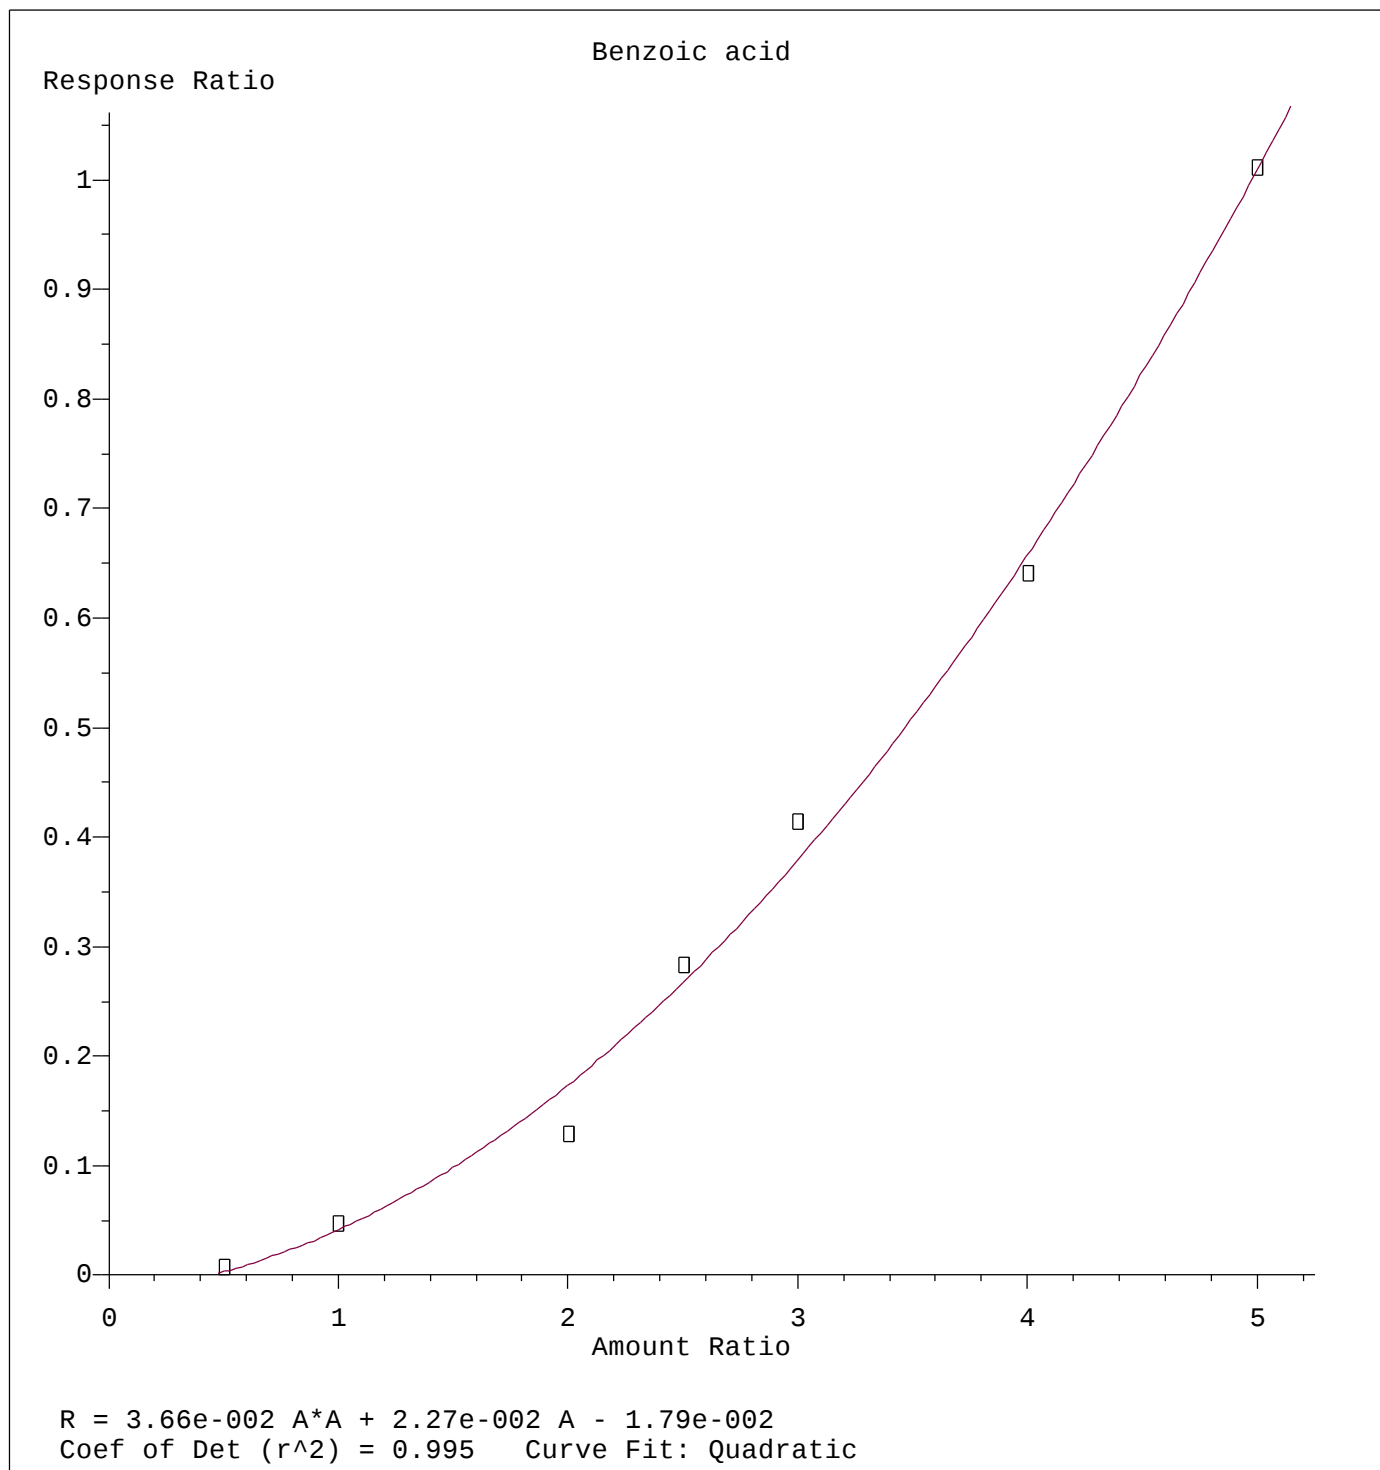

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061419.M
Calibration Table Last Updated: Fri Jun 14 15:26:06 2019

Hexachlorocyclopentadiene

Response Ratio

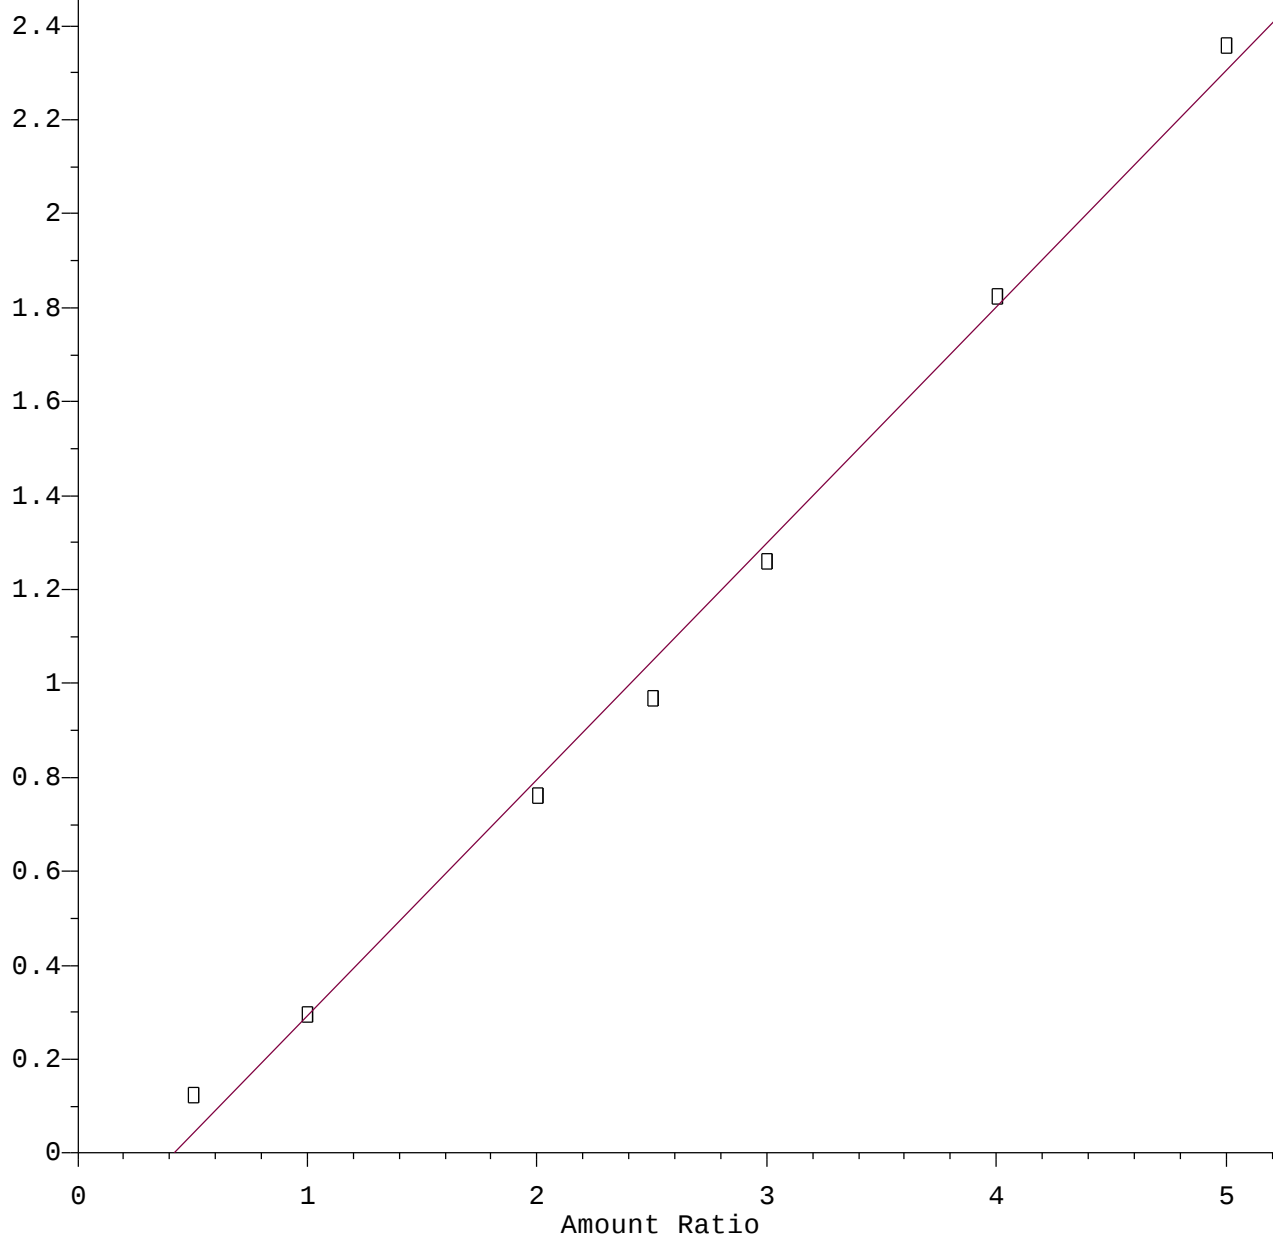


Resp Ratio = $5.03 \times 10^{-1} \times \text{Amt} - 2.10 \times 10^{-1}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061419.M
Calibration Table Last Updated: Fri Jun 14 15:26:06 2019

2,4-Dinitrophenol

Response Ratio

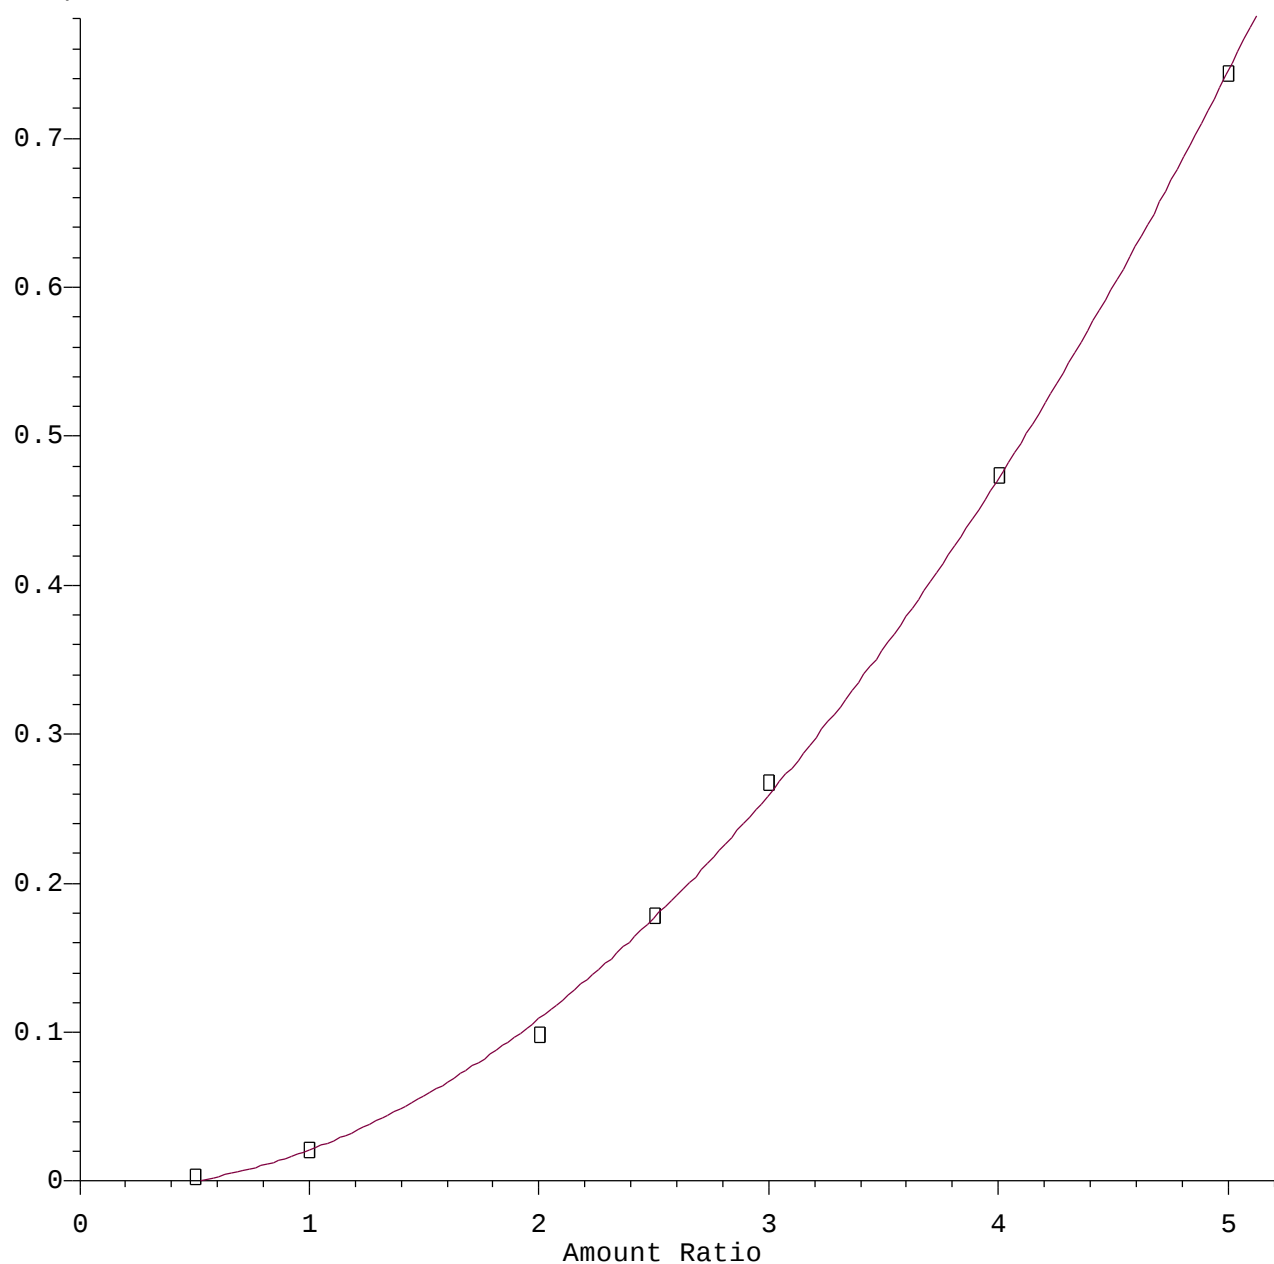


$R = 3.09e-002 A^2 - 4.26e-003 A - 5.98e-003$
Coef of Det (r^2) = 1.000 Curve Fit: Quadratic

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061419.M
Calibration Table Last Updated: Fri Jun 14 15:26:06 2019


4-Nitrophenol

Response Ratio

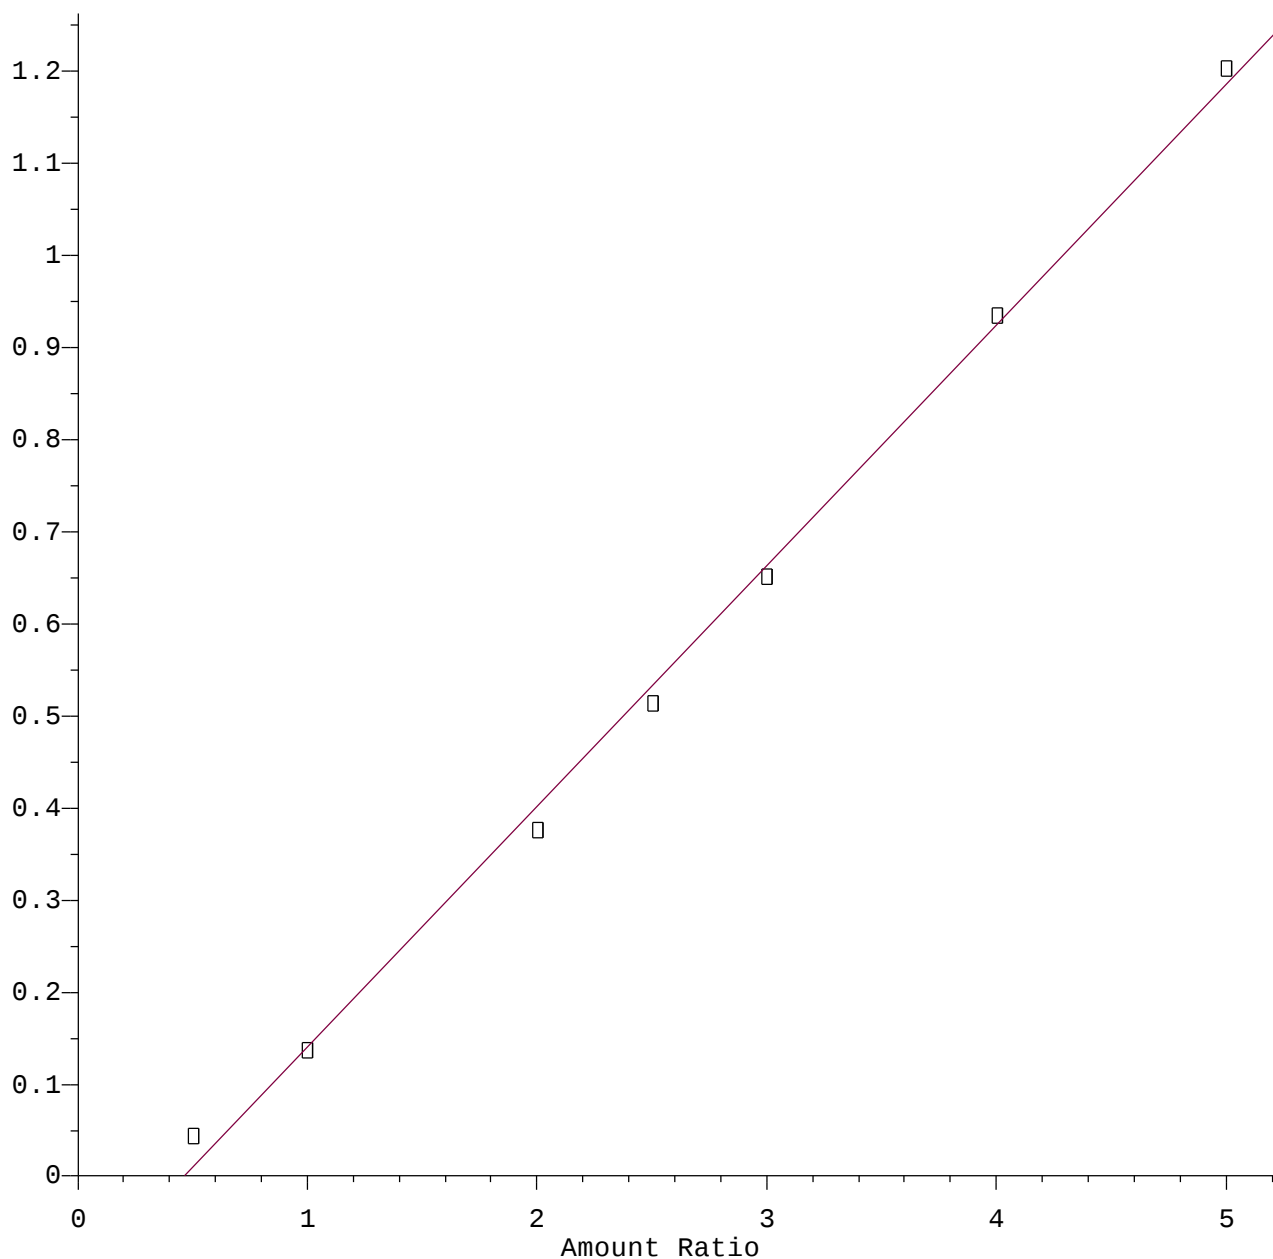


Resp Ratio = $2.61 \times 10^{-1} \times \text{Amt} - 1.22 \times 10^{-1}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061419.M
Calibration Table Last Updated: Fri Jun 14 15:26:06 2019

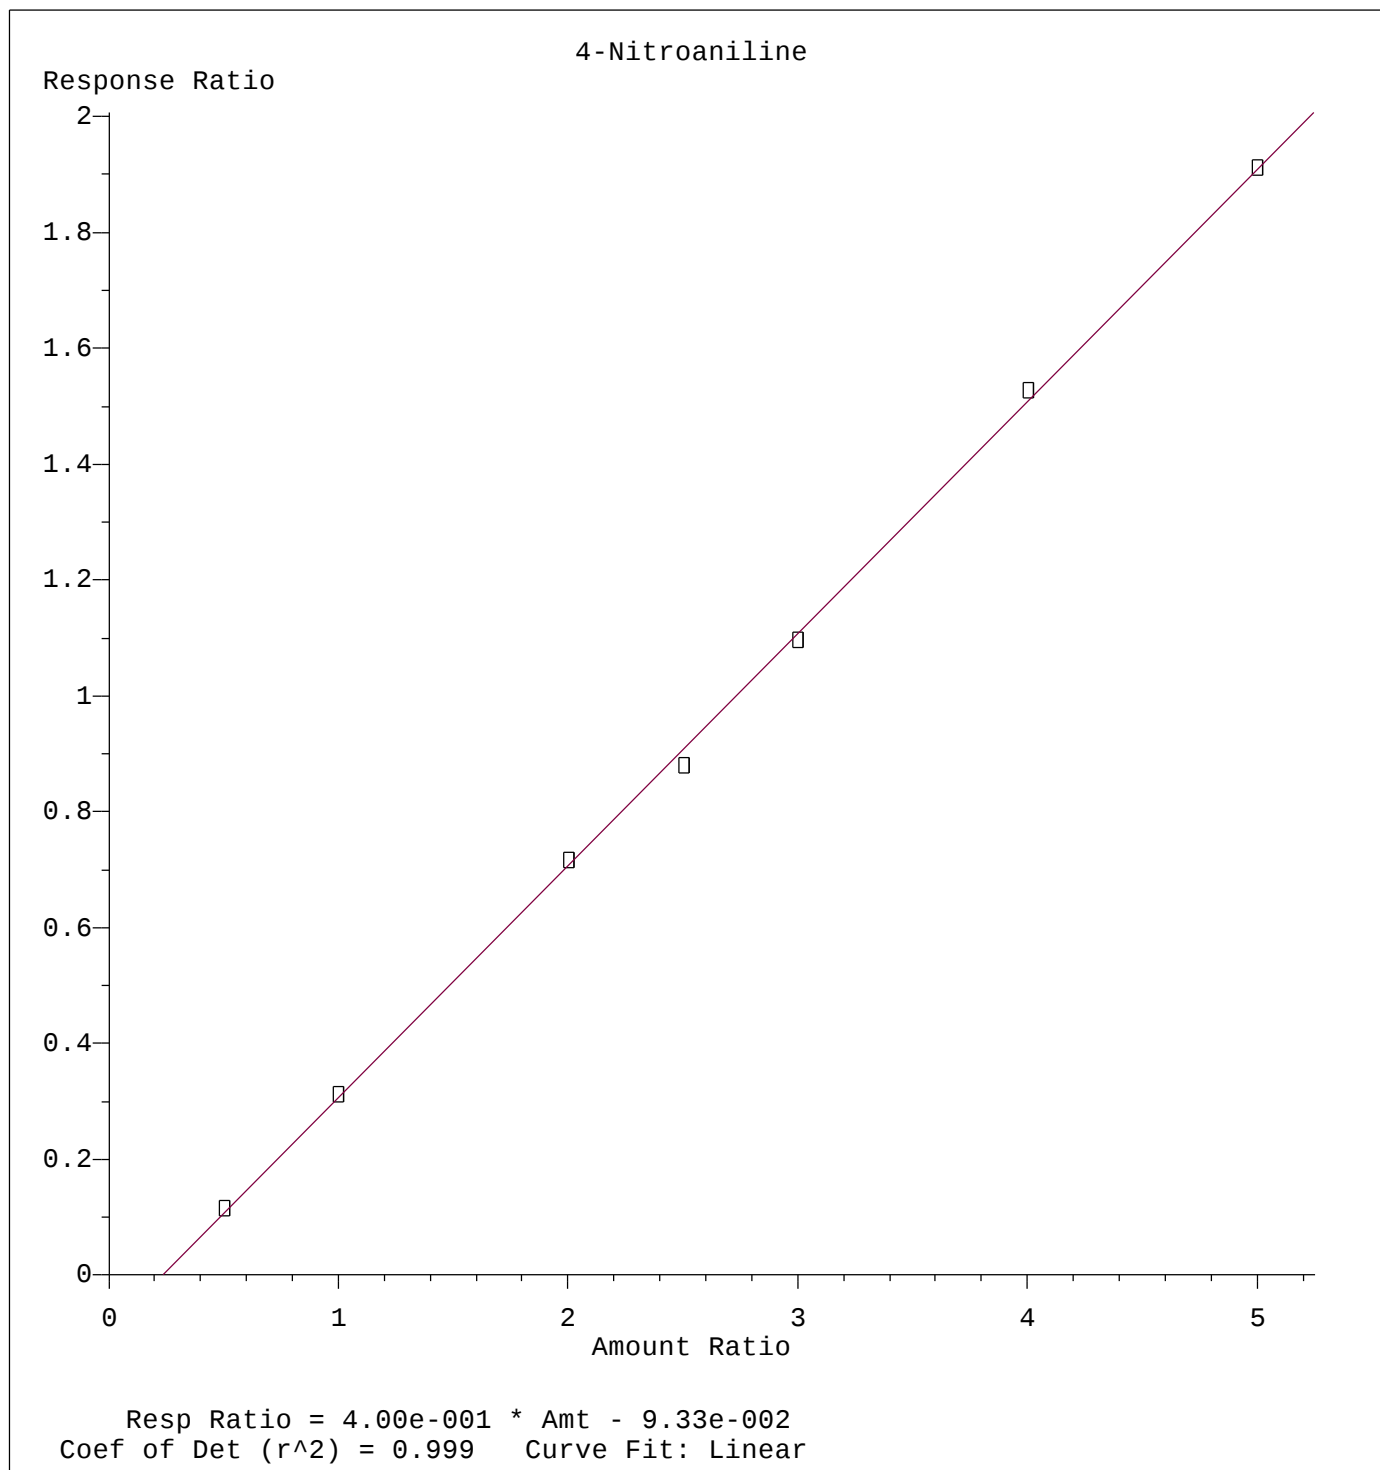


Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061419.M
Calibration Table Last Updated: Fri Jun 14 15:26:06 2019

4,6-Dinitro-2-methylphenol

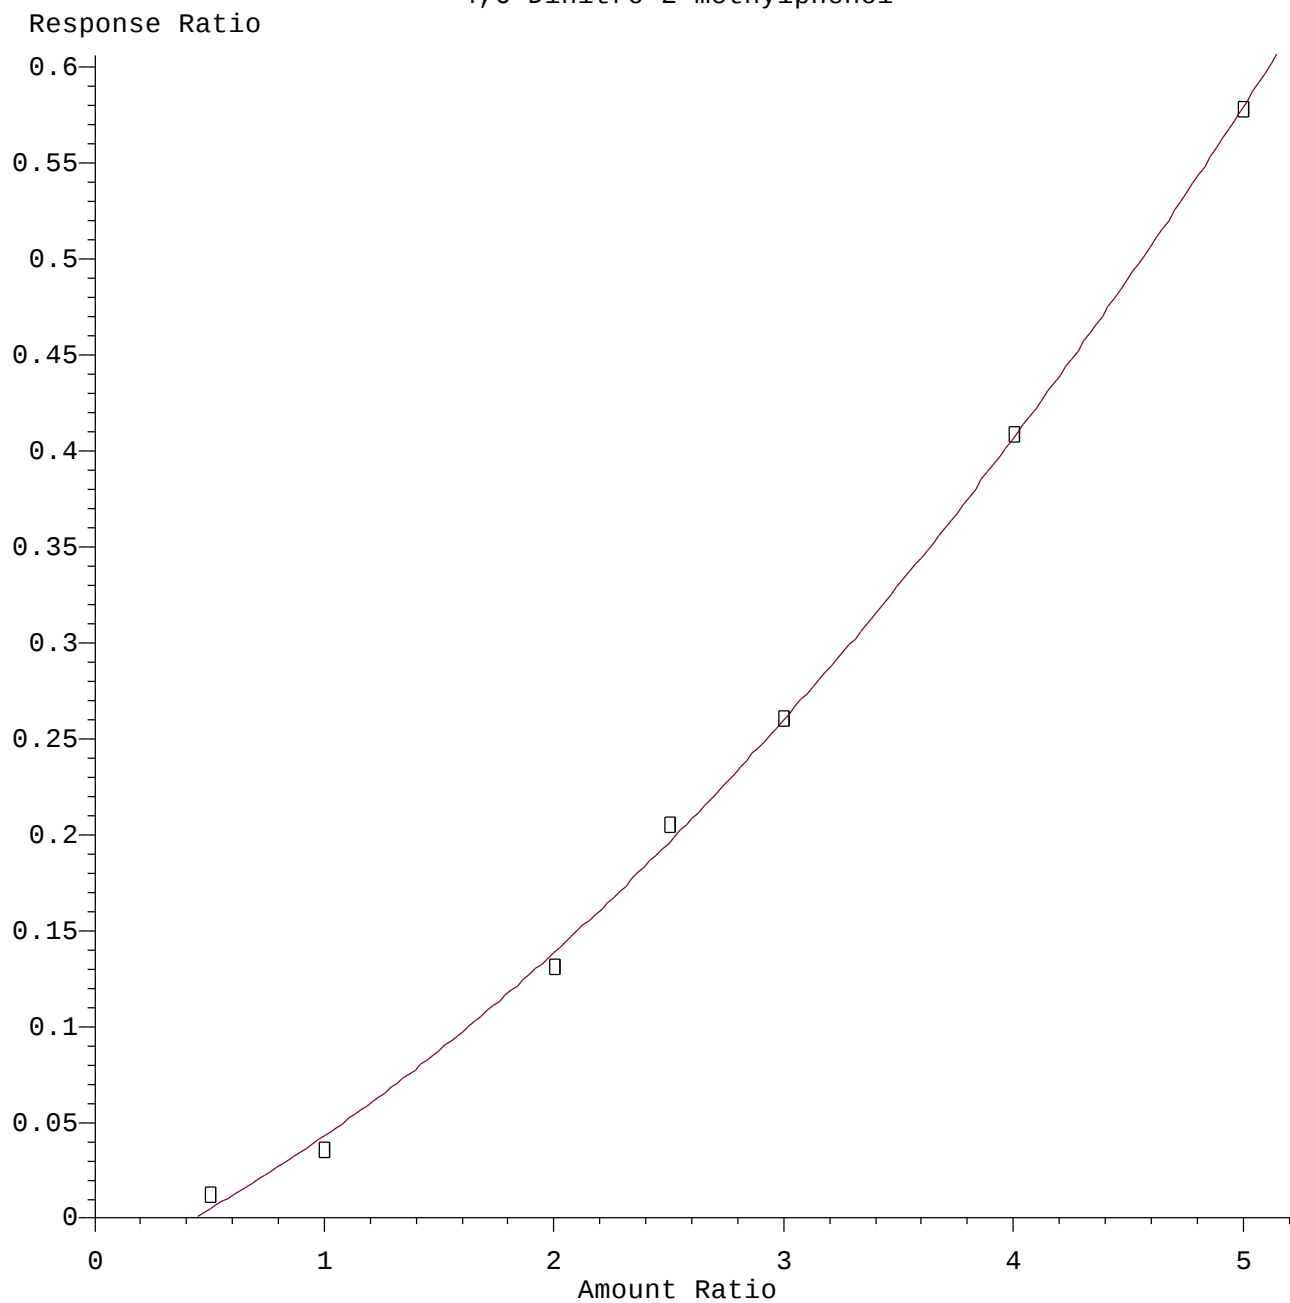

$R = 1.29e-002 A^2 + 5.70e-002 A - 2.68e-002$
Coef of Det (r^2) = 0.999 Curve Fit: Quadratic


Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061419.M
Calibration Table Last Updated: Fri Jun 14 15:26:06 2019

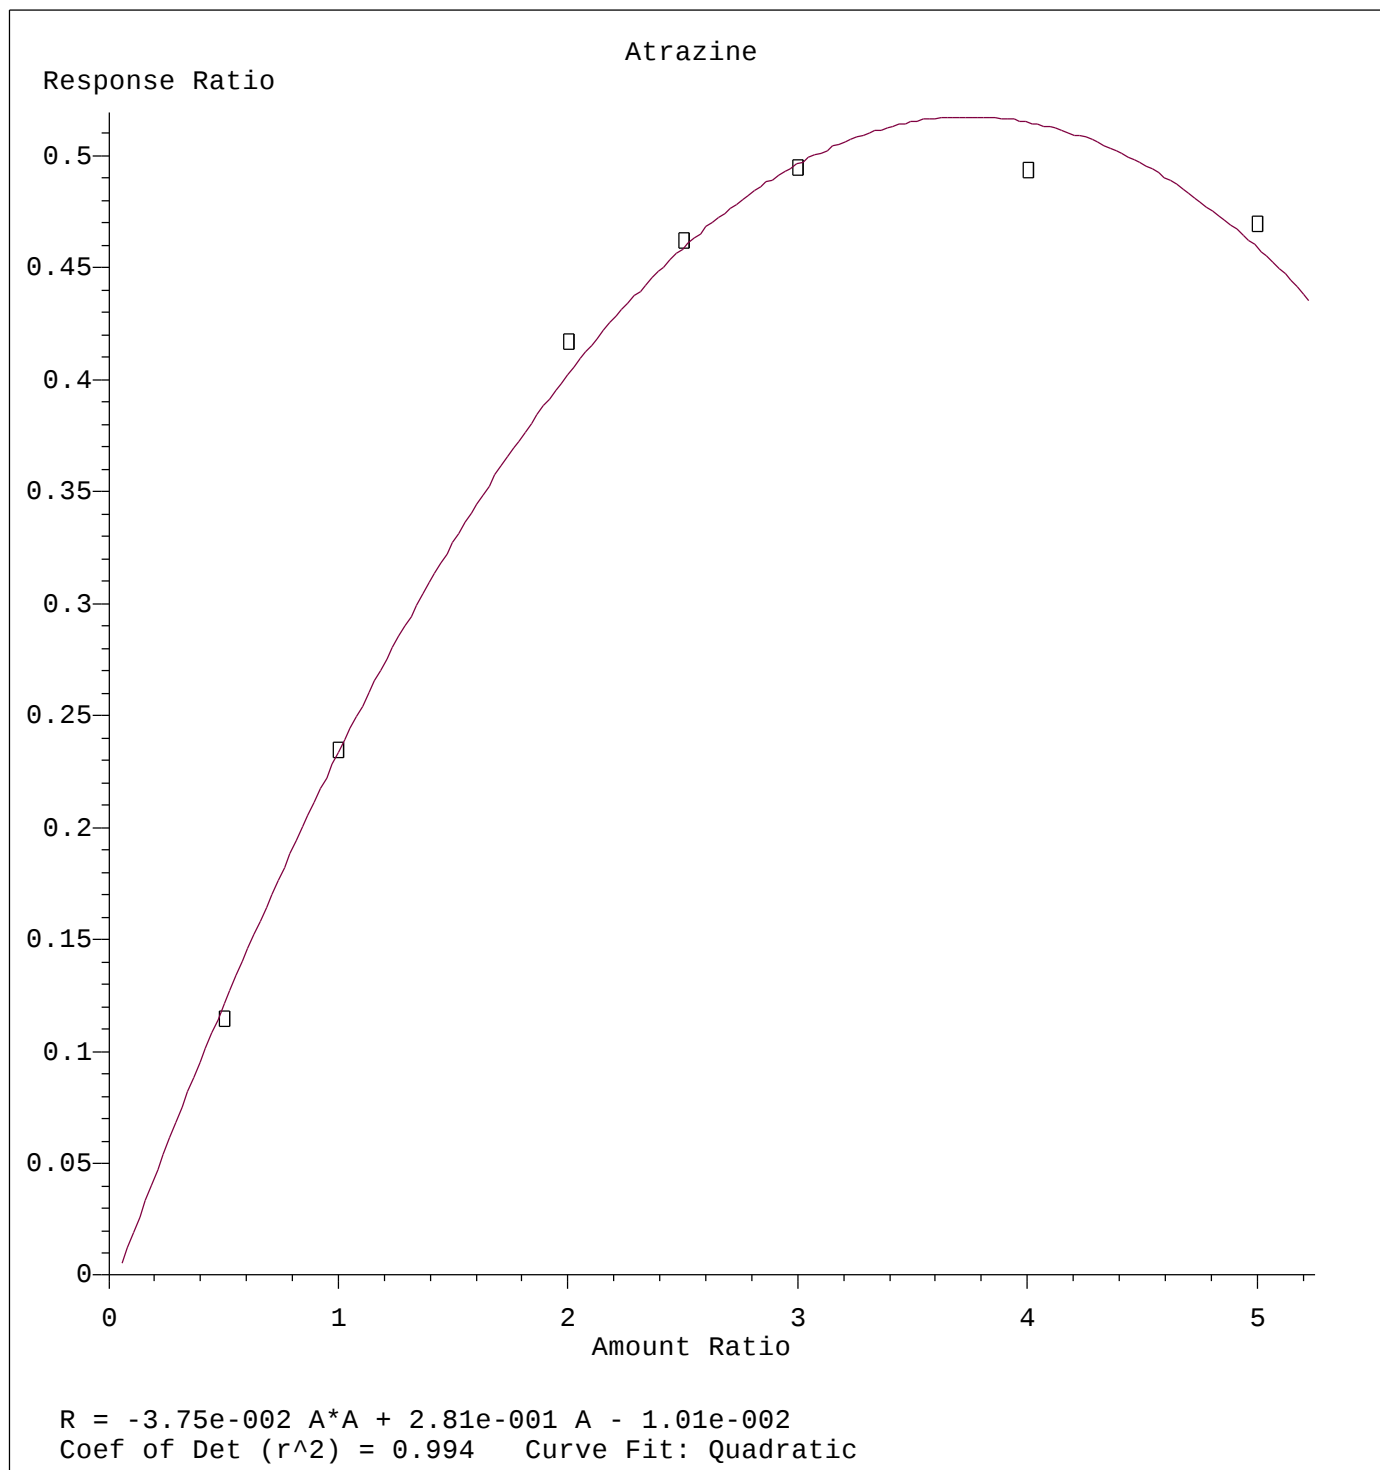

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061419.M
Calibration Table Last Updated: Fri Jun 14 15:26:06 2019

Pentachlorophenol

Response Ratio

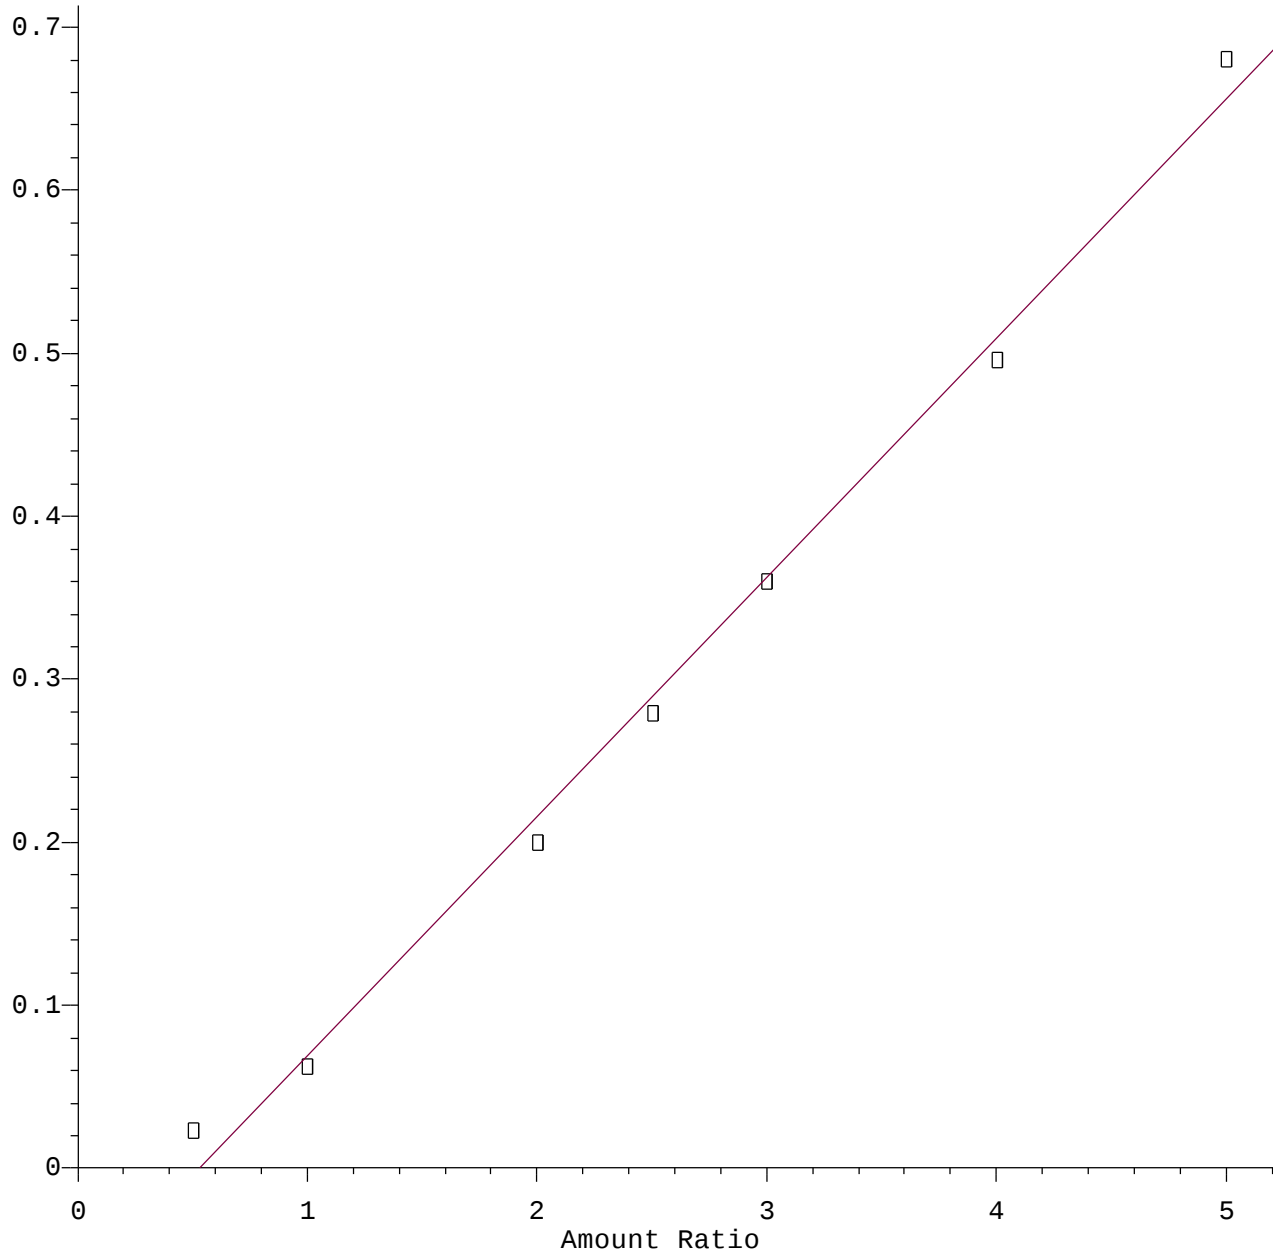

Resp Ratio = $1.47 \times 10^{-1} \times \text{Amt} - 7.79 \times 10^{-2}$
Coef of Det (r^2) = 0.994 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061419.M
Calibration Table Last Updated: Fri Jun 14 15:26:06 2019