


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061419\
 Data File : BG041245.D
 Acq On : 14 Jun 2019 9:07
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 14 15:26:06 2019

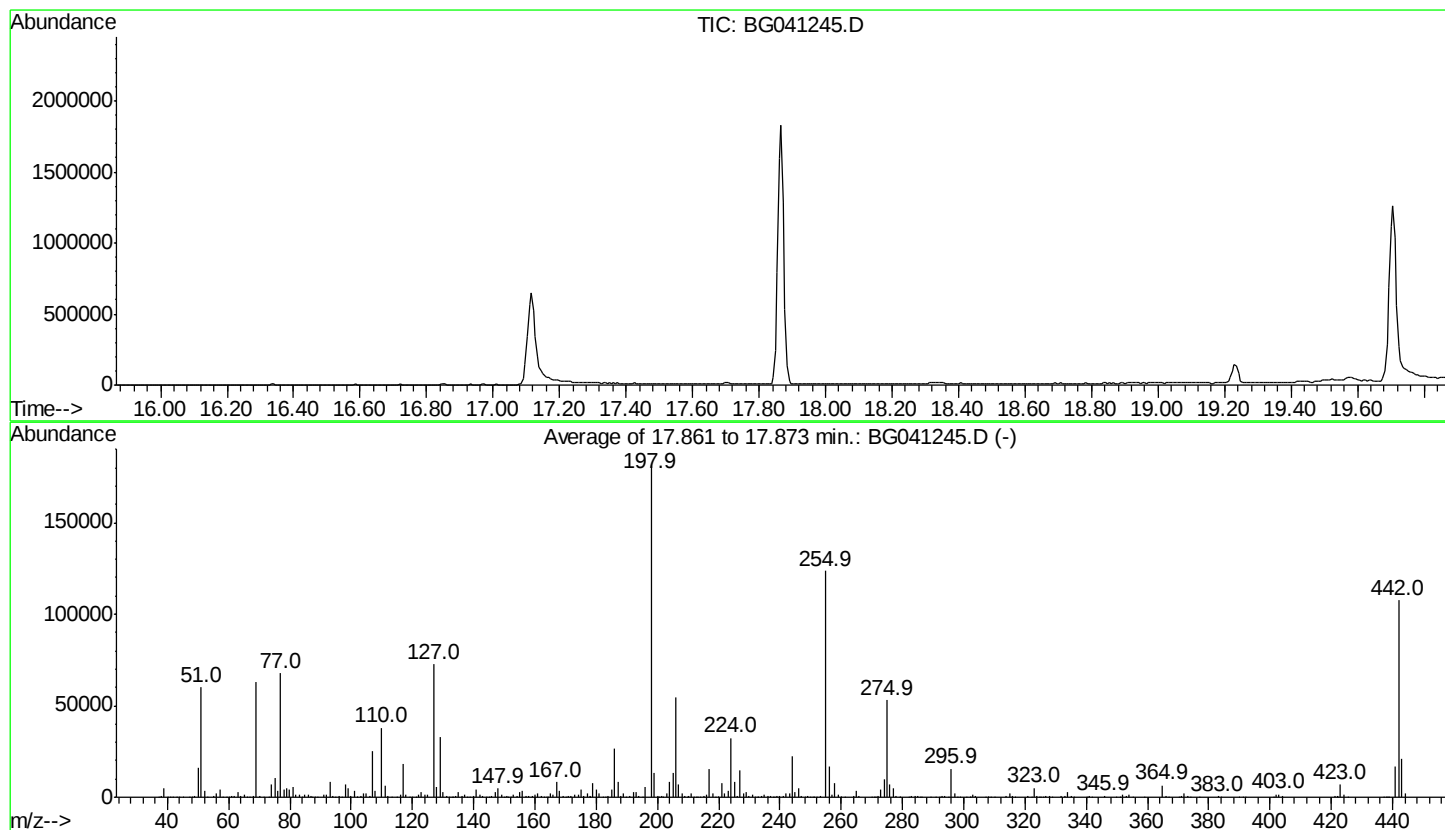

AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.0	59864	PASS
68	69	0.00	2	0.6	385	PASS
69	198	0.00	100	34.7	62848	PASS
70	69	0.00	2	0.7	439	PASS
127	198	10	80	40.0	72541	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	181141	PASS
199	198	5	9	7.3	13190	PASS
275	198	10	60	29.3	52986	PASS
365	198	1	100	3.6	6556	PASS
441	198	0.01	100	9.4	16940	PASS
442	198	50	100	59.3	107466	PASS
443	442	15	24	19.3	20749	PASS