


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061419\
 Data File : BG041255.D
 Acq On : 14 Jun 2019 16:13
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 14 15:26:06 2019

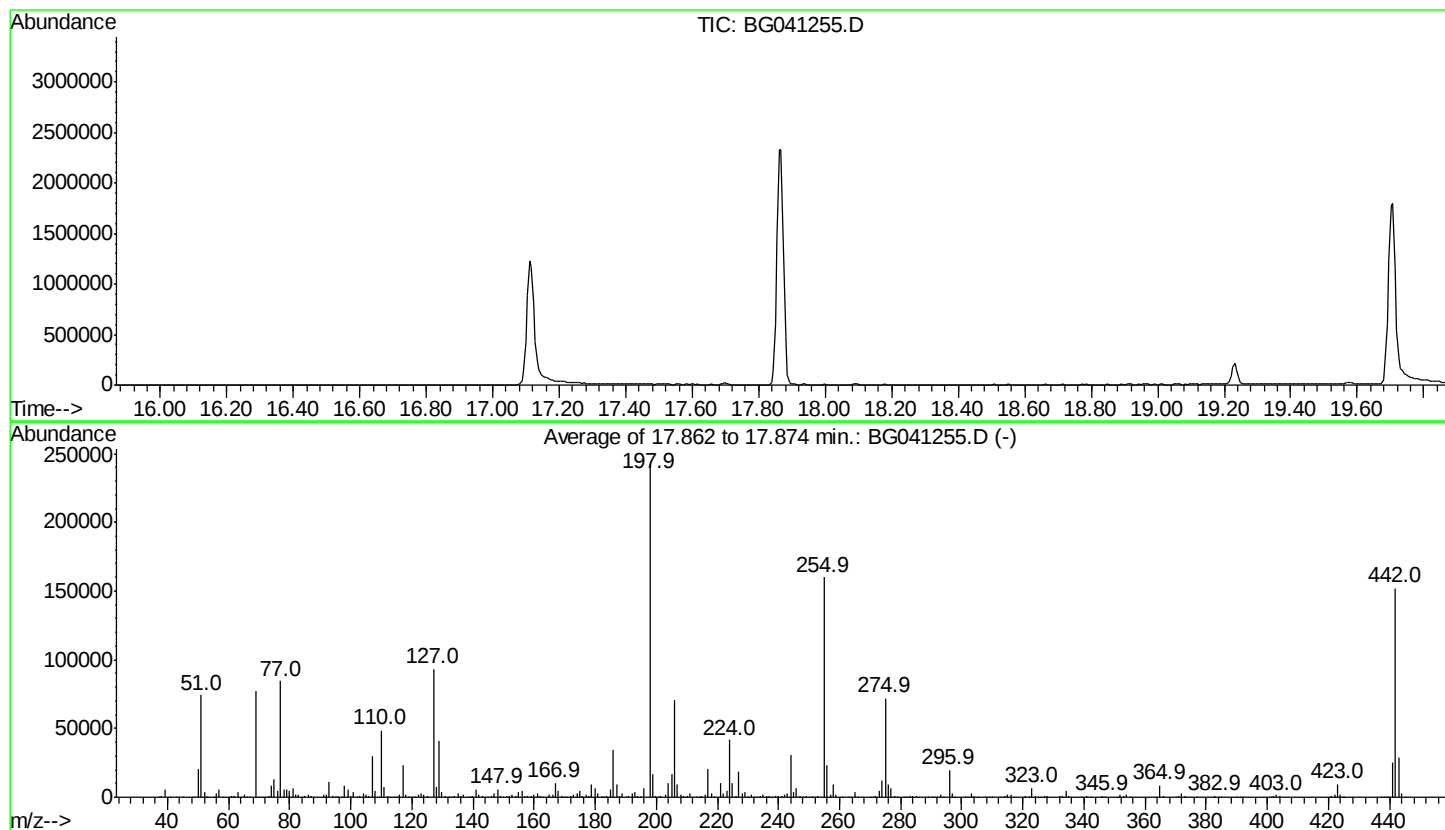

AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.8	74216	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.2	77656	PASS
70	69	0.00	2	0.6	476	PASS
127	198	10	80	38.7	93306	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	241258	PASS
199	198	5	9	6.9	16537	PASS
275	198	10	60	29.8	71777	PASS
365	198	1	100	3.5	8395	PASS
441	198	0.01	100	10.5	25312	PASS
442	198	50	100	63.1	152170	PASS
443	442	15	24	19.3	29341	PASS