

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061423\
 Data File : BG057715.D
 Acq On : 14 Jun 2023 20:06
 Operator : CG/JU
 Sample : 03074-08
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GT-GW-1

Quant Time: Jun 15 01:24:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 14 03:52:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.938	152	36744	20.000	ng	0.00
21) Naphthalene-d8	10.741	136	153496	20.000	ng	0.00
39) Acenaphthene-d10	14.566	164	101411	20.000	ng	0.00
64) Phenanthrene-d10	17.309	188	223488	20.000	ng	0.00
76) Chrysene-d12	21.569	240	190914	20.000	ng	0.00
86) Perylene-d12	24.736	264	230653	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.506	112	11408	5.055	ng	0.00
7) Phenol-d6	7.086	99	11872	3.425	ng	0.00
23) Nitrobenzene-d5	9.096	82	17995	20.555	ng	0.00
42) 2,4,6-Tribromophenol	16.052	330	6557	5.795	ng	0.00
45) 2-Fluorobiphenyl	13.191	172	43545	6.401	ng	0.00
79) Terphenyl-d14	19.930	244	58986	5.712	ng	0.00
Target Compounds						
84) Bis(2-ethylhexyl)phtha...	21.475	149	29303	4.379	ng	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061423\
Data File : BG057715.D
Acq On : 14 Jun 2023 20:06
Operator : CG/JU
Sample : 03074-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GT-GW-1

Quant Time: Jun 15 01:24:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 14 03:52:08 2023
Response via : Initial Calibration




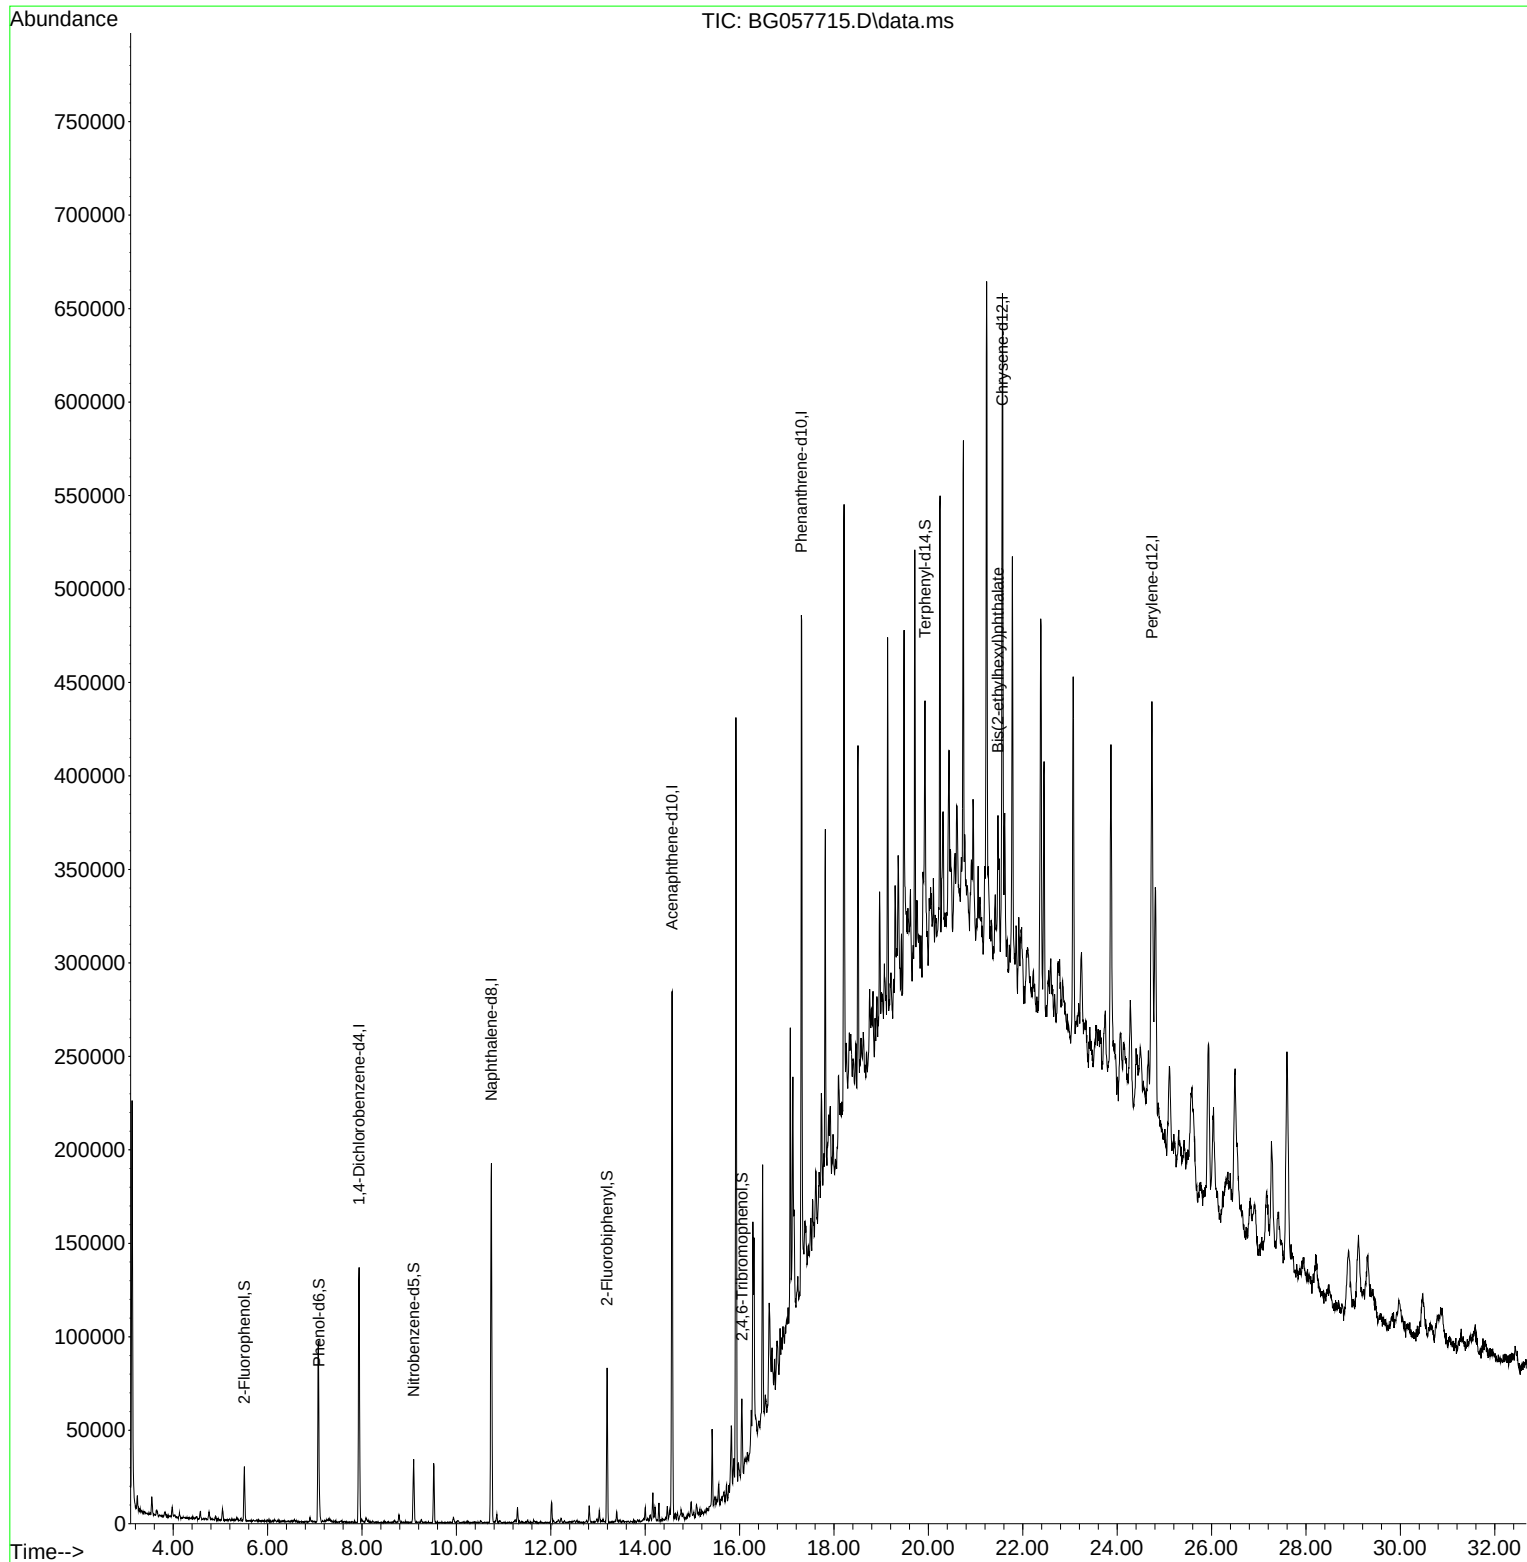




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.938 min Scan# 81
Delta R.T. -0.003 min
Lab File: BG057715.D
Acq: 14 Jun 2023 20:06




Instrument :
BNA_G
ClientSampleId :
GT-GW-1


Tgt Ion:152 Resp: 36744
Ion Ratio Lower Upper
152 100
150 157.2 120.8 181.2
115 62.3 49.4 74.2

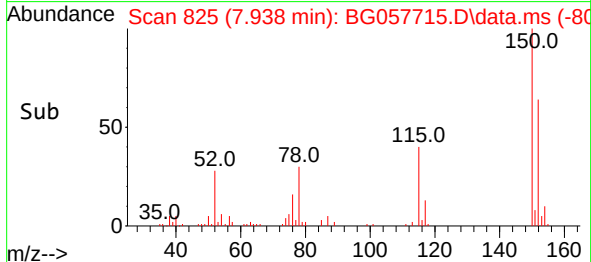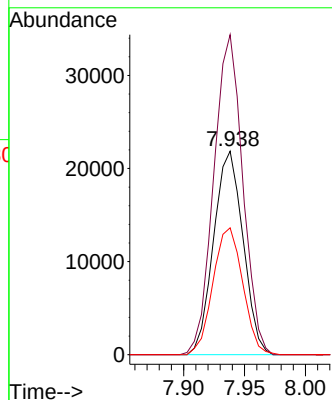

#5
2-Fluorophenol
Concen: 5.055 ng
RT: 5.506 min Scan# 411
Delta R.T. -0.003 min
Lab File: BG057715.D
Acq: 14 Jun 2023 20:06

Tgt Ion:112 Resp: 11408
Ion Ratio Lower Upper
112 100
64 73.6 62.3 93.5
63 38.8 31.5 47.3

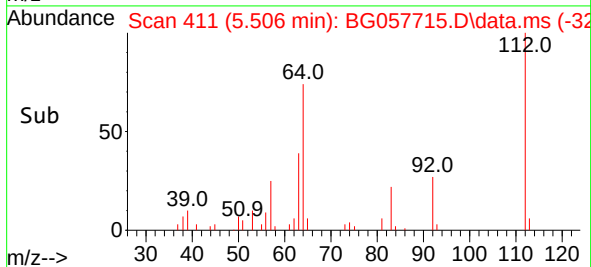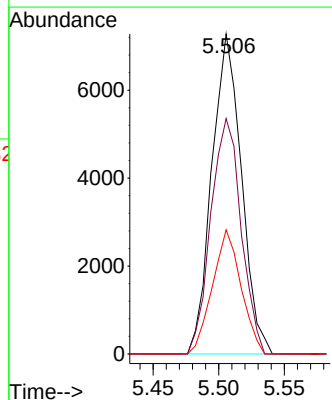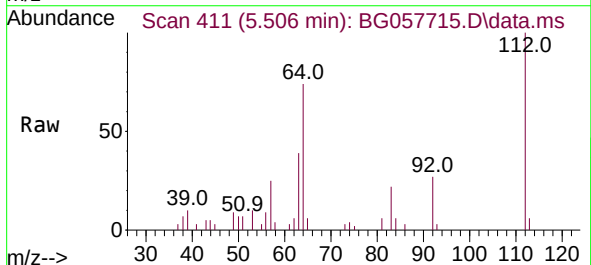



#7

Phenol-d6

Concen: 3.425 ng

RT: 7.086 min Scan# 61

Delta R.T. -0.009 min

Lab File: BG057715.D


Acq: 14 Jun 2023 20:06

Instrument :

BNA_G

ClientSampleId :

GT-GW-1

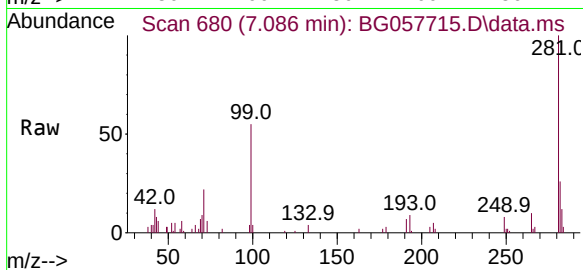




Tgt Ion: 99 Resp: 11872

Ion Ratio Lower Upper

99 100

42 21.1 18.3 27.5

71 39.6 27.5 41.3

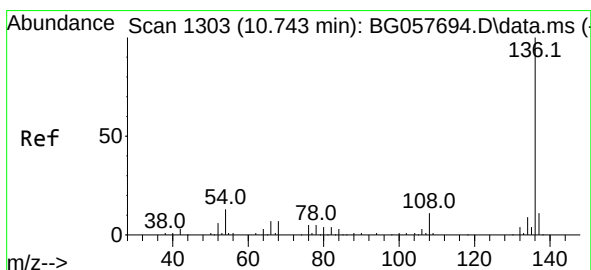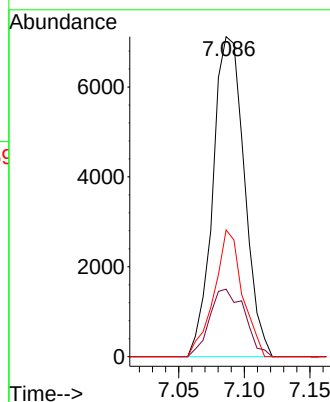

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.741 min Scan# 1302

Delta R.T. -0.002 min

Lab File: BG057715.D

Acq: 14 Jun 2023 20:06

Tgt Ion: 136 Resp: 153496




Ion Ratio Lower Upper


136 100

137 11.5 8.6 13.0

54 12.7 10.8 16.2

68 6.9 5.7 8.5

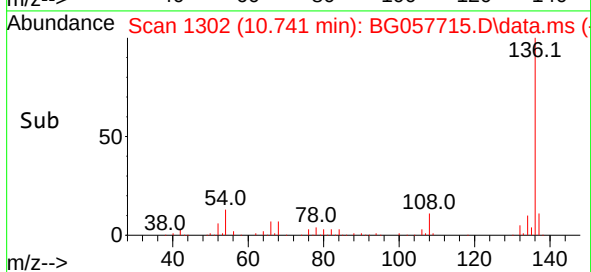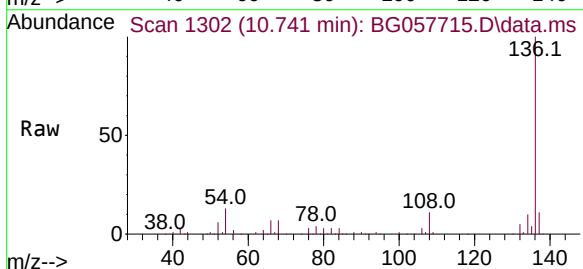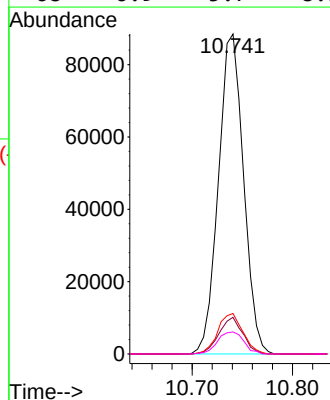



#23

Nitrobenzene-d5

Concen: 20.555 ng

RT: 9.096 min Scan# 1022

Delta R.T. -0.008 min

Lab File: BG057715.D

Acq: 14 Jun 2023 20:06

Instrument :

BNA_G

ClientSampleId :

GT-GW-1





Tgt Ion: 82 Resp: 17995

Ion Ratio Lower Upper

82 100

128 36.8 27.7 41.5

54 68.1 53.8 80.8

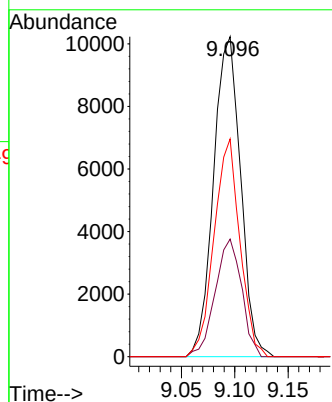

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.566 min Scan# 1953

Delta R.T. -0.008 min

Lab File: BG057715.D

Acq: 14 Jun 2023 20:06




Tgt Ion: 164 Resp: 101411


Ion Ratio Lower Upper

164 100

162 97.2 77.7 116.5

160 42.7 35.1 52.7

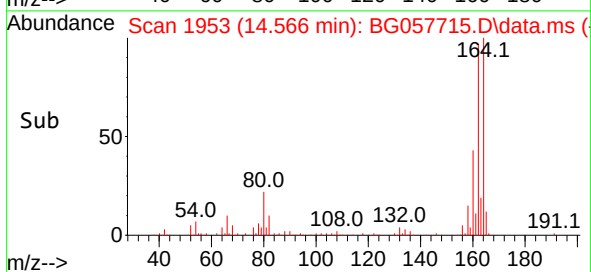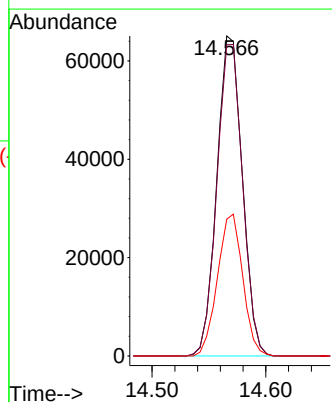



#42

2,4,6-Tribromophenol

Concen: 5.795 ng

RT: 16.052 min Scan# 21

Delta R.T. -0.009 min

Lab File: BG057715.D


Acq: 14 Jun 2023 20:06

Instrument :

BNA_G

ClientSampleId :

GT-GW-1






Tgt Ion:330 Resp: 6557

Ion Ratio Lower Upper

330 100

332 97.4 79.0 118.6

141 38.4 25.0 37.6#

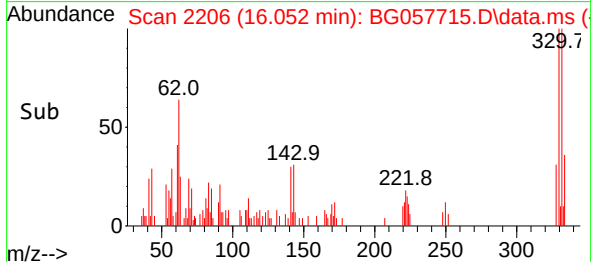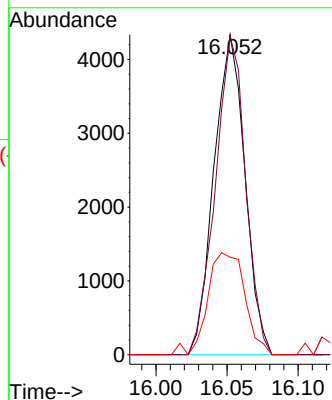

#45

2-Fluorobiphenyl

Concen: 6.401 ng

RT: 13.191 min Scan# 1719

Delta R.T. -0.009 min

Lab File: BG057715.D

Acq: 14 Jun 2023 20:06




Tgt Ion:172 Resp: 43545


Ion Ratio Lower Upper

172 100

171 33.1 27.9 41.9

170 22.4 18.2 27.4

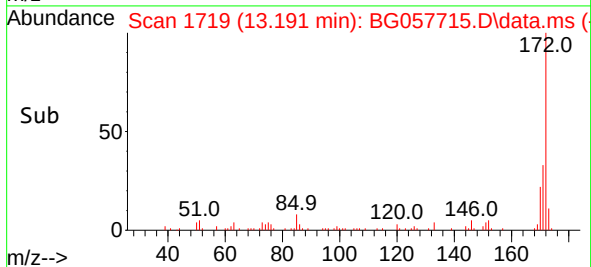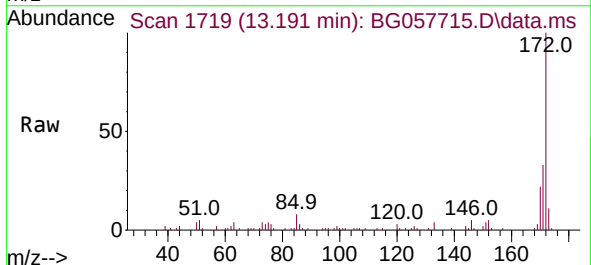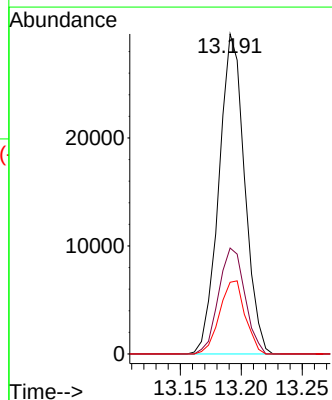



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.309 min Scan# 2420

Delta R.T. -0.009 min

Lab File: BG057715.D

Acq: 14 Jun 2023 20:06

Instrument :

BNA_G

ClientSampleId :

GT-GW-1





Tgt Ion:188 Resp: 223488

Ion Ratio Lower Upper

188 100

94 9.0 6.9 10.3

80 11.3 8.2 12.4

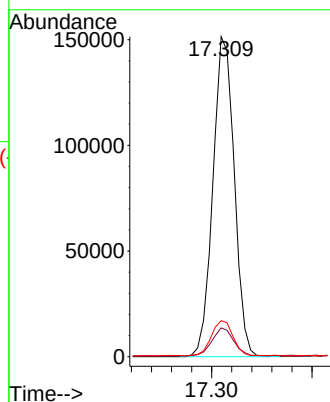

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.569 min Scan# 3145

Delta R.T. -0.003 min

Lab File: BG057715.D

Acq: 14 Jun 2023 20:06




Tgt Ion:240 Resp: 190914


Ion Ratio Lower Upper

240 100

120 11.3 8.1 12.1

236 26.8 20.7 31.1


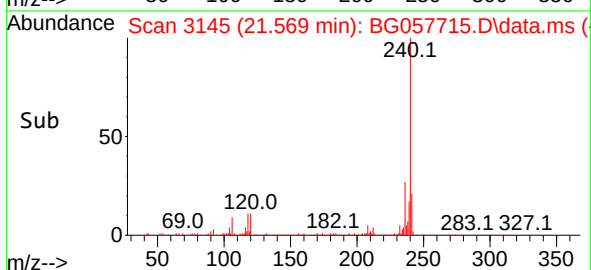
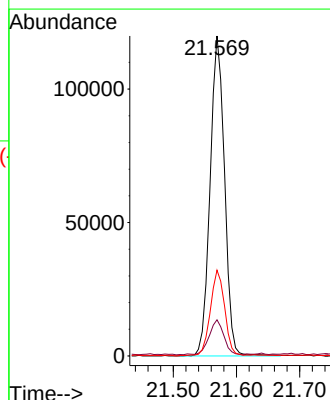





#79
 Terphenyl-d14
 Concen: 5.712 ng
 RT: 19.930 min Scan# 21
 Delta R.T. -0.003 min
 Lab File: BG057715.D
 Acq: 14 Jun 2023 20:06




Instrument :
 BNA_G
 ClientSampleId :
 GT-GW-1


Tgt Ion:244 Resp: 58986
 Ion Ratio Lower Upper
 244 100
 212 7.2 6.0 9.0
 122 10.8 7.7 11.5

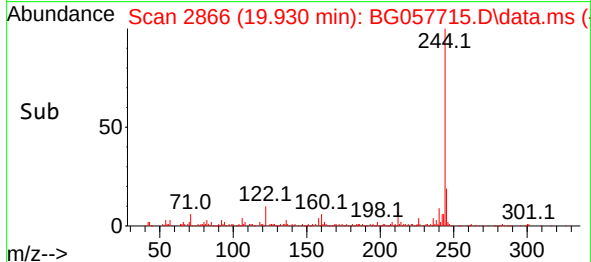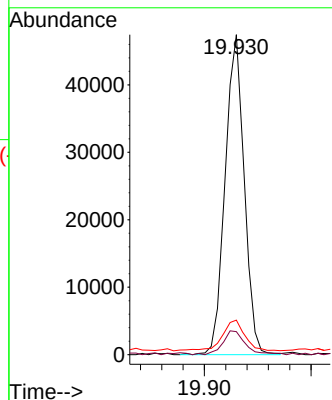

#84
 Bis(2-ethylhexyl)phthalate
 Concen: 4.379 ng
 RT: 21.475 min Scan# 3129
 Delta R.T. -0.003 min
 Lab File: BG057715.D
 Acq: 14 Jun 2023 20:06

Tgt Ion:149 Resp: 29303
 Ion Ratio Lower Upper
 149 100
 167 25.2 22.1 33.1
 279 4.2 3.0 4.4

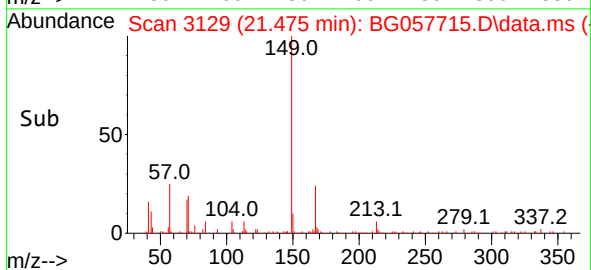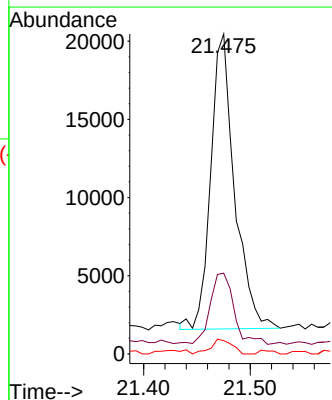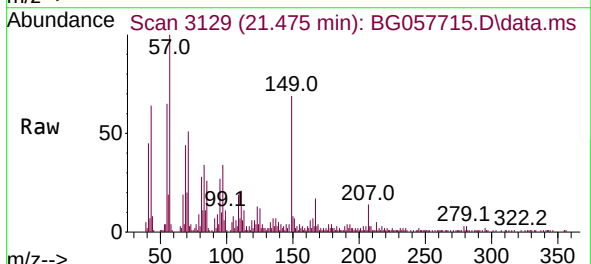



#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.736 min Scan# 30
 Delta R.T. -0.003 min
 Lab File: BG057715.D
 Acq: 14 Jun 2023 20:06

Instrument :
 BNA_G
 ClientSampleId :
 GT-GW-1

Tgt Ion:264 Resp: 230653
 Ion Ratio Lower Upper
 264 100
 260 22.5 17.3 25.9
 265 21.8 17.5 26.3

