

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061423\
 Data File : BG057704.D
 Acq On : 14 Jun 2023 12:19
 Operator : CG/JU
 Sample : 03156-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CONC-1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061323.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG057704.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.131	3	7	12	rBV	102459	141278	9.24%	1.750%
2	4.453	227	232	241	rVB	59271	87498	5.72%	1.084%
3	5.046	327	333	343	rVB	156007	230260	15.06%	2.852%
4	5.511	405	412	422	rBV	360604	553119	36.17%	6.850%
5	7.091	673	681	691	rBV	418481	694301	45.40%	8.598%
6	7.937	818	825	833	rVB	125286	213566	13.97%	2.645%
7	9.101	1014	1023	1031	rBV	221948	386231	25.26%	4.783%
8	10.740	1294	1302	1310	rBV	174295	303949	19.88%	3.764%
9	13.196	1713	1720	1727	rVB	657539	970906	63.49%	12.024%
10	14.571	1946	1954	1960	rVB2	262389	403986	26.42%	5.003%
11	15.922	2179	2184	2190	rBV	56491	79298	5.19%	0.982%
12	16.051	2200	2206	2216	rBV	249802	366220	23.95%	4.535%
13	17.314	2414	2421	2428	rVB	352664	535205	35.00%	6.628%
14	18.208	2568	2573	2575	rBV5	8996	17891	1.17%	0.222%
15	19.929	2860	2866	2877	rVB	1148964	1529139	100.00%	18.937%
16	20.405	2943	2947	2952	rVB2	39240	53379	3.49%	0.661%
17	20.575	2971	2976	2979	rBV	49196	60906	3.98%	0.754%
18	20.611	2979	2982	2990	rVB6	26211	52932	3.46%	0.656%
19	21.228	3083	3087	3092	rBV2	75059	111774	7.31%	1.384%
20	21.304	3098	3100	3103	rVB	16557	16910	1.11%	0.209%
21	21.339	3103	3106	3111	rVB6	17059	24967	1.63%	0.309%
22	21.568	3138	3145	3153	rBV2	324371	542449	35.47%	6.718%
23	22.220	3252	3256	3260	rVB3	11538	15363	1.00%	0.190%
24	22.379	3279	3283	3291	rVB3	13741	28931	1.89%	0.358%
25	23.866	3530	3536	3542	rBV2	33630	67987	4.45%	0.842%
26	24.729	3673	3683	3693	rBV	195992	553950	36.23%	6.860%
27	26.034	3899	3905	3911	rBV8	11781	32358	2.12%	0.401%




Sum of corrected areas: 8074753

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061423\
Data File : BG057704.D
Acq On : 14 Jun 2023 12:19
Operator : CG/JU
Sample : 03156-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CONC-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

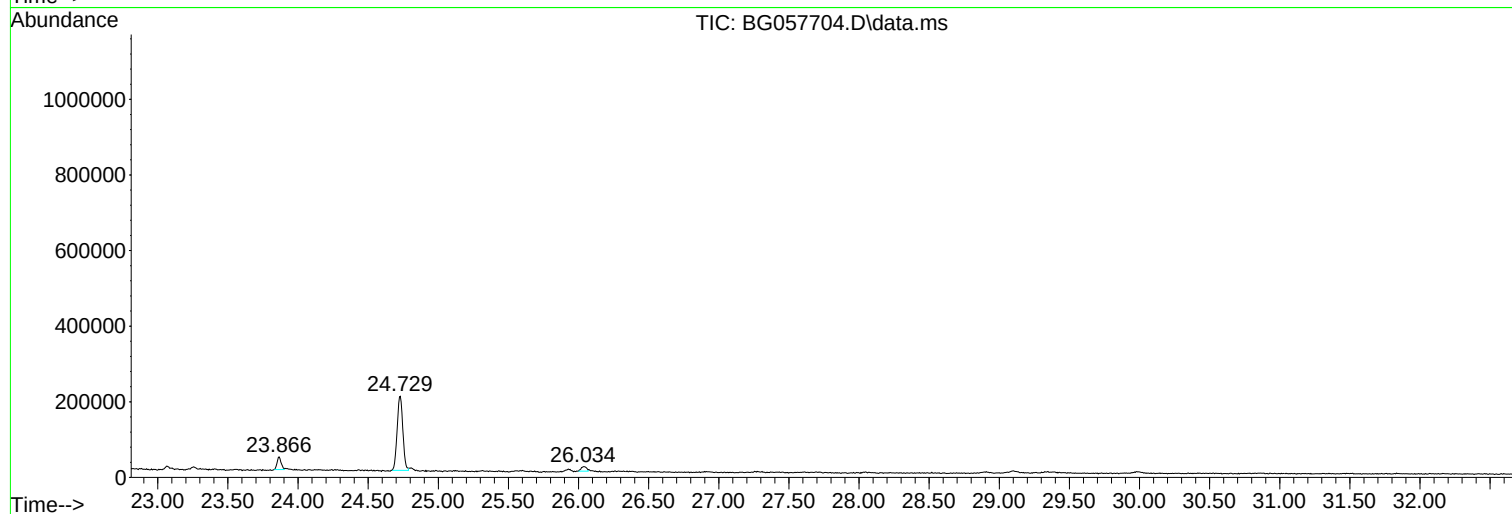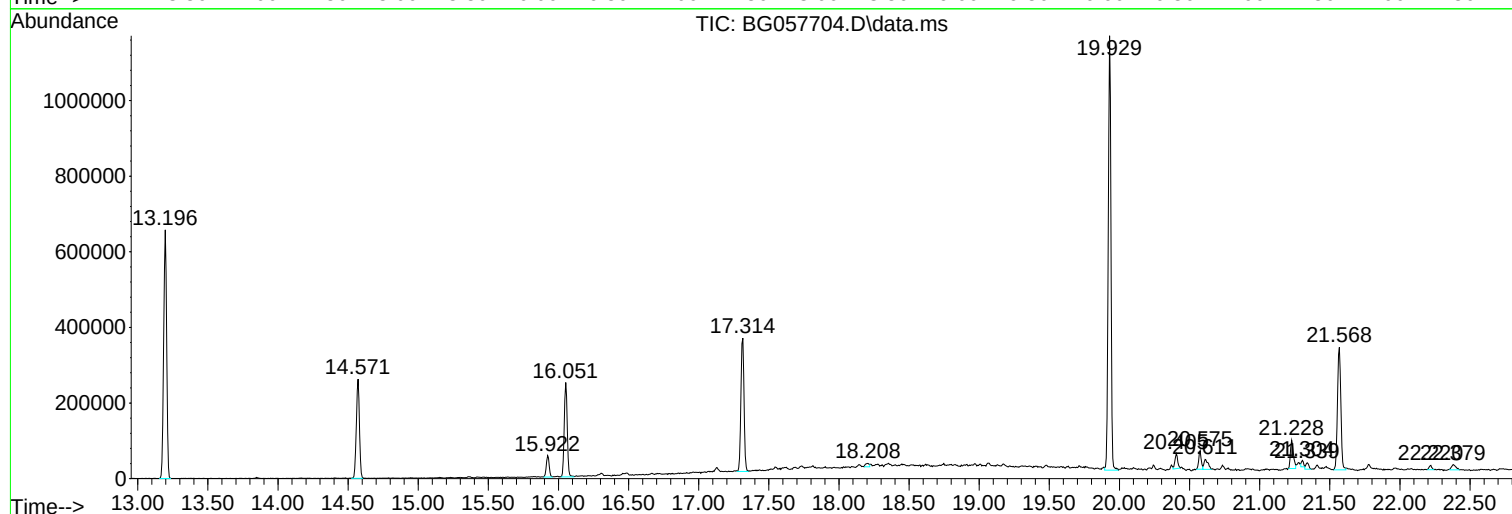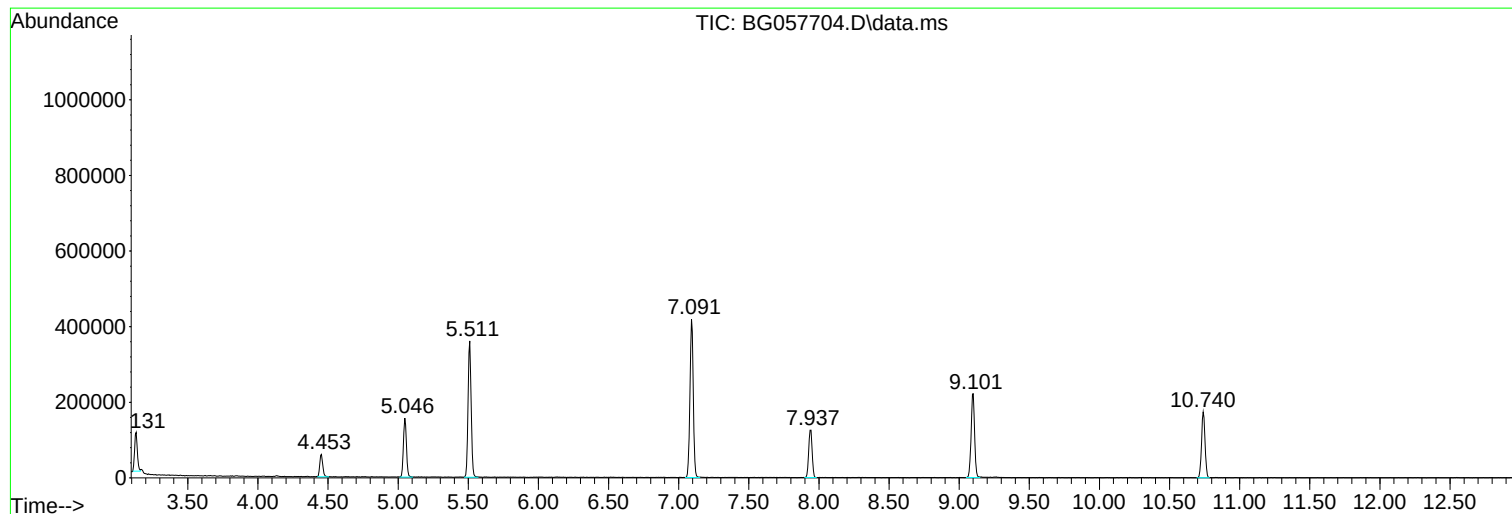

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061423\
Data File : BG057704.D
Acq On : 14 Jun 2023 12:19
Operator : CG/JU
Sample : 03156-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CONC-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061423\
Data File : BG057704.D
Acq On : 14 Jun 2023 12:19
Operator : CG/JU
Sample : 03156-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CONC-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------