


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061423\
Data File : BG057700.D
Acq On : 14 Jun 2023 9:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061323.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jun 14 03:52:08 2023

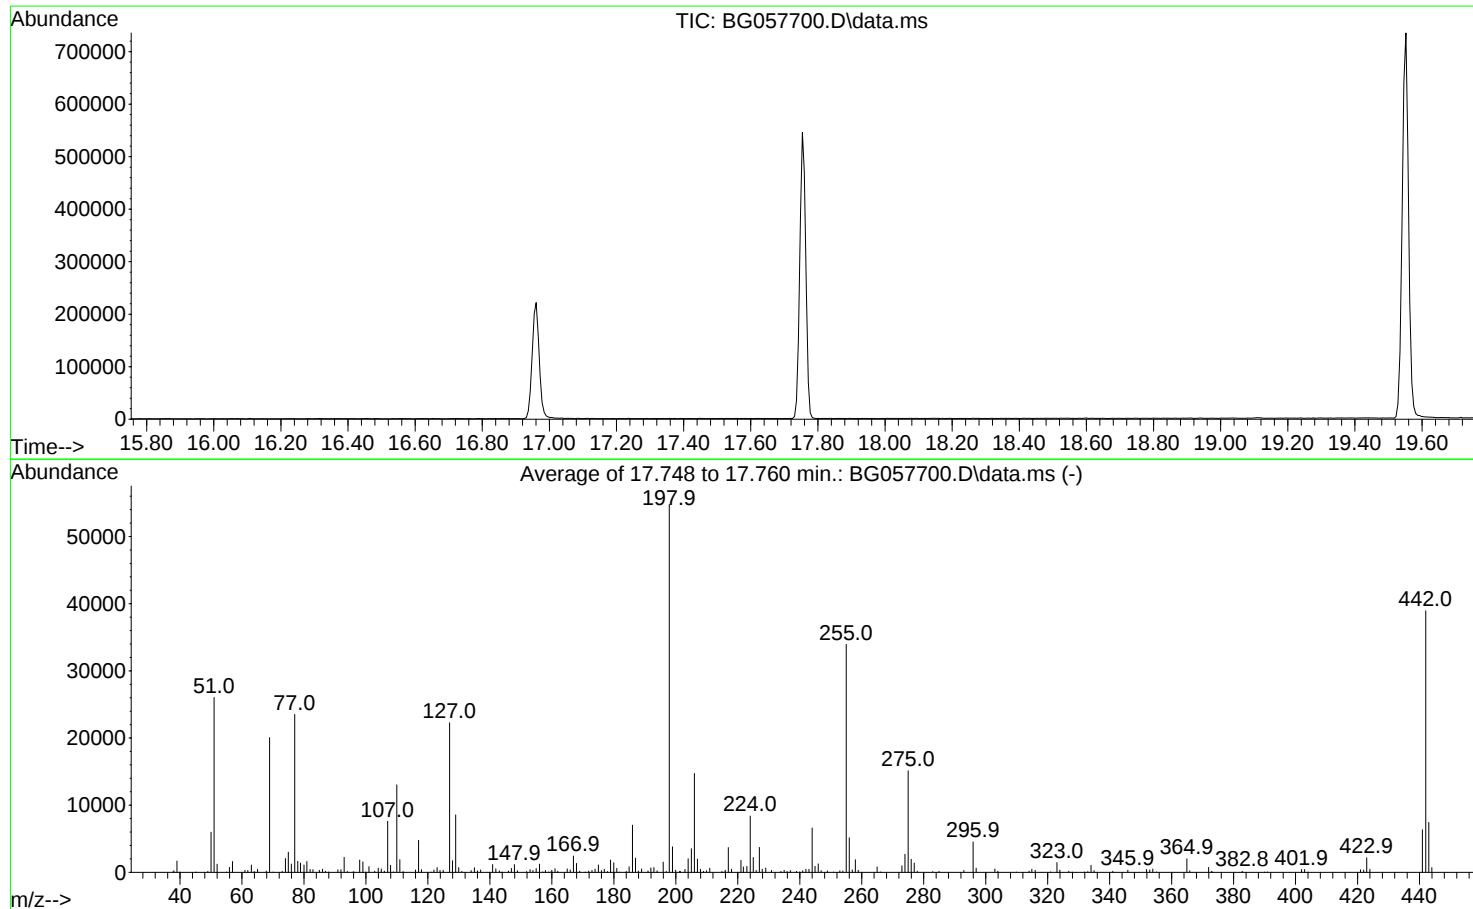

AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.6	26045	PASS
68	69	0.00	2	0.9	183	PASS
69	198	0.00	100	36.6	20048	PASS
70	69	0.00	2	0.2	50	PASS
127	198	10	80	40.7	22277	PASS
197	198	0.00	2	0.3	144	PASS
198	198	100	100	100.0	54768	PASS
199	198	5	9	7.0	3812	PASS
275	198	10	60	27.6	15117	PASS
365	198	1	100	3.7	2026	PASS
441	198	0.01	100	11.6	6348	PASS
442	442	50	100	100.0	38944	PASS
443	442	15	24	19.1	7422	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/14/2023	BNA_G	<u>BG057700.D</u>
Compound Name	Response	Retention Time
DDT	110366	20.786
DDD	1253	20.398
DDE	0	20.162
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1253	111619	1.12

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061423\
Data File : BG057700.D
Acq On : 14 Jun 2023 9:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 15 02:31:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 14 03:52:08 2023
Response via : Initial Calibration

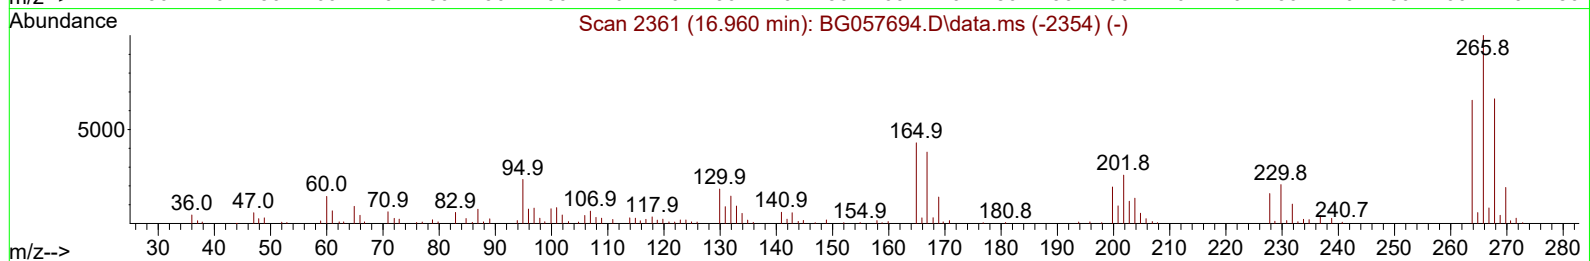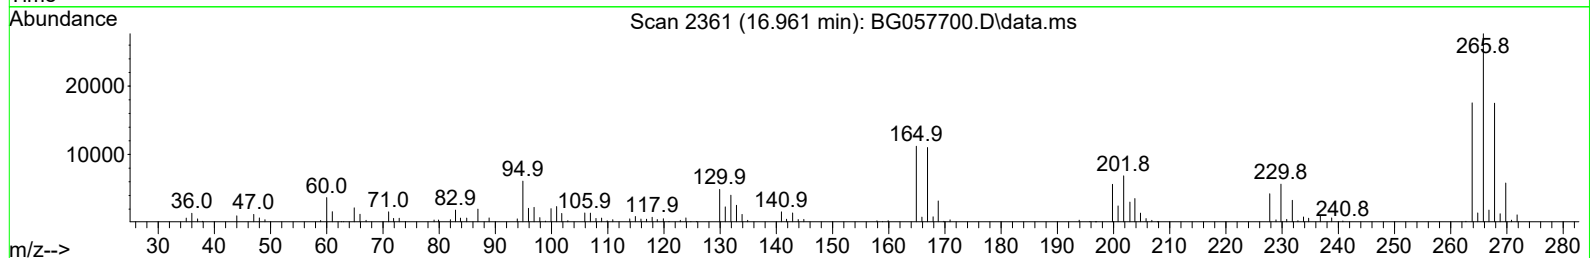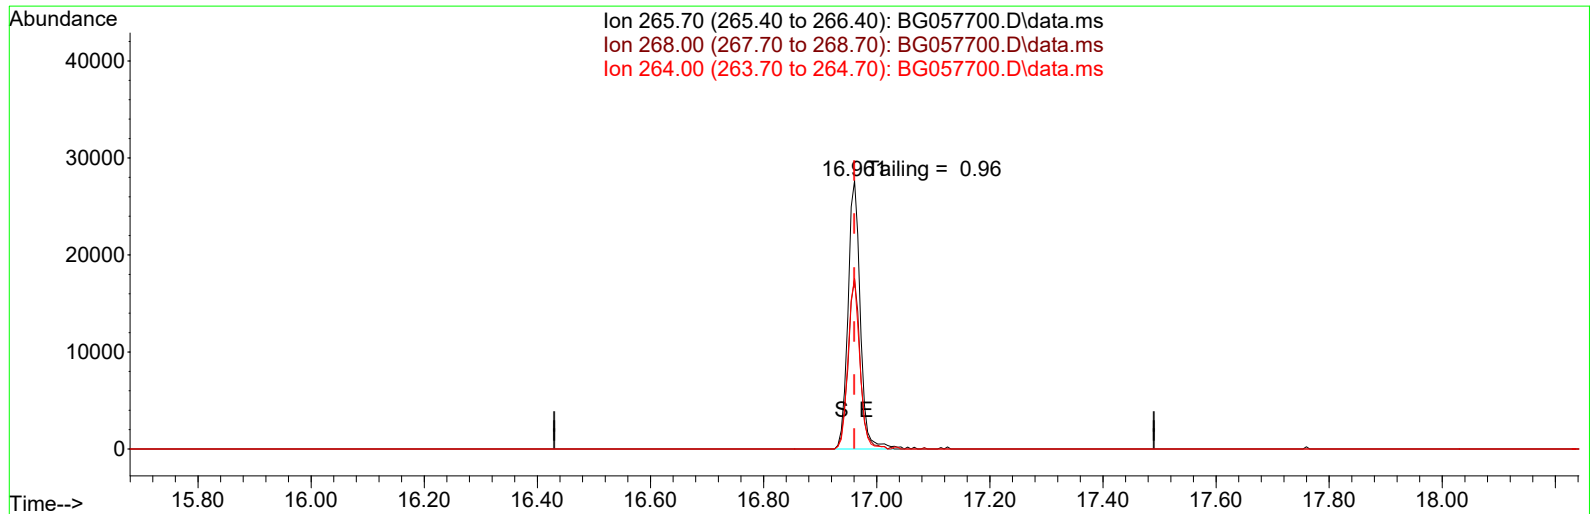

TIC: BG057700.D\data.ms

(70) Pentachlorophenol (C)

16.961min (+ 0.001) 32591.69 ng




response 41851

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	63.27
264.00	65.50	63.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061423\
Data File : BG057700.D
Acq On : 14 Jun 2023 9:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 15 02:31:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 14 03:52:08 2023
Response via : Initial Calibration

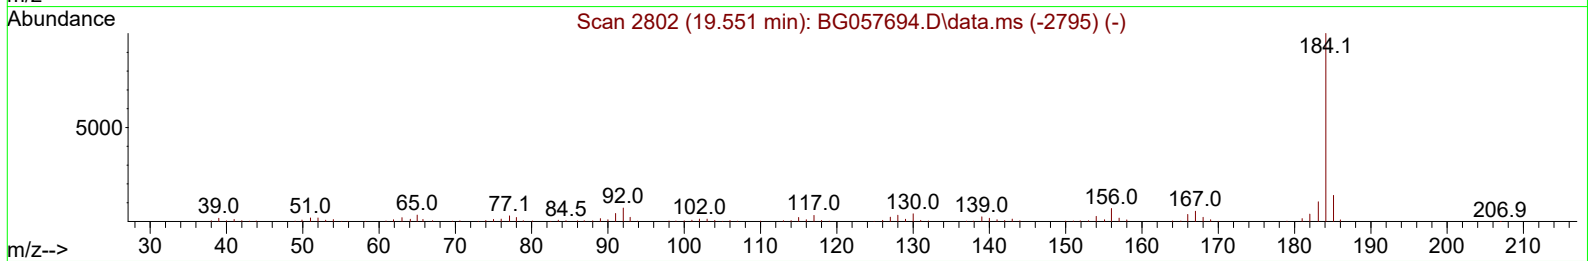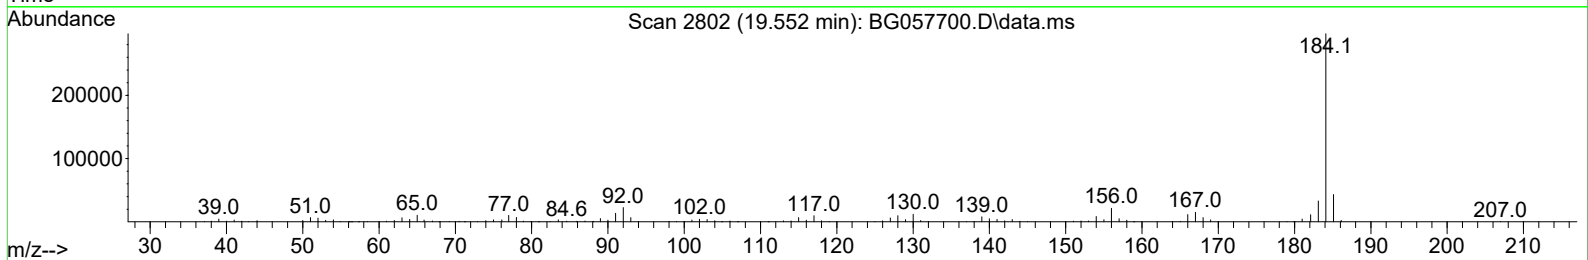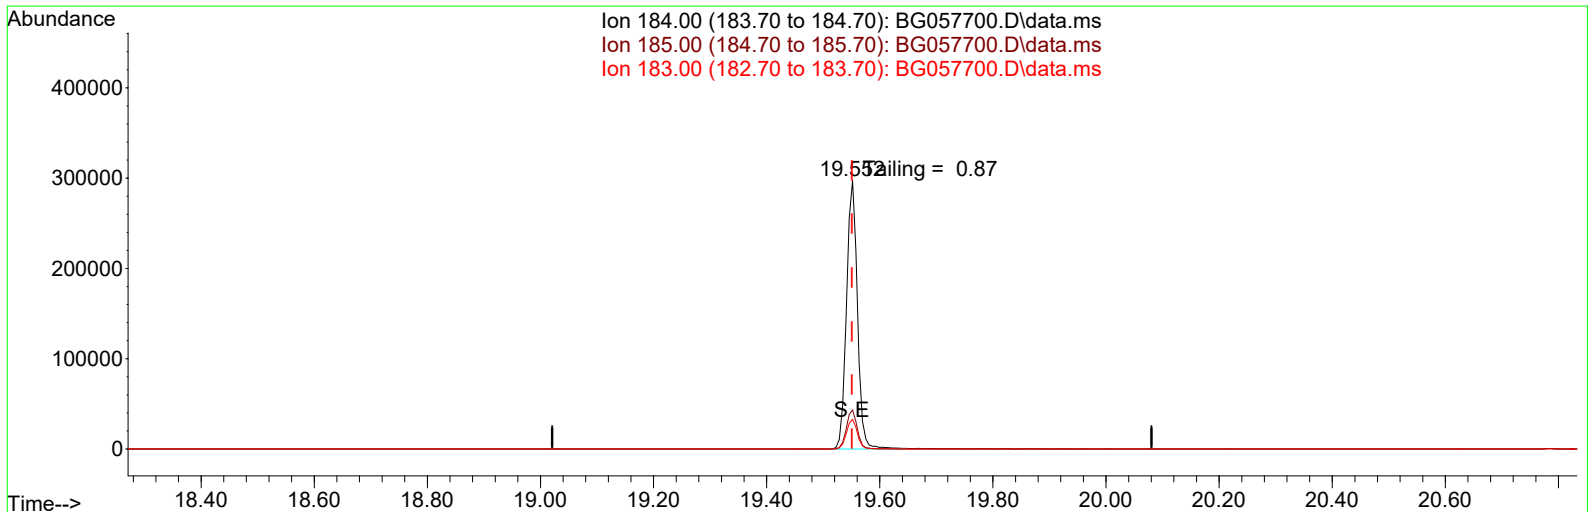

TIC: BG057700.D\data.ms

(77) Benzidine

19.552min (+ 0.001) 0.00 ng

response 399991

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.56
183.00	10.50	11.12
0.00	0.00	0.00