
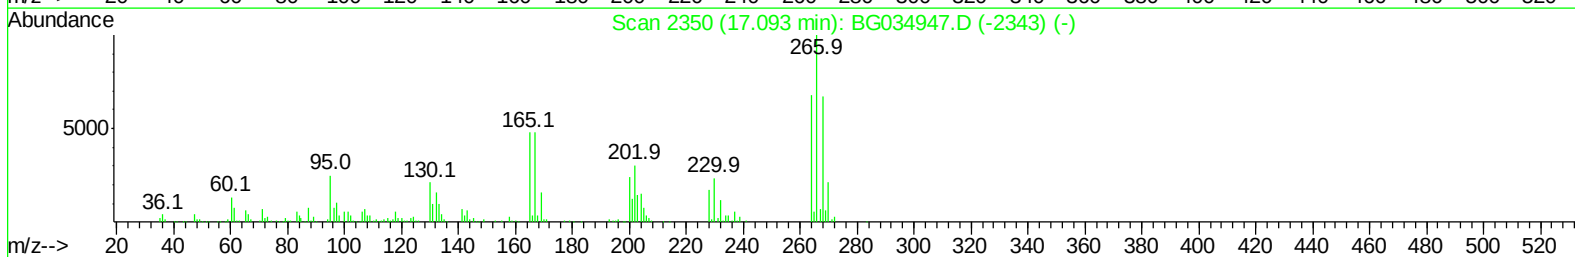
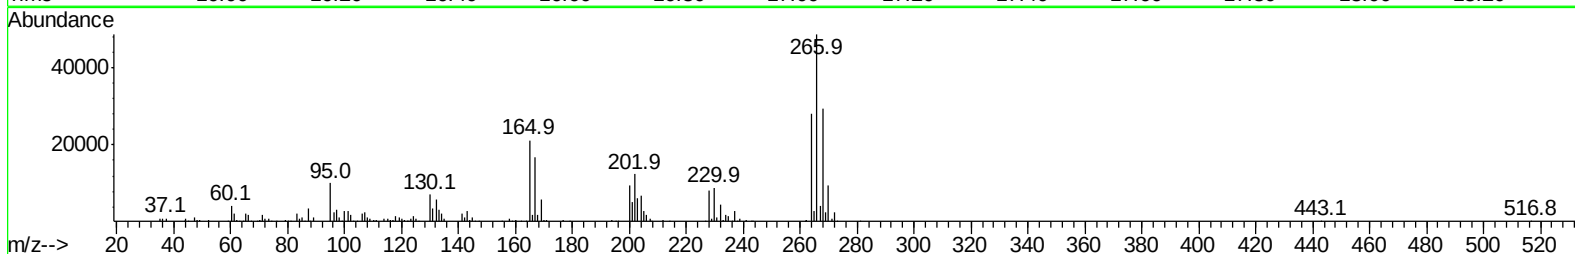


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061518\
Data File : BG035174.D
Acq On : 15 Jun 2018 15:51
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 18 06:59:13 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

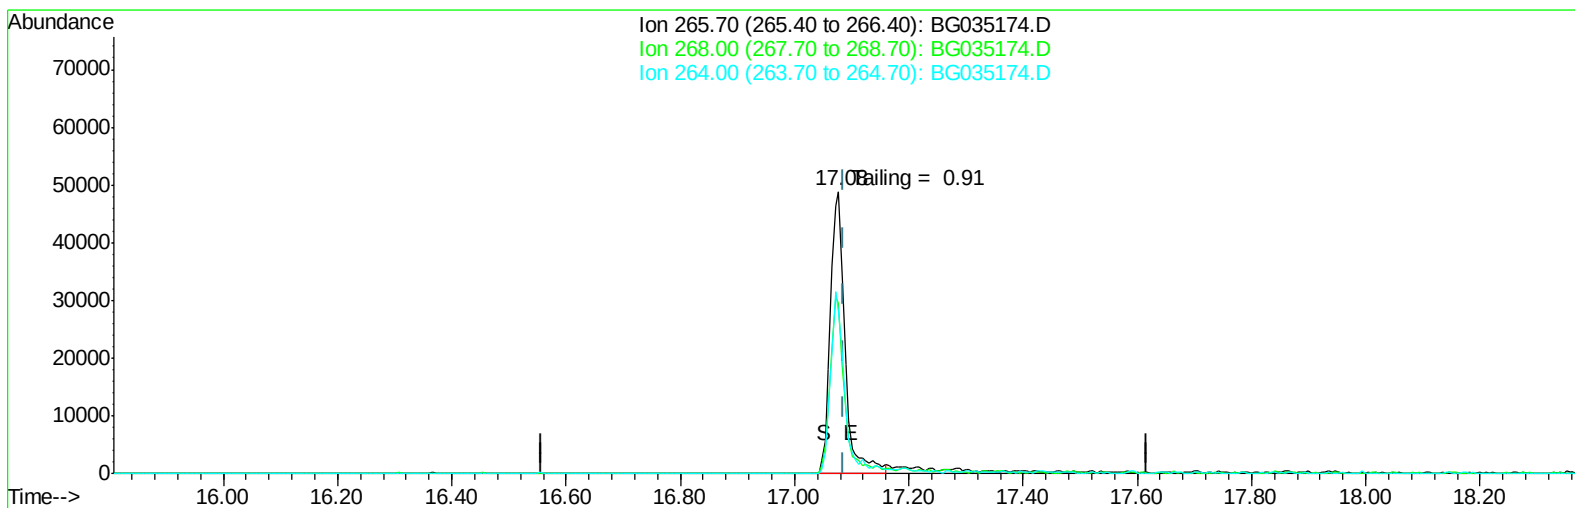

TIC: BG035174.D

(69) Pentachlorophenol (C)




17.077min (-0.010) 15697.10ng m

response 86165

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.25
264.00	62.00	57.65
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061518\
Data File : BG035174.D
Acq On : 15 Jun 2018 15:51
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 18 06:59:13 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

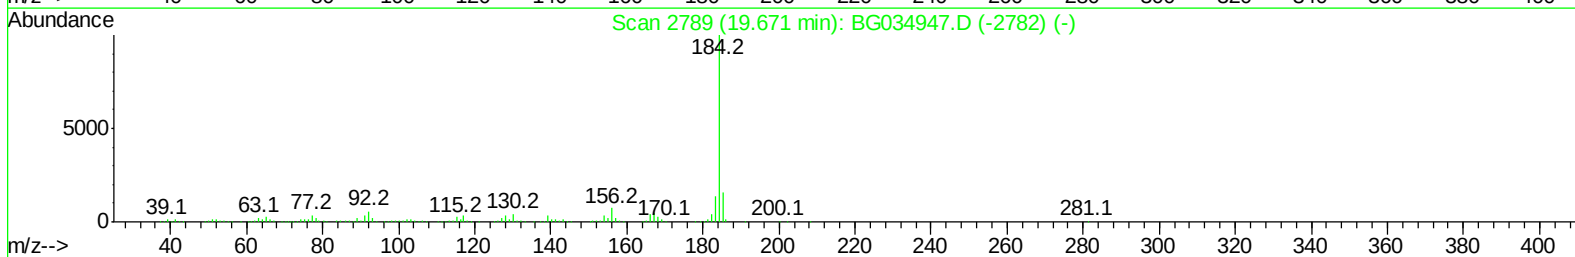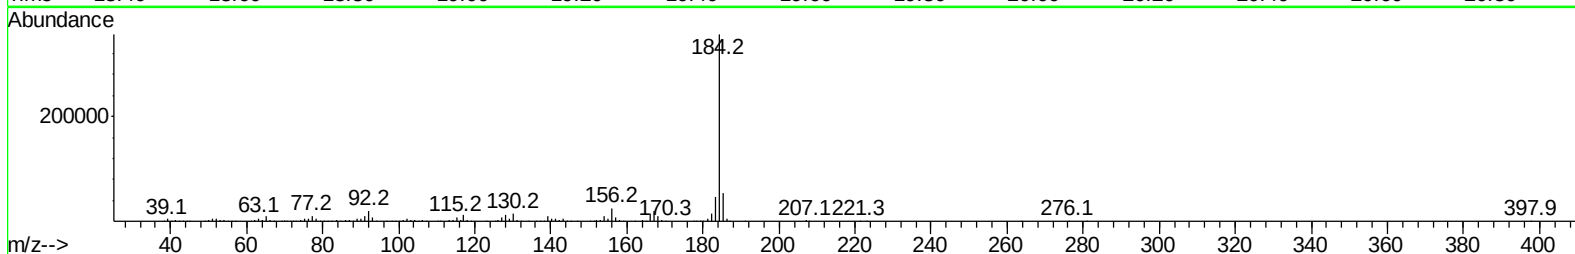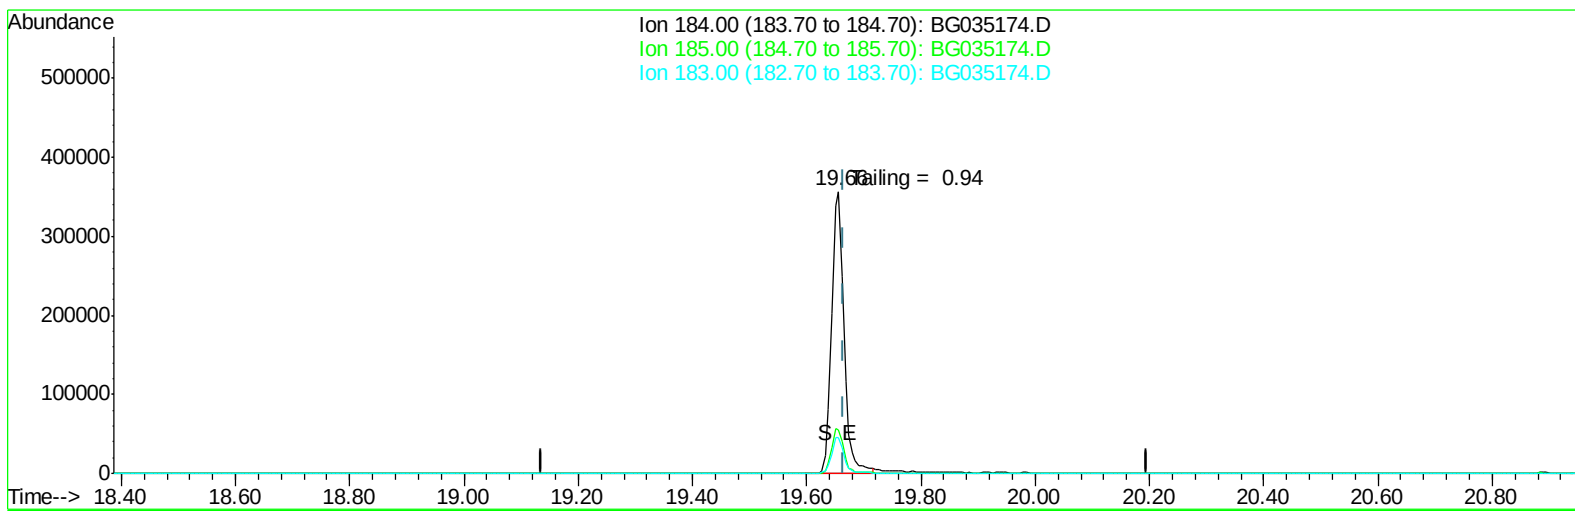

TIC: BG035174.D

(76) Benzidine

19.656min (-0.010) 212922.55ng

response 546583

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.28
183.00	13.30	12.81
0.00	0.00	0.00