
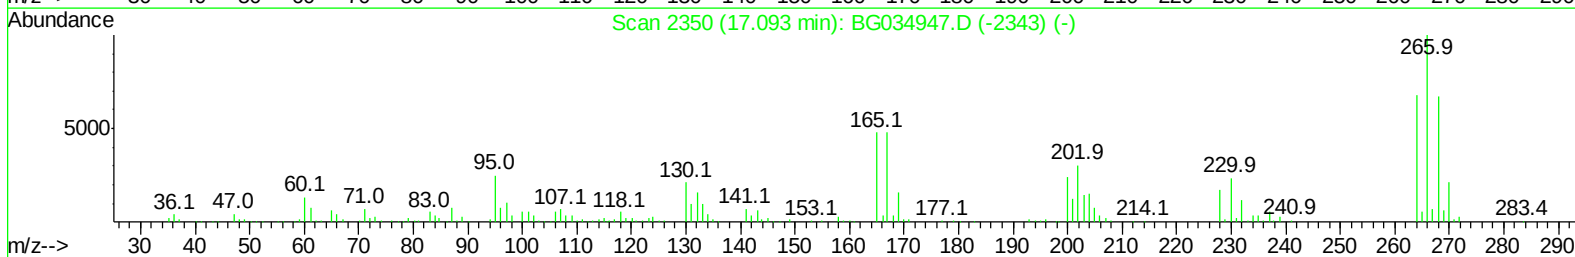
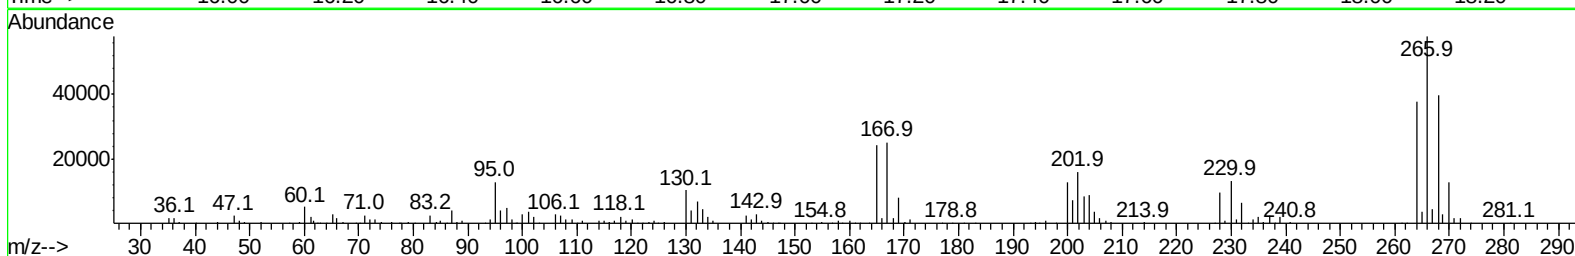


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061518\
Data File : BG035192.D
Acq On : 16 Jun 2018 4:45
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 18 07:02:39 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

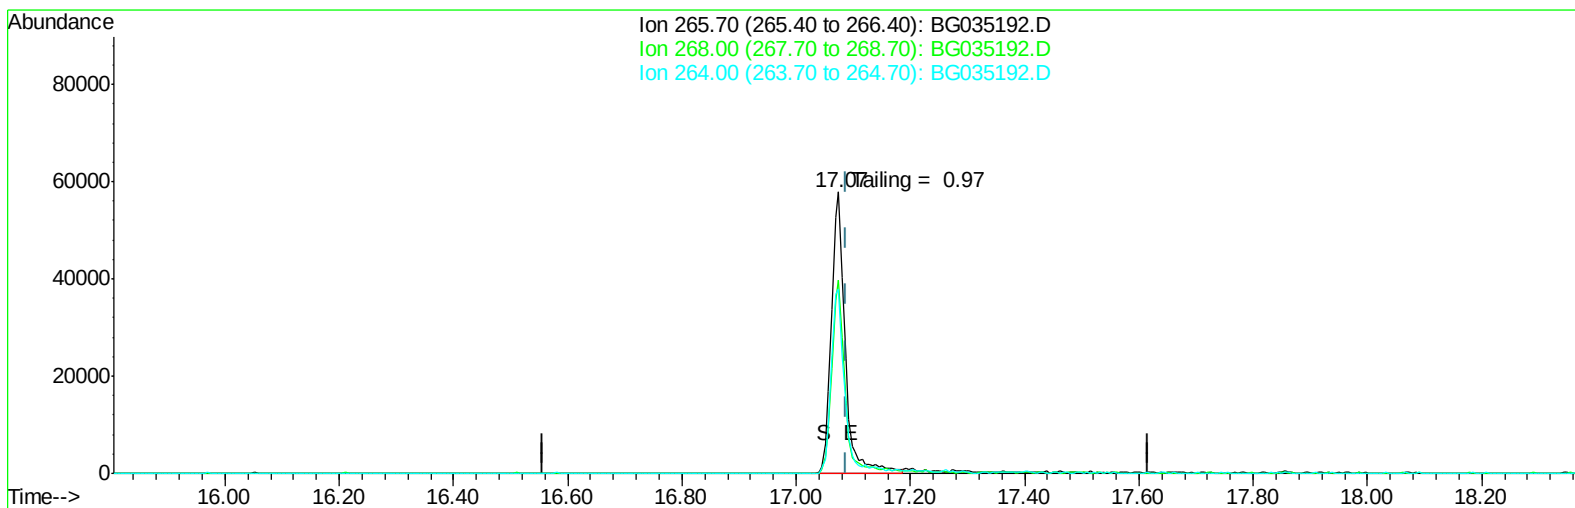

TIC: BG035192.D

(69) Pentachlorophenol (C)




17.074min (-0.013) 117607.36ng

response 96933

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	68.49
264.00	62.00	65.48
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061518\
 Data File : BG035192.D
 Acq On : 16 Jun 2018 4:45
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 18 07:02:39 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 08 17:16:28 2018
 Response via : Initial Calibration

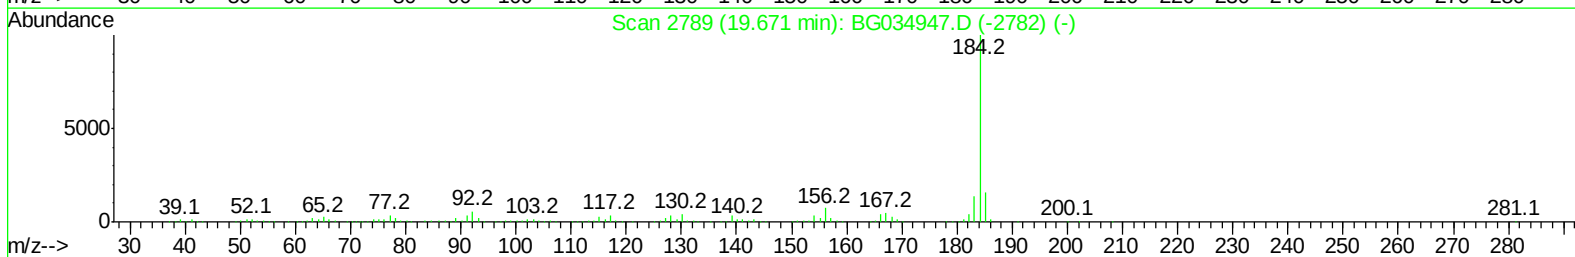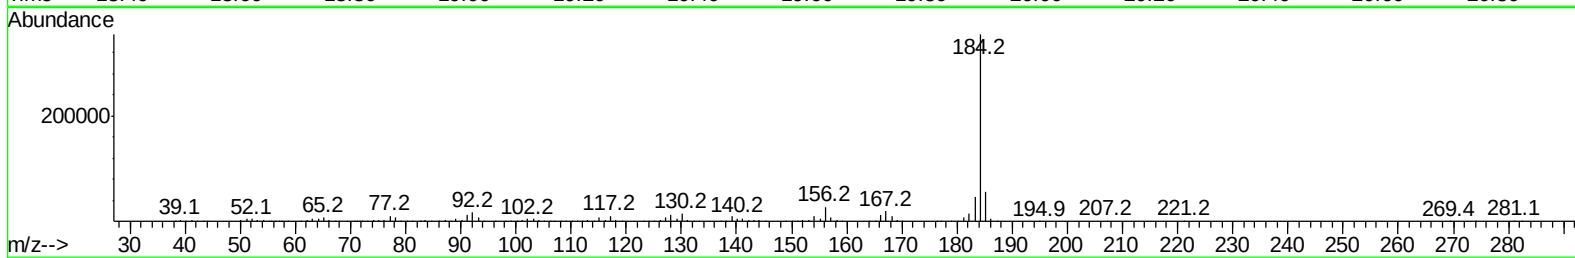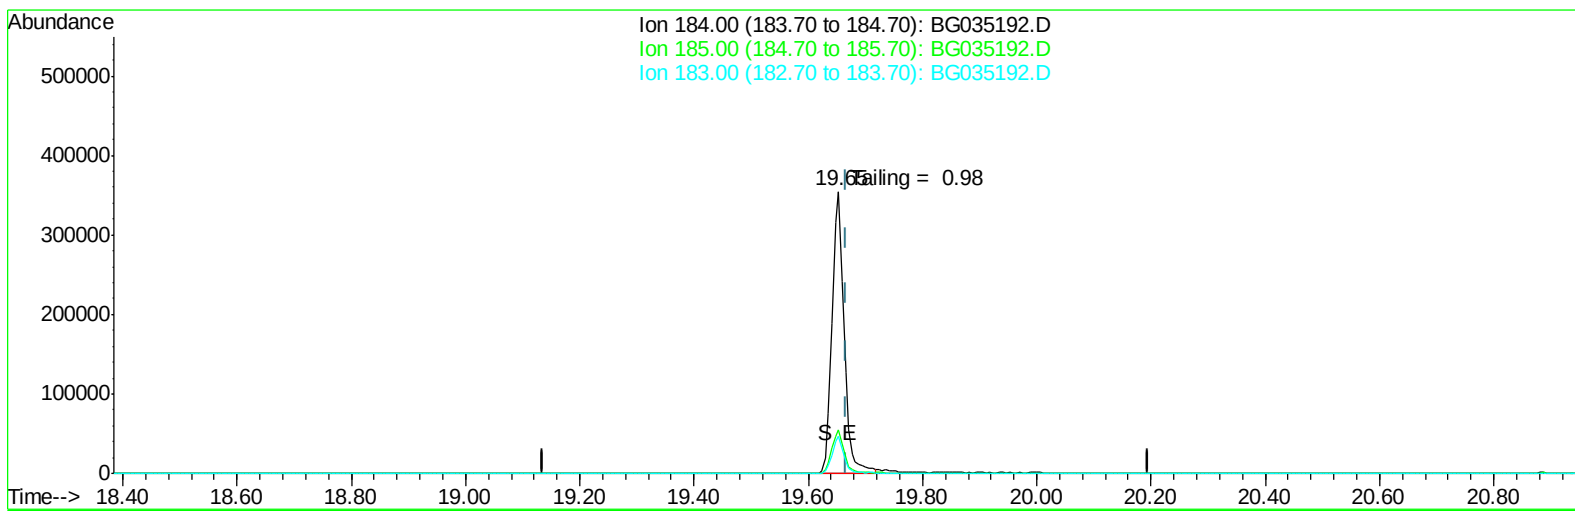

TIC: BG035192.D

(76) Benzidine

19.653min (-0.013) 192330.82ng

response 529500

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.50
183.00	13.30	13.04
0.00	0.00	0.00