

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061518\
 Data File : BG035189.D
 Acq On : 16 Jun 2018 2:10
 Operator : SJ/JU
 Sample : J3518-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EPE-106-7(65-67)

Quant Time: Jun 16 04:06:30 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 08 17:16:28 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	42873	20.00	ng	-0.01
21) Naphthalene-d8	10.87	136	174777	20.00	ng	-0.02
38) Acenaphthene-d10	14.68	164	130027	20.00	ng	-0.01
63) Phenanthrene-d10	17.42	188	356797	20.00	ng	-0.02
75) Chrysene-d12	21.69	240	390365	20.00	ng	-0.02
86) Perylene-d12	24.92	264	357383	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	355644	139.99	ng	0.00
7) Phenol-d6	7.22	99	547948	146.14	ng	0.00
23) Nitrobenzene-d5	9.22	82	350769	95.40	ng	-0.02
41) 2,4,6-Tribromophenol	16.17	330	261192	156.92	ng	-0.01
44) 2-Fluorobiphenyl	13.31	172	800681	80.05	ng	-0.02
78) Terphenyl-d14	20.03	244	1356331	72.78	ng	-0.02
Target Compounds						
49) Dimethylphthalate	14.13	163	101882	8.985	ng	Qvalue # 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061518\
Data File : BG035189.D
Acq On : 16 Jun 2018 2:10
Operator : SJ/JU
Sample : J3518-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EPE-106-7(65-67)

Quant Time: Jun 16 04:06:30 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

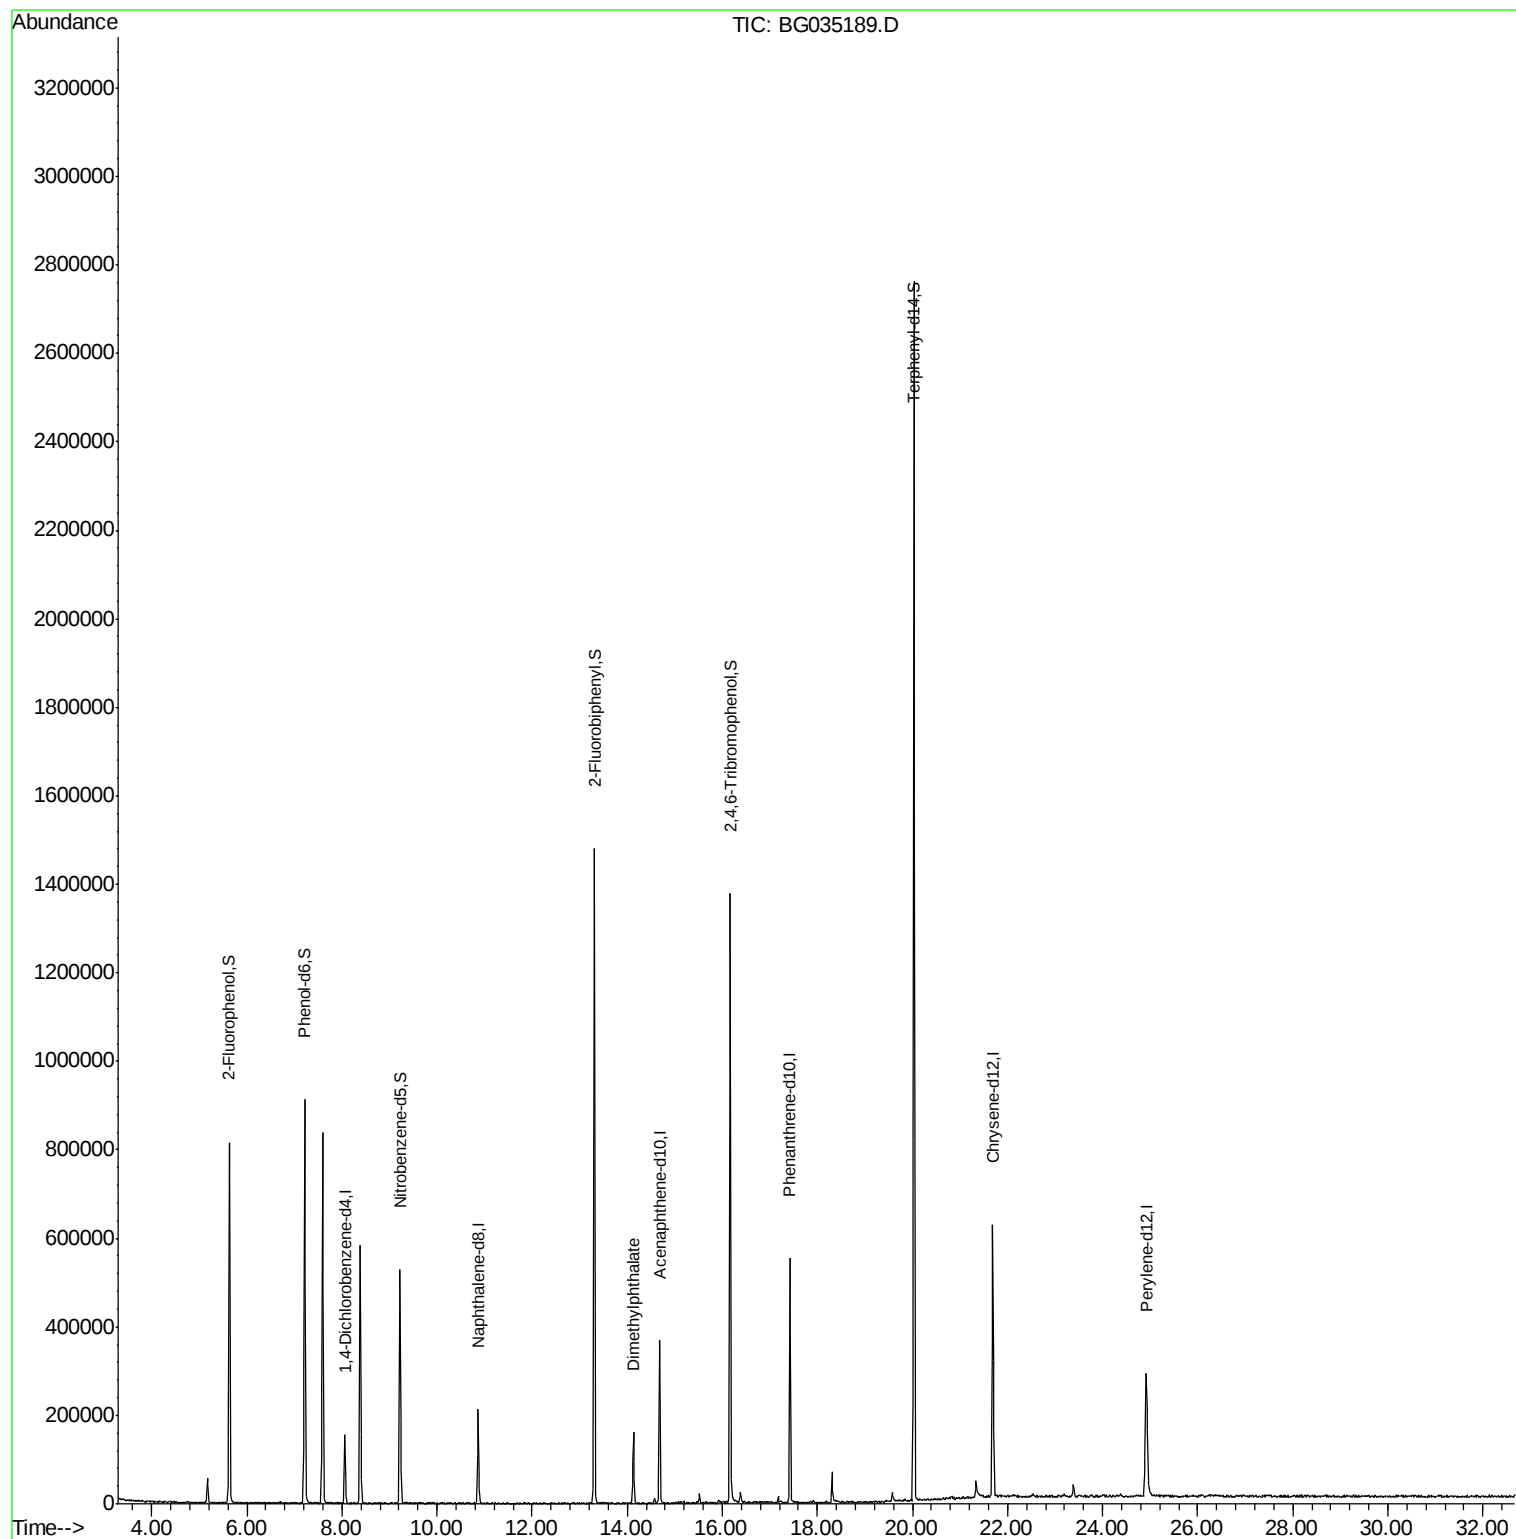




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.06 min Scan# 813
Delta R.T. -0.01 min
Lab File: BG035189.D
Acq: 16 Jun 2018 2:10

Instrument :
BNA_G
ClientSampleId :
EPE-106-7(65-67)

Tot Ion:152 Resp: 42873
Ion Ratio Lower Upper
152 100
150 154.9 126.6 189.8
115 60.3 53.0 79.4

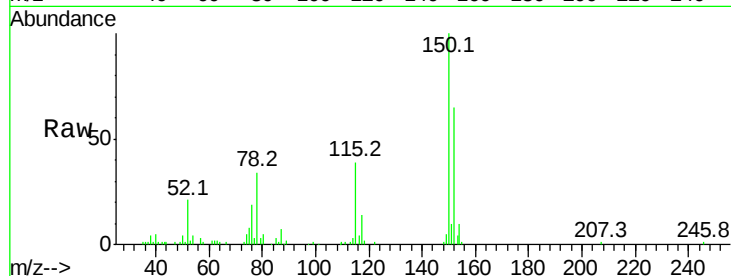


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

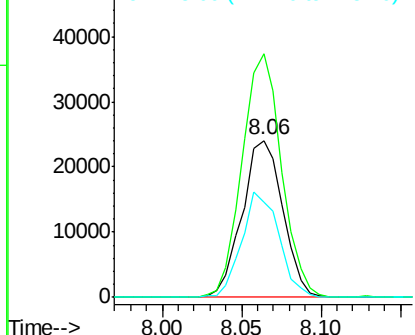



#5


2-Fluorophenol
Concen: 139.992 ng
RT: 5.64 min Scan# 400
Delta R.T. -0.01 min
Lab File: BG035189.D
Acq: 16 Jun 2018 2:10

Tgt Ion:112 Resp: 355644
Ion Ratio Lower Upper
112 100
64 62.2 56.3 84.5
63 33.7 30.1 45.1

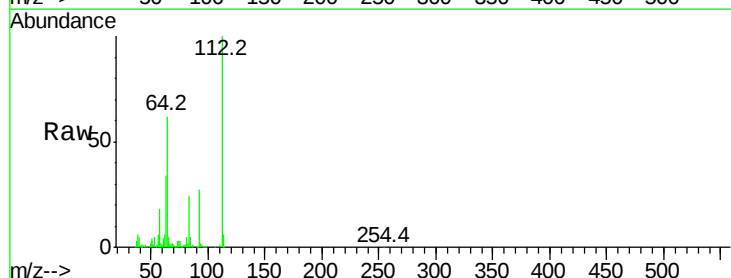

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

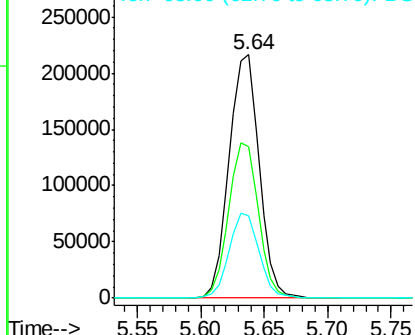

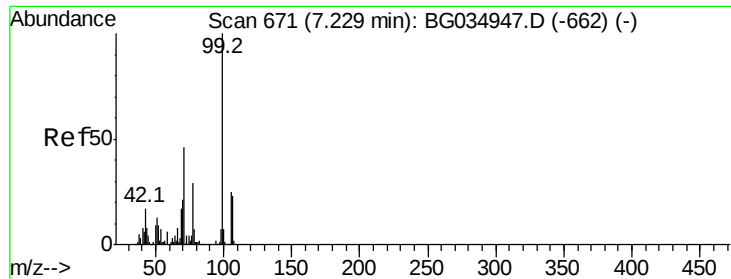

#7

Phenol-d6

Concen: 146.136 ng

RT: 7.22 min Scan# 669

Delta R.T. -0.01 min

Lab File: BG035189.D

Acq: 16 Jun 2018 2:10

Instrument :

BNA_G

ClientSampleId :

EPE-106-7(65-67)





Tot Ion: 99 Resp: 547948

Ion Ratio Lower Upper

99 100

42 16.2 14.1 21.1

71 42.6 26.1 39.1#

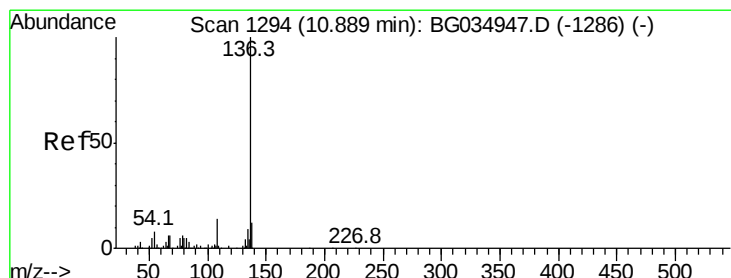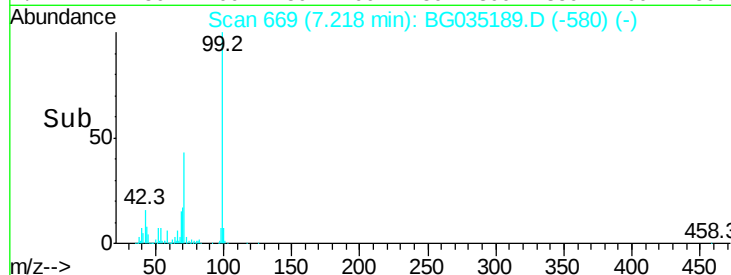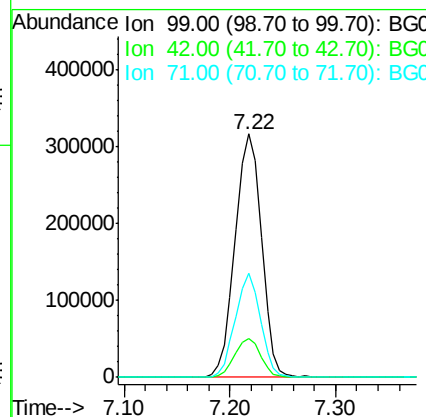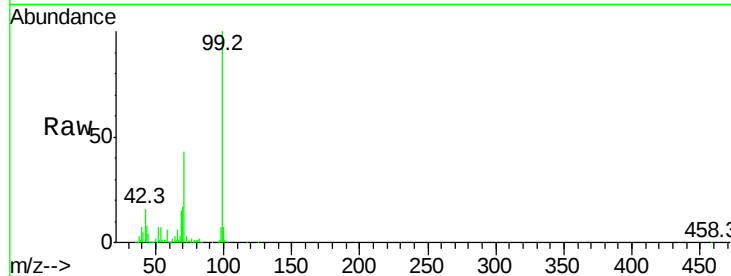

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.87 min Scan# 1290

Delta R.T. -0.02 min

Lab File: BG035189.D

Acq: 16 Jun 2018 2:10

Tgt Ion: 136 Resp: 174777




Ion Ratio Lower Upper


136 100

137 11.7 9.2 13.8

54 5.7 10.3 15.5#

68 4.6 4.5 6.7

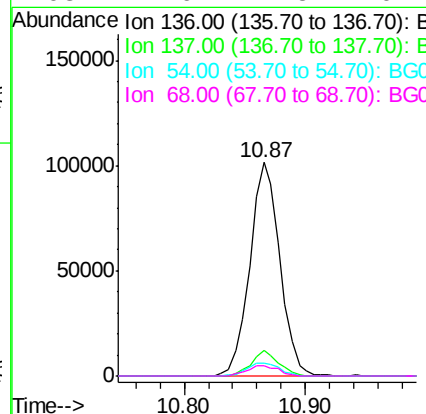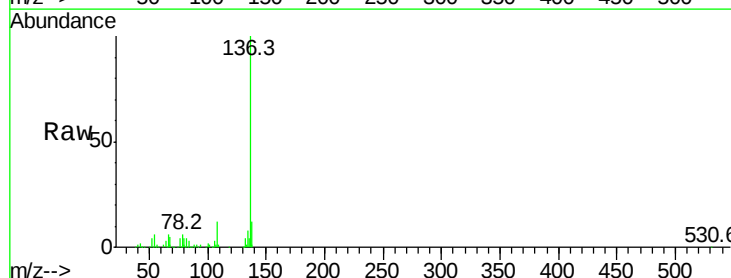

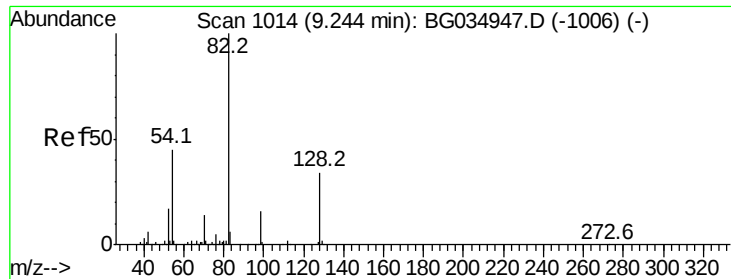

#23

Nitrobenzene-d5

Concen: 95.399 ng

RT: 9.22 min Scan# 1010

Delta R.T. -0.02 min

Lab File: BG035189.D

Acq: 16 Jun 2018 2:10

Instrument :

BNA_G

ClientSampleId :

EPE-106-7(65-67)





Tot Ion: 82 Resp: 350769

Ion Ratio Lower Upper

82 100

128 35.3 29.7 44.5

54 42.5 43.1 64.7#

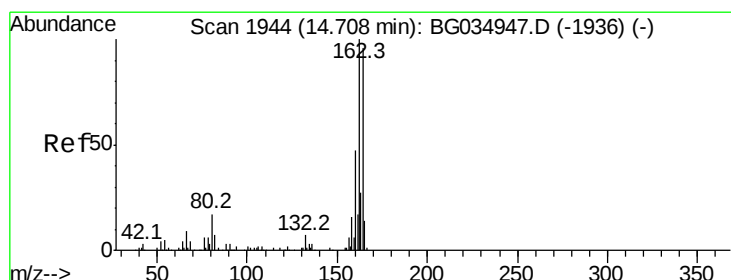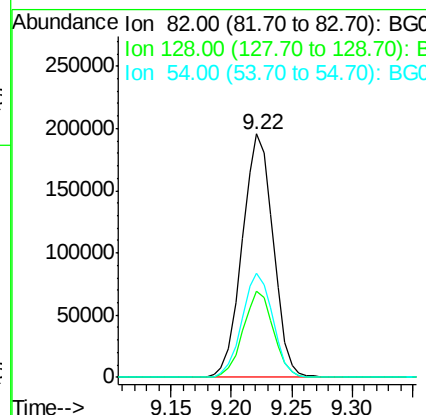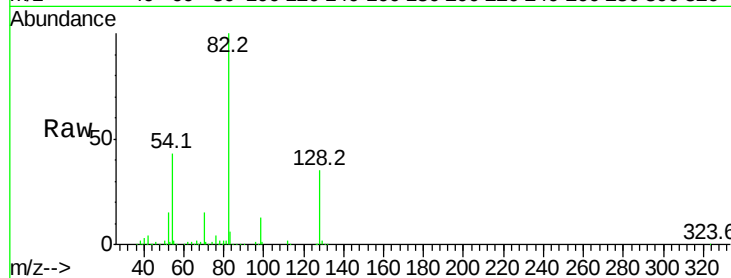

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.68 min Scan# 1940

Delta R.T. -0.01 min

Lab File: BG035189.D

Acq: 16 Jun 2018 2:10




Tgt Ion: 164 Resp: 130027


Ion Ratio Lower Upper

164 100

162 99.3 78.8 118.2

160 46.5 35.4 53.0


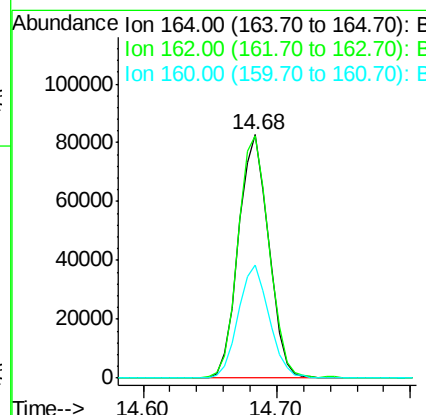
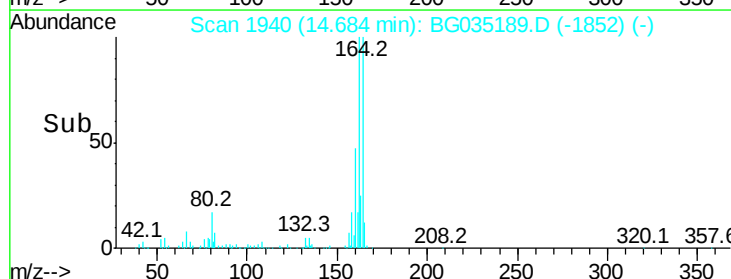
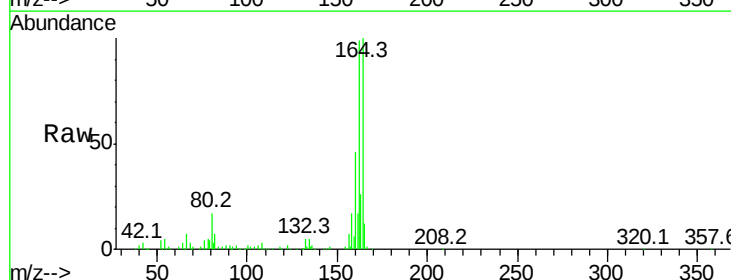


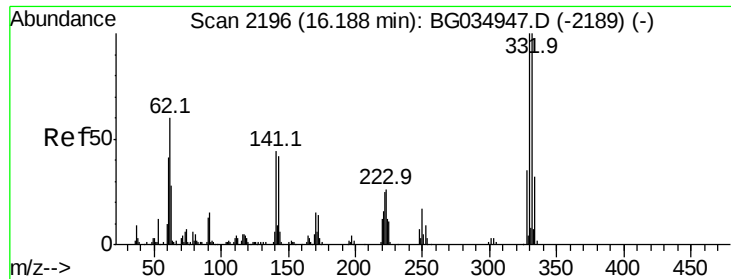

#41
 2,4,6-Tribromophenol
 Concen: 156.918 ng
 RT: 16.17 min Scan# 2193
 Delta R.T. -0.01 min
 Lab File: BG035189.D
 Acq: 16 Jun 2018 2:10




Instrument :
 BNA_G
 ClientSampleId :
 EPE-106-7(65-67)


Tot Ion	Ratio	Lower	Upper
330	100		
332	95.9	77.0	115.6
141	38.8	25.2	37.8#

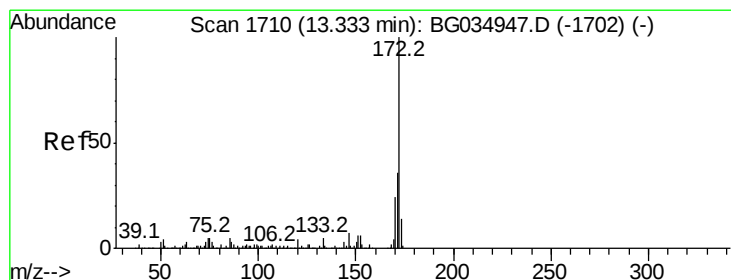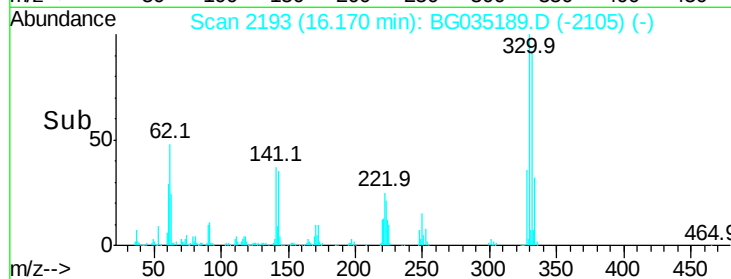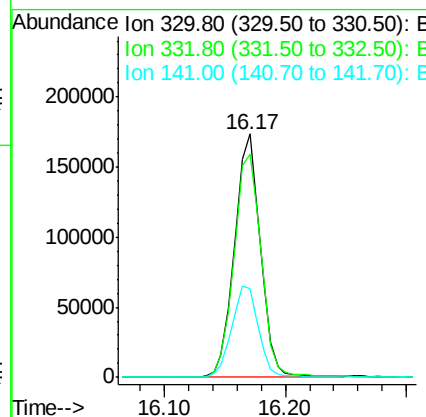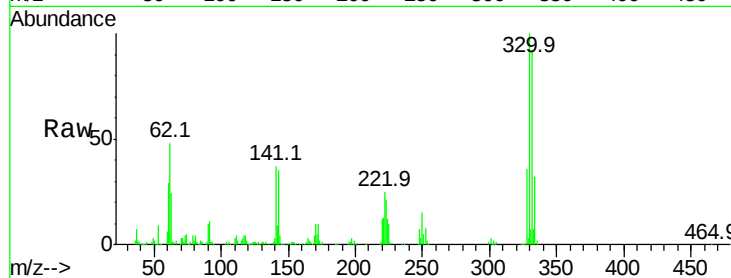

#44
 2-Fluorobiphenyl
 Concen: 80.051 ng
 RT: 13.31 min Scan# 1706
 Delta R.T. -0.02 min
 Lab File: BG035189.D
 Acq: 16 Jun 2018 2:10

Tgt Ion	Ratio	Lower	Upper
172	100		
171	34.5	30.0	45.0
170	23.7	19.5	29.3


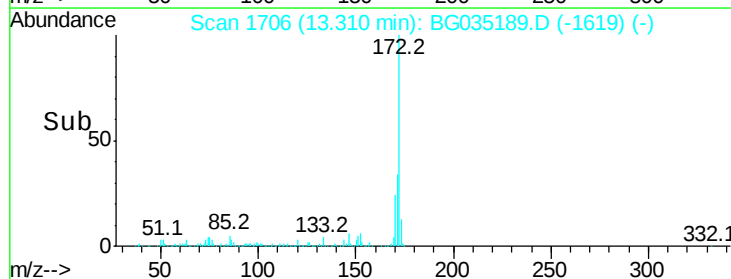
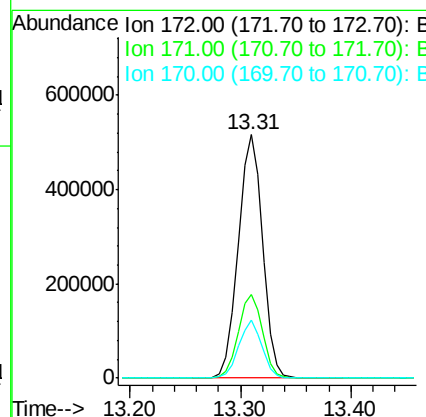
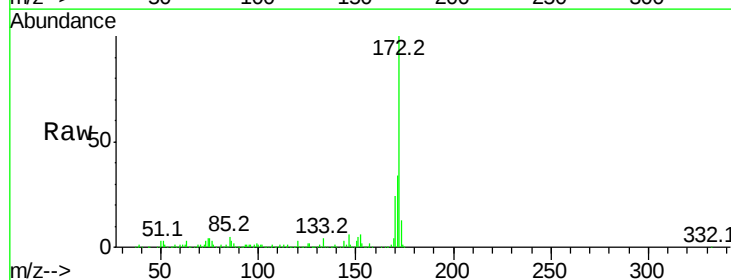


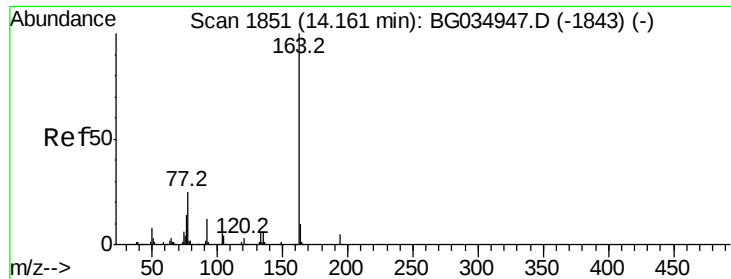

#49
Dimethylphthalate
Concen: 8.985 ng
RT: 14.13 min Scan# 1846
Delta R.T. -0.02 min
Lab File: BG035189.D
Acq: 16 Jun 2018 2:10




Instrument :
BNA_G
ClientSampleId :
EPE-106-7(65-67)


Tot Ion:163 Resp: 101882
Ion Ratio Lower Upper
163 100
194 5.5 3.4 5.2#
164 10.4 8.2 12.4

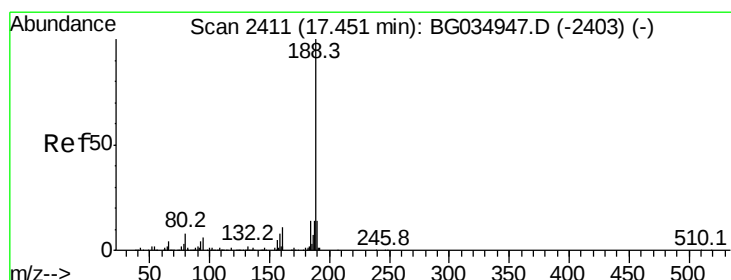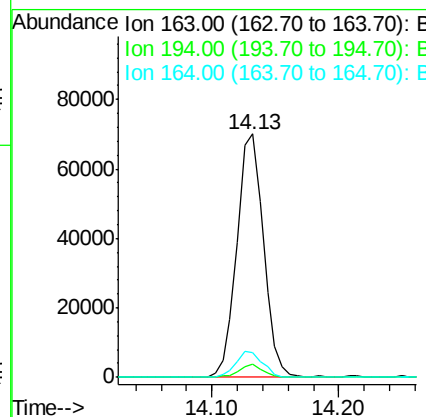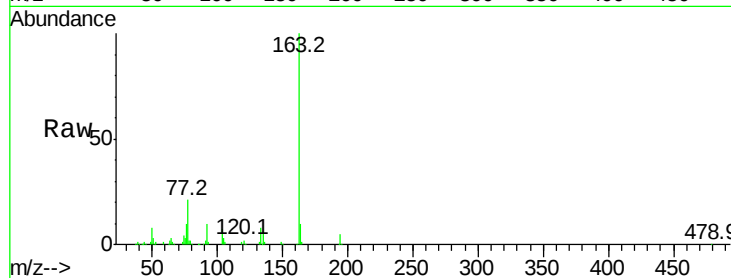

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.42 min Scan# 2406
Delta R.T. -0.02 min
Lab File: BG035189.D
Acq: 16 Jun 2018 2:10

Tgt Ion:188 Resp: 356797
Ion Ratio Lower Upper
188 100
94 5.6 6.9 10.3#
80 7.6 7.7 11.5#

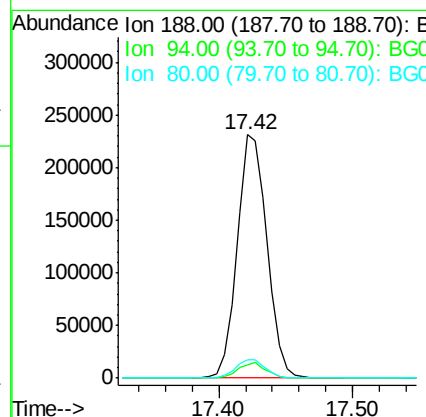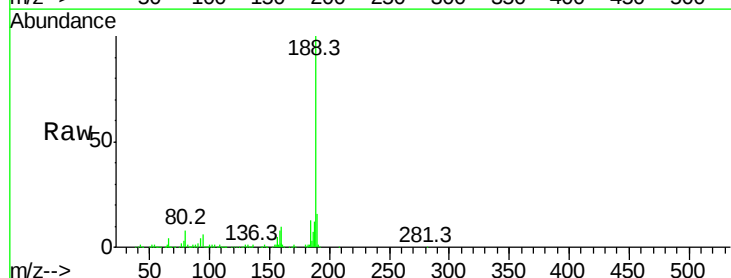



#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.69 min Scan# 3133

Delta R.T. -0.02 min

Lab File: BG035189.D

Acq: 16 Jun 2018 2:10

Instrument :

BNA_G

ClientSampleId :

EPE-106-7(65-67)





Tot Ion:240 Resp: 390365

Ion Ratio Lower Upper

240 100

120 5.9 6.8 10.2#

236 25.5 20.9 31.3

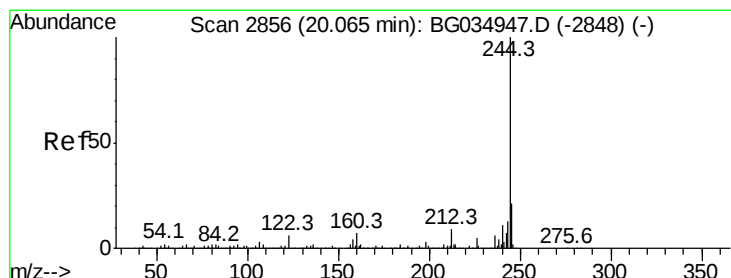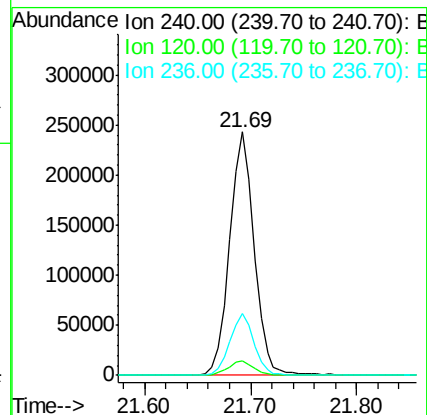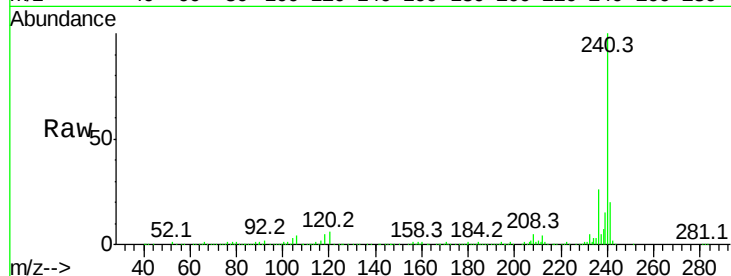

#78

Terphenyl-d14

Concen: 72.780 ng

RT: 20.03 min Scan# 2850

Delta R.T. -0.02 min

Lab File: BG035189.D

Acq: 16 Jun 2018 2:10




Tgt Ion:244 Resp: 1356331


Ion Ratio Lower Upper

244 100

212 8.9 5.8 8.8#

122 6.9 7.0 10.4#

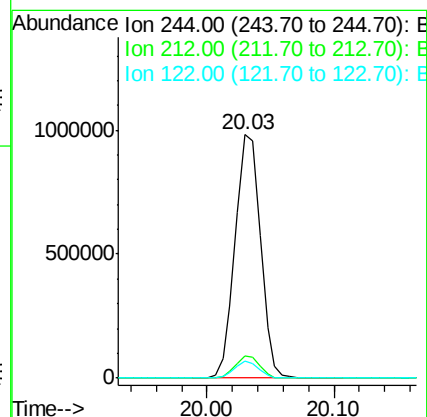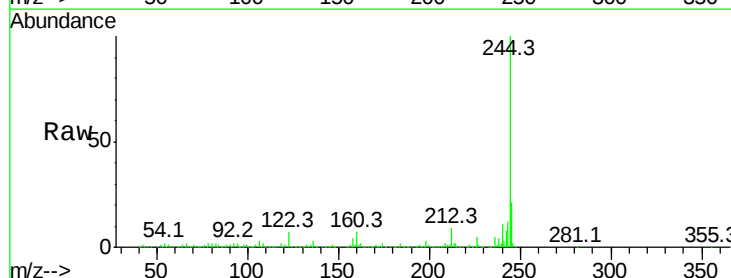


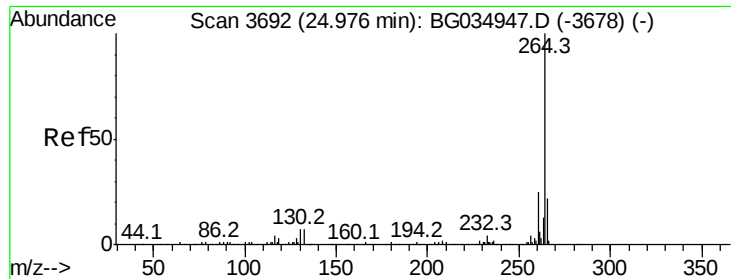

#86
Pervlene-d12
Concen: 20.000 ng
RT: 24.92 min Scan# 3682
Delta R.T. -0.04 min
Lab File: BG035189.D
Acq: 16 Jun 2018 2:10

Instrument :
BNA_G
ClientSampleId :
EPE-106-7(65-67)

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.2	17.4	26.0
265	19.3	17.7	26.5

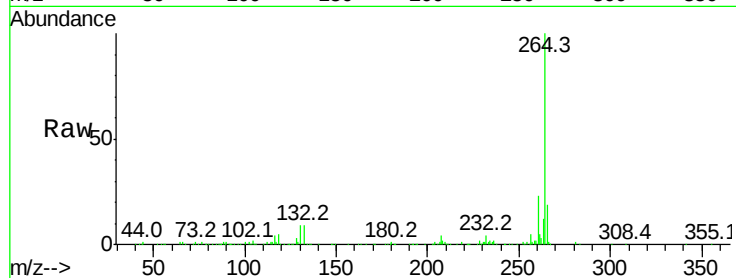

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

