


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG061518\
 Data File : BG035192.D
 Acq On : 16 Jun 2018 4:45
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG060718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 08 17:16:28 2018

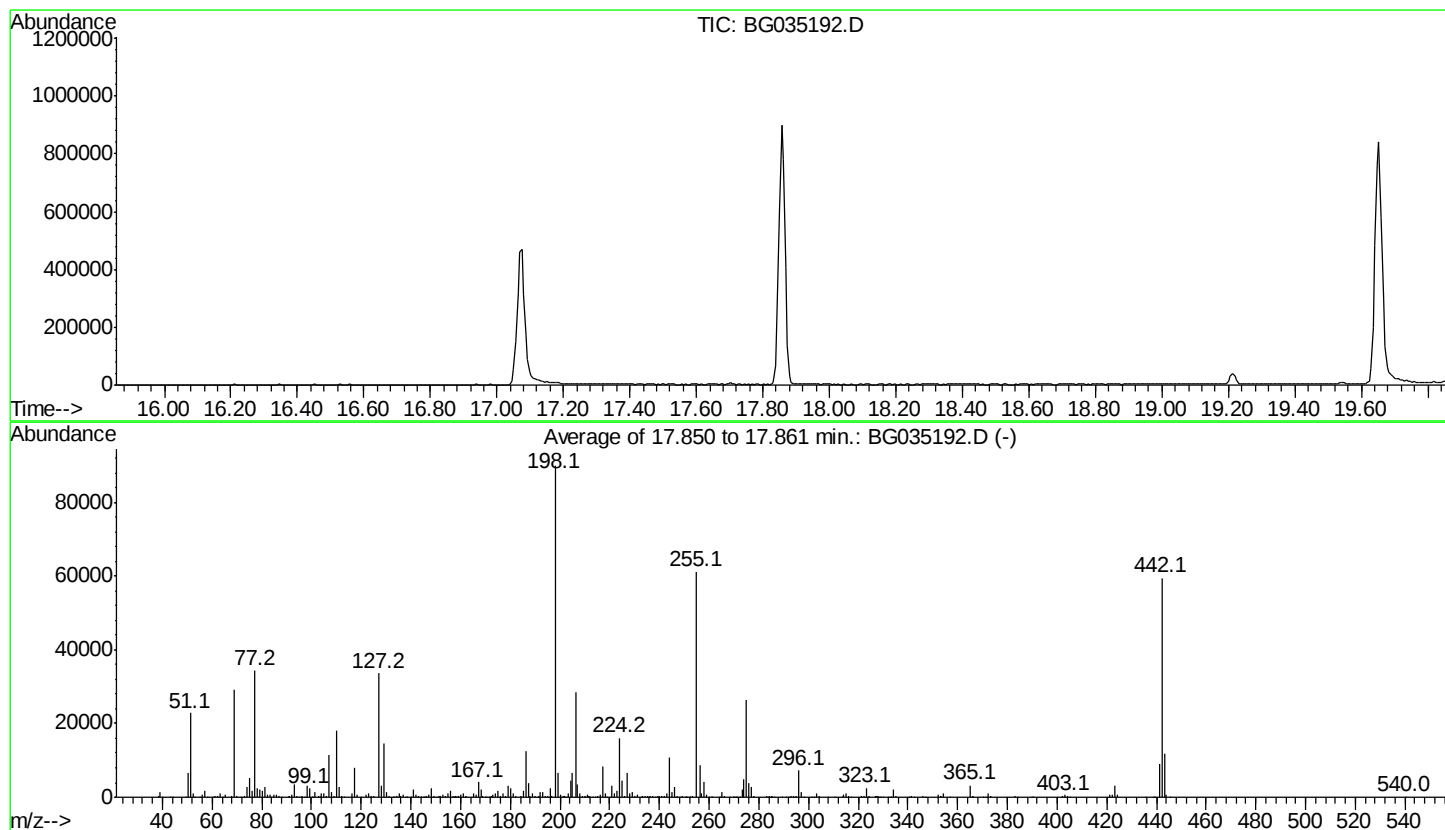

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.4	22810	PASS
68	69	0.00	2	1.6	463	PASS
69	198	0.00	100	32.5	29200	PASS
70	69	0.00	2	0.8	223	PASS
127	198	10	80	37.3	33568	PASS
197	198	0.00	2	0.4	387	PASS
198	198	100	100	100.0	89928	PASS
199	198	5	9	7.3	6582	PASS
275	198	10	60	29.3	26360	PASS
365	198	1	100	3.6	3235	PASS
441	443	0.01	100	78.5	9195	PASS
442	198	50	100	66.2	59538	PASS
443	442	15	24	19.7	11716	PASS