
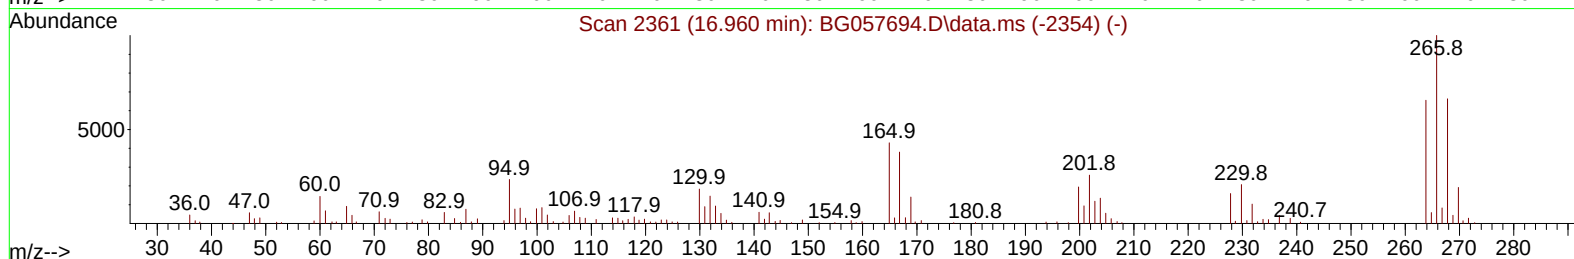
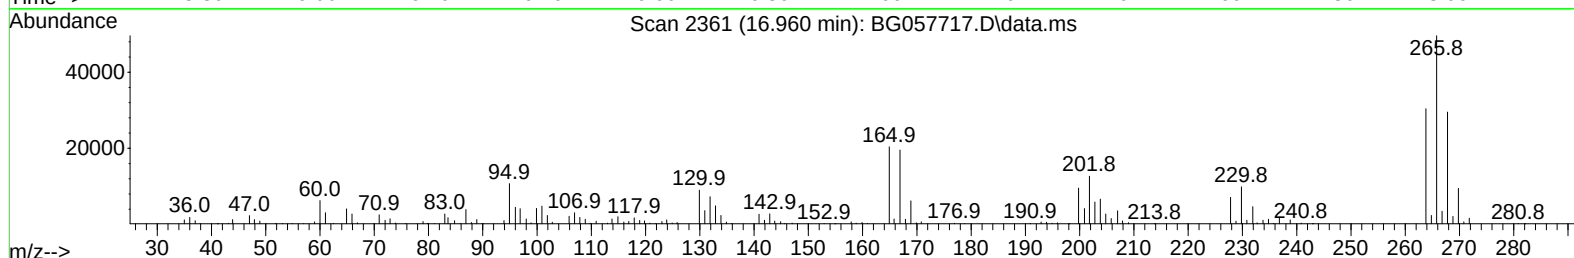


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061523\
Data File : BG057717.D
Acq On : 15 Jun 2023 9:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 02:19:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 15 15:28:07 2023
Response via : Initial Calibration

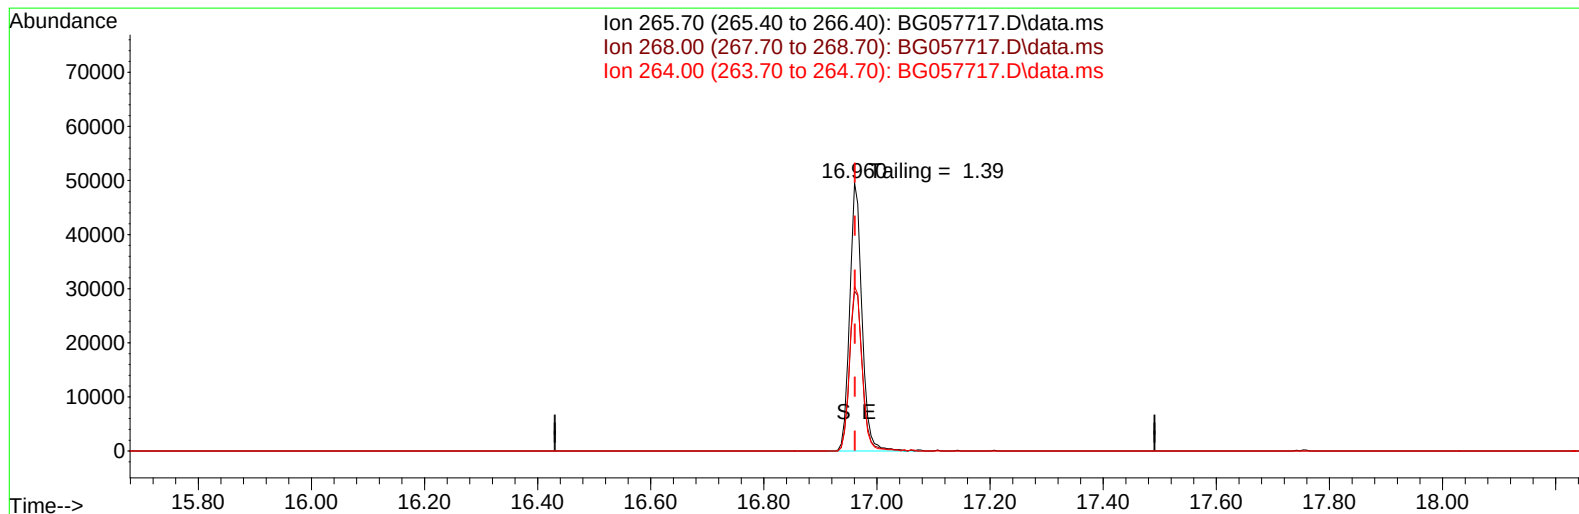

TIC: BG057717.D\data.ms

(70) Pentachlorophenol (C)




16.960min (-0.001) 46880.05 ng

response 74874

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	59.54
264.00	65.50	61.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061523\
Data File : BG057717.D
Acq On : 15 Jun 2023 9:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 02:19:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 15 15:28:07 2023
Response via : Initial Calibration

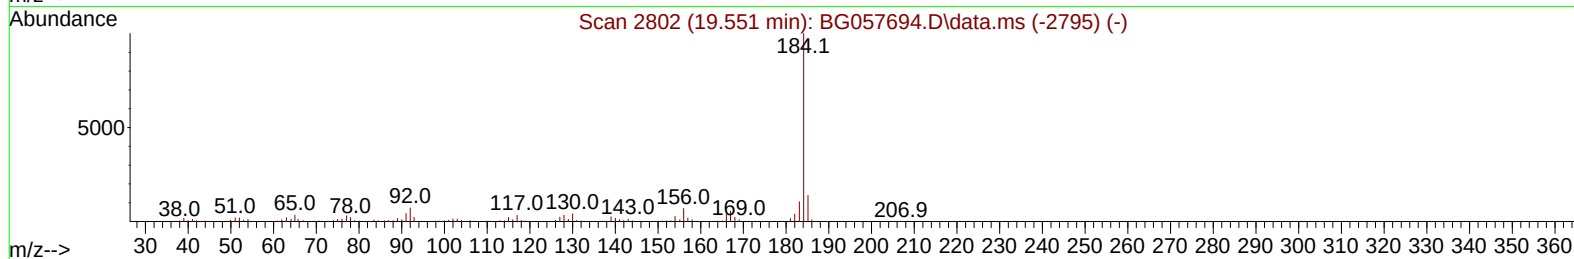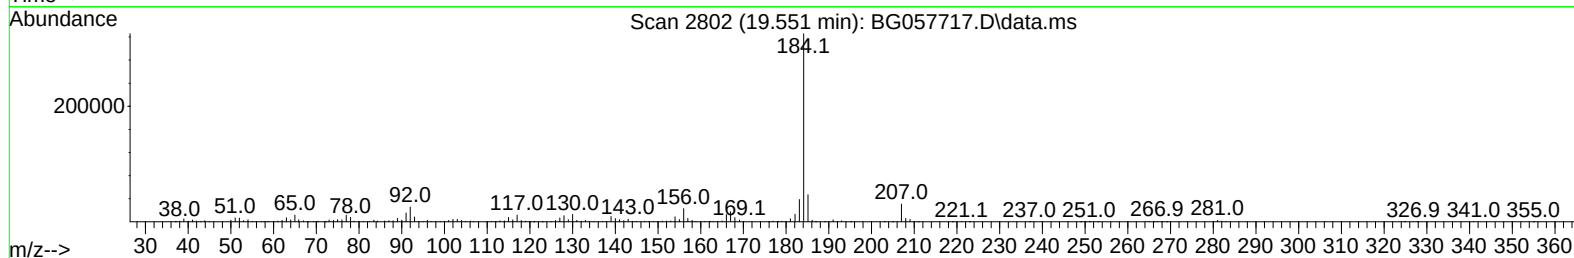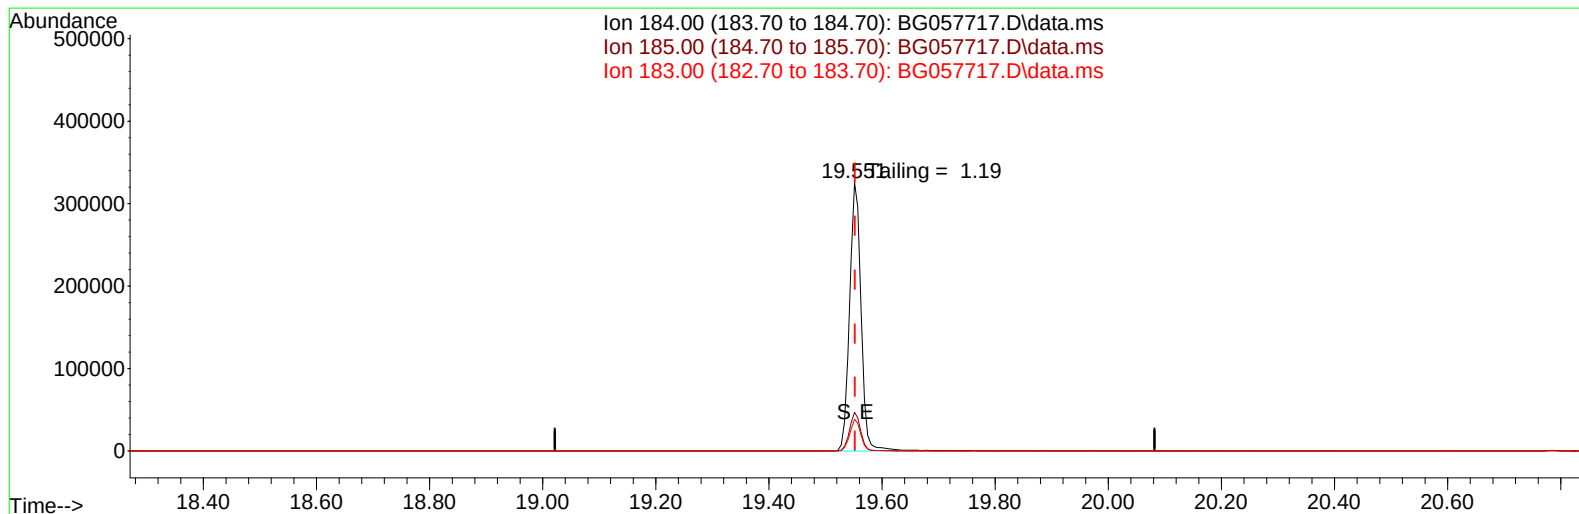

TIC: BG057717.D\data.ms

(77) Benzidine

19.551min (-0.001) 0.00 ng

response 460743

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.45
183.00	10.50	11.84
0.00	0.00	0.00