


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061523\
Data File : BG057717.D
Acq On : 15 Jun 2023 9:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061323.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jun 15 15:28:07 2023

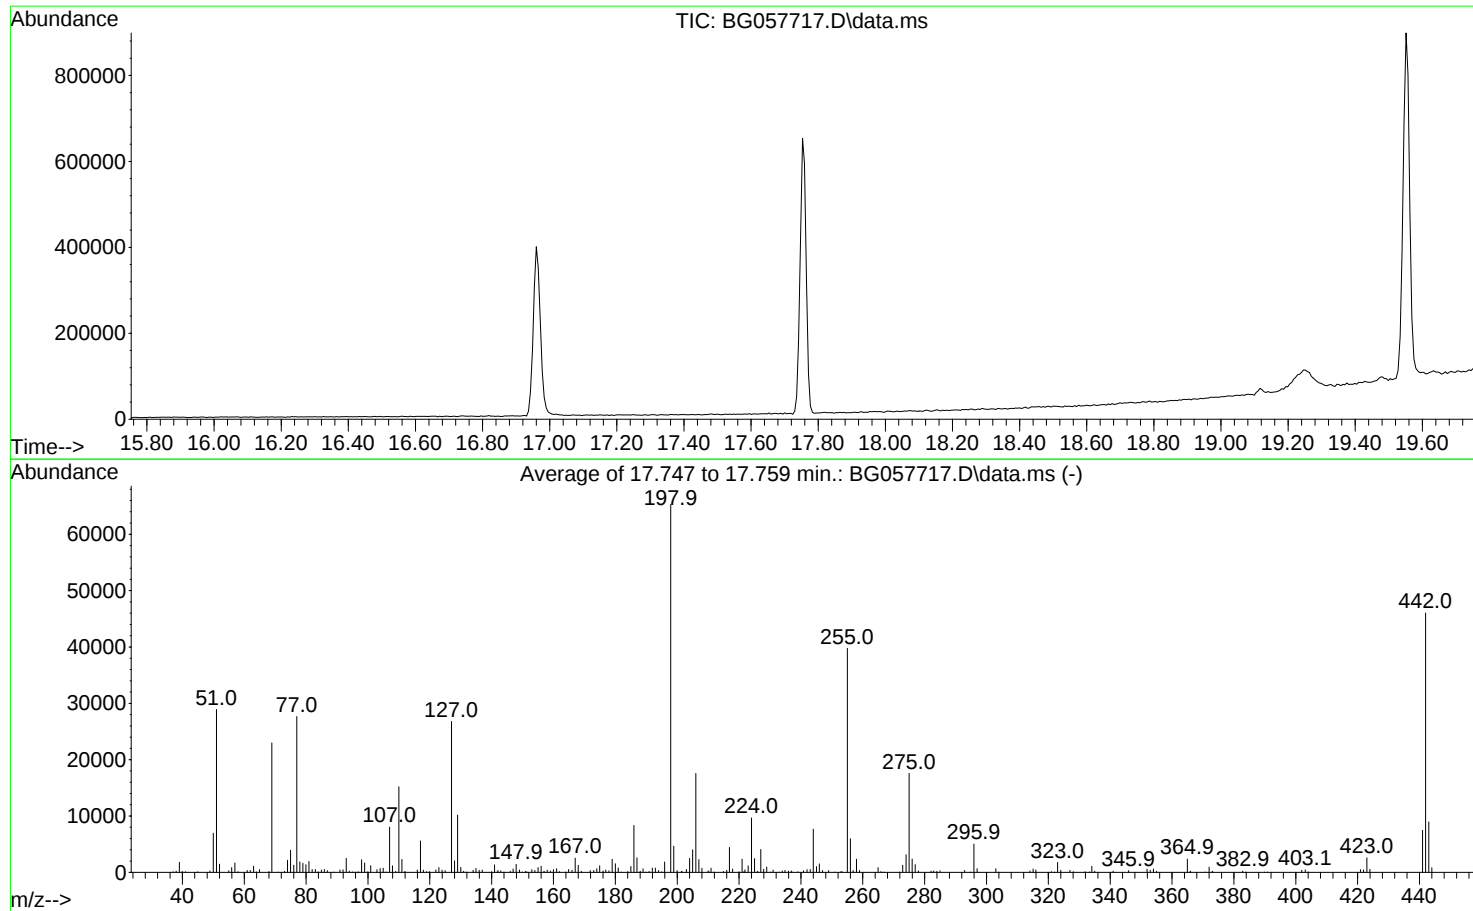

AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.3	28915	PASS
68	69	0.00	2	0.6	145	PASS
69	198	0.00	100	35.2	22987	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.0	26781	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	65293	PASS
199	198	5	9	7.2	4670	PASS
275	198	10	60	26.9	17570	PASS
365	198	1	100	3.6	2375	PASS
441	198	0.01	100	11.4	7467	PASS
442	442	50	100	100.0	46040	PASS
443	442	15	24	19.4	8953	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/15/2023	BNA_G	<u>BG057717.D</u>
Compound Name	Response	Retention Time
DDT	171889	20.785
DDD	3710	20.397
DDE	0	20.162
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3710	175599	2.11

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061523\
Data File : BG057717.D
Acq On : 15 Jun 2023 9:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 16 02:19:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 15 15:28:07 2023
Response via : Initial Calibration

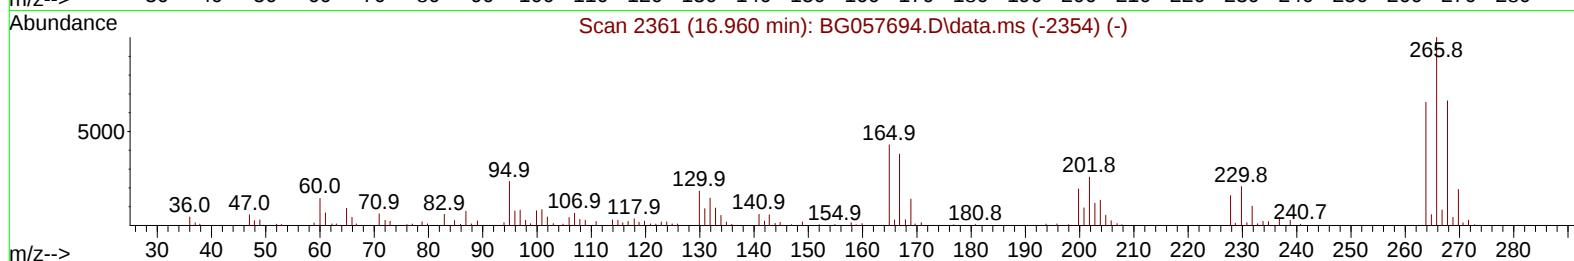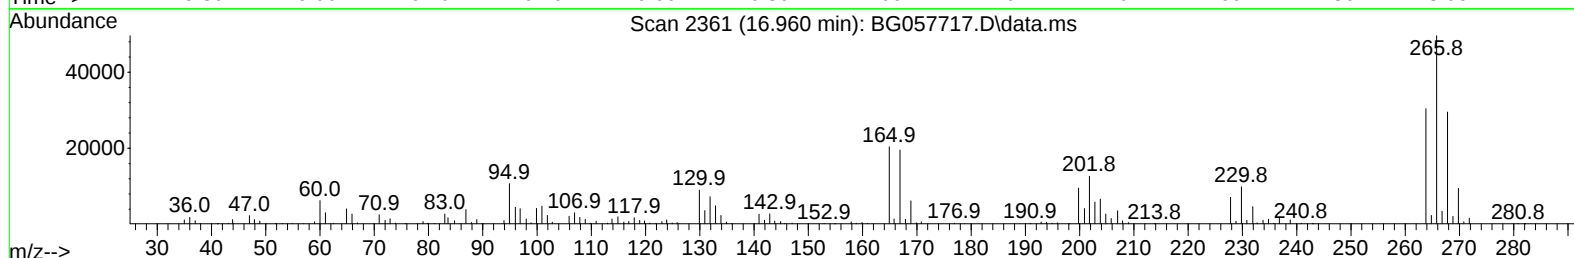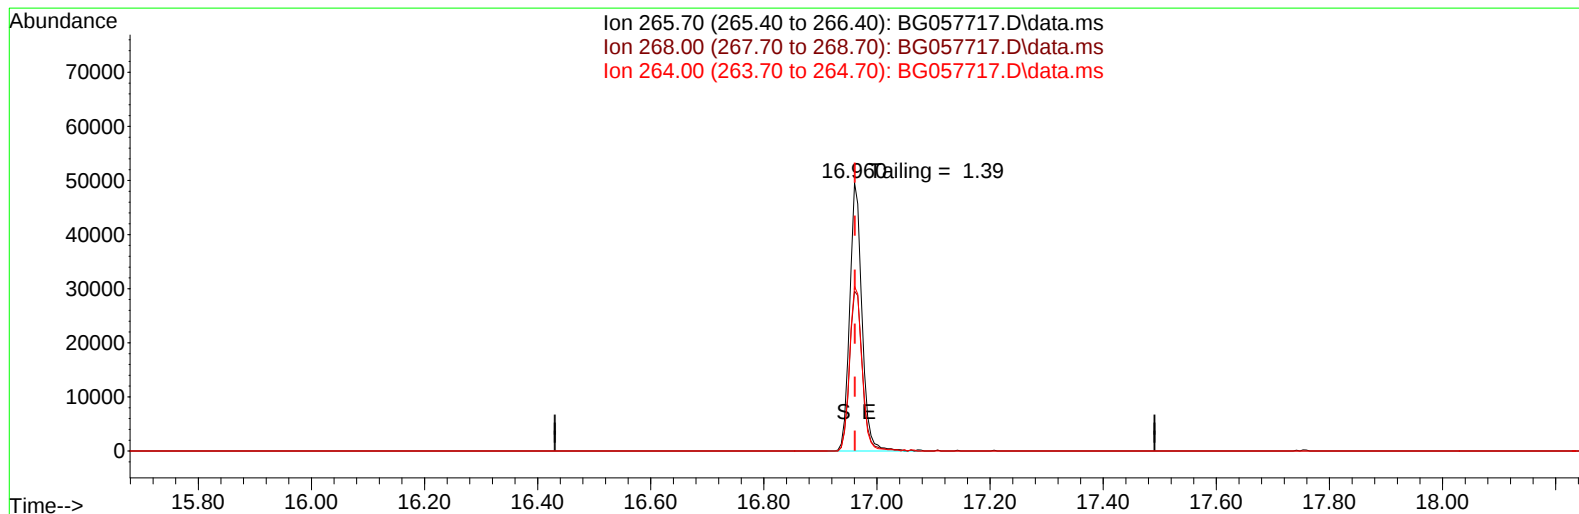

TIC: BG057717.D\data.ms

(70) Pentachlorophenol (C)

16.960min (-0.001) 46880.05 ng




response 74874

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	59.54
264.00	65.50	61.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061523\
 Data File : BG057717.D
 Acq On : 15 Jun 2023 9:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jun 16 02:19:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 15 15:28:07 2023
 Response via : Initial Calibration

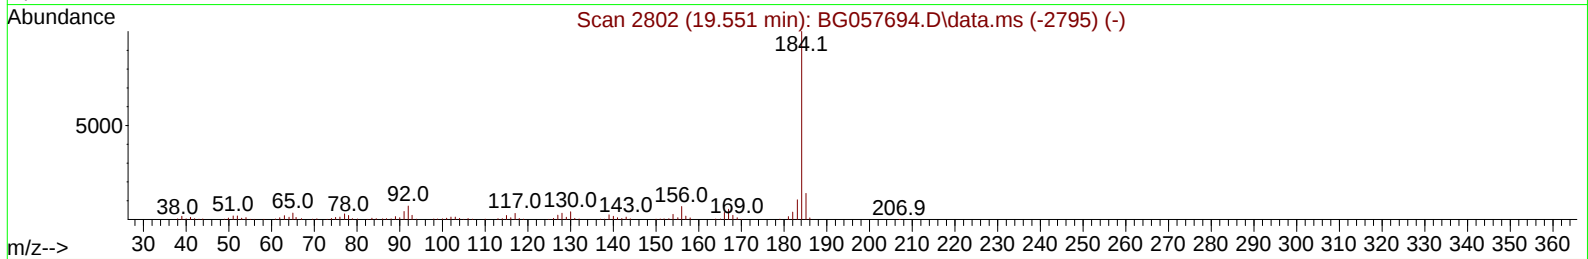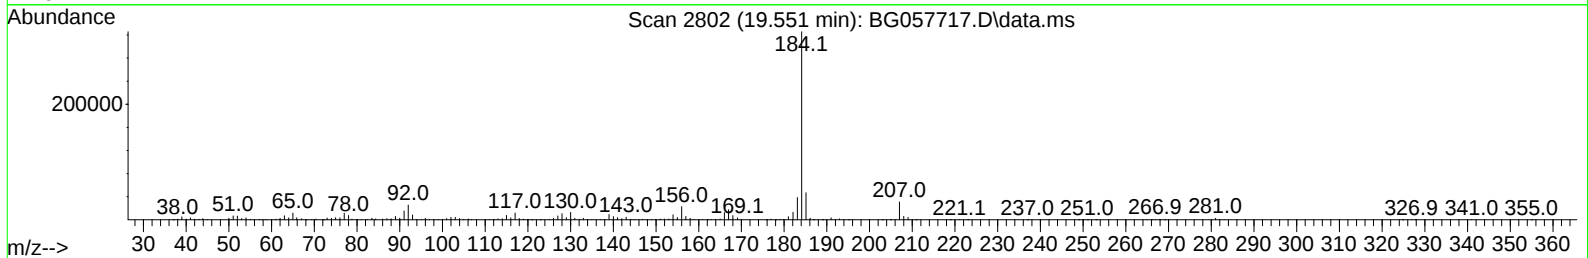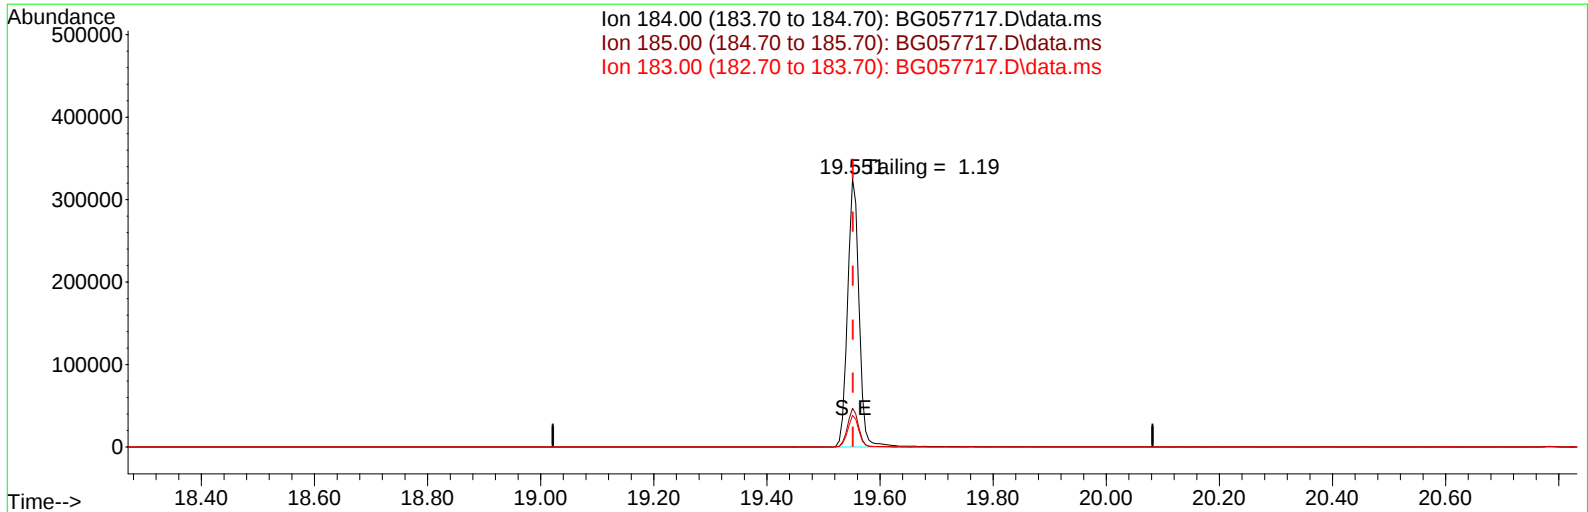

TIC: BG057717.D\data.ms

(77) Benzidine

19.551min (-0.001) 0.00 ng

response 460743

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.45
183.00	10.50	11.84
0.00	0.00	0.00