
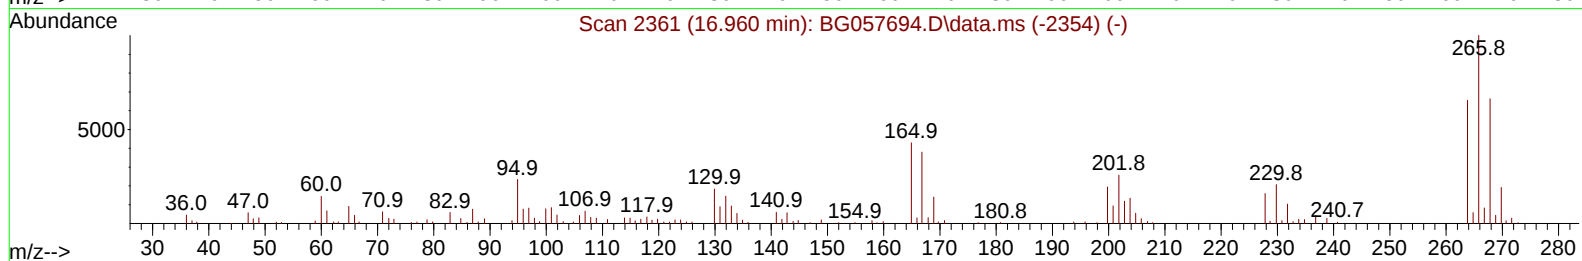
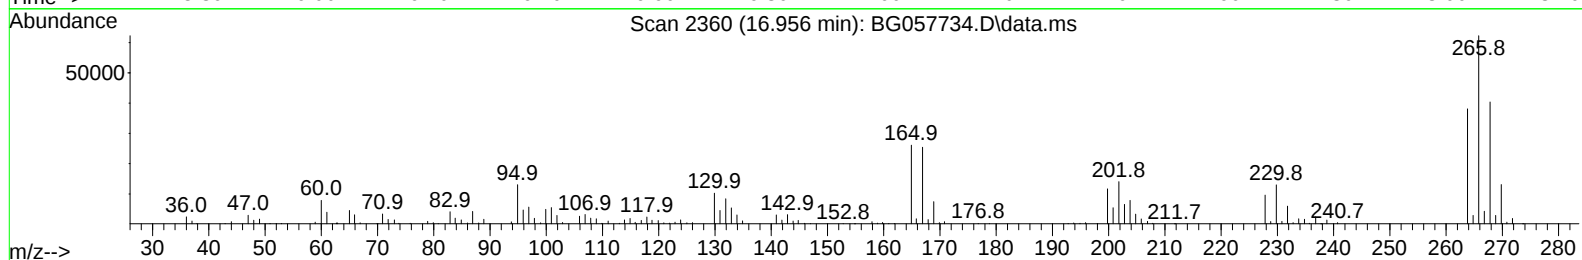


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061623\
Data File : BG057734.D
Acq On : 16 Jun 2023 14:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 05:53:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 15 15:28:07 2023
Response via : Initial Calibration

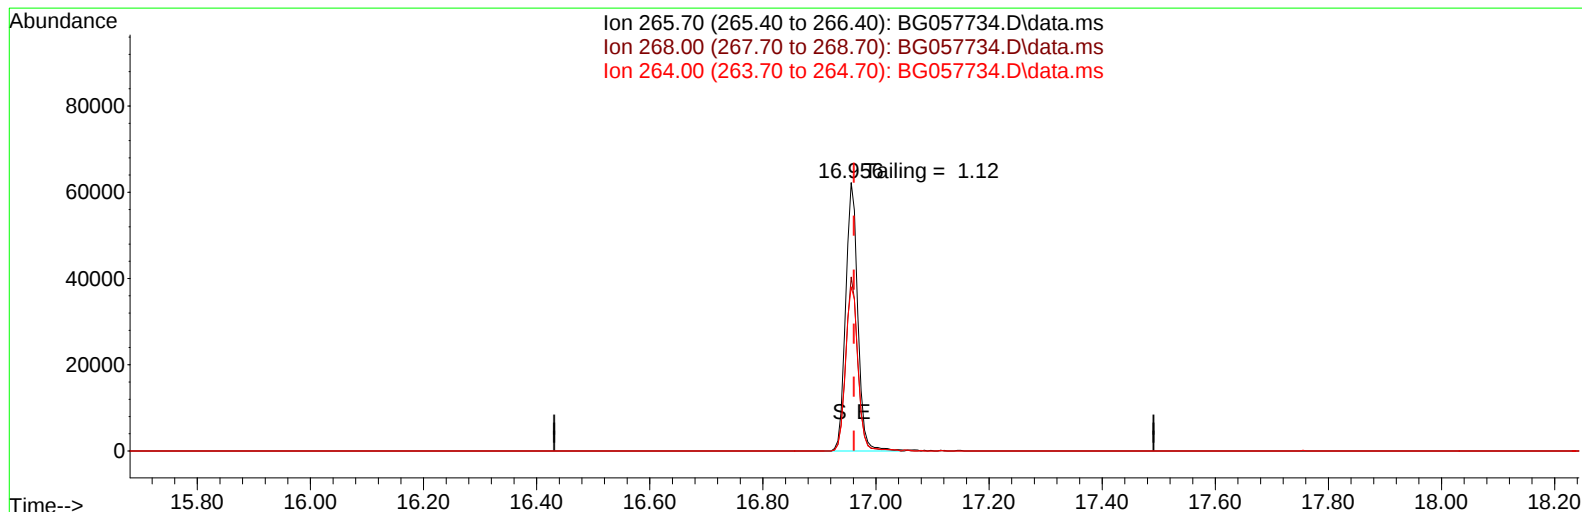

TIC: BG057734.D\data.ms

(70) Pentachlorophenol (C)




16.956min (-0.005) 41900.96 ng

response 93155

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	64.84
264.00	65.50	61.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061623\
Data File : BG057734.D
Acq On : 16 Jun 2023 14:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 05:53:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 15 15:28:07 2023
Response via : Initial Calibration

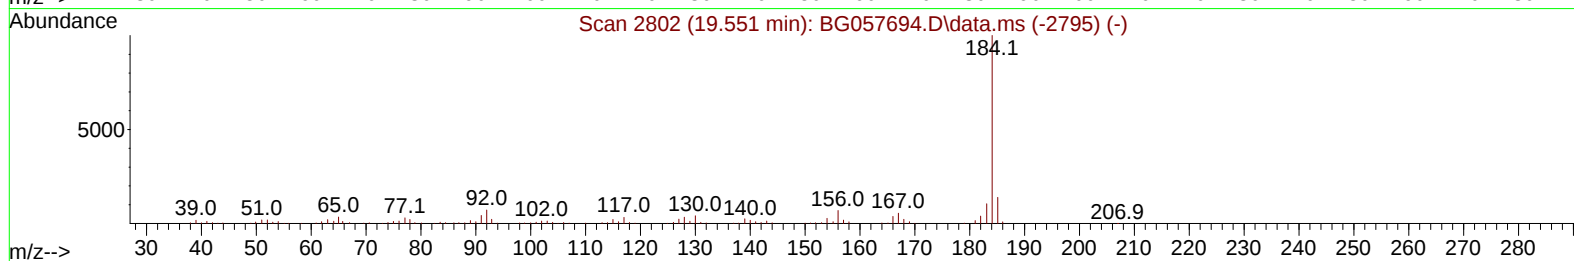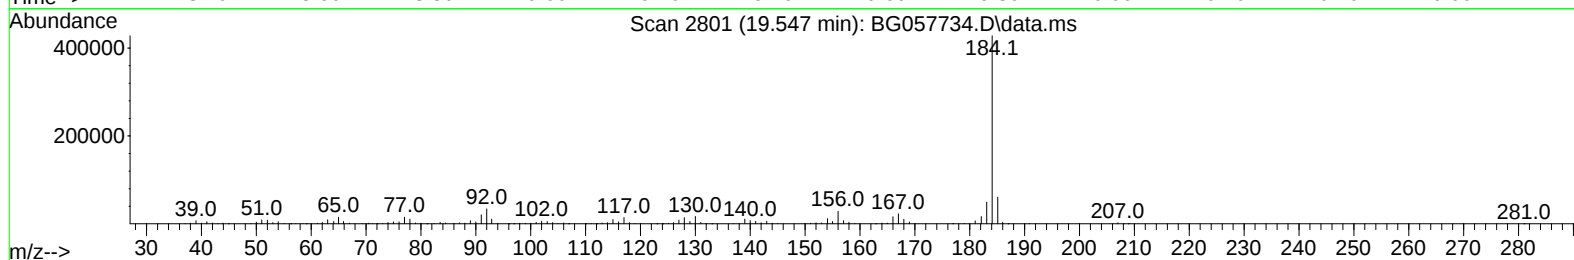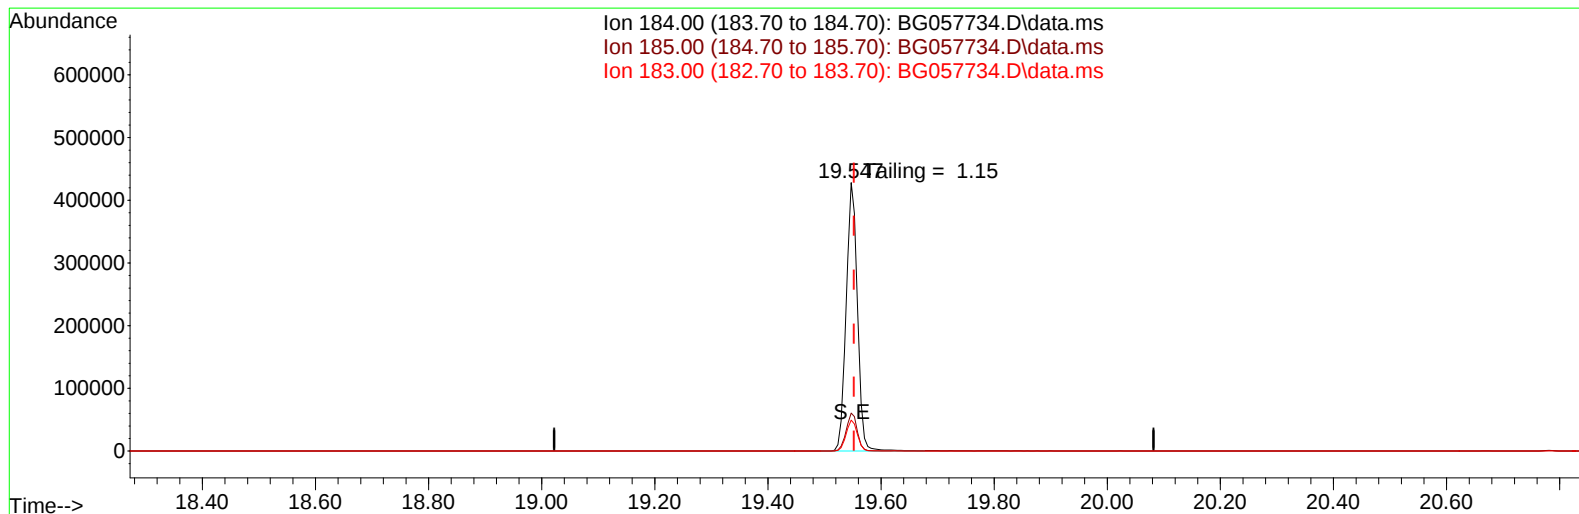

TIC: BG057734.D\data.ms

(77) Benzidine

19.547min (-0.005) 0.00 ng

response 594405

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.16
183.00	10.50	11.51
0.00	0.00	0.00