
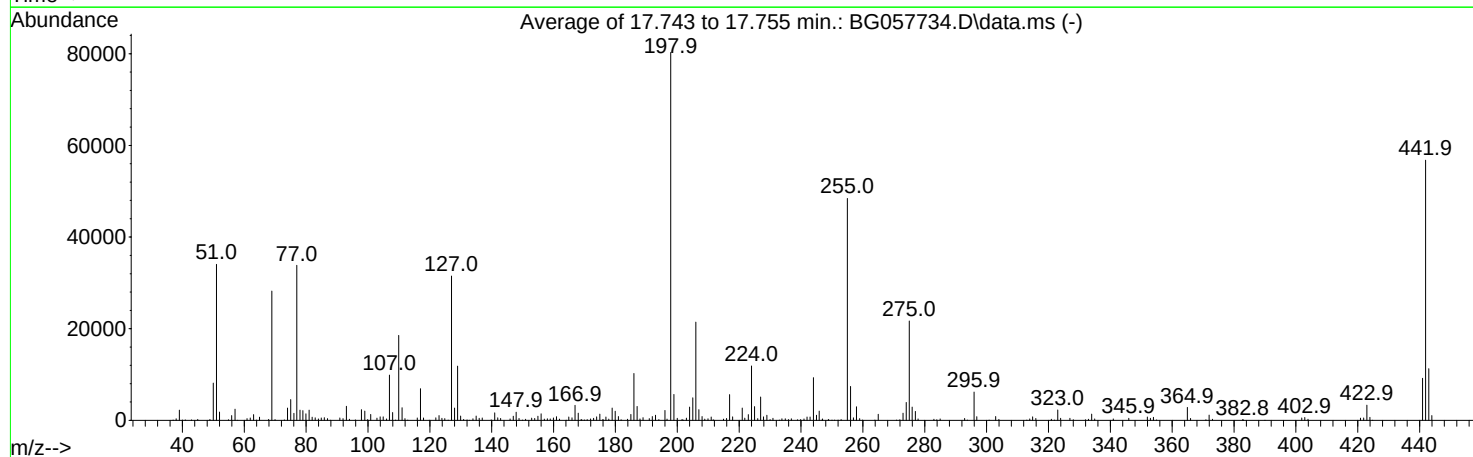


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061623\
Data File : BG057734.D
Acq On : 16 Jun 2023 14:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061323.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jun 15 15:28:07 2023

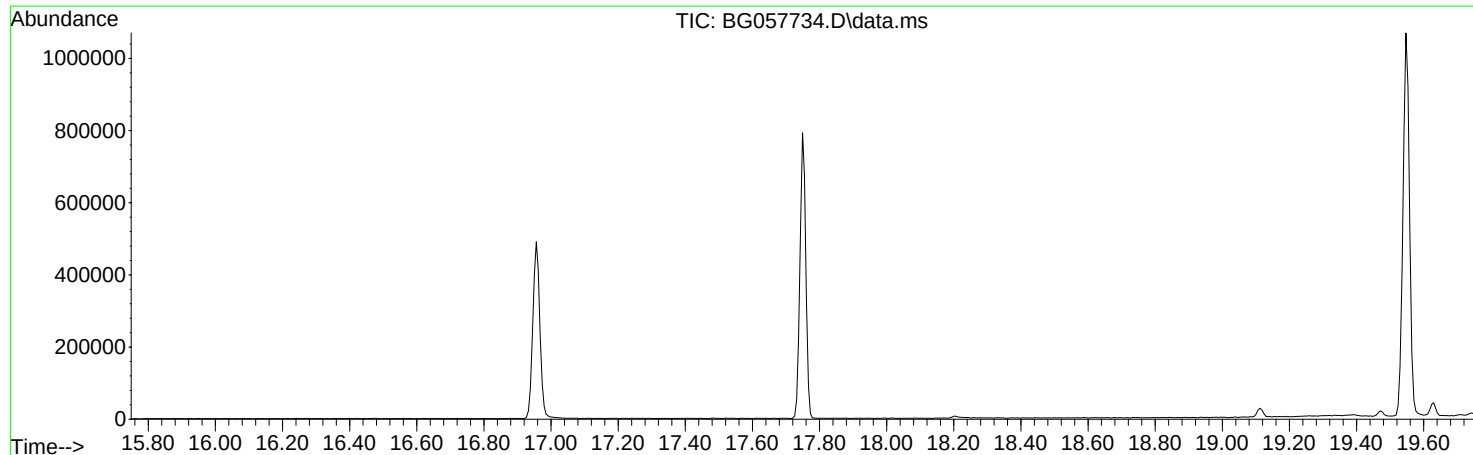

AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.4	34053	PASS
68	69	0.00	2	0.7	210	PASS
69	198	0.00	100	35.1	28208	PASS
70	69	0.00	2	0.6	176	PASS
127	198	10	80	39.2	31488	PASS
197	198	0.00	2	0.3	271	PASS
198	198	100	100	100.0	80272	PASS
199	198	5	9	7.1	5668	PASS
275	198	10	60	27.0	21669	PASS
365	198	1	100	3.5	2812	PASS
441	198	0.01	100	11.4	9175	PASS
442	442	50	100	100.0	56771	PASS
443	442	15	24	19.9	11270	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/16/2023	BNA_G	<u>BG057734.D</u>
Compound Name	Response	Retention Time
DDT	229062	20.781
DDD	4083	20.399
DDE	0	20.162
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4083	233145	1.75

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061623\
Data File : BG057734.D
Acq On : 16 Jun 2023 14:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 17 05:53:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 15 15:28:07 2023
Response via : Initial Calibration

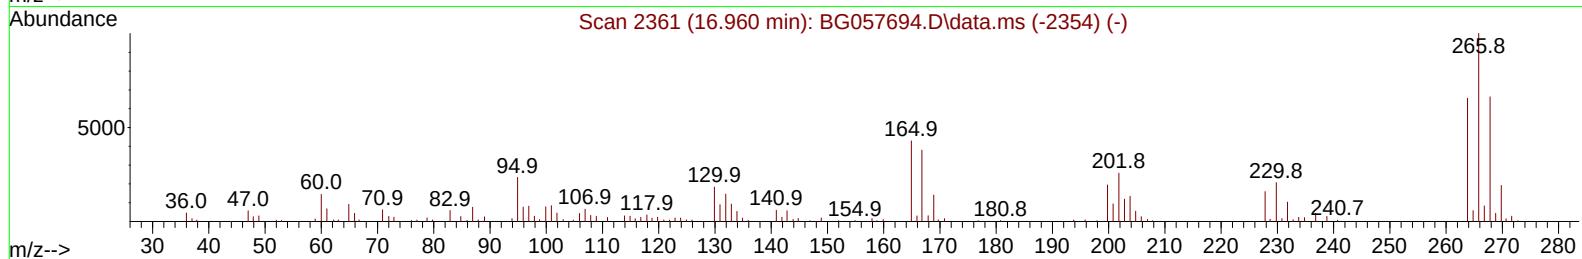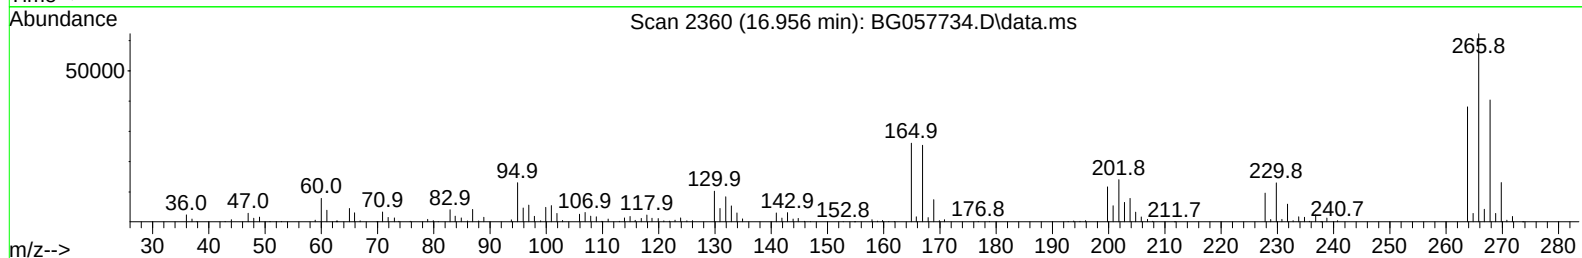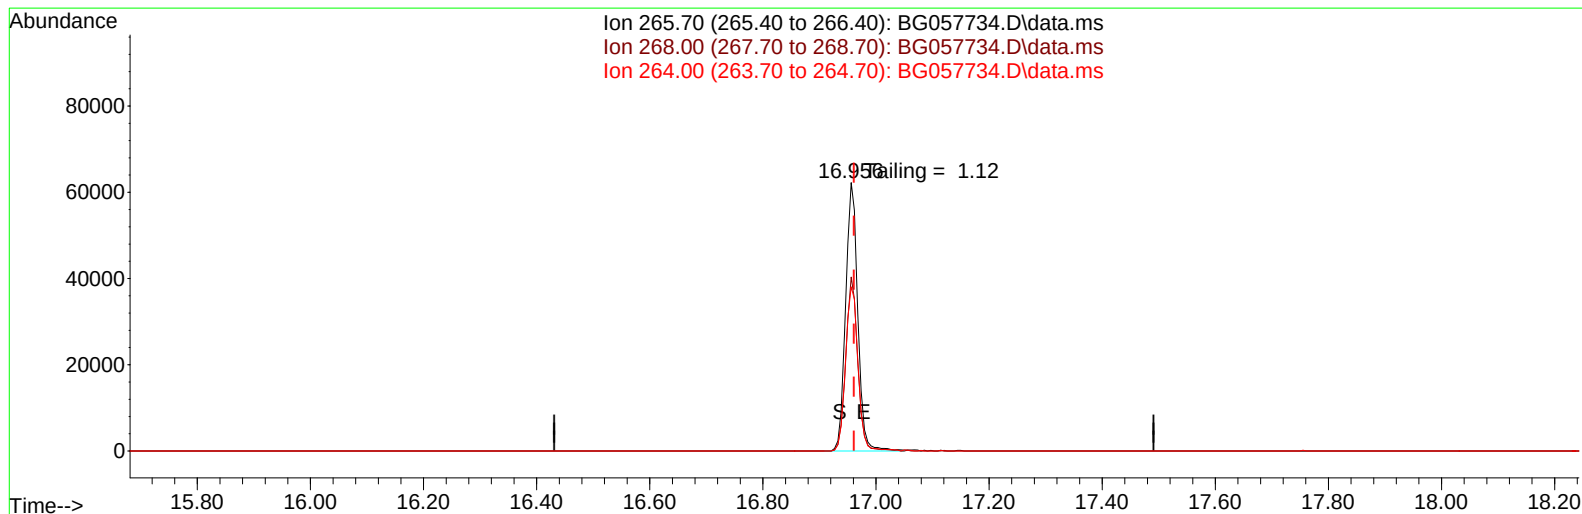

TIC: BG057734.D\data.ms

(70) Pentachlorophenol (C)

16.956min (-0.005) 41900.96 ng




response 93155

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	64.84
264.00	65.50	61.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061623\
 Data File : BG057734.D
 Acq On : 16 Jun 2023 14:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jun 17 05:53:28 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 15 15:28:07 2023
 Response via : Initial Calibration

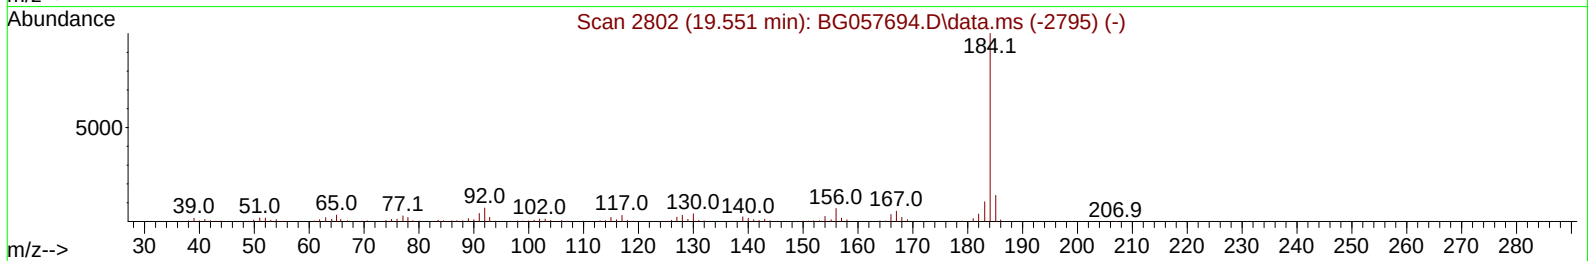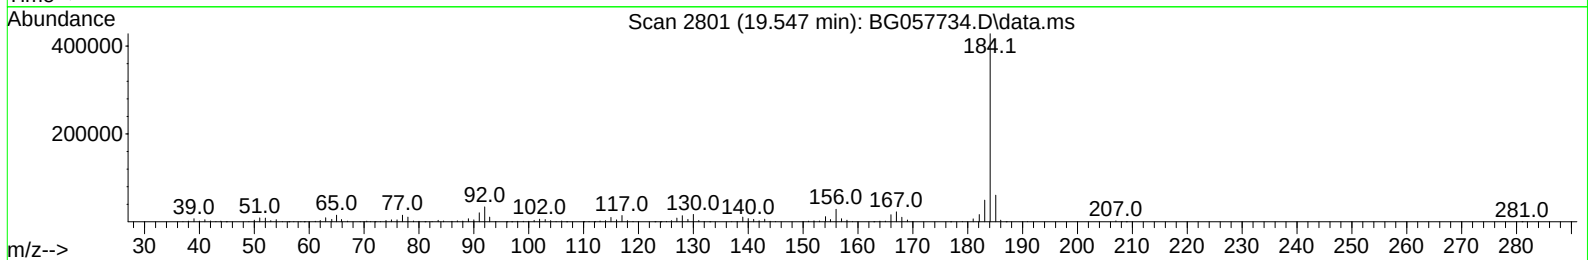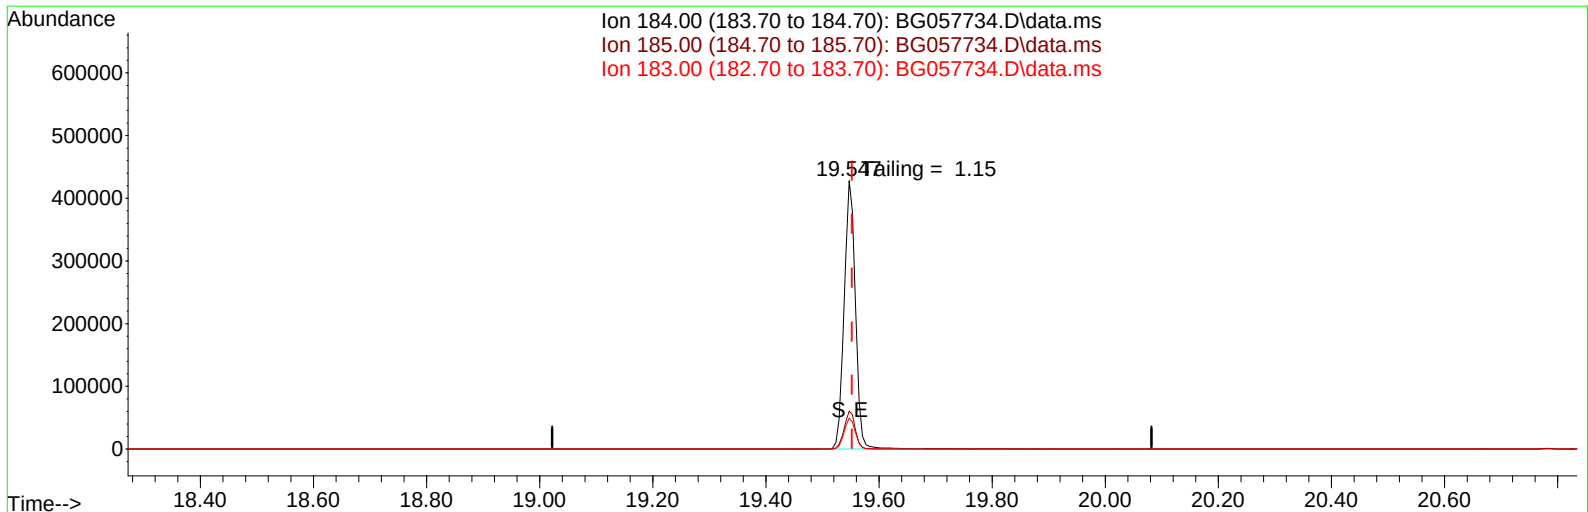

TIC: BG057734.D\data.ms

(77) Benzidine

19.547min (-0.005) 0.00 ng

response 594405

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.16
183.00	10.50	11.51
0.00	0.00	0.00