

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061719\
 Data File : BG041276.D
 Acq On : 17 Jun 2019 17:09
 Operator : HP/JU
 Sample : K3156-03RE
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Jun 17 17:44:56 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 14:58:02 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.08	152	72061	20.00	ng	0.00
21) Naphthalene-d8	10.91	136	278859	20.00	ng	0.00
39) Acenaphthene-d10	14.71	164	183090	20.00	ng	0.00
64) Phenanthrene-d10	17.46	188	427640	20.00	ng	0.00
76) Chrysene-d12	21.74	240	444304	20.00	ng	0.00
87) Perylene-d12	25.05	264	496016	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.62	112	314898	80.29	ng	0.00
7) Phenol-d6	7.24	99	462640	81.38	ng	0.00
23) Nitrobenzene-d5	9.26	82	336413	50.74	ng	0.00
42) 2,4,6-Tribromophenol	16.21	330	205237	73.02	ng	0.00
45) 2-Fluorobiphenyl	13.34	172	682751	50.68	ng	0.00
79) Terphenyl-d14	20.06	244	1023569	45.66	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	9.26	70	48371	10.520	ng	Qvalue # 75
50) Dimethylphthalate	14.16	163	134340	8.246	ng	99
56) 4-Nitrophenol	14.90	139	66	3.240	ng	# 1
57) 2,4-Dinitrotoluene	14.71	165	24922	4.963	ng	# 20
67) 4-Bromophenyl-phenylether	16.21	248	15468	2.797	ng	# 1
75) Fluoranthene	19.51	202	112559	3.715	ng	97
78) Pyrene	19.87	202	98758	3.296	ng	99
81) Benzo(a)anthracene	21.71	228	63195	2.101	ng	95
83) Chrysene	21.78	228	71370	2.467	ng	98
88) Benzo(b)fluoranthene	23.98	252	101688	3.308	ng	# 92
89) Benzo(k)fluoranthene	23.98	252	101688	3.339	ng	94
90) Benzo(a)pyrene	24.89	252	69267	2.386	ng	# 95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061719\
Data File : BG041276.D
Acq On : 17 Jun 2019 17:09
Operator : HP/JU
Sample : K3156-03RE
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Jun 17 17:44:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 14:58:02 2019
Response via : Initial Calibration

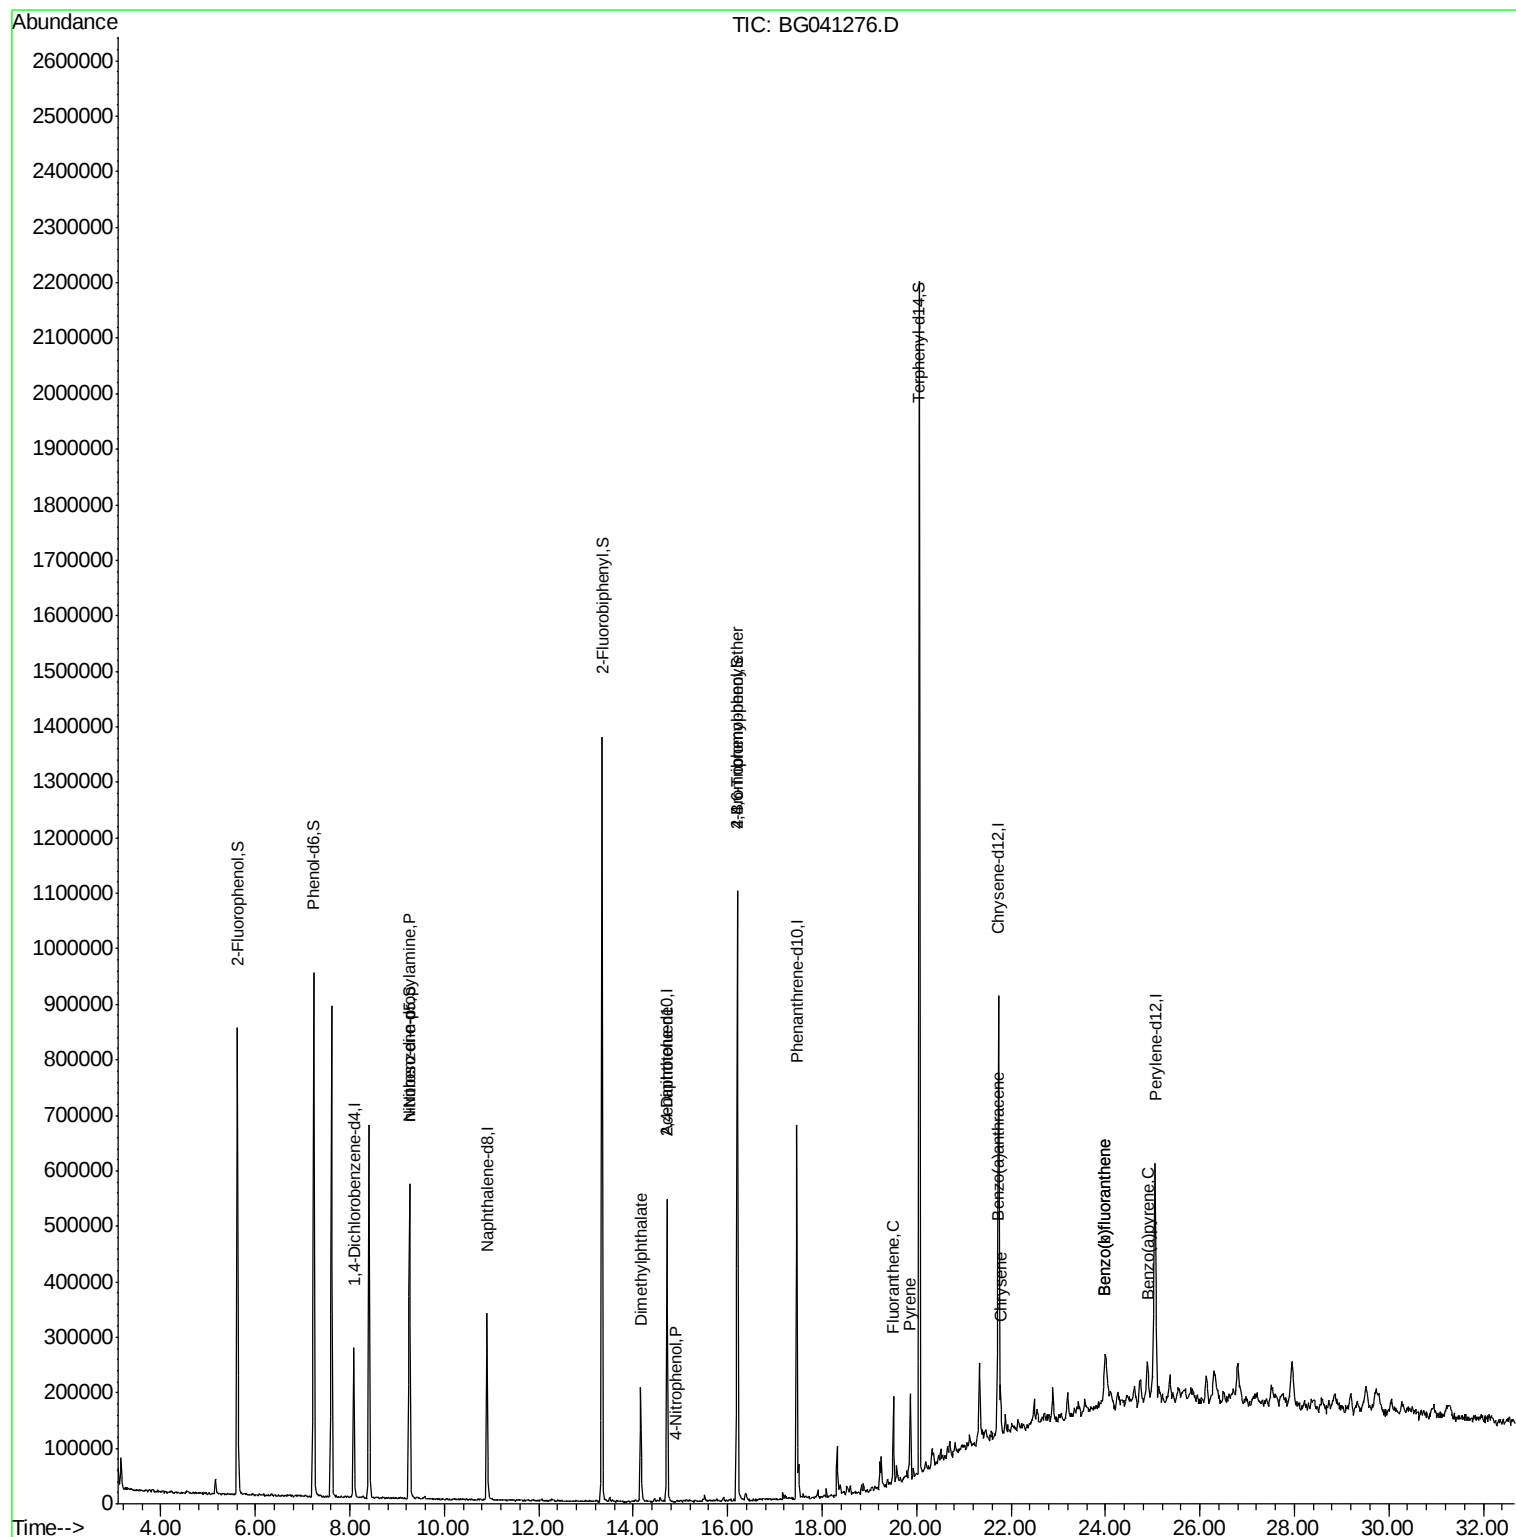




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.08 min Scan# 850
Delta R.T. 0.00 min
Lab File: BG041276.D
Acq: 17 Jun 2019 17:09

Instrument :
BNA_G
ClientSampleId :

Tot Ion:152 Resp: 72061
Ion Ratio Lower Upper
152 100
150 159.5 120.6 181.0
115 57.6 47.9 71.9

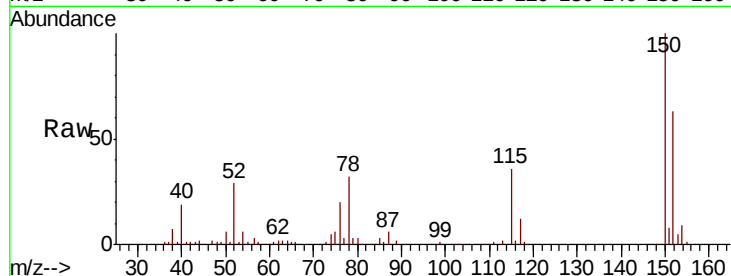


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

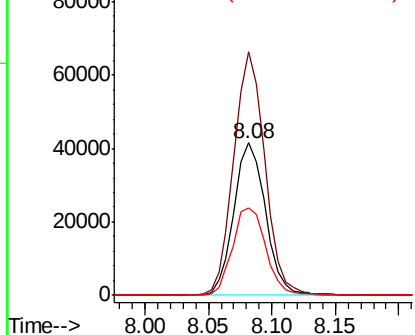



#5


2-Fluorophenol
Concen: 80.293 ng
RT: 5.62 min Scan# 431
Delta R.T. 0.00 min
Lab File: BG041276.D
Acq: 17 Jun 2019 17:09

Tgt Ion:112 Resp: 314898
Ion Ratio Lower Upper
112 100
64 74.2 55.9 83.9
63 42.5 34.6 51.8



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

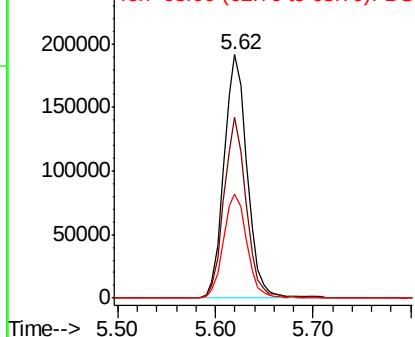

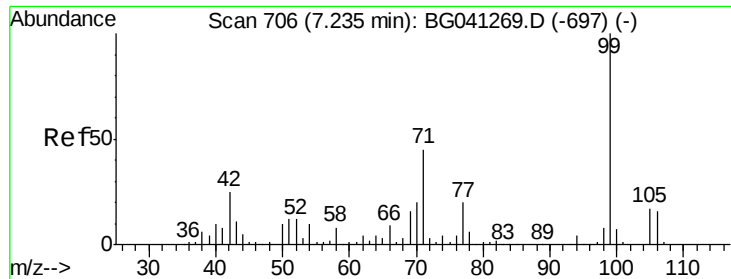

#7

Phenol-d6

Concen: 81.382 ng

RT: 7.24 min Scan# 706

Delta R.T. 0.00 min

Lab File: BG041276.D

Acq: 17 Jun 2019 17:09

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 99 Resp: 462640

Ion Ratio Lower Upper




99 100

42 25.7 19.9 29.9

71 46.1 36.4 54.6

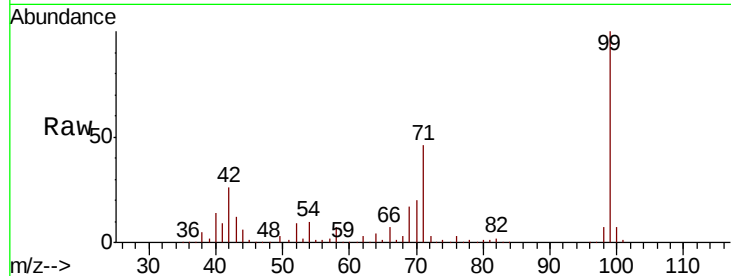

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

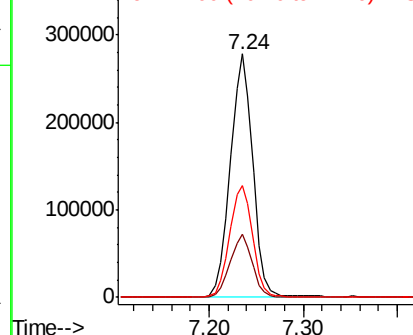

#19

n-Nitroso-di-n-propylamine

Concen: 10.520 ng

RT: 9.26 min Scan# 1051

Delta R.T. 0.38 min

Lab File: BG041276.D

Acq: 17 Jun 2019 17:09

Tgt Ion: 70 Resp: 48371


Ion Ratio Lower Upper

70 100



42 48.5 51.4 77.2#

101 0.0 8.2 12.2#

130 1.3 15.2 22.8#



Abundance Ion 70.00 (69.70 to 70.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 101.00 (100.70 to 101.70): BGC
Ion 130.00 (129.70 to 130.70): BGC



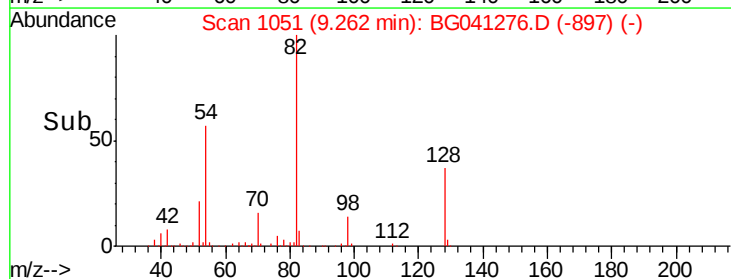
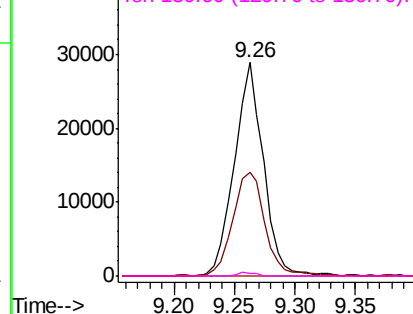




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.91 min Scan# 1331
Delta R.T. 0.00 min
Lab File: BG041276.D
Acq: 17 Jun 2019 17:09




Instrument :
BNA_G
ClientSampleId :


Tot Ion:136	Resp:	278859
Ion	Ratio	Lower Upper
136	100	
137	10.9	8.8 13.2
54	8.7	6.4 9.6
68	3.6	4.8 7.2#

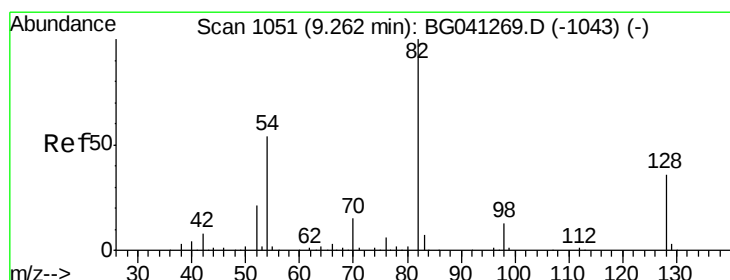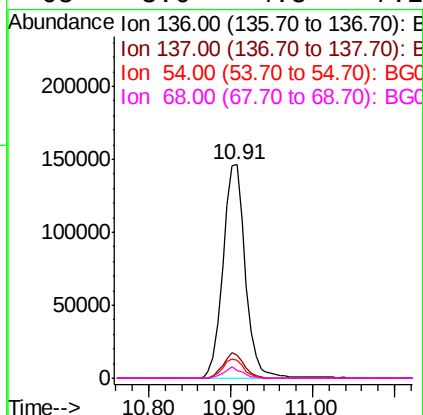

#23
Nitrobenzene-d5
Concen: 50.736 ng
RT: 9.26 min Scan# 1051
Delta R.T. 0.00 min
Lab File: BG041276.D
Acq: 17 Jun 2019 17:09

Tgt Ion: 82	Resp:	336413
Ion	Ratio	Lower Upper
82	100	
128	36.9	29.2 43.8
54	57.3	43.4 65.0

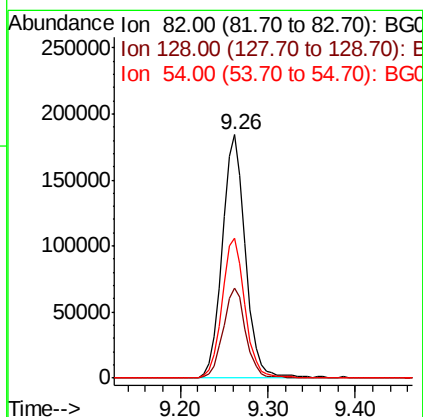

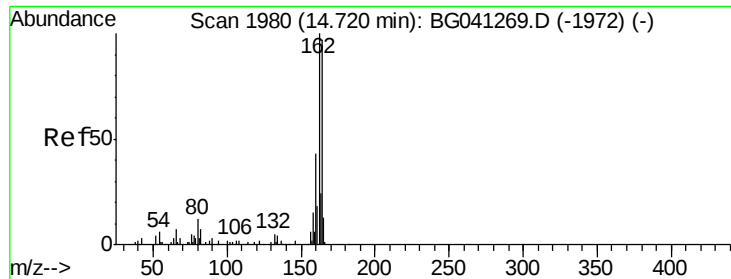

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.71 min Scan# 1979

Delta R.T. -0.01 min

Lab File: BG041276.D

Acq: 17 Jun 2019 17:09





Instrument :

BNA_G

ClientSampleId :

Tot Ion:164 Resp: 183090

Ion	Ratio	Lower	Upper
164	100		
162	104.1	82.8	124.2
160	47.7	35.8	53.8

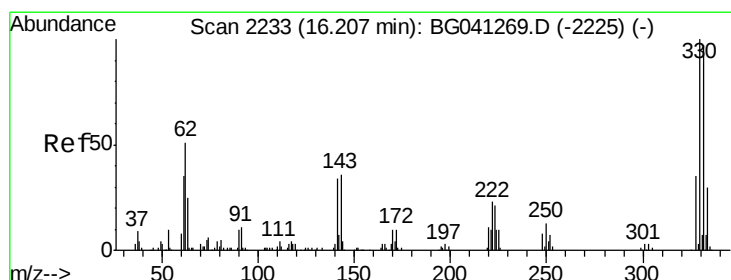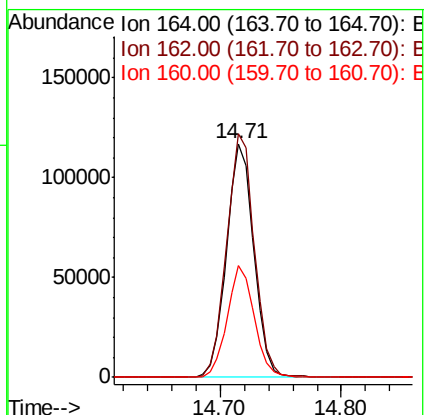

#42

2,4,6-Tribromophenol

Concen: 73.016 ng

RT: 16.21 min Scan# 2233




Delta R.T. 0.00 min


Lab File: BG041276.D

Acq: 17 Jun 2019 17:09

Tgt Ion:330 Resp: 205237

Ion	Ratio	Lower	Upper
330	100		
332	95.9	75.5	113.3
141	38.0	29.0	43.4


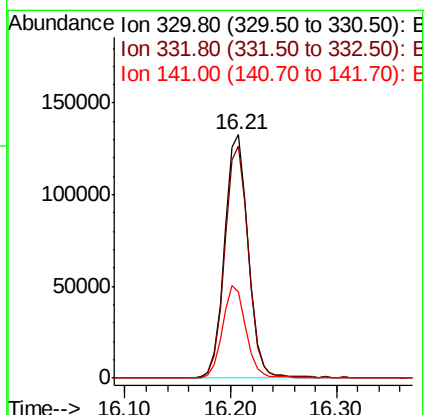
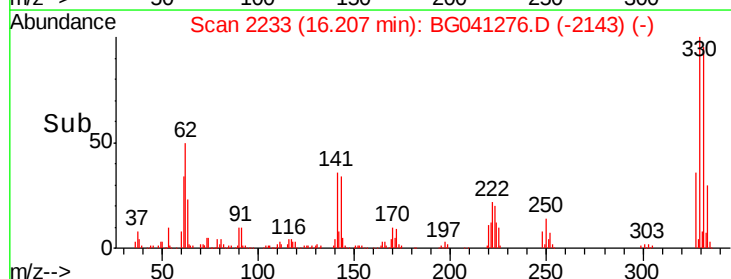
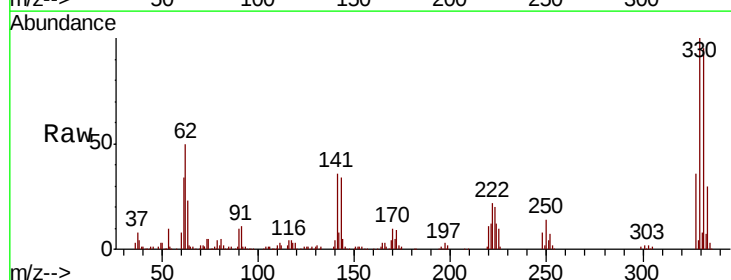




#45
2-Fluorobiphenyl
Concen: 50.684 ng
RT: 13.34 min Scan# 1745
Delta R.T. 0.00 min
Lab File: BG041276.D
Acq: 17 Jun 2019 17:09




Instrument :
BNA_G
ClientSampleId :


Tot Ion:172 Resp: 682751
Ion Ratio Lower Upper
172 100
171 37.6 30.0 45.0
170 24.5 19.8 29.6

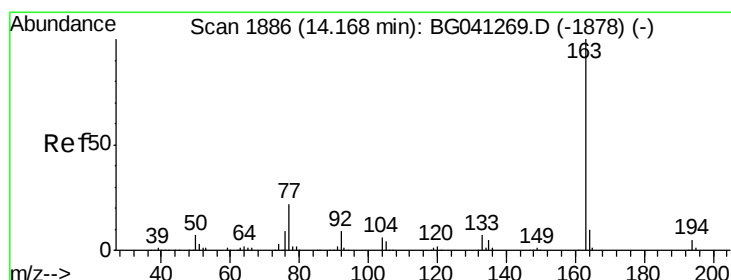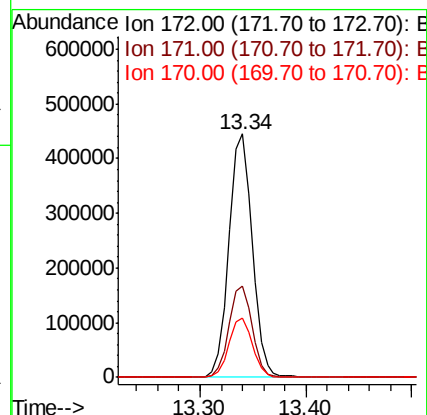

#50
Dimethylphthalate
Concen: 8.246 ng
RT: 14.16 min Scan# 1885
Delta R.T. -0.01 min
Lab File: BG041276.D
Acq: 17 Jun 2019 17:09

Tgt Ion:163 Resp: 134340
Ion Ratio Lower Upper
163 100
194 5.0 3.9 5.9
164 10.1 8.3 12.5

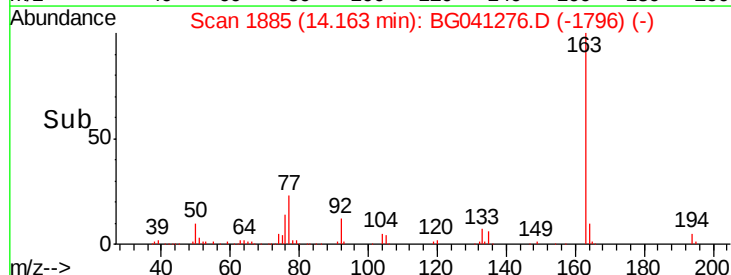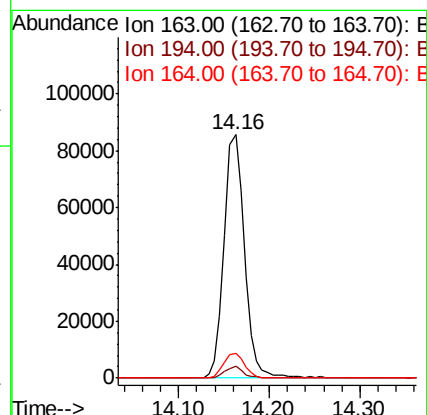

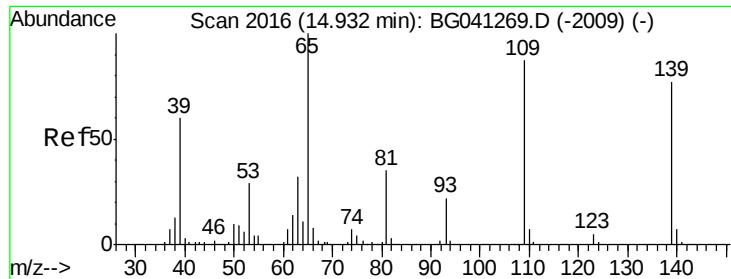

#56

4-Nitrophenol

Concen: 3.240 ng

RT: 14.90 min Scan# 2010

Delta R.T. -0.03 min

Lab File: BG041276.D


Acq: 17 Jun 2019 17:09

Instrument :

BNA_G

ClientSampleId :

Tot Ion	Ratio	Lower	Upper
139	100		
109	0.0	93.2	133.2#
65	0.0	110.2	150.2#






Abundance

Ion 139.00 (138.70 to 139.70): E

Ion 109.00 (108.70 to 109.70): E

Ion 65.00 (64.70 to 65.70): BGC

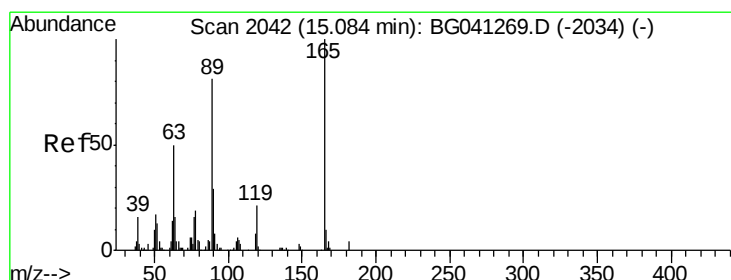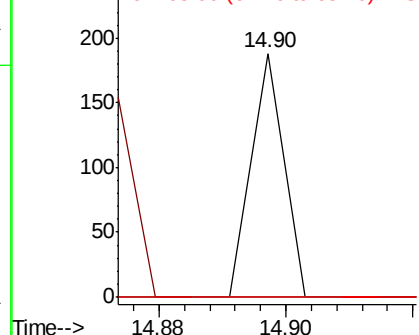

#57

2,4-Dinitrotoluene

Concen: 4.963 ng

RT: 14.71 min Scan# 1979

Delta R.T. -0.37 min

Lab File: BG041276.D

Acq: 17 Jun 2019 17:09

Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.9	40.0	60.0#
89	2.1	64.6	96.8#
182	0.0	2.9	4.3#




Abundance


Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BGC

Ion 89.00 (88.70 to 89.70): BGC

Ion 182.00 (181.70 to 182.70): E

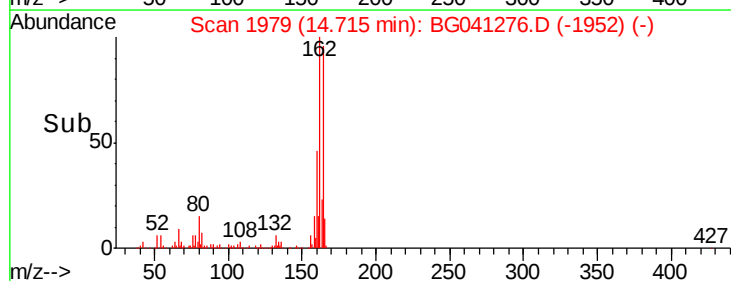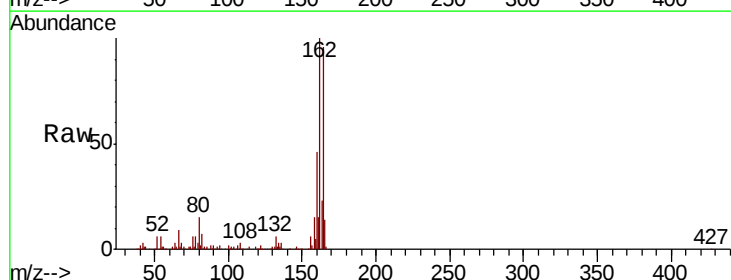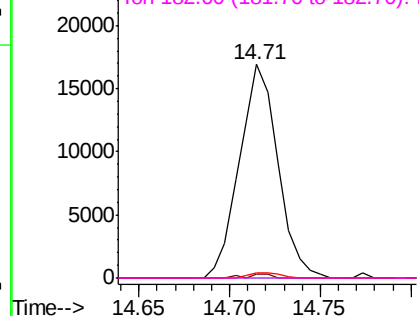



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.46 min Scan# 2447

Delta R.T. 0.00 min

Lab File: BG041276.D

Acq: 17 Jun 2019 17:09

Instrument :

BNA_G

ClientSampleId :


Tot Ion:188 Resp: 427640

Ion Ratio Lower Upper

188 100

94 5.2 3.6 5.4




80 6.0 4.8 7.2



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG

Ion 80.00 (79.70 to 80.70): BG

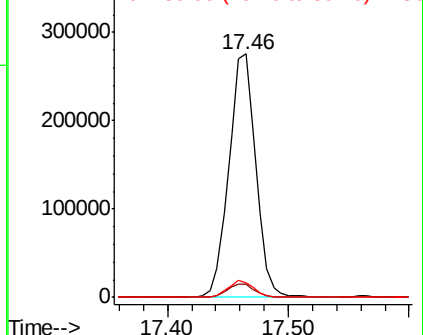

#67

4-Bromophenyl-phenylether

Concen: 2.797 ng

RT: 16.21 min Scan# 2233

Delta R.T. -0.43 min

Lab File: BG041276.D

Acq: 17 Jun 2019 17:09


Tgt Ion:248 Resp: 15468

Ion Ratio Lower Upper

248 100

250 181.9 79.8 119.8#



141 454.6 55.8 83.6#




Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E

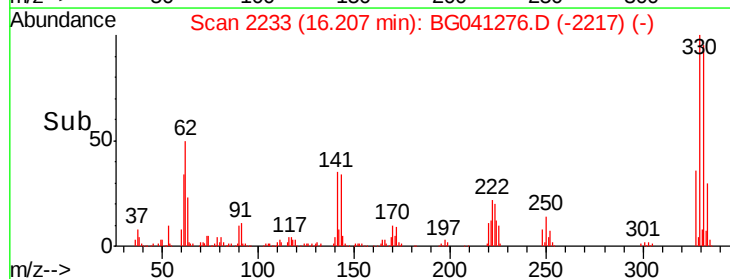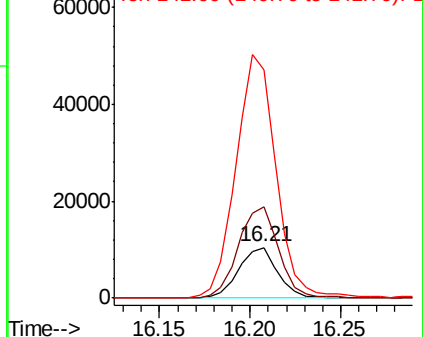



#75

Fluoranthene

Concen: 3.715 ng

RT: 19.51 min Scan# 2795

Delta R.T. 0.00 min

Lab File: BG041276.D

Acq: 17 Jun 2019 17:09

Instrument :

BNA_G

ClientSampleId :


Tot Ion:202 Resp: 112559

Ion Ratio Lower Upper

202 100

101 4.0 0.0 26.0

203 18.7 0.0 37.7



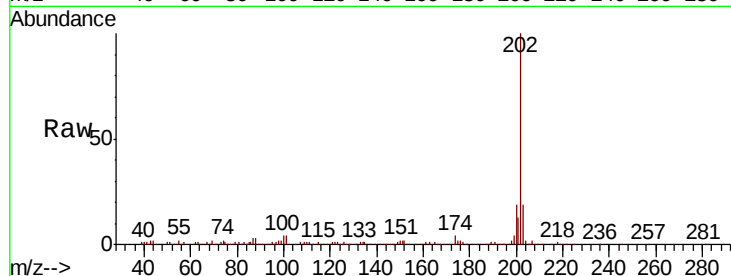


Abundance

Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

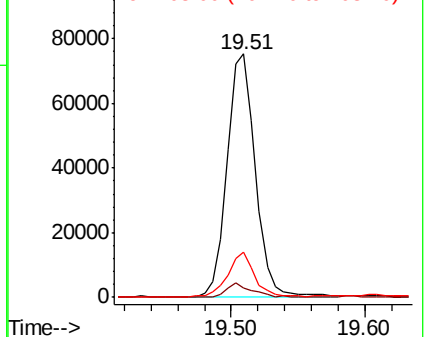

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.74 min Scan# 3174

Delta R.T. -0.01 min

Lab File: BG041276.D

Acq: 17 Jun 2019 17:09


Tgt Ion:240 Resp: 444304

Ion Ratio Lower Upper

240 100

120 4.6 3.7 5.5

236 27.4 21.1 31.7






Abundance

Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

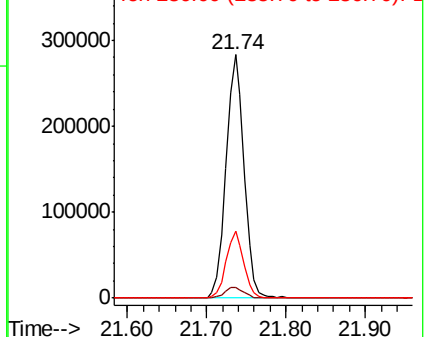



#78

Pvrene

Concen: 3.296 ng

RT: 19.87 min Scan# 2856

Delta R.T. -0.01 min

Lab File: BG041276.D

Acq: 17 Jun 2019 17:09

Instrument :

BNA_G

ClientSampleId :


Tot Ion:202 Resp: 98758

Ion Ratio Lower Upper




202 100

200 20.2 16.8 25.2

203 18.6 14.6 21.8



Abundance Ion 202.00 (201.70 to 202.70): E
Ion 200.00 (199.70 to 200.70): E
Ion 203.00 (202.70 to 203.70): E

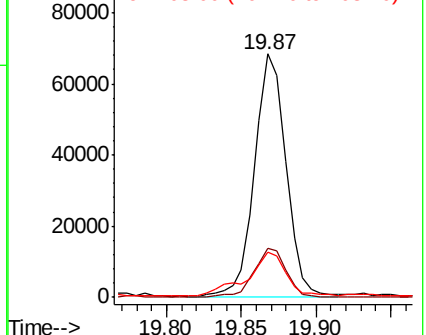

#79

Terphenyl-d14

Concen: 45.656 ng

RT: 20.06 min Scan# 2888

Delta R.T. -0.01 min

Lab File: BG041276.D

Acq: 17 Jun 2019 17:09


Tgt Ion:244 Resp: 1023569

Ion Ratio Lower Upper



244 100


212 8.2 6.6 10.0

122 6.5 5.0 7.4



Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E



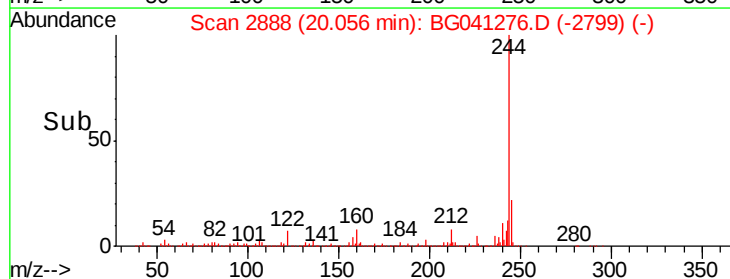
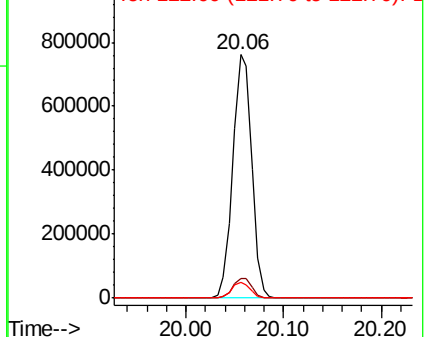


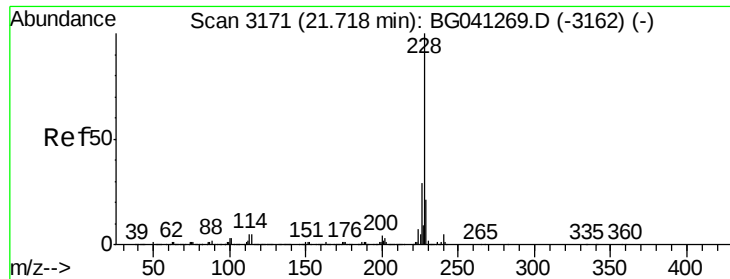

#81
Benzo(a)anthracene
Concen: 2.101 ng
RT: 21.71 min Scan# 3170
Delta R.T. -0.01 min
Lab File: BG041276.D
Acq: 17 Jun 2019 17:09




Instrument :
BNA_G
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
228	100		
226	24.7	23.2	34.8
229	21.8	16.8	25.2

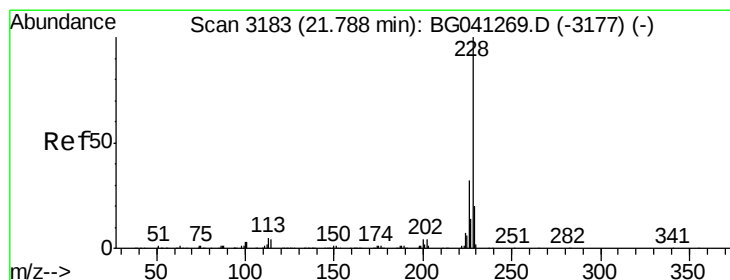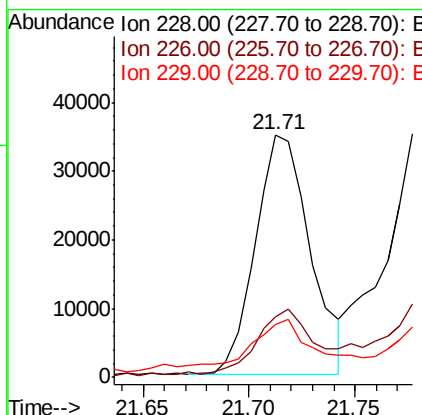

#83
Chrysene
Concen: 2.467 ng
RT: 21.78 min Scan# 3181
Delta R.T. -0.01 min
Lab File: BG041276.D
Acq: 17 Jun 2019 17:09

Tgt Ion	Ratio	Lower	Upper
228	100		
226	30.0	25.4	38.0
229	20.8	16.2	24.2

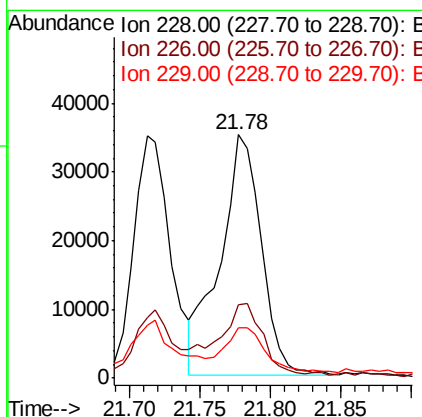

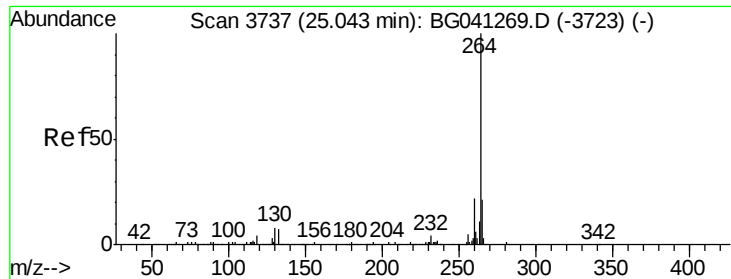

#87

Pervlene-d12

Concen: 20.000 ng

RT: 25.05 min Scan# 3738

Delta R.T. 0.01 min

Lab File: BG041276.D

Acq: 17 Jun 2019 17:09


Instrument :

BNA_G

ClientSampleId :

Tot Ion:264 Resp: 496016

Ion	Ratio	Lower	Upper
264	100		
260	24.4	17.4	26.2
265	22.0	17.2	25.8



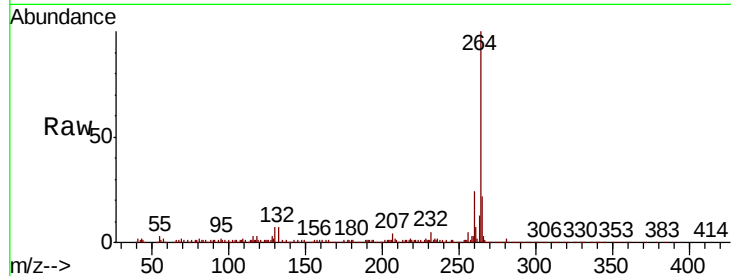


Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

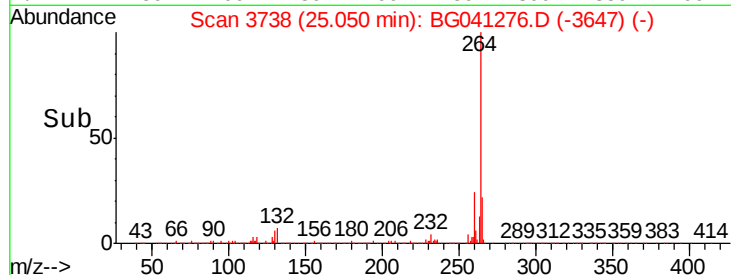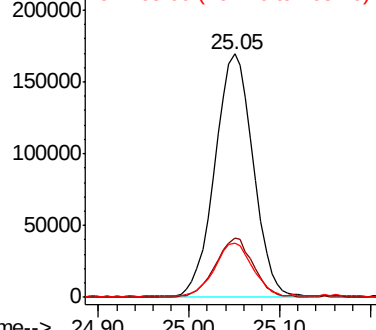

#88

Benzo(b)fluoranthene

Concen: 3.308 ng

RT: 23.98 min Scan# 3556


Delta R.T. -0.01 min

Lab File: BG041276.D

Acq: 17 Jun 2019 17:09

Tgt Ion:252 Resp: 101688

Ion	Ratio	Lower	Upper
252	100		
253	26.3	17.4	26.0#
125	5.5	3.9	5.9






Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

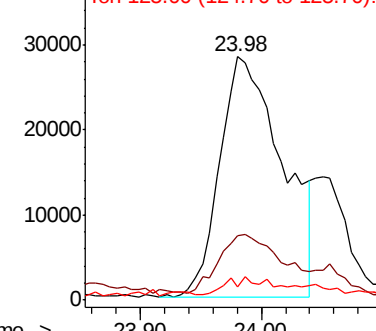



#89

Benzo(k)fluoranthene

Concen: 3.339 ng

RT: 23.98 min Scan# 3556

Delta R.T. -0.08 min

Lab File: BG041276.D

Acq: 17 Jun 2019 17:09

Instrument :

BNA_G

ClientSampleId :


Tot Ion:252 Resp: 101688

Ion Ratio Lower Upper




252 100

253 26.3 18.0 27.0

125 5.5 4.3 6.5



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

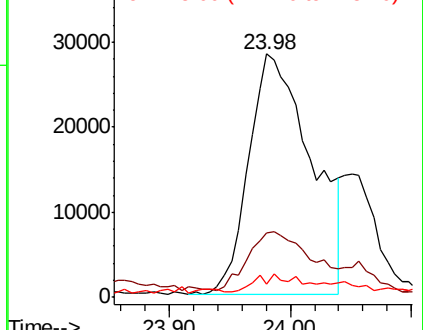

#90

Benzo(a)pyrene

Concen: 2.386 ng

RT: 24.89 min Scan# 3711

Delta R.T. 0.00 min

Lab File: BG041276.D

Acq: 17 Jun 2019 17:09


Tgt Ion:252 Resp: 69267

Ion Ratio Lower Upper

252 100

253 24.0 17.8 26.6

125 8.2 4.2 6.4#



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

