
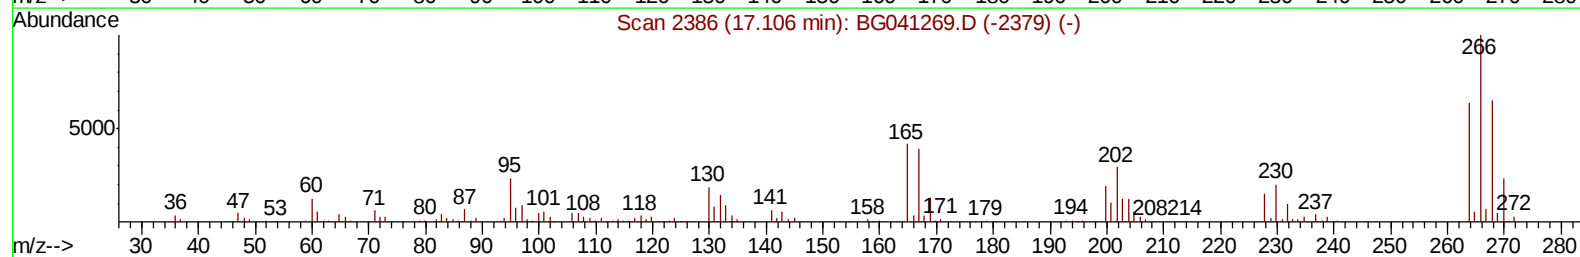
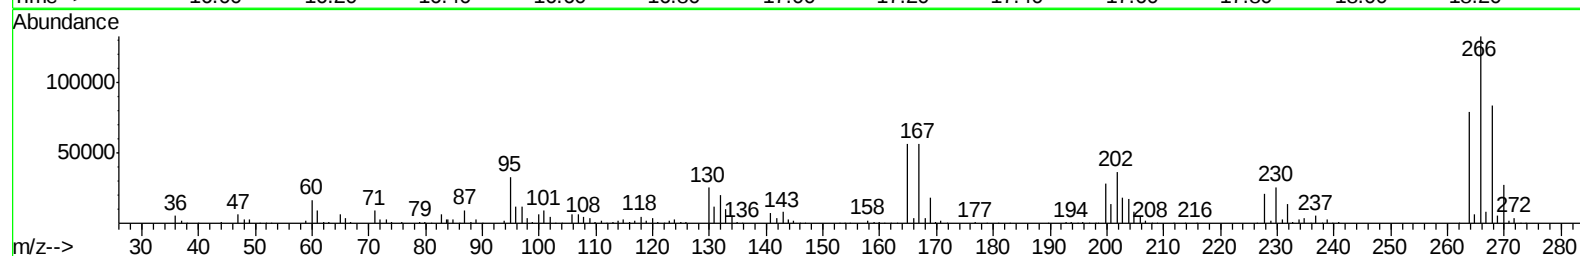


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061719\
Data File : BG041266.D
Acq On : 17 Jun 2019 9:16
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 15:22:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 14:58:02 2019
Response via : Initial Calibration

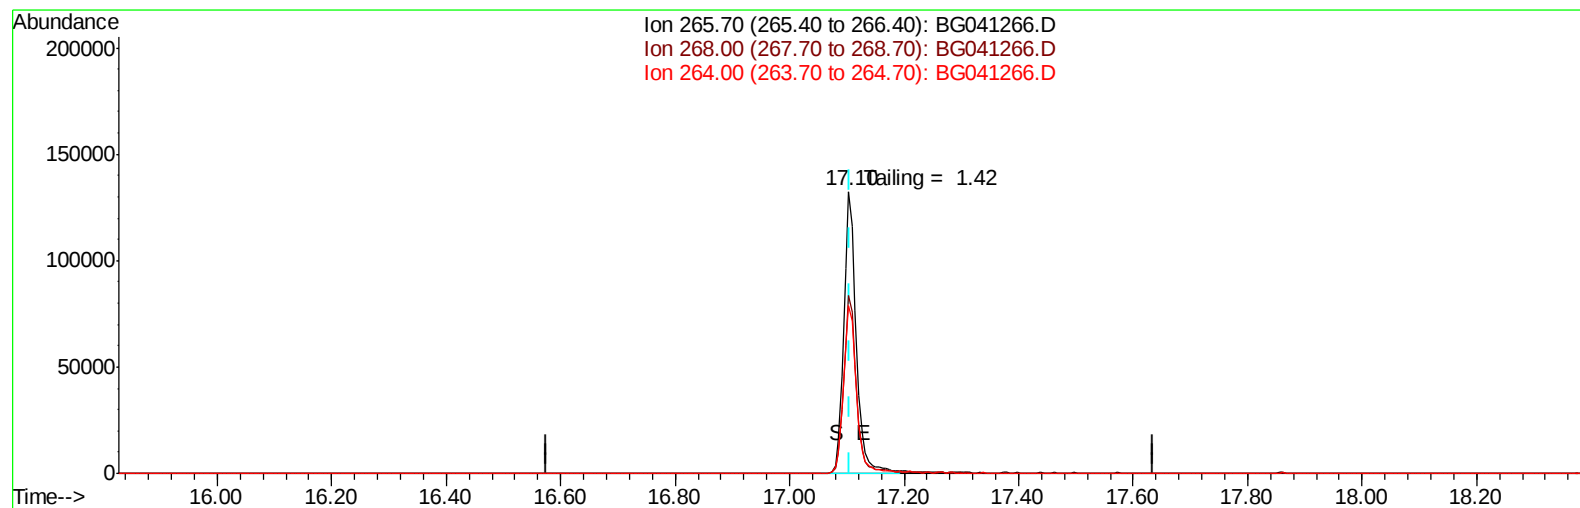

TIC: BG041266.D

(70) Pentachlorophenol (C)




17.103min (-0.002) 21845.09ng

response 206459

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	63.18
264.00	64.00	59.33
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061719\
 Data File : BG041266.D
 Acq On : 17 Jun 2019 9:16
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 15:22:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 14:58:02 2019
 Response via : Initial Calibration

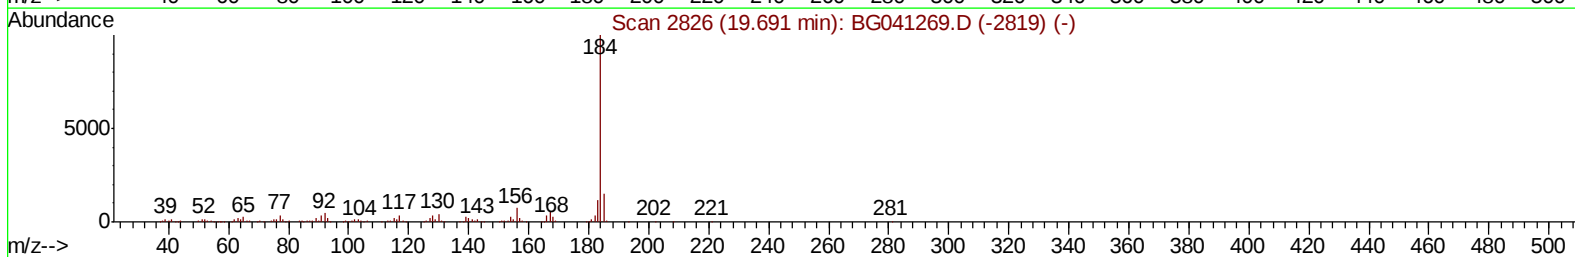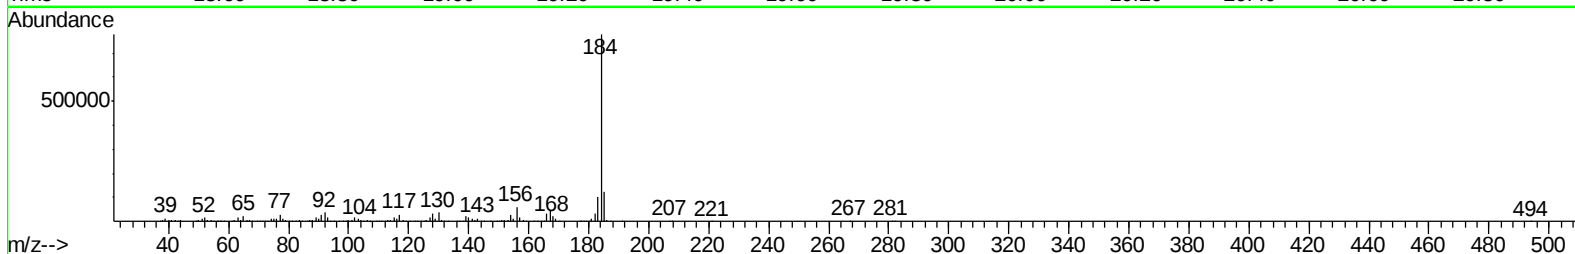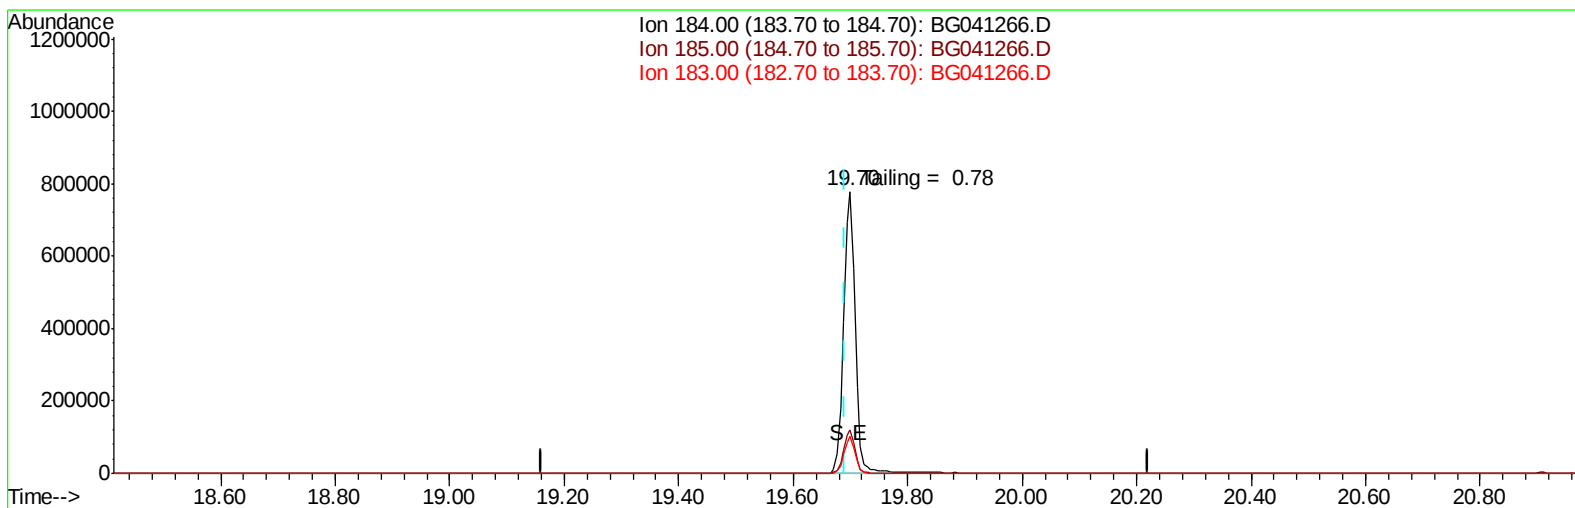

TIC: BG041266.D

(77) Benzidine

19.700min (+0.009) 0.00ng

response 1109507

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.68
183.00	12.00	13.12
0.00	0.00	0.00