


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG061719\
 Data File : BG041266.D
 Acq On : 17 Jun 2019 9:16
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 17 14:58:02 2019

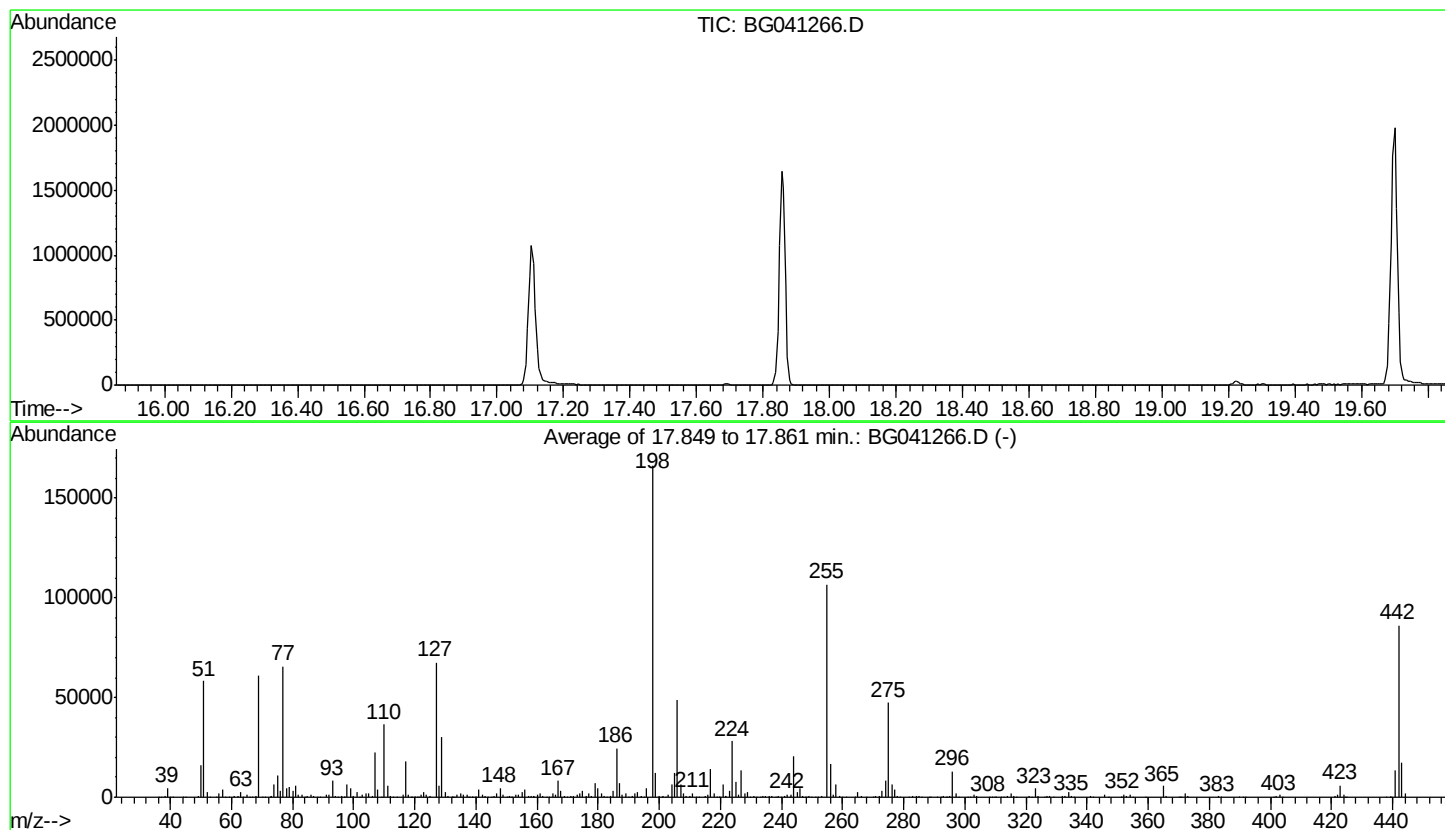

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	58312	PASS
68	69	0.00	2	1.0	580	PASS
69	198	0.00	100	36.6	60874	PASS
70	69	0.00	2	0.5	295	PASS
127	198	10	80	40.6	67442	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	166197	PASS
199	198	5	9	7.2	11986	PASS
275	198	10	60	28.5	47448	PASS
365	198	1	100	3.3	5522	PASS
441	198	0.01	100	8.3	13724	PASS
442	198	50	100	51.8	86008	PASS
443	442	15	24	20.0	17243	PASS