


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061719\
Data File : BG041277.D
Acq On : 17 Jun 2019 18:25
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061719.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jun 17 14:58:02 2019

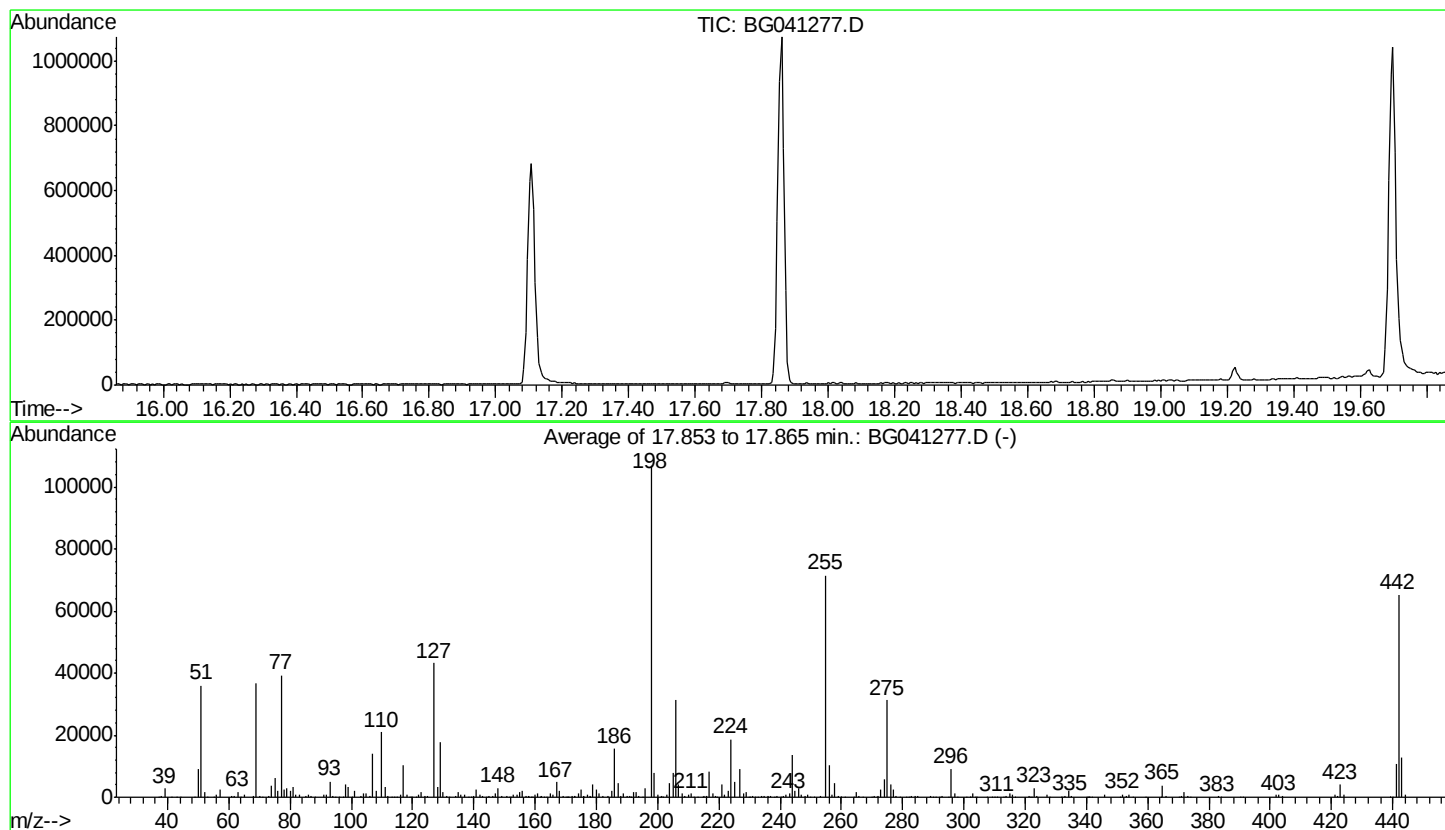

AutoFind: Scans 2513, 2514, 2515; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.6	35909	PASS
68	69	0.00	2	0.6	225	PASS
69	198	0.00	100	34.3	36641	PASS
70	69	0.00	2	0.9	331	PASS
127	198	10	80	40.5	43264	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	106818	PASS
199	198	5	9	7.3	7832	PASS
275	198	10	60	29.2	31221	PASS
365	198	1	100	3.5	3732	PASS
441	198	0.01	100	10.0	10644	PASS
442	198	50	100	61.0	65189	PASS
443	442	15	24	19.5	12738	PASS