
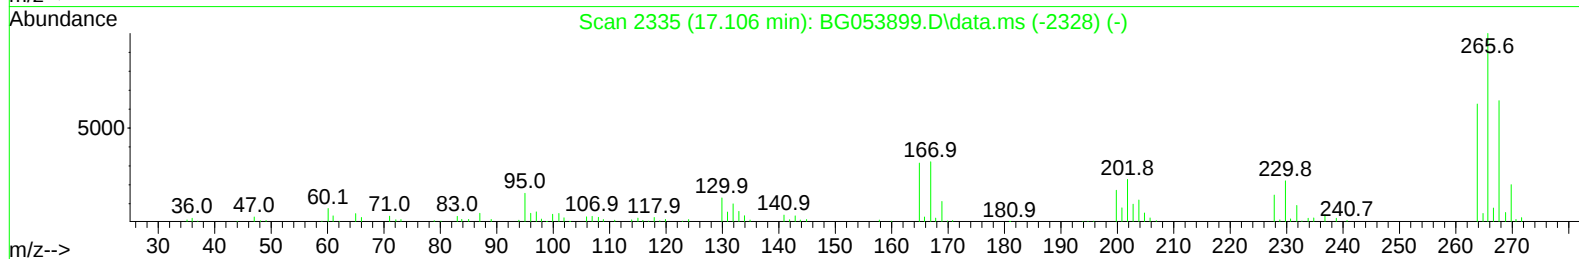
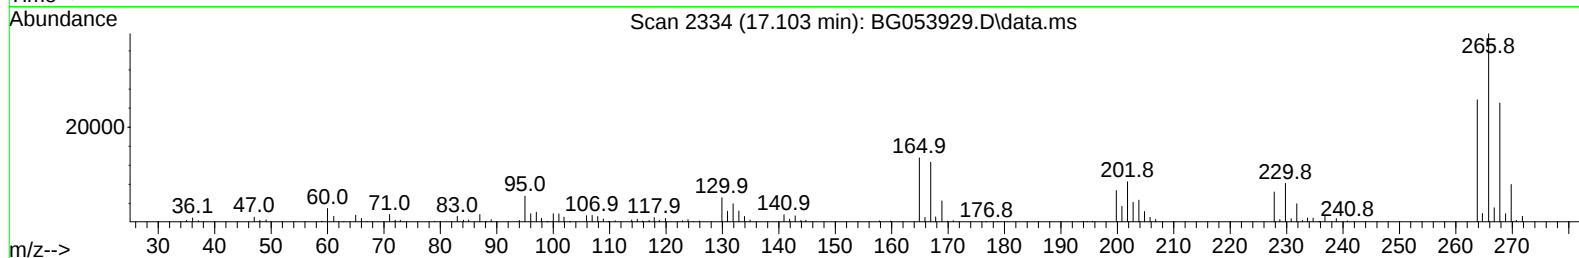


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061722\
Data File : BG053929.D
Acq On : 17 Jun 2022 10:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 18 01:47:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 15:49:31 2022
Response via : Initial Calibration

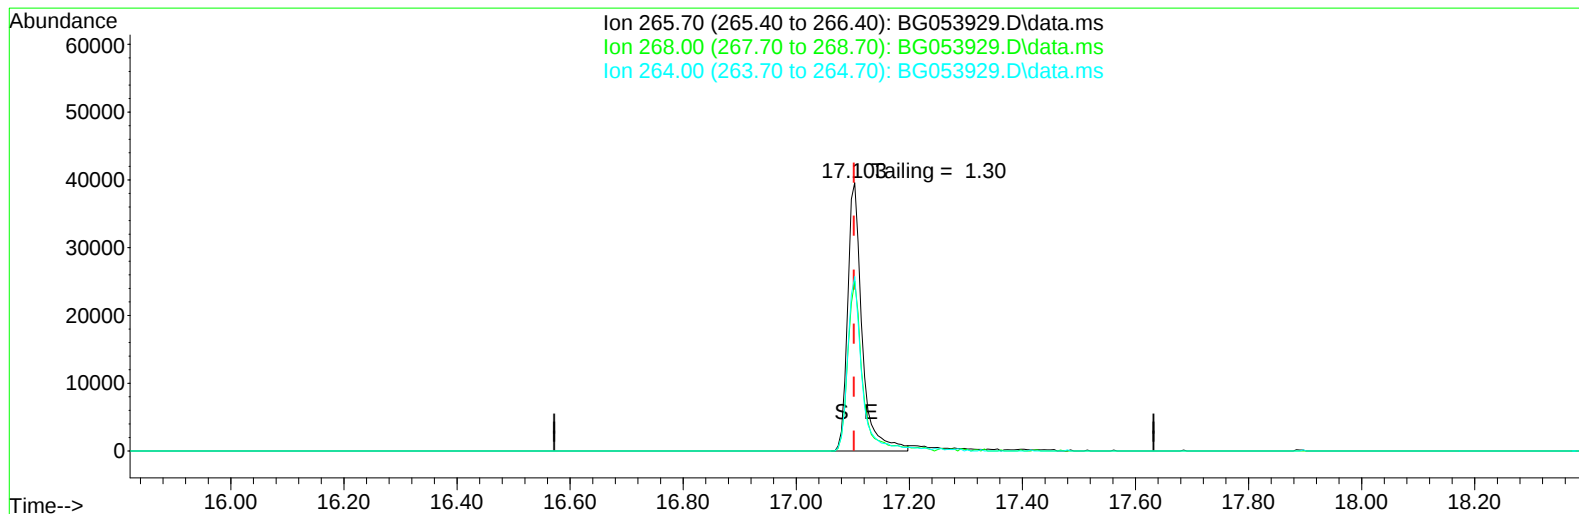

TIC: BG053929.D\data.ms

(70) Pentachlorophenol (C)




17.103min (+ 0.002) 37867.79 ng

response 70617

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	63.25
264.00	66.20	69.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061722\
Data File : BG053929.D
Acq On : 17 Jun 2022 10:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 18 01:47:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 15:49:31 2022
Response via : Initial Calibration

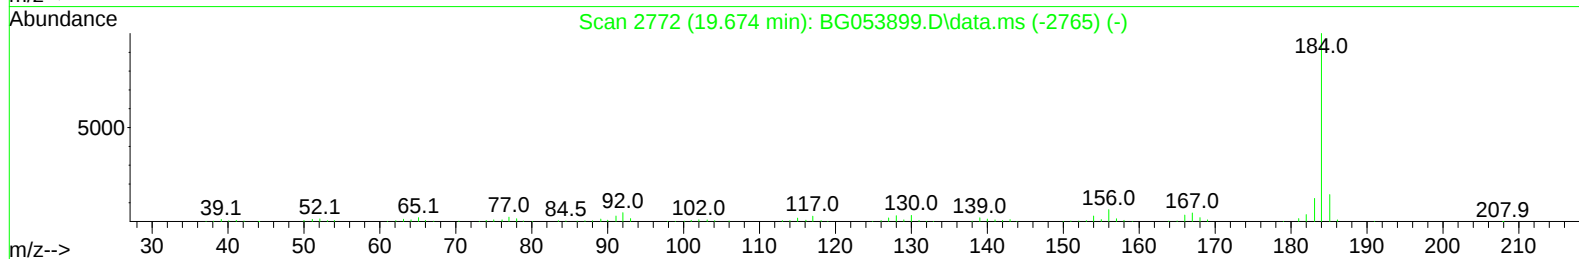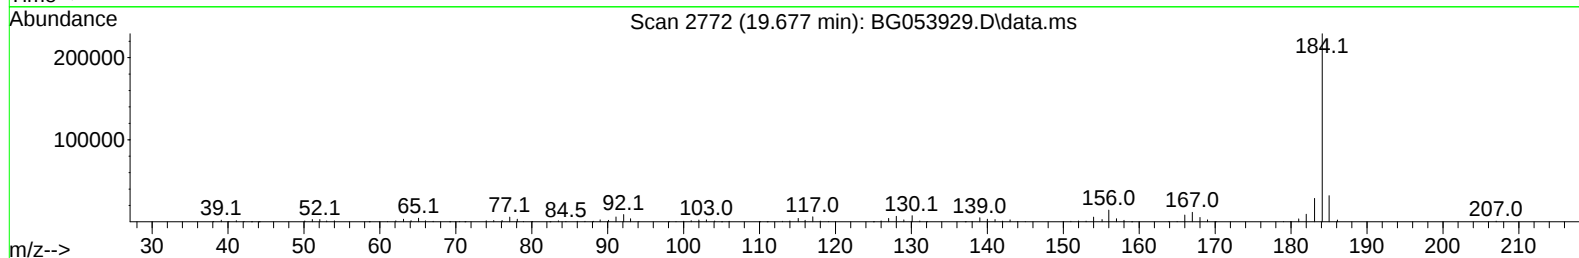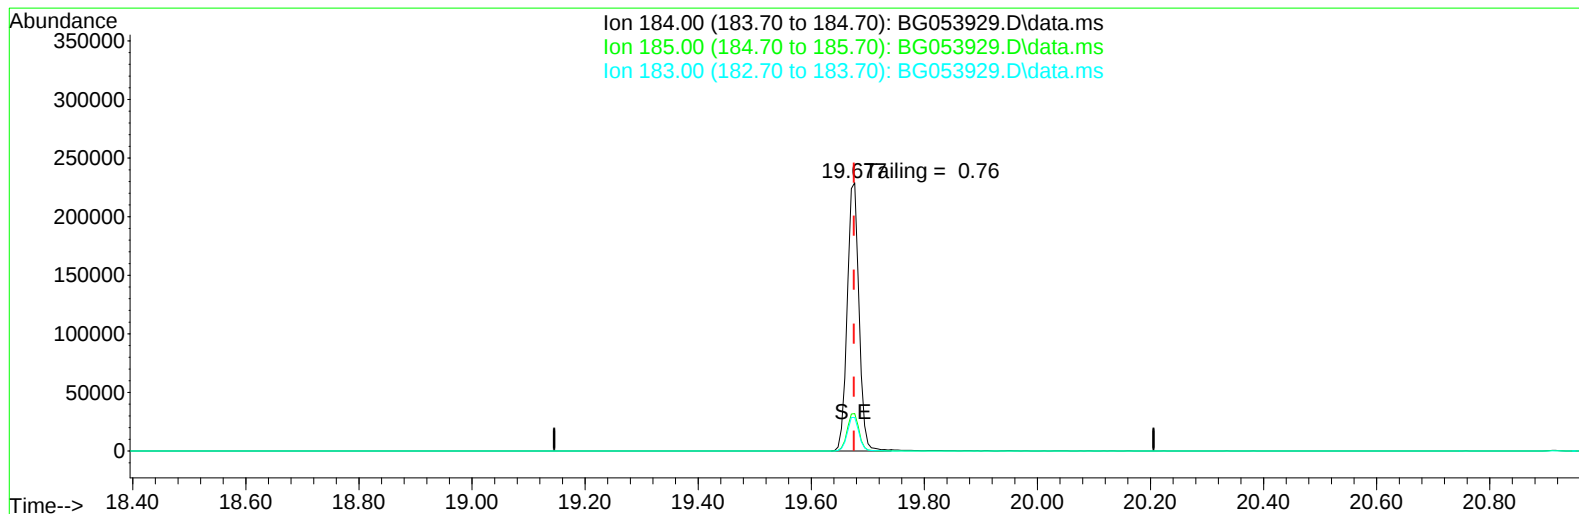

TIC: BG053929.D\data.ms

(77) Benzidine**19.677min (+ 0.002) 0.00 ng****response 332601**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.95
183.00	11.10	12.52
0.00	0.00	0.00