
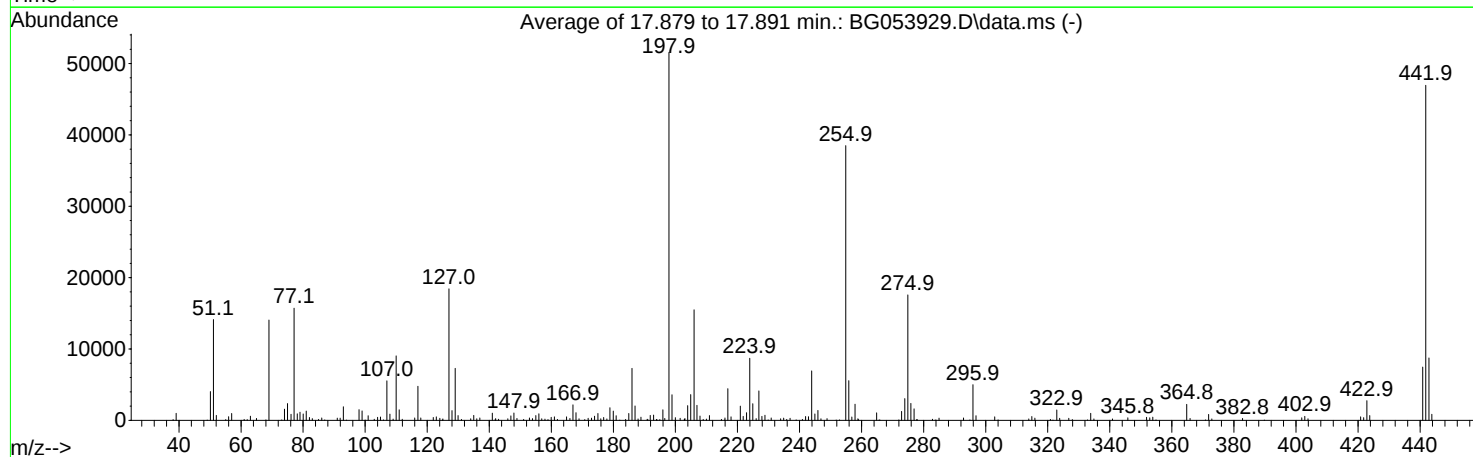


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061722\
 Data File : BG053929.D
 Acq On : 17 Jun 2022 10:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 13 15:49:31 2022

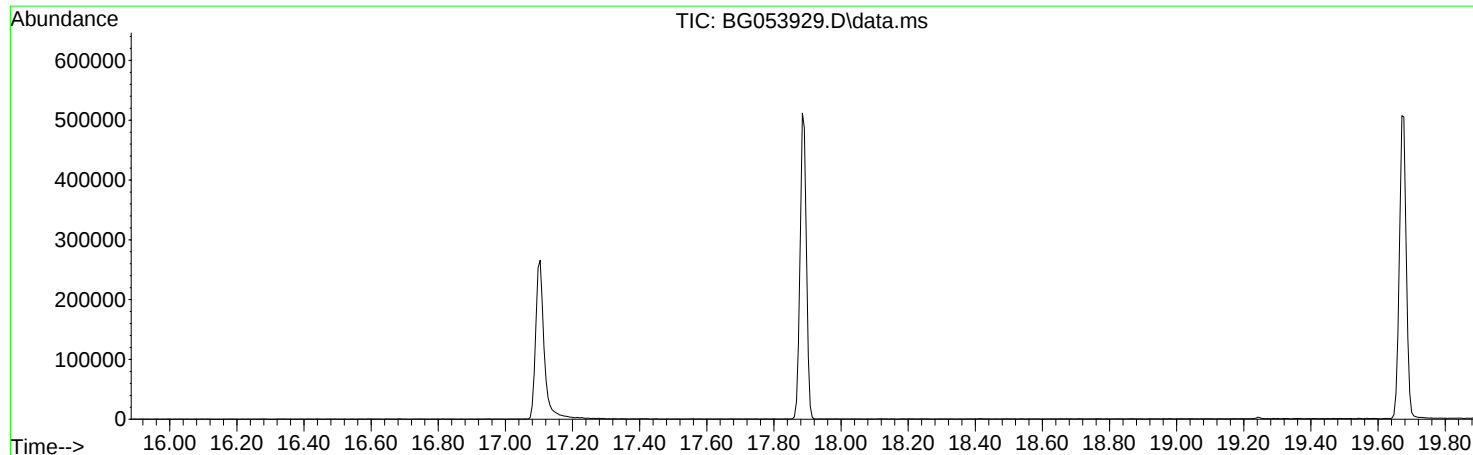




AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.4	14114	PASS
68	69	0.00	2	0.5	67	PASS
69	198	0.00	100	27.3	14067	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	35.7	18424	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51544	PASS
199	198	5	9	6.9	3581	PASS
275	198	10	60	34.1	17583	PASS
365	198	1	100	4.4	2252	PASS
441	198	0.01	100	14.5	7465	PASS
442	442	50	100	100.0	46955	PASS
443	442	15	24	18.6	8745	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061722\
Data File : BG053929.D
Acq On : 17 Jun 2022 10:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 18 01:47:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 15:49:31 2022
Response via : Initial Calibration

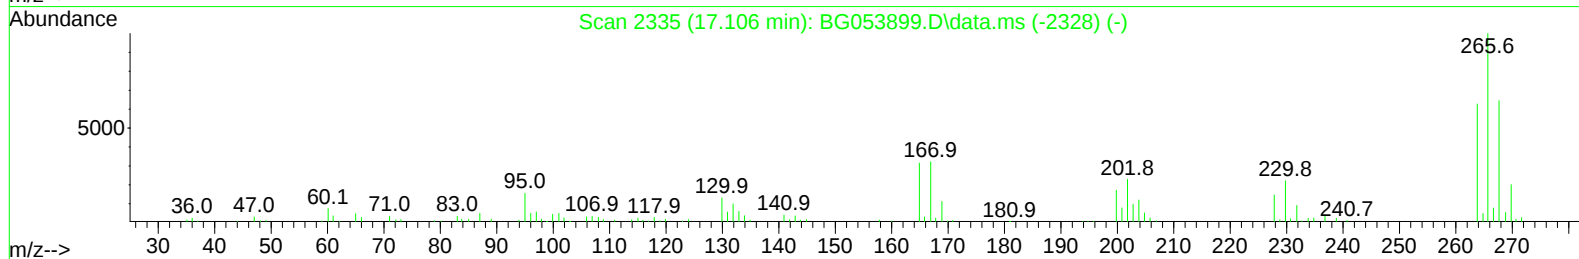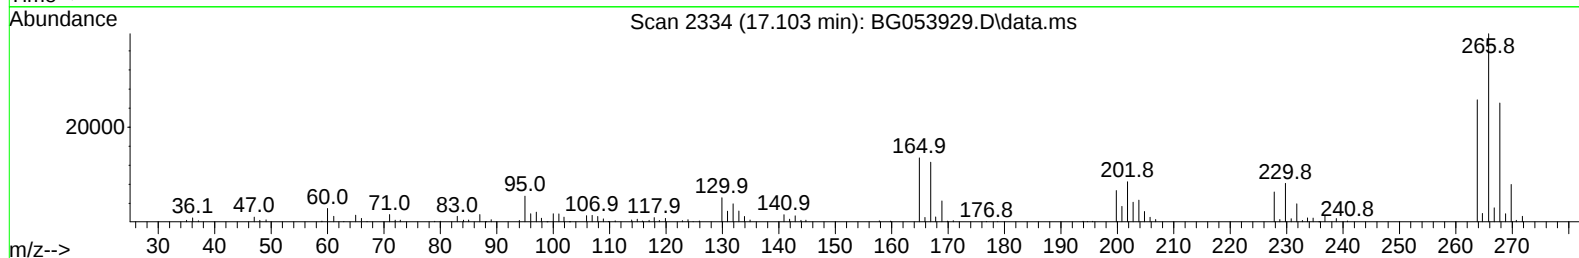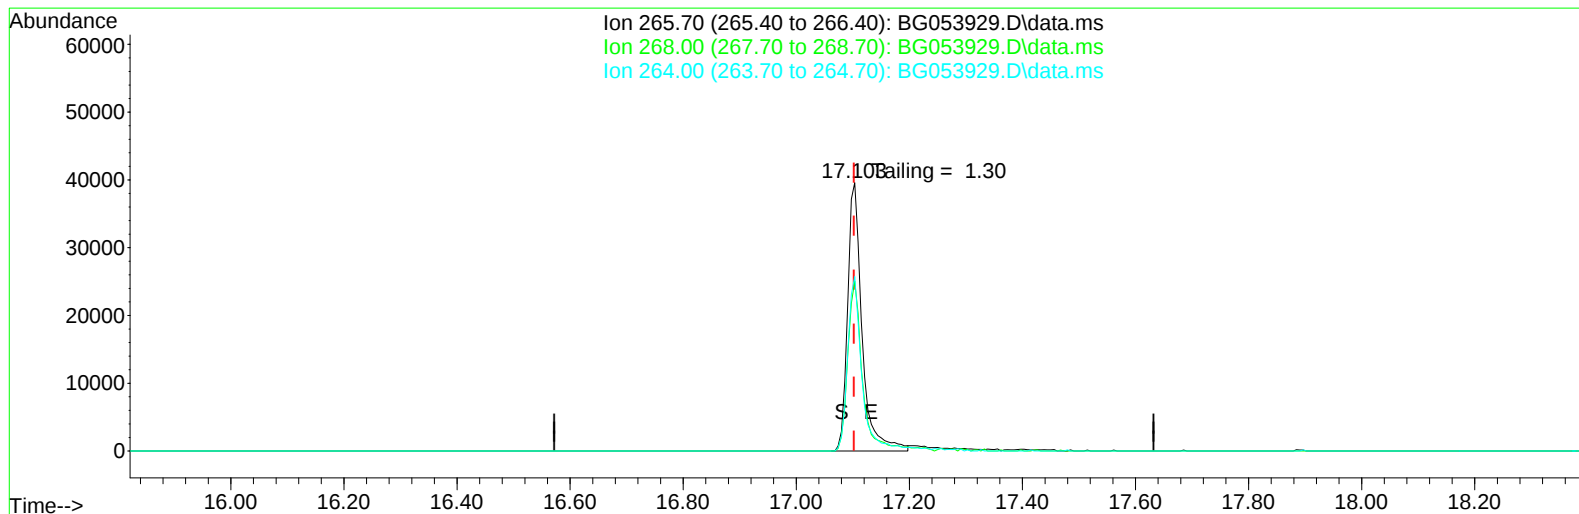

TIC: BG053929.D\data.ms

(70) Pentachlorophenol (C)

17.103min (+ 0.002) 37867.79 ng




response 70617

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	63.25
264.00	66.20	69.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061722\
Data File : BG053929.D
Acq On : 17 Jun 2022 10:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 18 01:47:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 15:49:31 2022
Response via : Initial Calibration

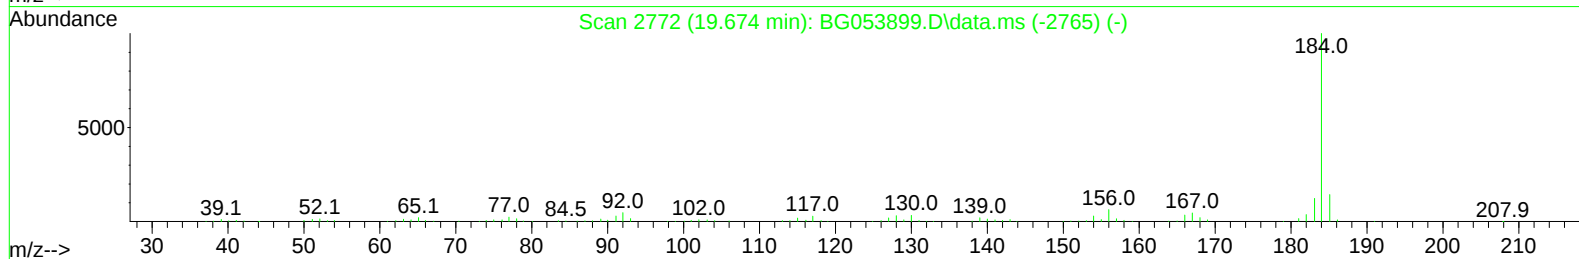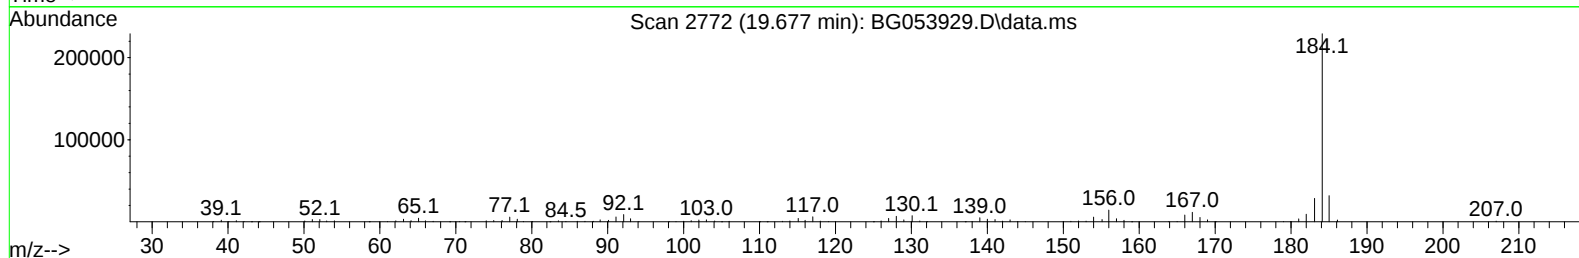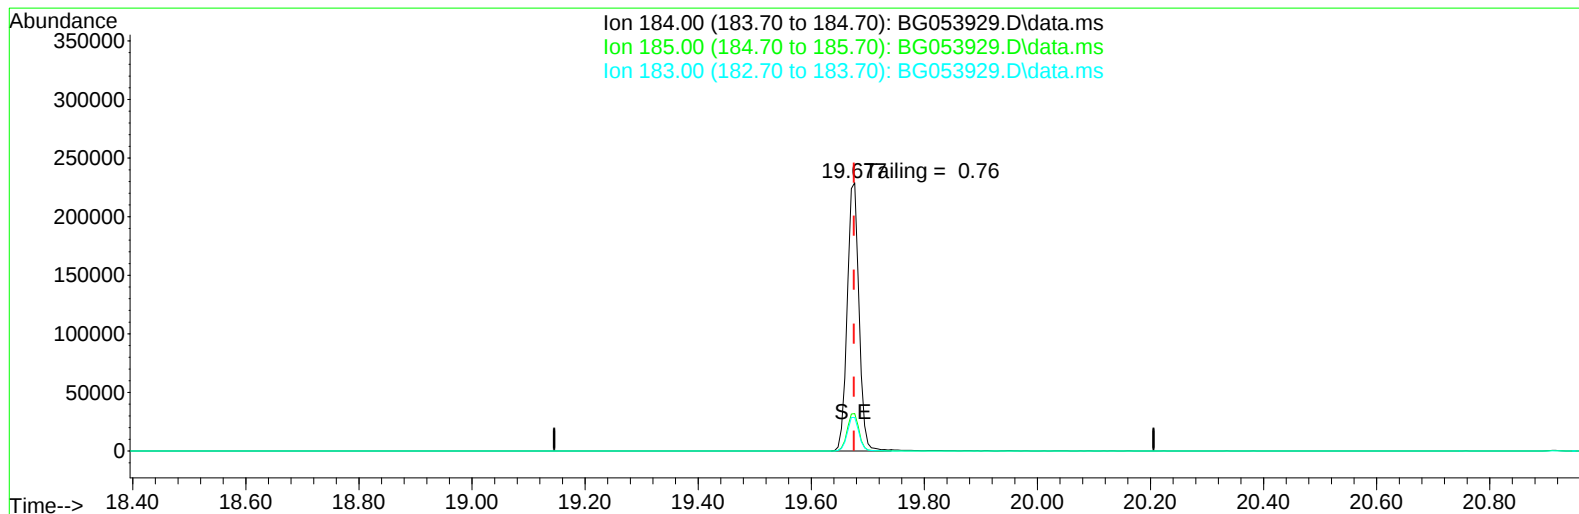

TIC: BG053929.D\data.ms

(77) Benzidine

19.677min (+ 0.002) 0.00 ng

response 332601

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.95
183.00	11.10	12.52
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/17/2022	BNA_G	<u>BG053929.D</u>
Compound Name	Response	Retention Time
DDT	189134	20.91
DDD	2314	20.47
DDE	0	19.97
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2314	191448	1.21

Instrument :
BNA_G
ClientSampleId :
DFTPP