
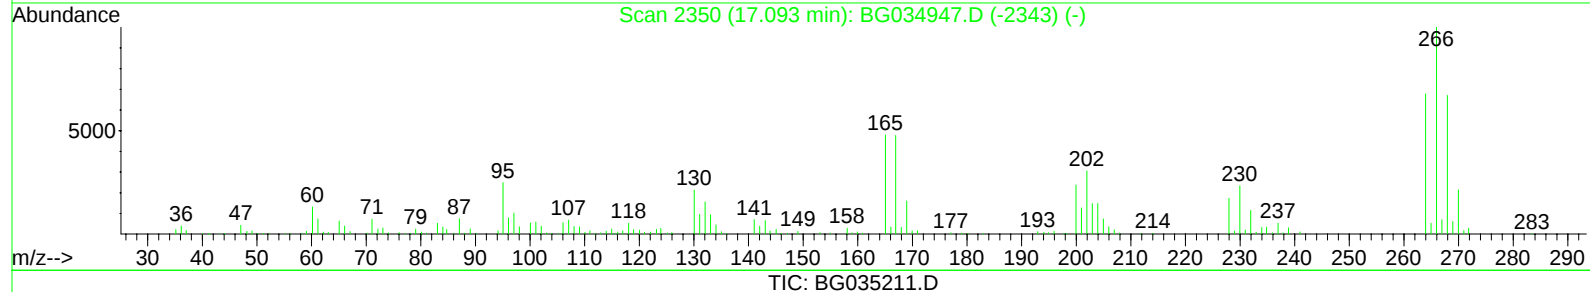
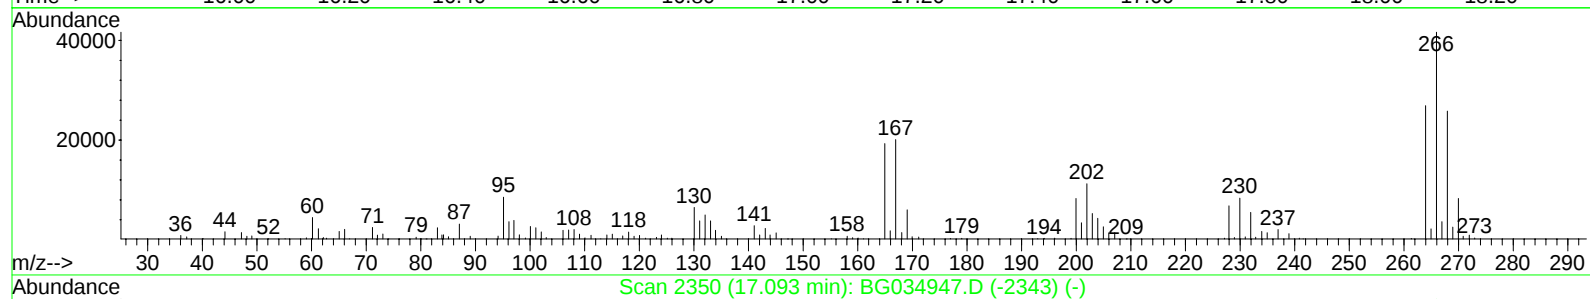


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG061818\  
Data File : BG035211.D  
Acq On : 18 Jun 2018 10:05  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 18 19:18:09 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Jun 08 17:16:28 2018  
Response via : Initial Calibration

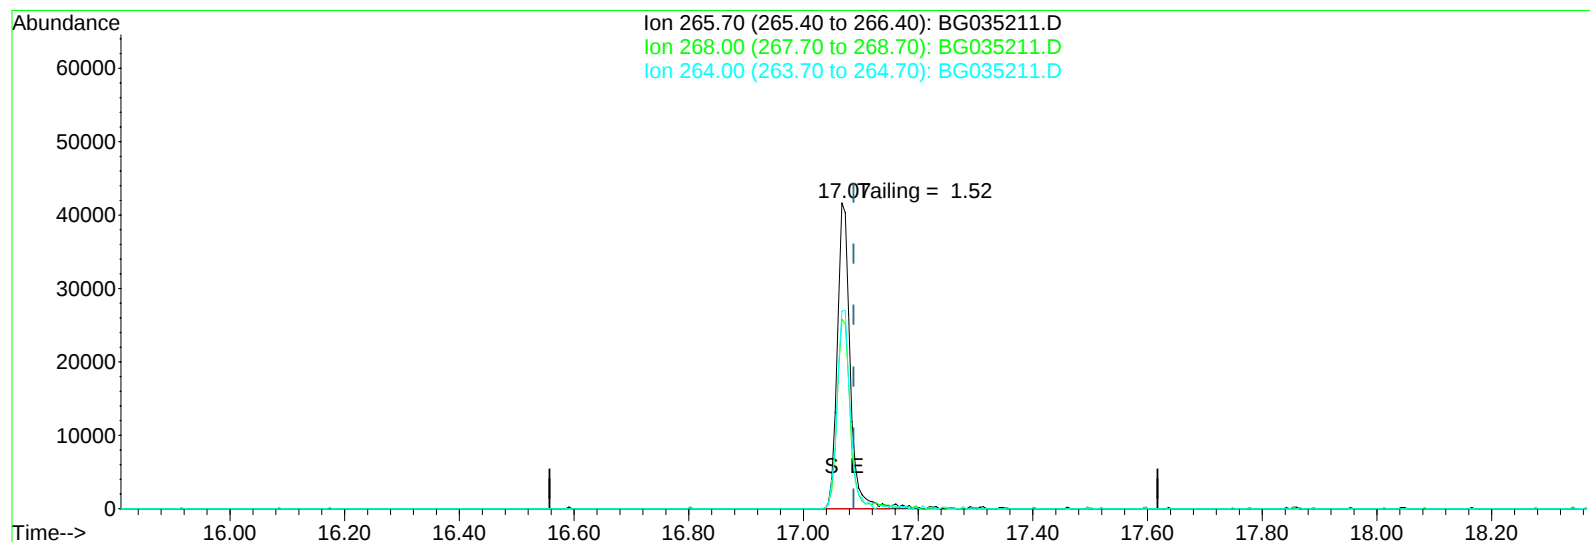

(69) Pentachlorophenol (C)




17.067min (-0.021) 15443.25ng

response 64406

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 61.97 |
| 264.00 | 62.00 | 64.64 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG061818\  
Data File : BG035211.D  
Acq On : 18 Jun 2018 10:05  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 18 19:18:09 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Jun 08 17:16:28 2018  
Response via : Initial Calibration

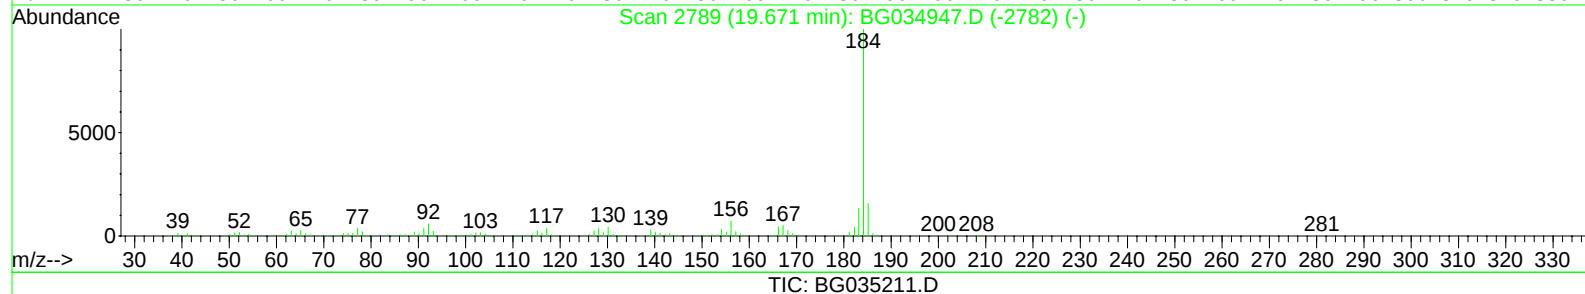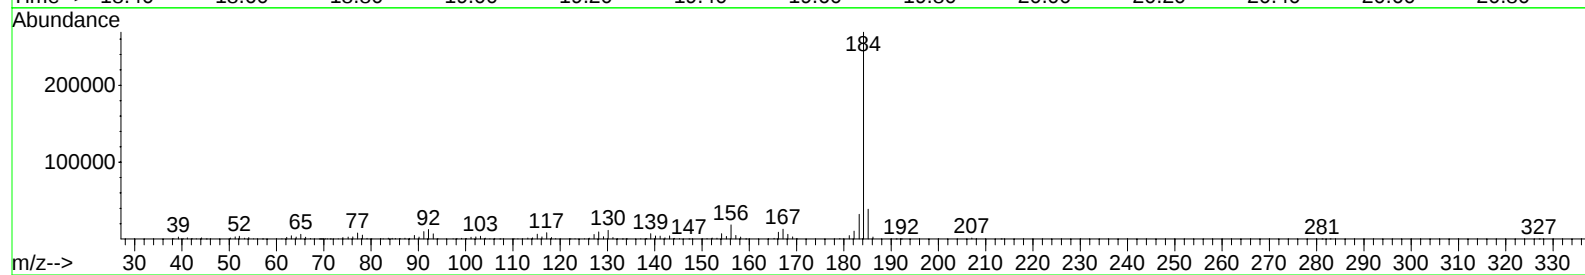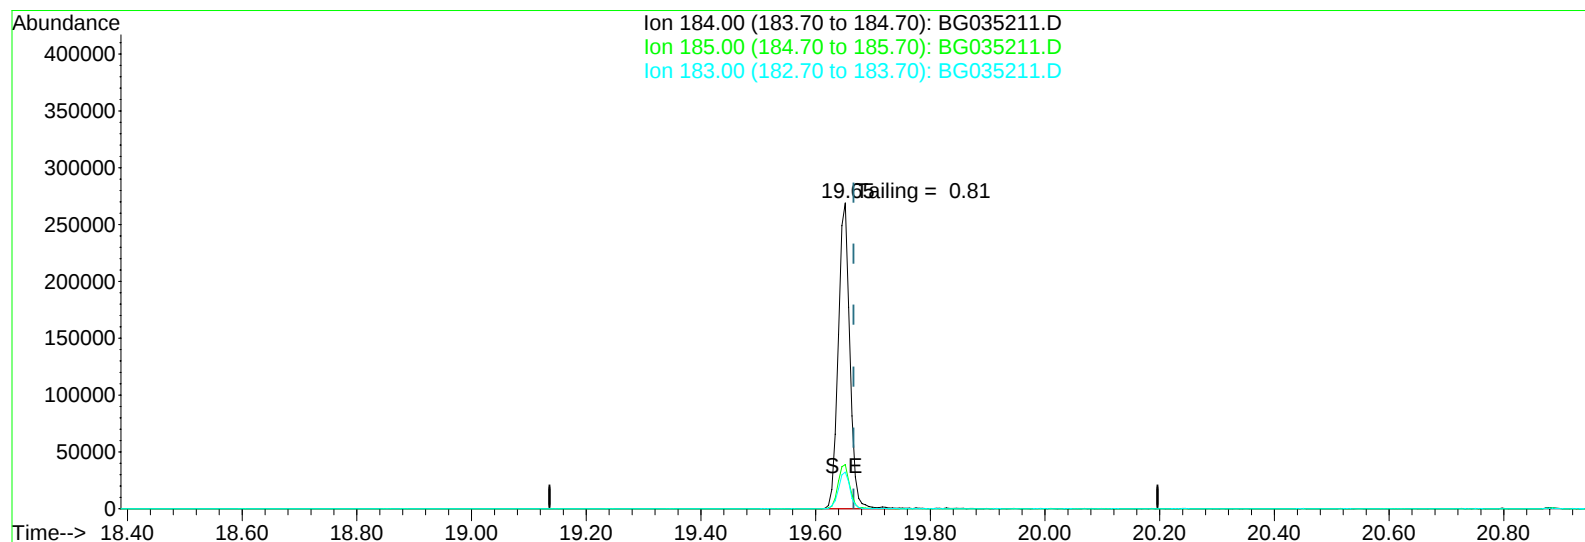

(76) Benzidine

19.652min (-0.015) 163863.60ng

response 341394

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 13.90 | 14.47 |
| 183.00 | 13.30 | 11.96 |
| 0.00   | 0.00  | 0.00  |