

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061818\
 Data File : BG035217.D
 Acq On : 18 Jun 2018 13:58
 Operator : SJ/JU
 Sample : J3504-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB-51COMP

Quant Time: Jun 18 16:52:38 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 08 17:16:28 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.07	152	60832	20.00	ng	0.00
21) Naphthalene-d8	10.86	136	202629	20.00	ng	-0.02
38) Acenaphthene-d10	14.68	164	128507	20.00	ng	-0.02
63) Phenanthrene-d10	17.42	188	318891	20.00	ng	-0.02
75) Chrysene-d12	21.69	240	446060	20.00	ng	-0.03
86) Perylene-d12	24.92	264	429408	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.63	112	424251	117.70	ng	0.00
7) Phenol-d6	7.22	99	523868	98.47	ng	0.00
23) Nitrobenzene-d5	9.22	82	434053	101.82	ng	-0.02
41) 2,4,6-Tribromophenol	16.17	330	245672	149.34	ng	-0.02
44) 2-Fluorobiphenyl	13.31	172	894184	90.46	ng	-0.02
78) Terphenyl-d14	20.03	244	1777254	83.46	ng	-0.02
Target Compounds						
37) 2-Methylnaphthalene	12.52	142	16136	2.022	ng	Qvalue 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061818\
Data File : BG035217.D
Acq On : 18 Jun 2018 13:58
Operator : SJ/JU
Sample : J3504-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-51COMP

Quant Time: Jun 18 16:52:38 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

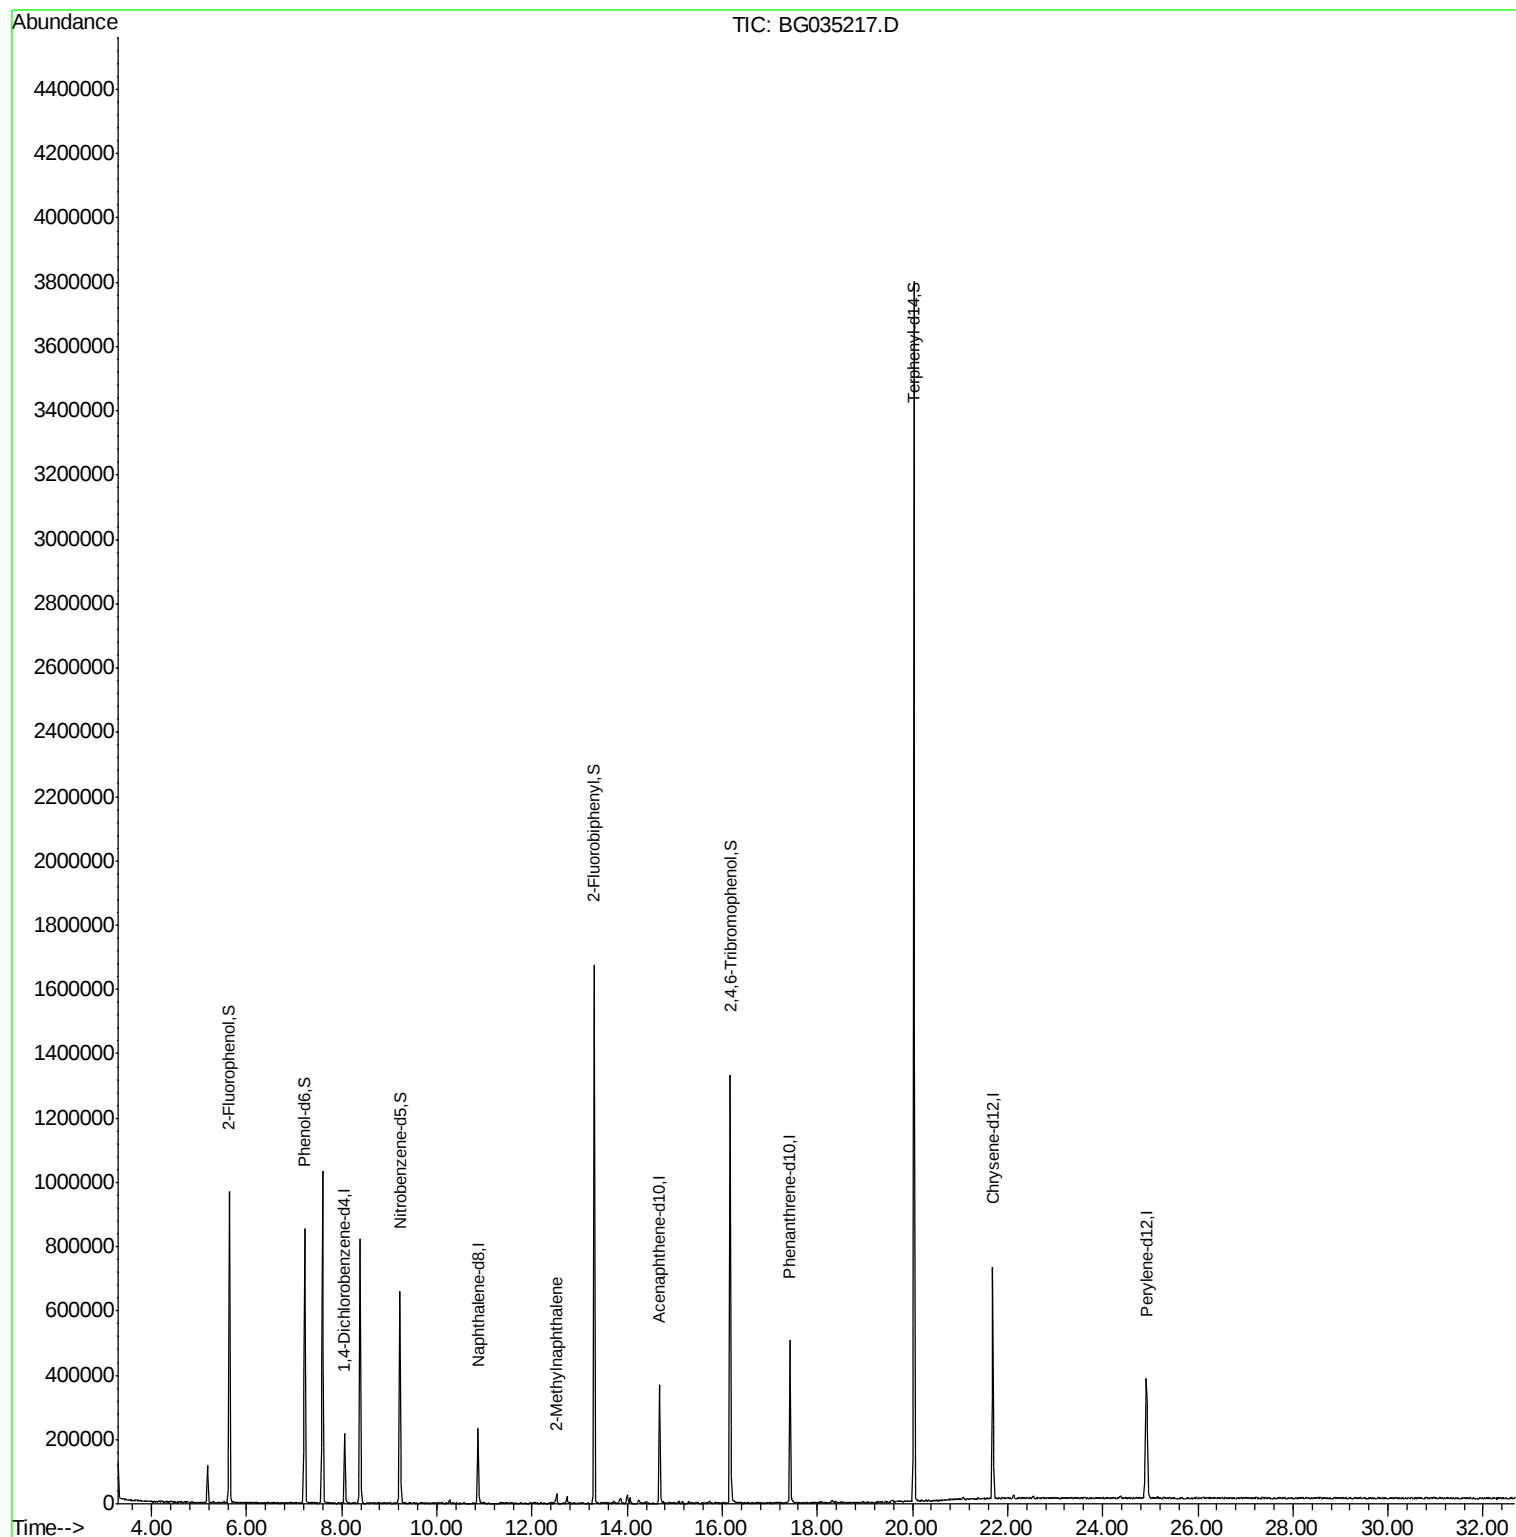






#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.07 min Scan# 813
Delta R.T. -0.01 min
Lab File: BG035217.D
Acq: 18 Jun 2018 13:58

Instrument :
BNA_G
ClientSampleId :
SB-51COMP




Tot Ion:152 Resp: 60832
Ion Ratio Lower Upper
152 100
150 143.9 126.6 189.8
115 58.8 53.0 79.4

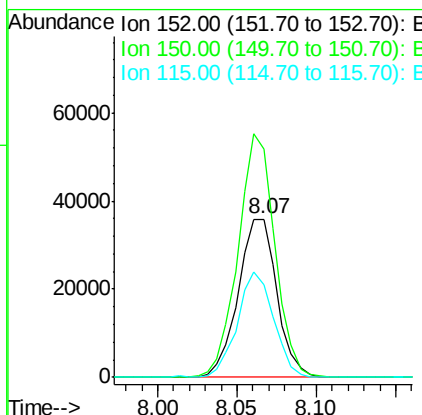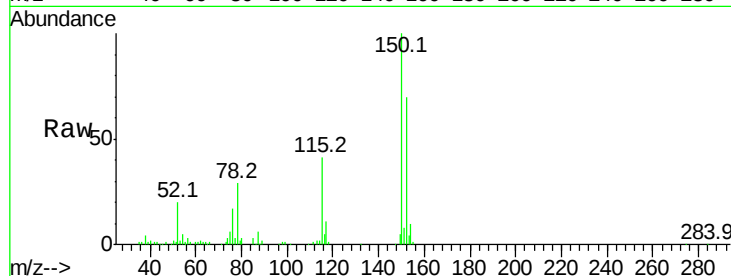

#5

2-Fluorophenol
Concen: 117.696 ng
RT: 5.63 min Scan# 399
Delta R.T. -0.01 min
Lab File: BG035217.D
Acq: 18 Jun 2018 13:58

Tgt Ion:112 Resp: 424251
Ion Ratio Lower Upper
112 100
64 64.1 56.3 84.5
63 34.6 30.1 45.1

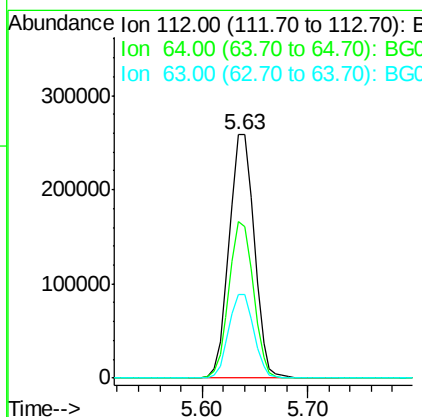



#7

Phenol-d6

Concen: 98.467 ng

RT: 7.22 min Scan# 669

Delta R.T. -0.00 min

Lab File: BG035217.D

Acq: 18 Jun 2018 13:58

Instrument :

BNA_G

ClientSampleId :

SB-51COMP


Tot Ion: 99 Resp: 523868

Ion Ratio Lower Upper




99 100

42 14.4 14.1 21.1

71 38.9 26.1 39.1

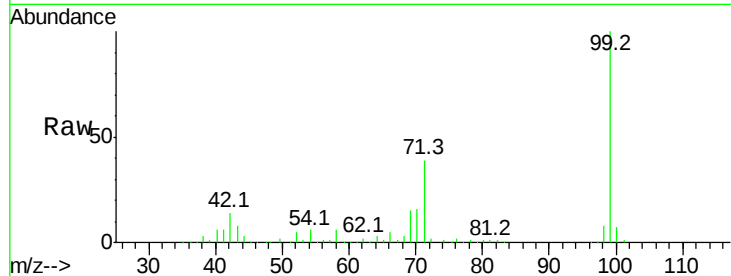

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

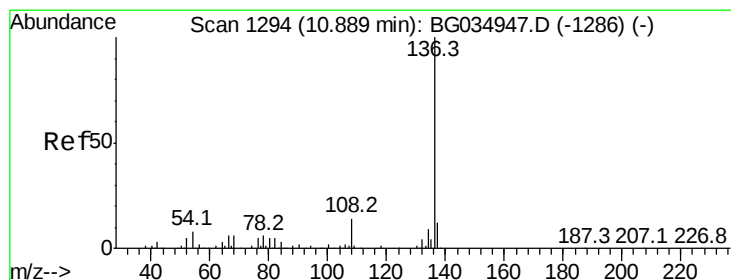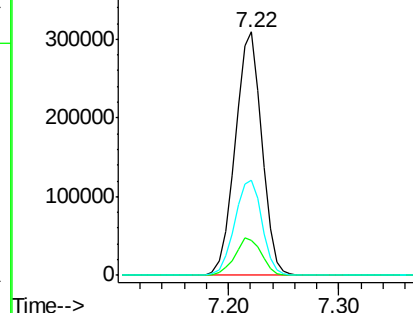

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.86 min Scan# 1289

Delta R.T. -0.02 min

Lab File: BG035217.D

Acq: 18 Jun 2018 13:58

Tgt Ion: 136 Resp: 202629


Ion Ratio Lower Upper

136 100



137 11.1 9.2 13.8


54 6.4 10.3 15.5#

68 5.0 4.5 6.7



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

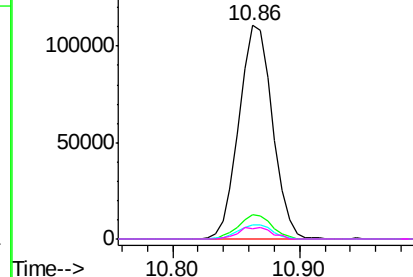



#23

Nitrobenzene-d5

Concen: 101.824 ng

RT: 9.22 min Scan# 1010

Delta R.T. -0.02 min

Lab File: BG035217.D

Acq: 18 Jun 2018 13:58

Instrument :

BNA_G

ClientSampleId :

SB-51COMP


Tot Ion: 82 Resp: 434053

Ion Ratio Lower Upper




82 100

128 37.6 29.7 44.5

54 43.7 43.1 64.7

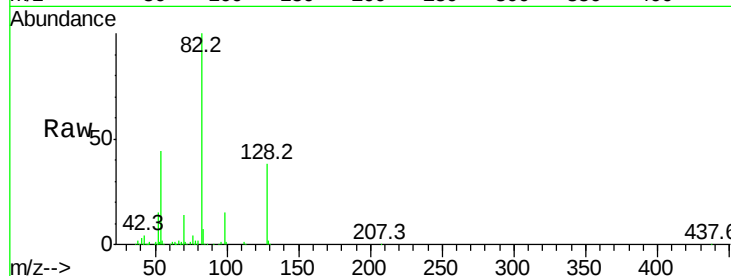

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

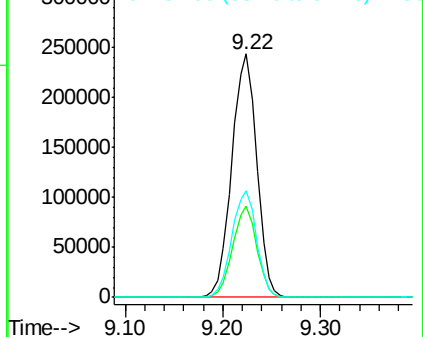

#37

2-Methylnaphthalene

Concen: 2.022 ng

RT: 12.52 min Scan# 1571

Delta R.T. -0.02 min

Lab File: BG035217.D

Acq: 18 Jun 2018 13:58


Tgt Ion: 142 Resp: 16136

Ion Ratio Lower Upper



142 100


141 71.2 67.1 100.7

115 38.1 30.7 46.1



Abundance Ion 142.00 (141.70 to 142.70): BGC
Ion 141.00 (140.70 to 141.70): BGC
Ion 115.00 (114.70 to 115.70): BGC




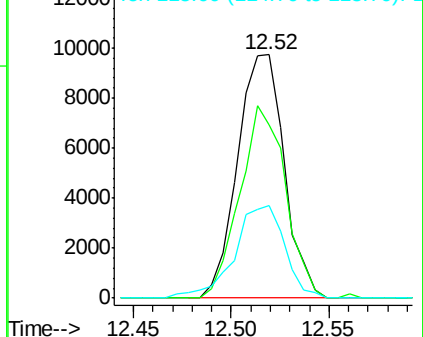


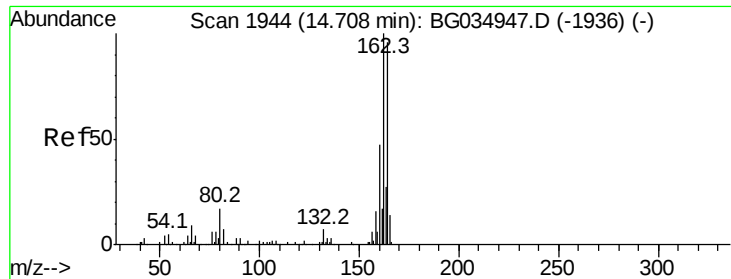

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.68 min Scan# 1939
Delta R.T. -0.02 min
Lab File: BG035217.D
Acq: 18 Jun 2018 13:58




Instrument :
BNA_G
ClientSampleId :
SB-51COMP


Tot Ion	Ratio	Lower	Upper
164	100		
162	99.8	78.8	118.2
160	44.9	35.4	53.0

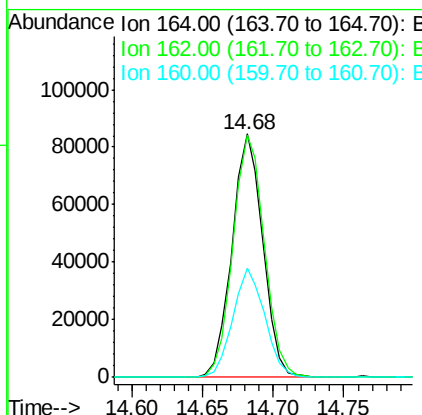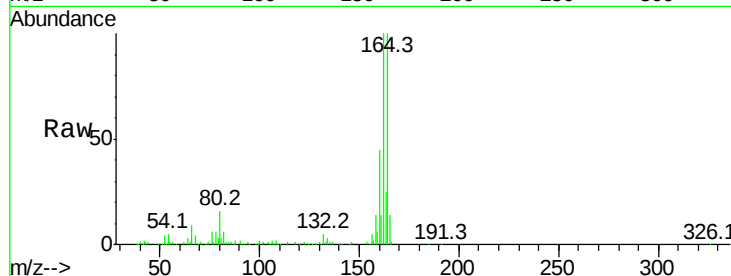

#41
2,4,6-Tribromophenol
Concen: 149.340 ng
RT: 16.17 min Scan# 2192
Delta R.T. -0.02 min
Lab File: BG035217.D
Acq: 18 Jun 2018 13:58

Tgt Ion	Ratio	Lower	Upper
330	100		
332	97.4	77.0	115.6
141	38.5	25.2	37.8#

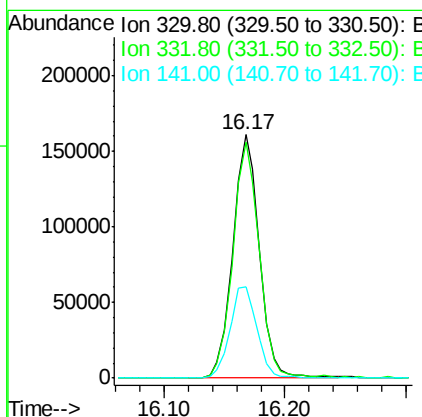







#44
2-Fluorobiphenyl
Concen: 90.457 ng
RT: 13.31 min Scan# 1705
Delta R.T. -0.02 min
Lab File: BG035217.D
Acq: 18 Jun 2018 13:58

Instrument :
BNA_G
ClientSampleId :
SB-51COMP

Tot Ion:172 Resp: 894184
Ion Ratio Lower Upper
172 100
171 35.3 30.0 45.0
170 22.8 19.5 29.3

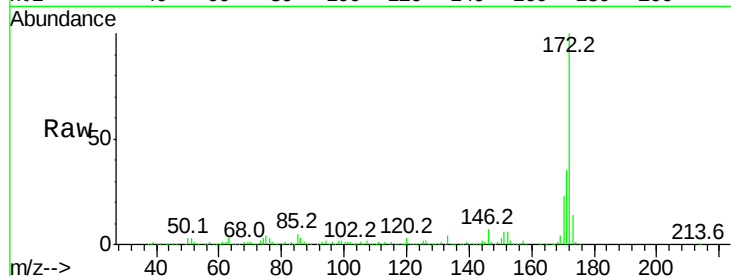


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E


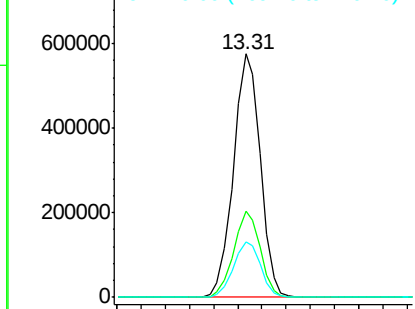



#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.42 min Scan# 2406
Delta R.T. -0.02 min
Lab File: BG035217.D
Acq: 18 Jun 2018 13:58

Tgt Ion:188 Resp: 318891
Ion Ratio Lower Upper
188 100
94 5.8 6.9 10.3#
80 7.5 7.7 11.5#



Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

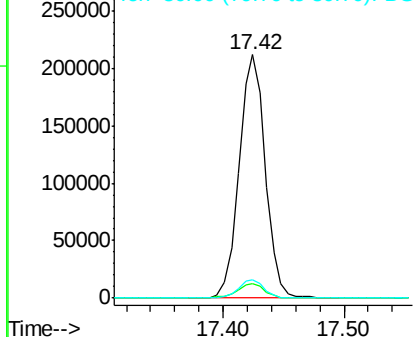



#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.69 min Scan# 3132

Delta R.T. -0.03 min

Lab File: BG035217.D

Acq: 18 Jun 2018 13:58

Instrument :

BNA_G

ClientSampleId :

SB-51COMP


Tot Ion:240 Resp: 446060

Ion Ratio Lower Upper

240 100

120 5.5 6.8 10.2#




236 25.6 20.9 31.3



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

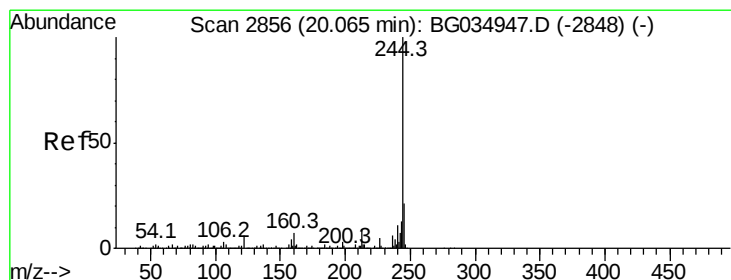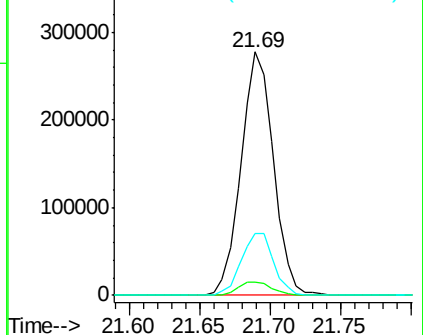

#78

Terphenyl-d14

Concen: 83.459 ng

RT: 20.03 min Scan# 2850

Delta R.T. -0.02 min

Lab File: BG035217.D

Acq: 18 Jun 2018 13:58


Tgt Ion:244 Resp: 1777254

Ion Ratio Lower Upper

244 100

212 9.4 5.8 8.8#



122 7.1 7.0 10.4




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

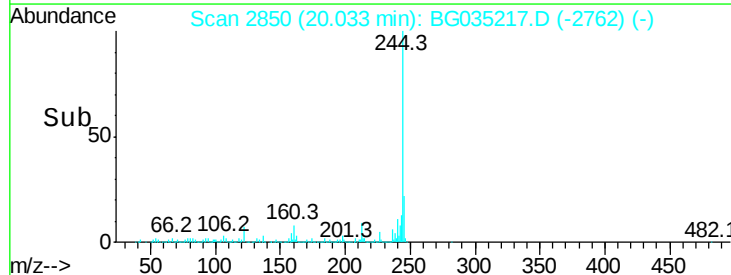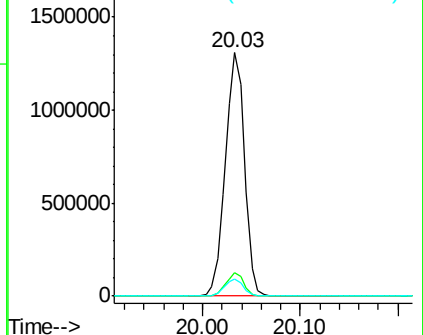


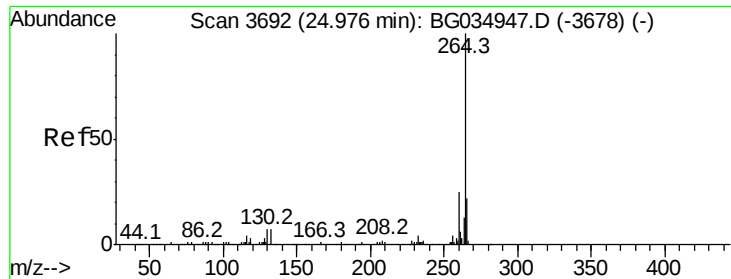

#86
Pervlene-d12
Concen: 20.000 ng
RT: 24.92 min Scan# 3682
Delta R.T. -0.03 min
Lab File: BG035217.D
Acq: 18 Jun 2018 13:58

Instrument :
BNA_G
ClientSampleId :
SB-51COMP

Tot Ion	Ratio	Lower	Upper
264	100		
260	25.3	17.4	26.0
265	20.5	17.7	26.5

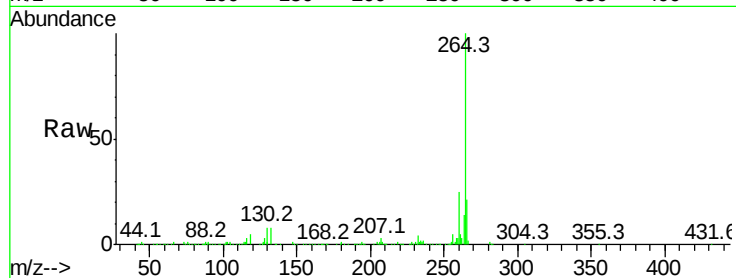

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

