

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061818\
 Data File : BG035246.D
 Acq On : 19 Jun 2018 10:05
 Operator : SJ/JU
 Sample : J3566-16
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TP-6-S

Quant Time: Jun 19 11:59:11 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 08 17:16:28 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	41089	20.00	ng	-0.01
21) Naphthalene-d8	10.86	136	145986	20.00	ng	-0.02
38) Acenaphthene-d10	14.68	164	93438	20.00	ng	-0.01
63) Phenanthrene-d10	17.42	188	324161	20.00	ng	-0.02
75) Chrysene-d12	21.69	240	330031	20.00	ng	-0.03
86) Perylene-d12	24.92	264	84717	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	365310	150.04	ng	0.00
7) Phenol-d6	7.22	99	460906	128.26	ng	0.00
23) Nitrobenzene-d5	9.22	82	371630	121.01	ng	-0.02
41) 2,4,6-Tribromophenol	16.17	330	294136	245.91	ng	-0.01
44) 2-Fluorobiphenyl	13.31	172	802531	111.66	ng	-0.02
78) Terphenyl-d14	20.03	244	2347067	148.97	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061818\
Data File : BG035246.D
Acq On : 19 Jun 2018 10:05
Operator : SJ/JU
Sample : J3566-16
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-6-S

Quant Time: Jun 19 11:59:11 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

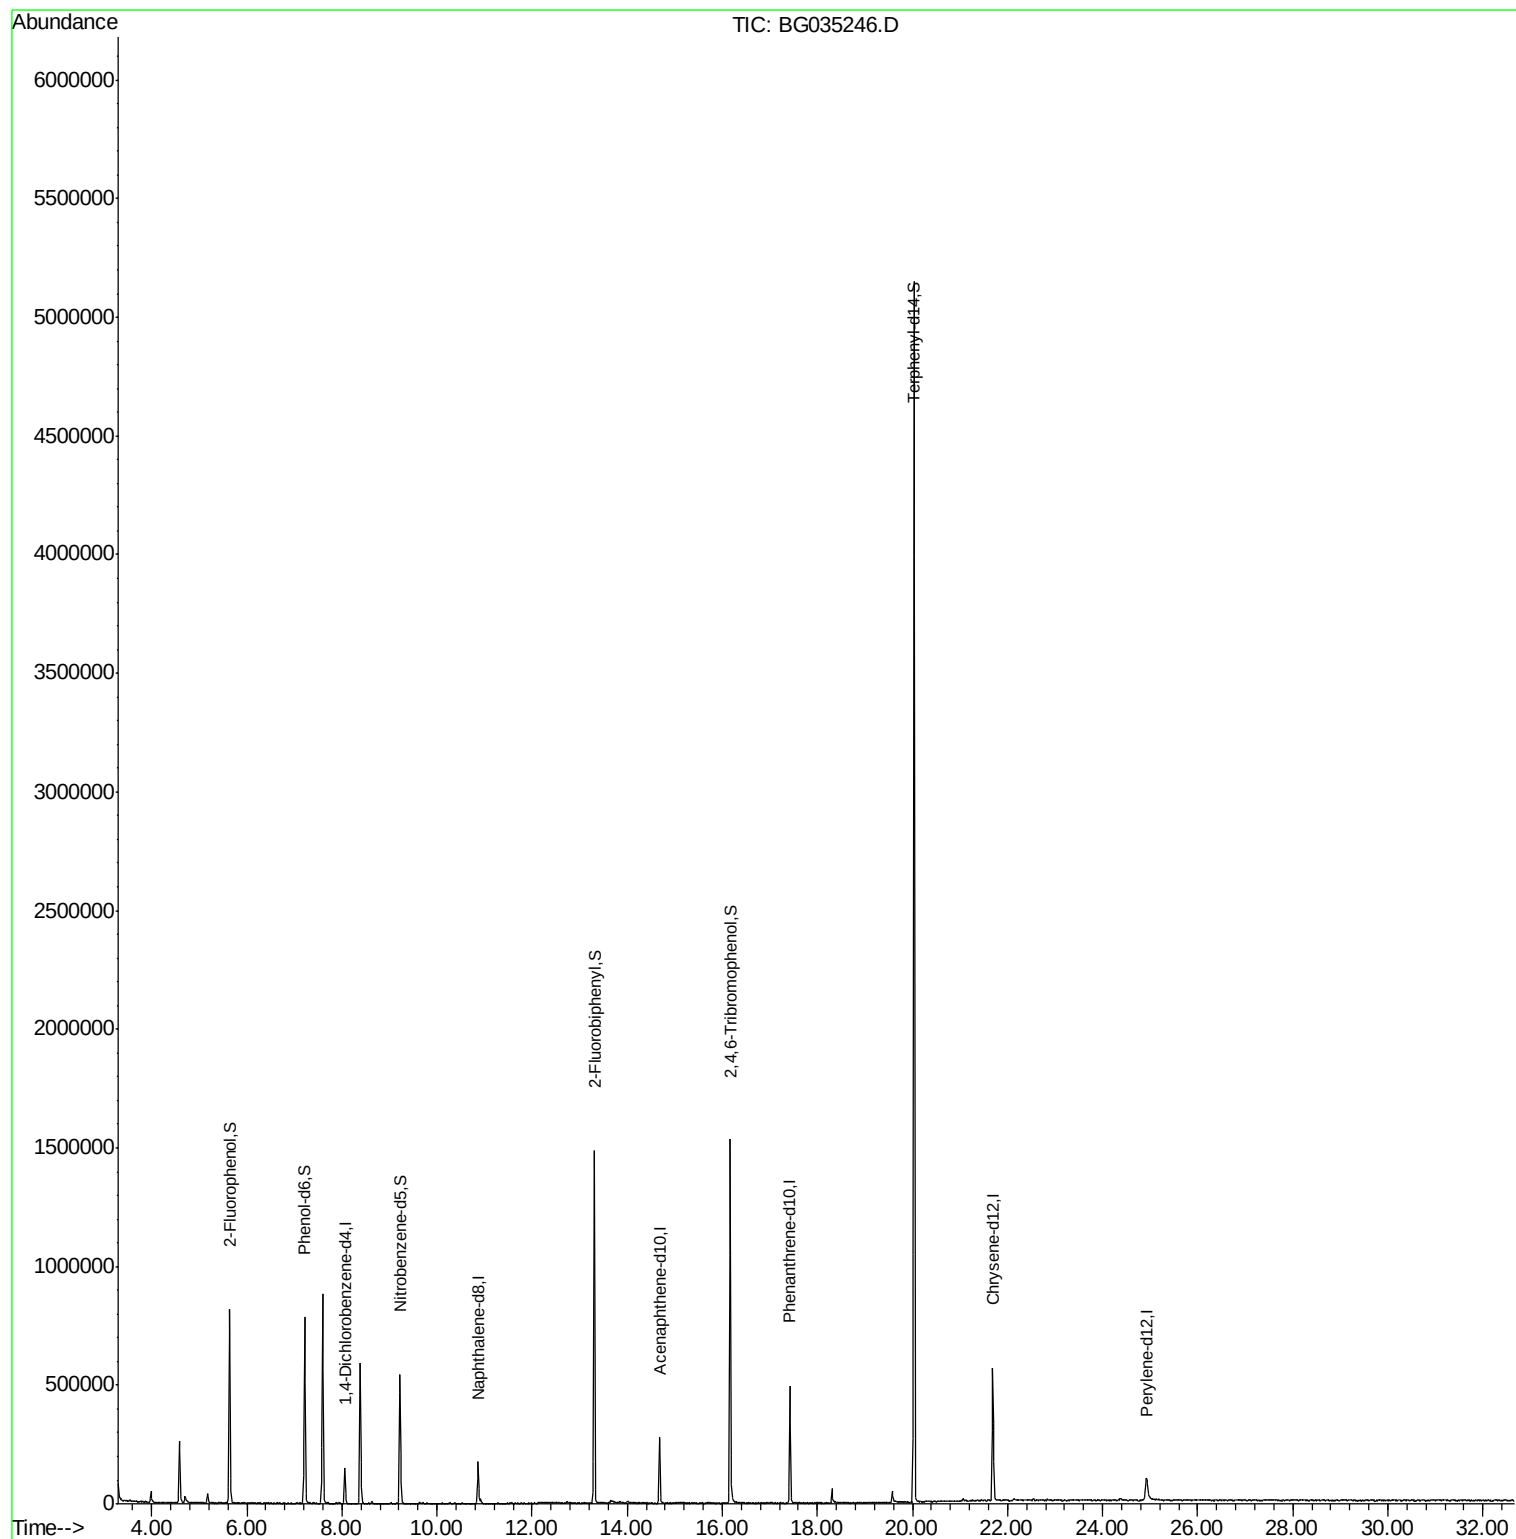

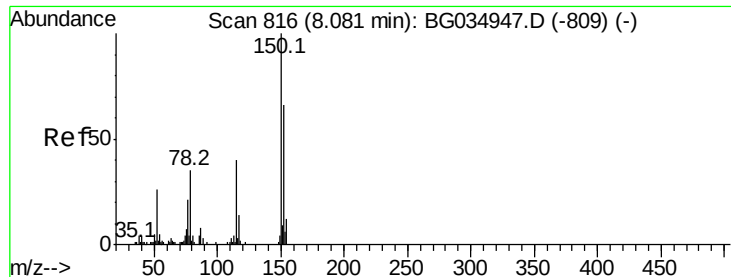


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.06 min Scan# 813
Delta R.T. -0.01 min
Lab File: BG035246.D
Acq: 19 Jun 2018 10:05

Instrument :
BNA_G
ClientSampled :
TP-6-S

Tot Ion:152 Resp: 41089
Ion Ratio Lower Upper
152 100
150 160.2 126.6 189.8
115 67.2 53.0 79.4

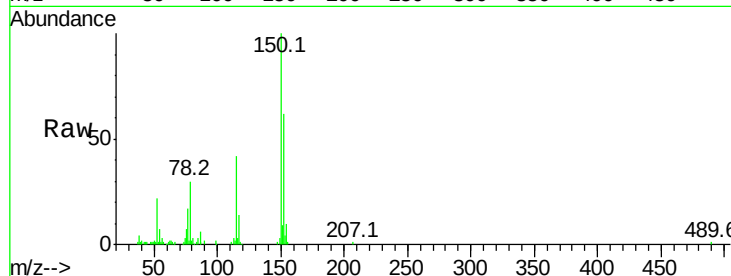


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

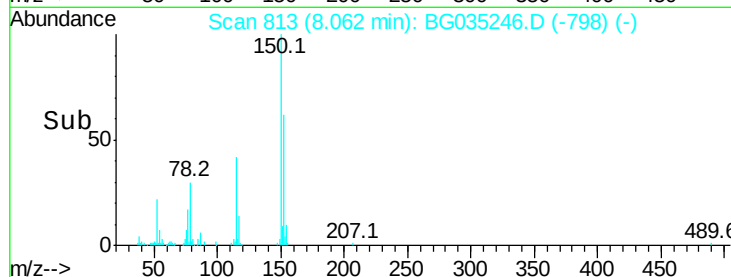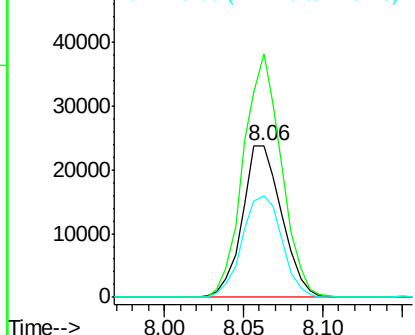



#5


2-Fluorophenol
Concen: 150.040 ng
RT: 5.64 min Scan# 400
Delta R.T. -0.01 min
Lab File: BG035246.D
Acq: 19 Jun 2018 10:05

Tgt Ion:112 Resp: 365310
Ion Ratio Lower Upper
112 100
64 63.1 56.3 84.5
63 35.5 30.1 45.1



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

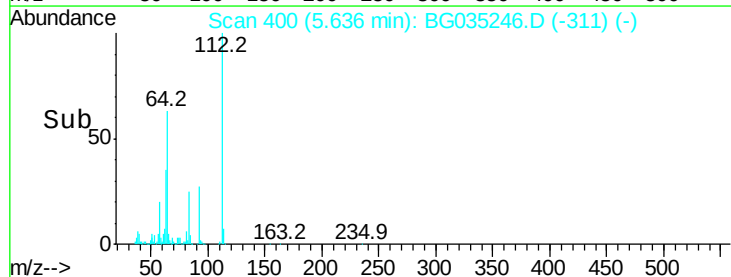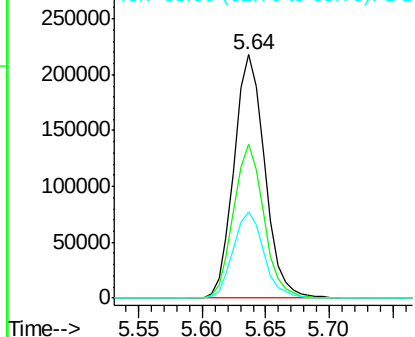

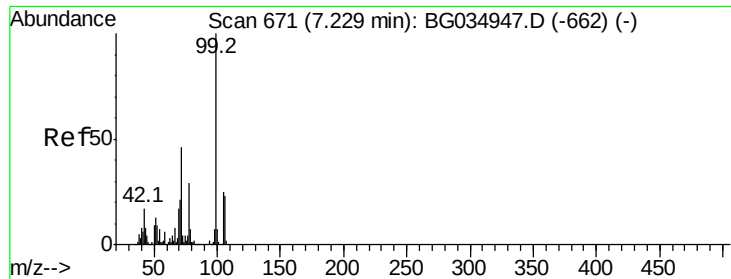

#7

Phenol-d6

Concen: 128.259 ng

RT: 7.22 min Scan# 669

Delta R.T. -0.01 min

Lab File: BG035246.D

Acq: 19 Jun 2018 10:05

Instrument :

BNA_G

ClientSampleId :

TP-6-S





Tot Ion: 99 Resp: 460906

Ion Ratio Lower Upper

99 100

42 16.2 14.1 21.1

71 43.4 26.1 39.1#

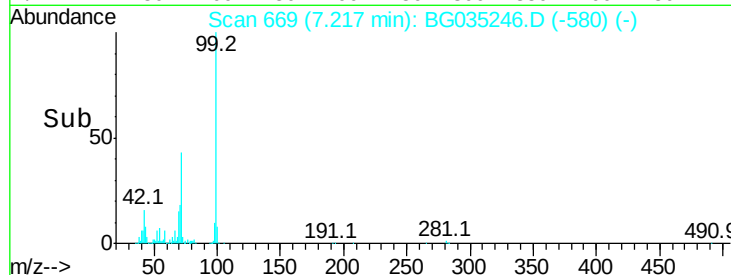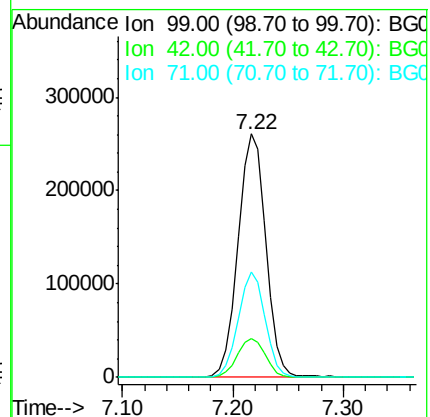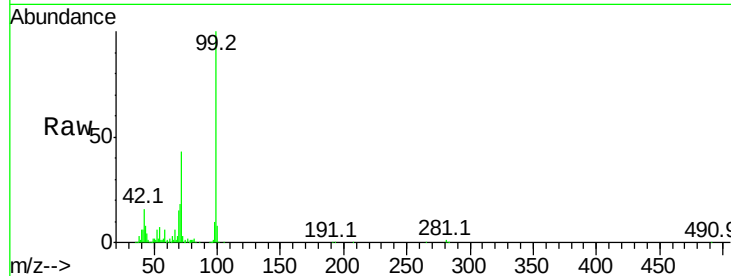

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.86 min Scan# 1290

Delta R.T. -0.02 min

Lab File: BG035246.D

Acq: 19 Jun 2018 10:05

Tgt Ion: 136 Resp: 145986




Ion Ratio Lower Upper


136 100

137 11.9 9.2 13.8

54 7.6 10.3 15.5#

68 5.2 4.5 6.7

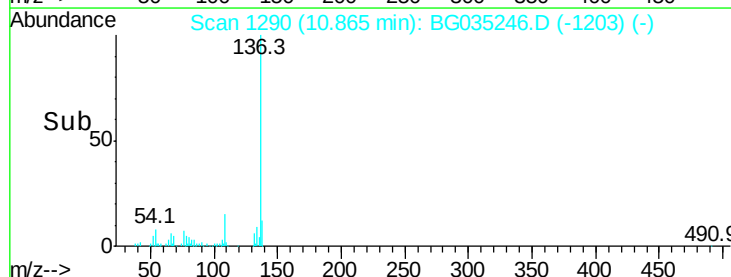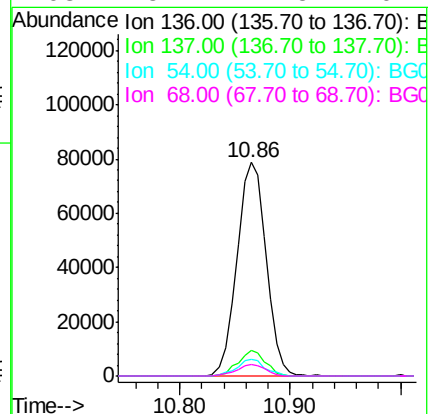

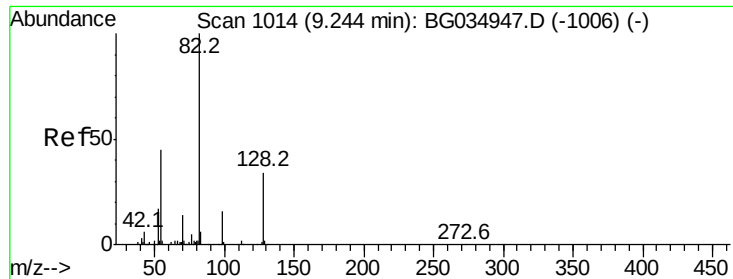

#23

Nitrobenzene-d5

Concen: 121.006 ng

RT: 9.22 min Scan# 1010

Delta R.T. -0.02 min

Lab File: BG035246.D

Acq: 19 Jun 2018 10:05

Instrument :

BNA_G

ClientSampleId :

TP-6-S


Tot Ion: 82 Resp: 371630

Ion Ratio Lower Upper




82 100

128 34.2 29.7 44.5

54 41.5 43.1 64.7#

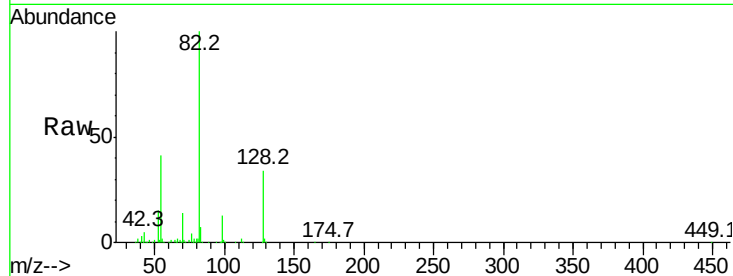

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

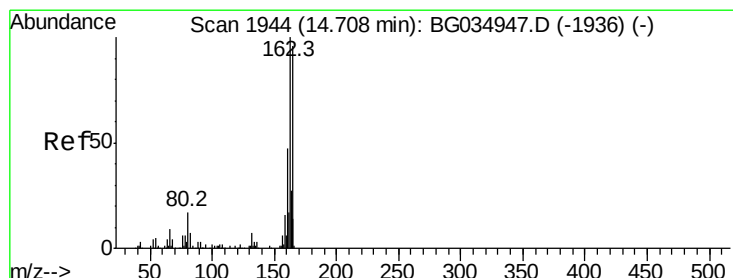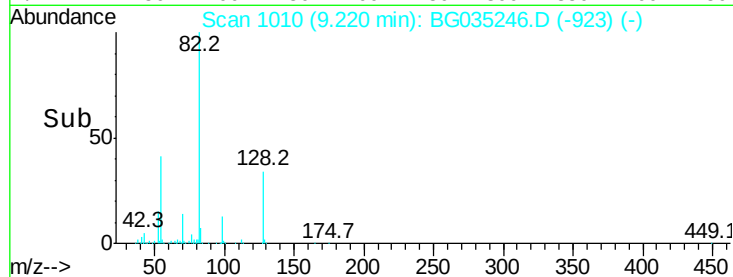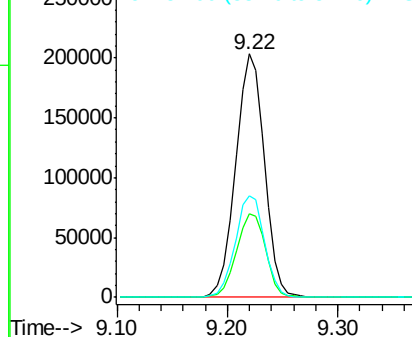

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.68 min Scan# 1940

Delta R.T. -0.01 min

Lab File: BG035246.D

Acq: 19 Jun 2018 10:05


Tgt Ion:164 Resp: 93438

Ion Ratio Lower Upper



164 100


162 107.3 78.8 118.2

160 48.2 35.4 53.0

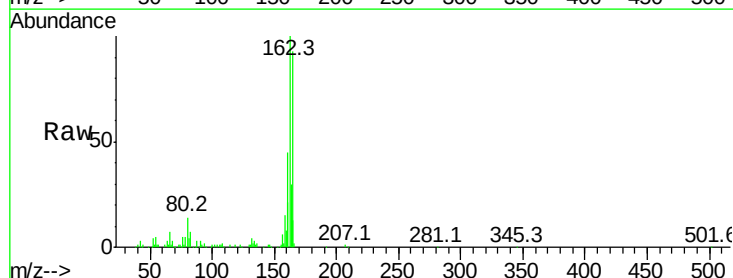

Abundance Ion 164.00 (163.70 to 164.70): BGC
Ion 162.00 (161.70 to 162.70): BGC
Ion 160.00 (159.70 to 160.70): BGC

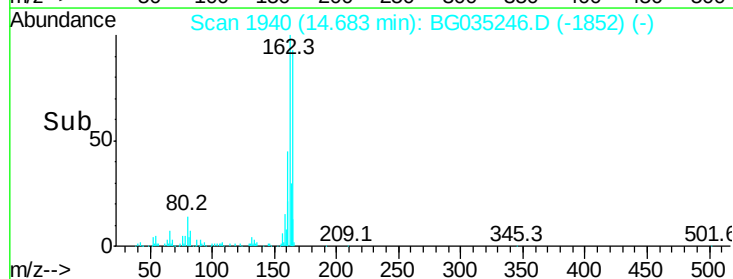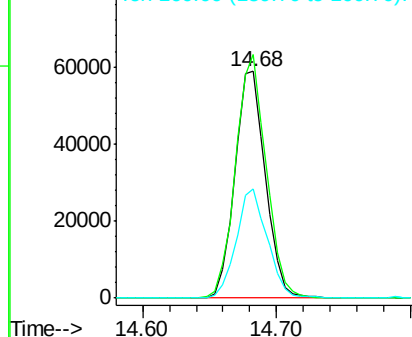


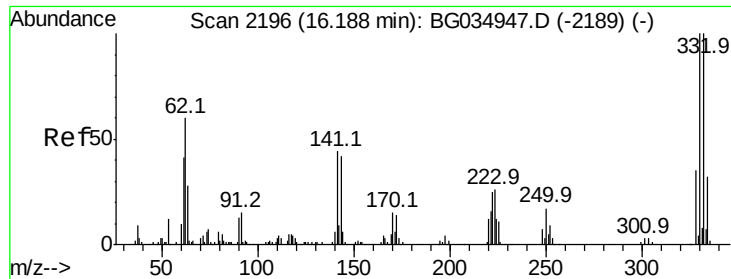




#41
 2,4,6-Tribromophenol
 Concen: 245.907 ng
 RT: 16.17 min Scan# 2193
 Delta R.T. -0.01 min
 Lab File: BG035246.D
 Acq: 19 Jun 2018 10:05

Instrument :
 BNA_G
 ClientSampled :
 TP-6-S

Tot Ion	Ratio	Lower	Upper
330	100		
332	94.6	77.0	115.6
141	37.9	25.2	37.8#




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

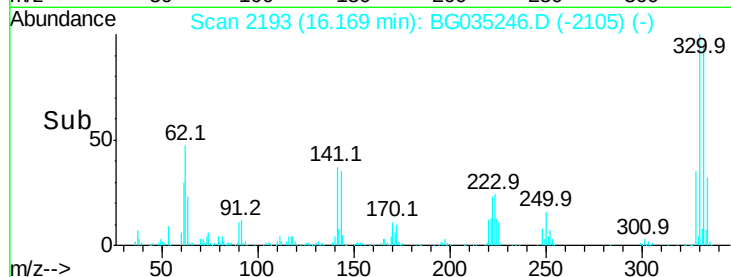
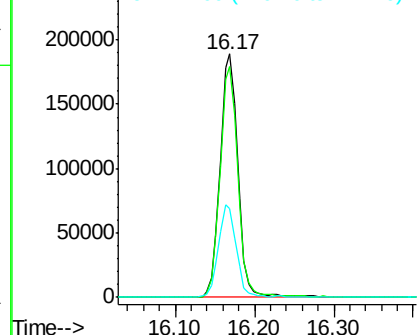



#44
 2-Fluorobiphenyl
 Concen: 111.656 ng
 RT: 13.31 min Scan# 1706
 Delta R.T. -0.02 min
 Lab File: BG035246.D
 Acq: 19 Jun 2018 10:05

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.4	30.0	45.0
170	23.7	19.5	29.3



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

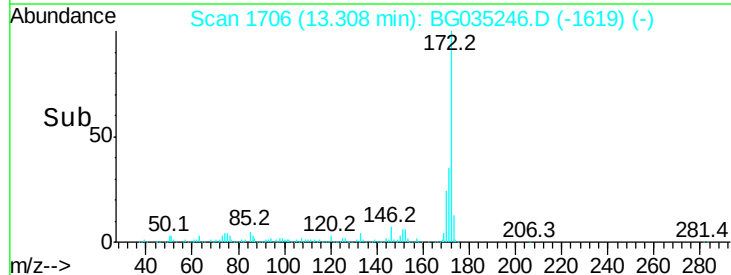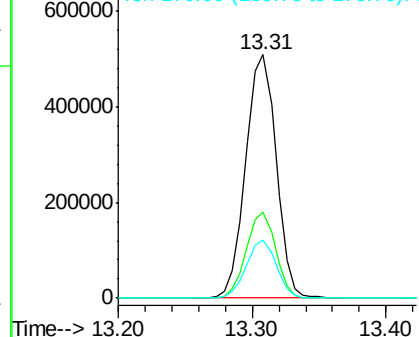

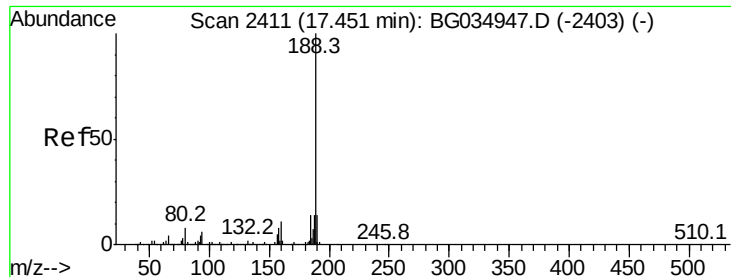

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.42 min Scan# 2406

Delta R.T. -0.02 min

Lab File: BG035246.D

Acq: 19 Jun 2018 10:05

Instrument :

BNA_G

ClientSampled :

TP-6-S


Tot Ion:188 Resp: 324161

Ion Ratio Lower Upper

188 100

94 5.9 6.9 10.3#




80 8.2 7.7 11.5

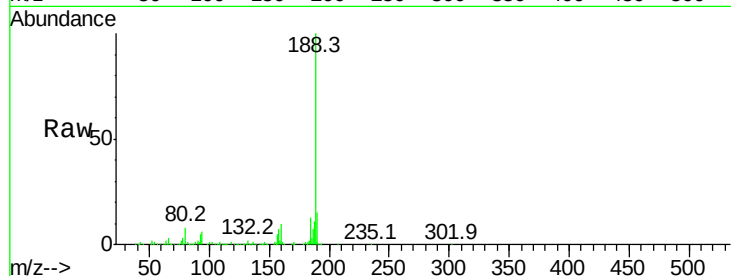

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

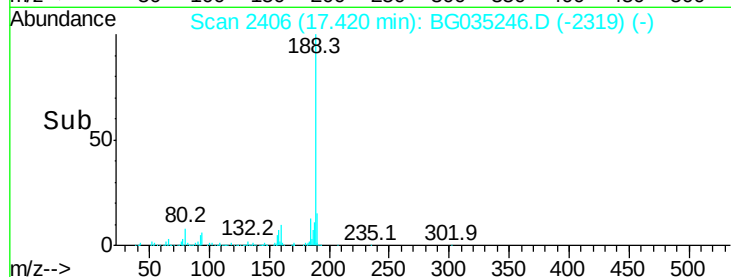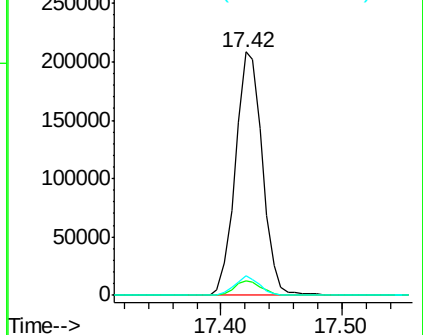

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.69 min Scan# 3133

Delta R.T. -0.03 min

Lab File: BG035246.D

Acq: 19 Jun 2018 10:05


Tgt Ion:240 Resp: 330031

Ion Ratio Lower Upper

240 100

120 5.6 6.8 10.2#



236 25.8 20.9 31.3




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

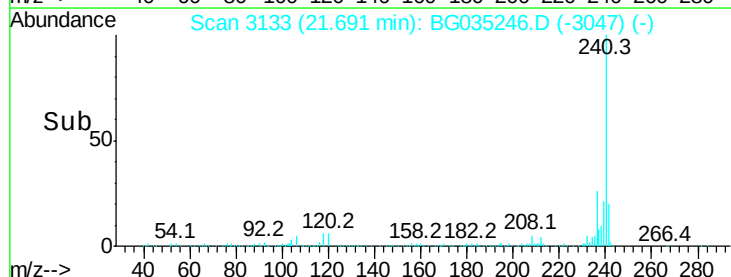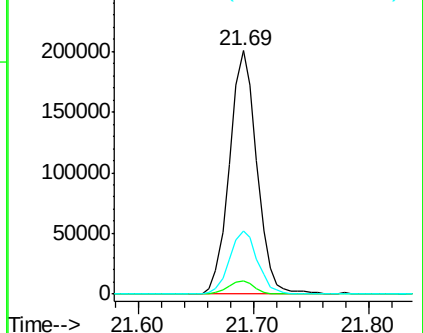

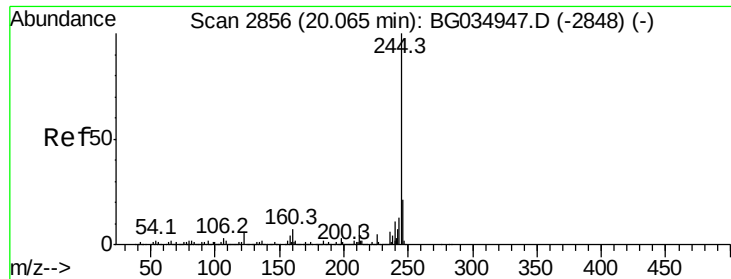

#78

Terphenyl-d14

Concen: 148.966 ng

RT: 20.03 min Scan# 2851

Delta R.T. -0.01 min

Lab File: BG035246.D

Acq: 19 Jun 2018 10:05

Instrument :

BNA_G

ClientSampleId :

TP-6-S


Tot Ion:244 Resp: 2347067

Ion Ratio Lower Upper

244 100

212 10.4 5.8 8.8#




122 7.5 7.0 10.4



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

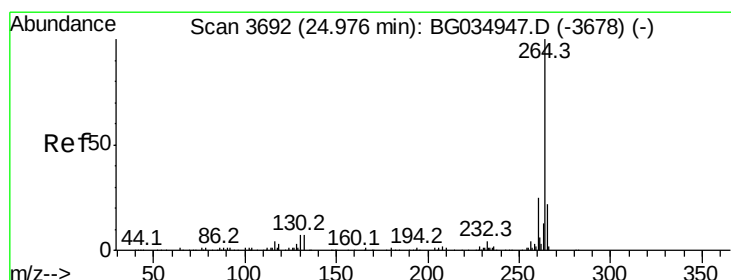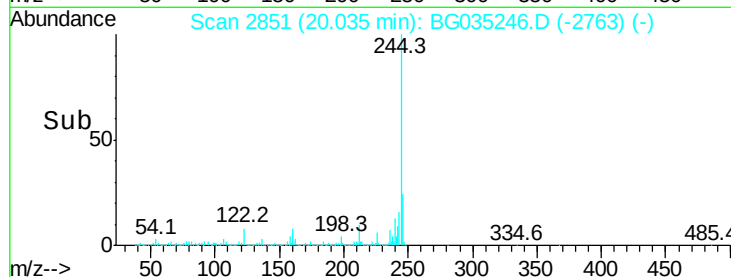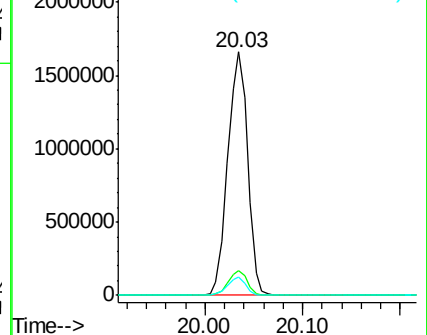

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.92 min Scan# 3683

Delta R.T. -0.03 min

Lab File: BG035246.D

Acq: 19 Jun 2018 10:05


Tgt Ion:264 Resp: 84717

Ion Ratio Lower Upper

264 100

260 30.5 17.4 26.0#

265 20.6 17.7 26.5



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

