


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG061818\
 Data File : BG035211.D
 Acq On : 18 Jun 2018 10:05
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG060718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 08 17:16:28 2018

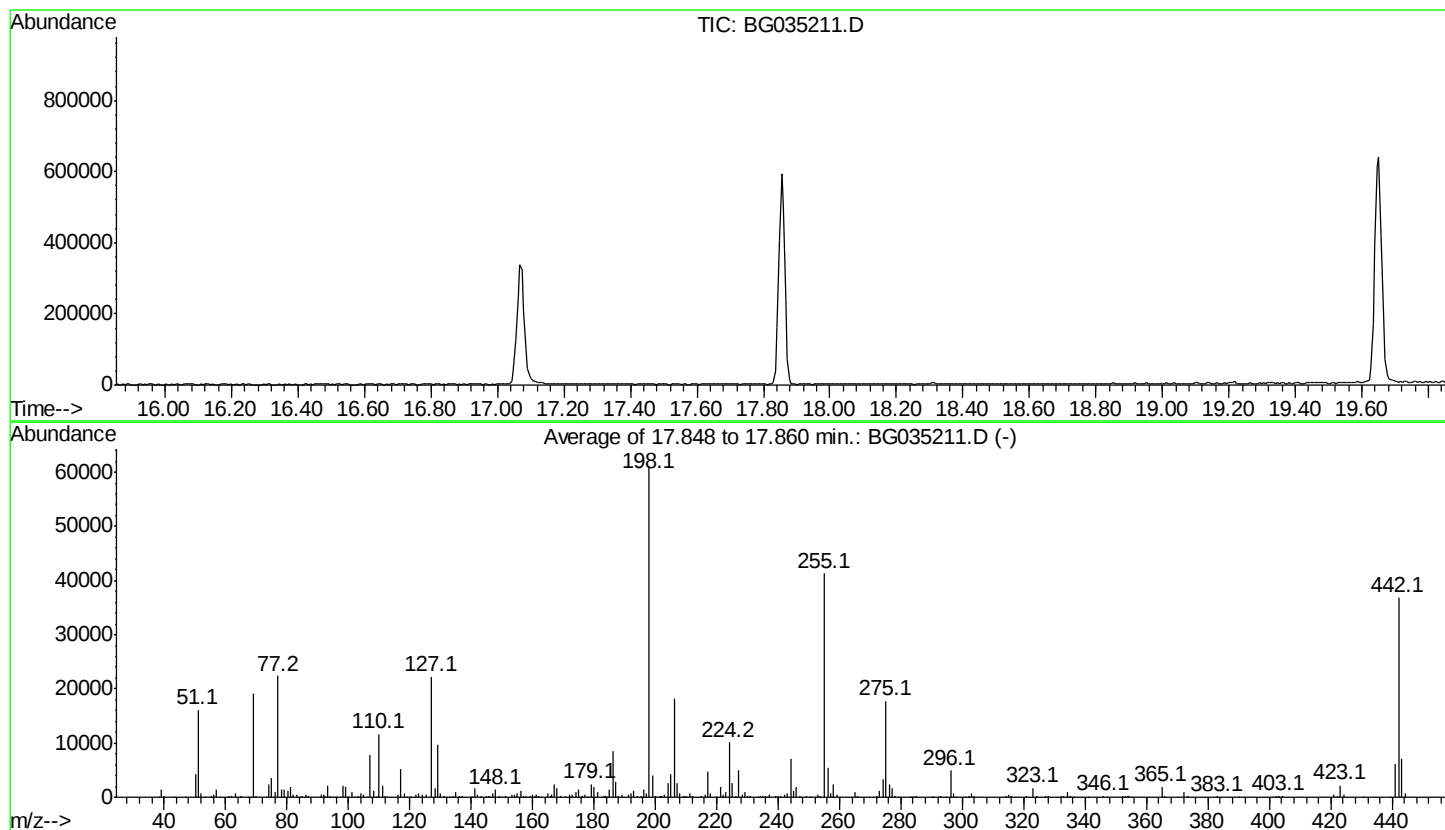

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.4	16133	PASS
68	69	0.00	2	0.6	116	PASS
69	198	0.00	100	31.3	19146	PASS
70	69	0.00	2	0.8	144	PASS
127	198	10	80	36.4	22250	PASS
197	198	0.00	2	1.3	777	PASS
198	198	100	100	100.0	61194	PASS
199	198	5	9	6.4	3947	PASS
275	198	10	60	29.1	17781	PASS
365	198	1	100	3.1	1890	PASS
441	443	0.01	100	85.4	6156	PASS
442	198	50	100	60.1	36778	PASS
443	442	15	24	19.6	7205	PASS