


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG061818\
 Data File : BG035230.D
 Acq On : 18 Jun 2018 23:43
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG060718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 08 17:16:28 2018

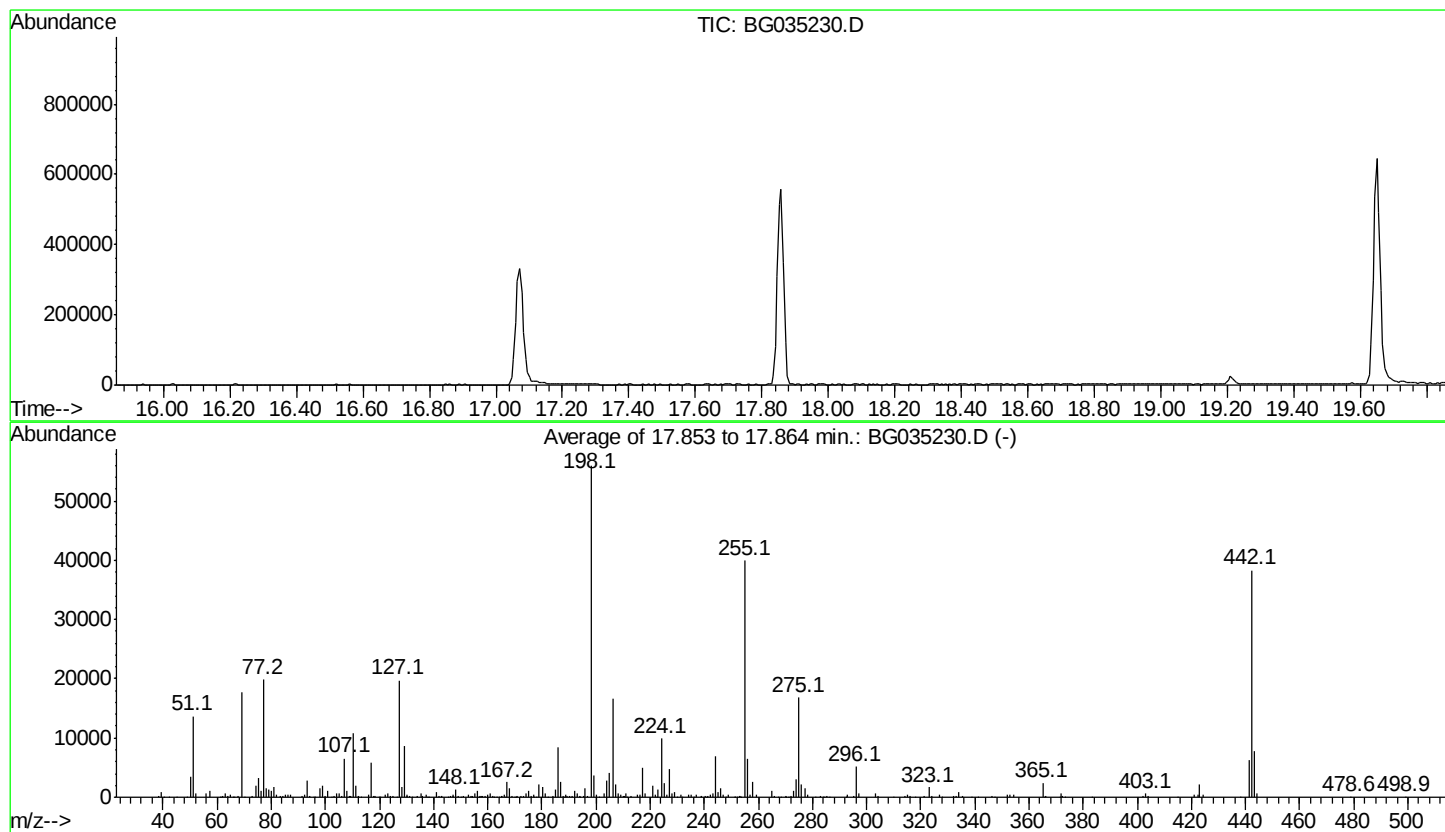

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.5	13714	PASS
68	69	0.00	2	0.8	134	PASS
69	198	0.00	100	31.7	17750	PASS
70	69	0.00	2	0.4	72	PASS
127	198	10	80	35.3	19766	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	55970	PASS
199	198	5	9	6.4	3590	PASS
275	198	10	60	29.9	16755	PASS
365	198	1	100	4.3	2417	PASS
441	443	0.01	100	81.3	6347	PASS
442	198	50	100	68.4	38282	PASS
443	442	15	24	20.4	7811	PASS