

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061819\
 Data File : BG041316.D
 Acq On : 19 Jun 2019 4:13
 Operator : HP/JU
 Sample : K3157-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CL-01-061719-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.167	8	13	23	rVB	649986	1035626	30.81%	6.155%
2	3.473	60	65	73	rBV	74163	98989	2.95%	0.588%
3	4.619	255	260	263	rBV	70718	112870	3.36%	0.671%
4	5.100	338	342	346	rBV2	32787	45181	1.34%	0.269%
5	5.147	346	350	356	rVB	82959	121471	3.61%	0.722%
6	5.617	423	430	444	rBV	671587	1083955	32.25%	6.442%
7	7.127	683	687	695	rVB	40643	62467	1.86%	0.371%
8	7.233	697	705	721	rVB	620320	1083642	32.24%	6.440%
9	7.603	761	768	784	rVB	759260	1322303	39.34%	7.859%
10	8.079	842	849	859	rVB2	126775	223167	6.64%	1.326%
11	8.402	896	904	911	rBV	572019	1003277	29.85%	5.963%
12	9.260	1042	1050	1059	rBV	495942	903347	26.88%	5.369%
13	10.899	1322	1329	1339	rBV	160102	293754	8.74%	1.746%
14	13.338	1736	1744	1757	rBV	1344827	2102497	62.56%	12.496%
15	14.713	1972	1978	1990	rBV2	273740	443297	13.19%	2.635%
16	16.205	2225	2232	2245	rBV	1040984	1676905	49.89%	9.966%
17	17.462	2439	2446	2460	rBV2	375905	575380	17.12%	3.420%
18	20.059	2882	2888	2898	rBV	2636466	3360958	100.00%	19.975%
19	21.740	3167	3174	3183	rBV	390043	654012	19.46%	3.887%
20	25.048	3728	3737	3752	rVB	208138	622810	18.53%	3.701%


Sum of corrected areas: 16825908

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061819\
Data File : BG041316.D
Acq On : 19 Jun 2019 4:13
Operator : HP/JU
Sample : K3157-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CL-01-061719-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

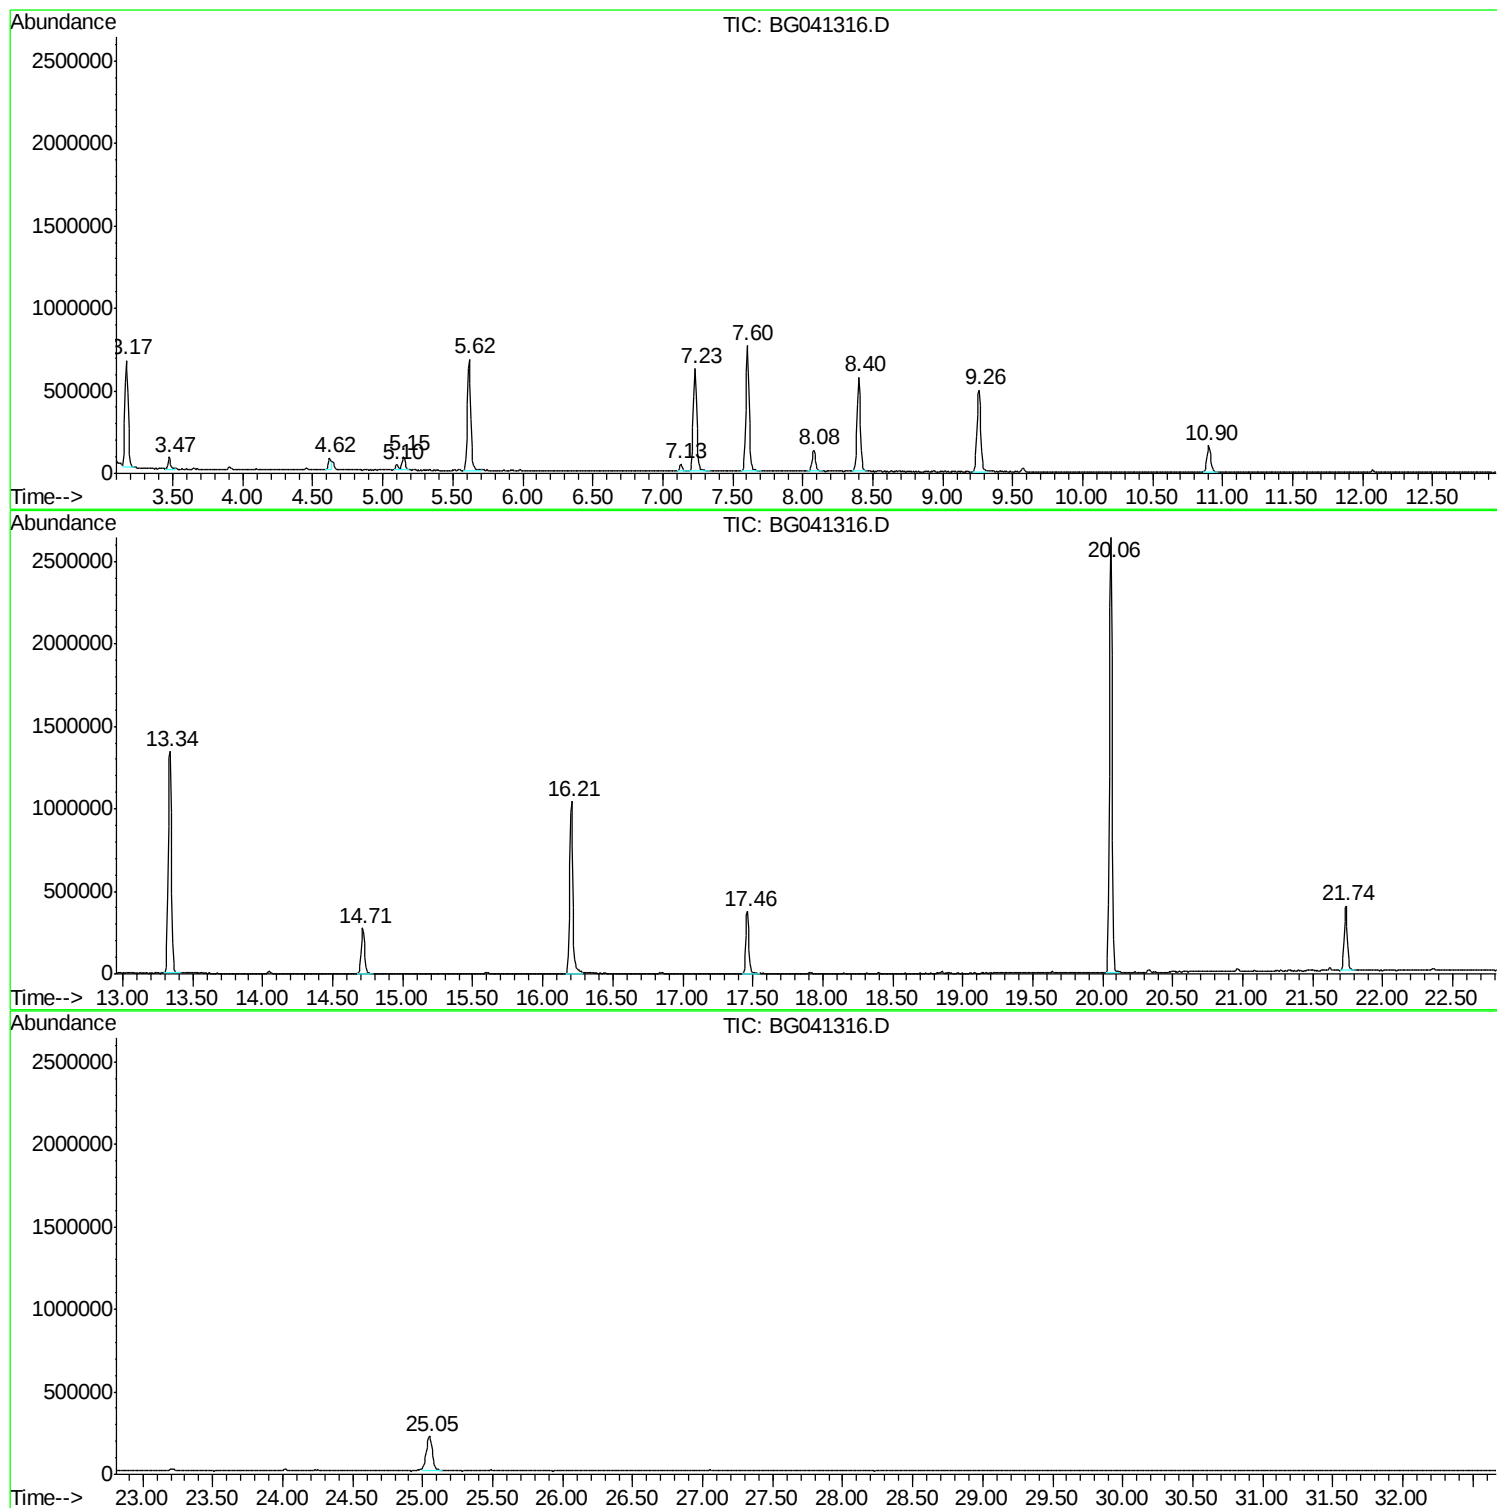

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG061819\
Data_File : BG041316.D
Acq_On : 19 Jun 2019 4:133
Operator : HP/JUU
Sample : K3157-044
Misc :
ALS_Vial : 20 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
CL-01-061719-B

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061719.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\Database\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
