

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061819\
 Data File : BG041317.D
 Acq On : 19 Jun 2019 4:51
 Operator : HP/JU
 Sample : K3157-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CL-01-061719-A

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.172	8	14	24	rVB	588260	984978	26.31%	5.357%
2	3.472	61	65	77	rVB	89849	116321	3.11%	0.633%
3	4.617	256	260	263	rBV	66860	103578	2.77%	0.563%
4	5.105	338	343	346	rBV	38236	54736	1.46%	0.298%
5	5.146	346	350	360	rVB	85773	139014	3.71%	0.756%
6	5.616	424	430	442	rBV	742604	1173250	31.33%	6.381%
7	7.132	683	688	693	rVB	42715	62044	1.66%	0.337%
8	7.232	697	705	719	rBV	669234	1141834	30.50%	6.210%
9	7.608	761	769	784	rVB	866157	1465993	39.15%	7.973%
10	8.078	843	849	860	rBV	144317	249625	6.67%	1.358%
11	8.401	896	904	913	rBV	655059	1128072	30.13%	6.135%
12	9.259	1042	1050	1065	rBV	555182	1022669	27.31%	5.562%
13	10.898	1322	1329	1341	rBV	170968	322130	8.60%	1.752%
14	13.336	1737	1744	1756	rBV	1530003	2322728	62.03%	12.632%
15	14.711	1972	1978	1988	rBV2	288154	478059	12.77%	2.600%
16	16.204	2225	2232	2256	rBV	1204963	1899333	50.73%	10.329%
17	17.461	2436	2446	2454	rBV2	402271	608942	16.26%	3.312%
18	20.058	2882	2888	2896	rBV	3020460	3744231	100.00%	20.363%
19	21.738	3167	3174	3181	rBV	430565	714389	19.08%	3.885%
20	25.046	3728	3737	3749	rVB2	226415	655846	17.52%	3.567%


Sum of corrected areas: 18387772

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061819\
Data File : BG041317.D
Acq On : 19 Jun 2019 4:51
Operator : HP/JU
Sample : K3157-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CL-01-061719-A

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

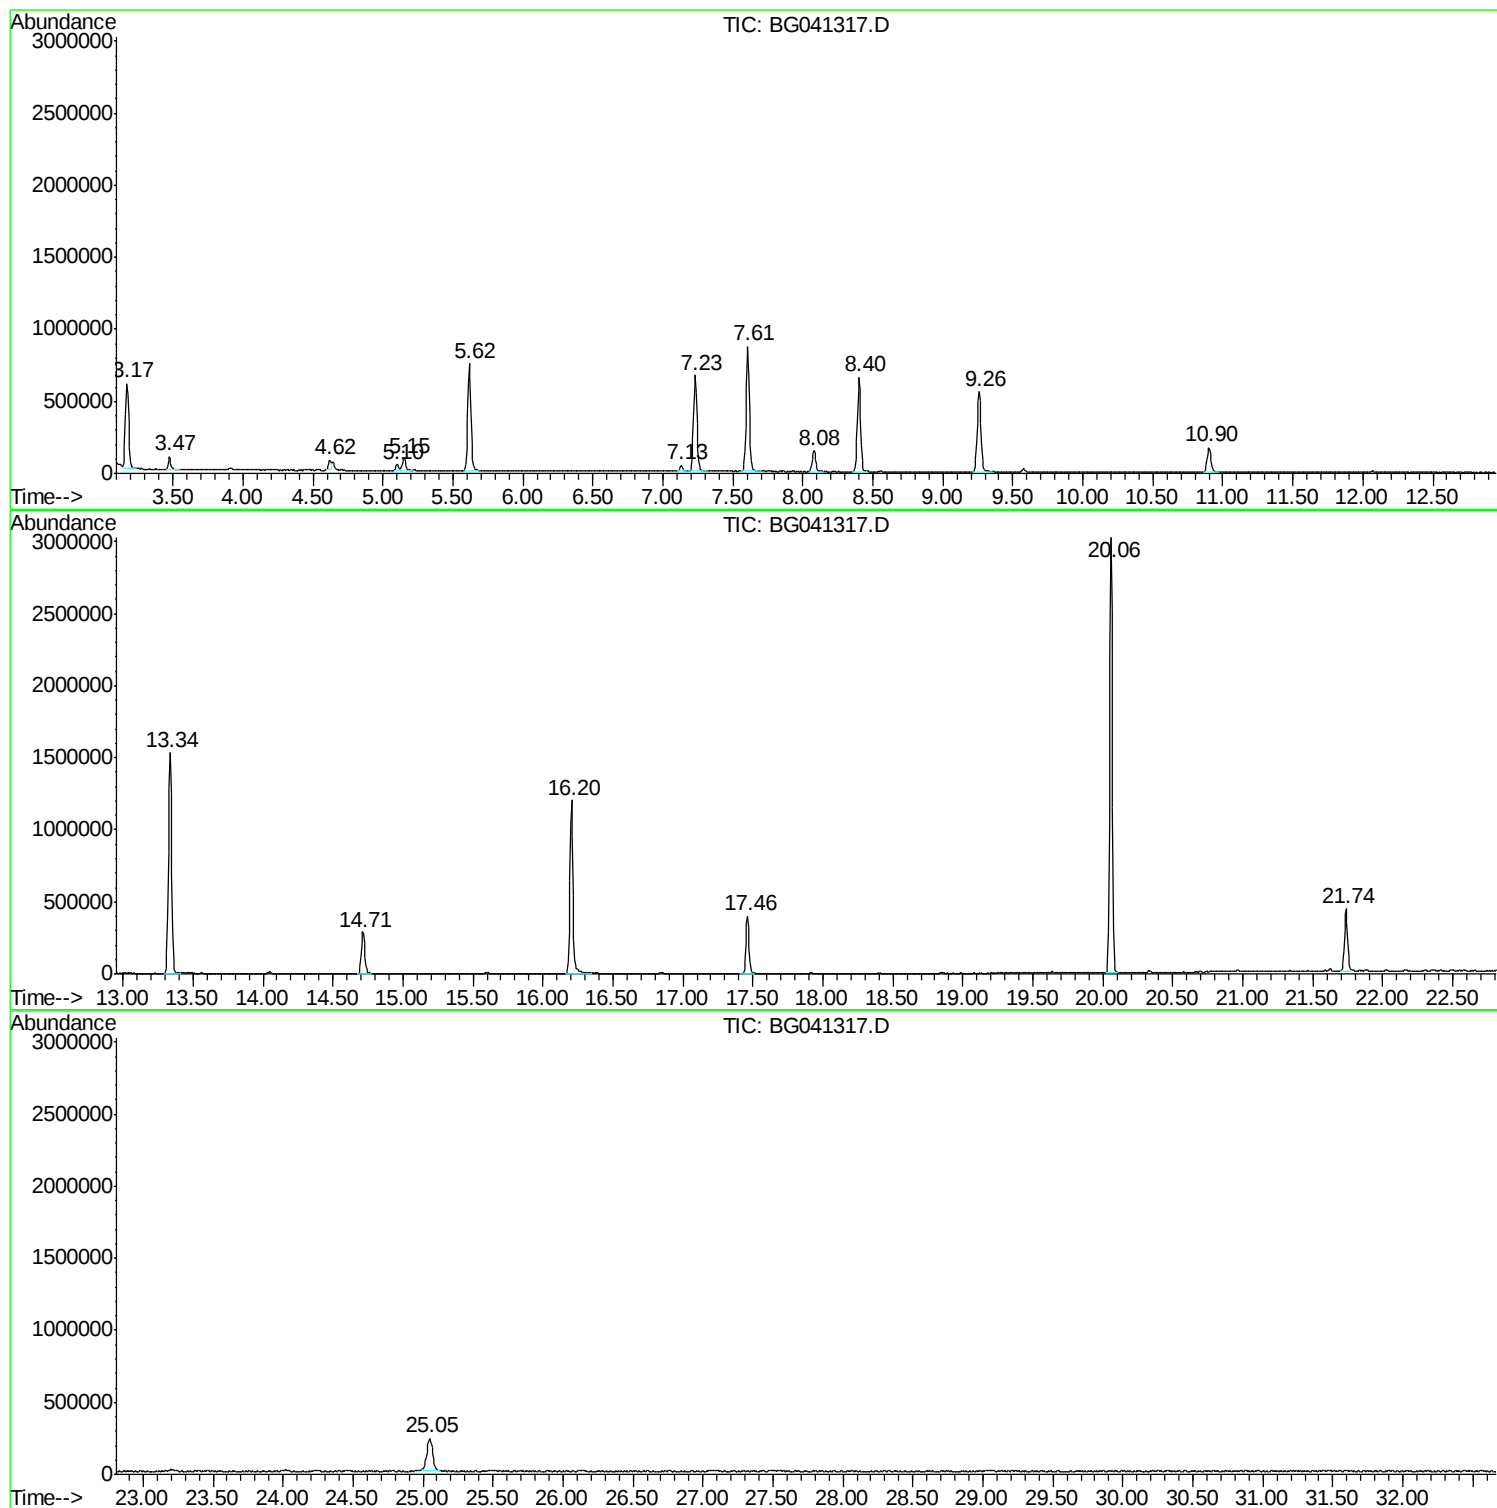

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG061819\
Data_File : BG041317.D
Acq_On : 19 Jun 2019 4:511
Operator : HP/JUU
Sample : K3157-022
Misc :
ALS_Vial : 21 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
CL-01-061719-A

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061719.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\Database\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
