

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061819\  
 Data File : BG041318.D  
 Acq On : 19 Jun 2019 5:29  
 Operator : HP/JU  
 Sample : K3157-06  
 Misc :  
 ALS Vial : 22 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 CL-01-061719-C

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG061719.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 3.172       | 8             | 14          | 27           | rVB      | 595366         | 988162        | 26.52%          | 5.485%        |
| 2         | 3.471       | 61            | 65          | 71           | rBV      | 59352          | 76242         | 2.05%           | 0.423%        |
| 3         | 4.623       | 256           | 261         | 263          | rBV      | 67936          | 104333        | 2.80%           | 0.579%        |
| 4         | 5.099       | 338           | 342         | 346          | rBV      | 38774          | 53379         | 1.43%           | 0.296%        |
| 5         | 5.146       | 346           | 350         | 358          | rVB      | 78217          | 122621        | 3.29%           | 0.681%        |
| 6         | 5.616       | 424           | 430         | 446          | rBV      | 713932         | 1134029       | 30.44%          | 6.295%        |
| 7         | 7.132       | 683           | 688         | 692          | rVB      | 43649          | 59994         | 1.61%           | 0.333%        |
| 8         | 7.232       | 698           | 705         | 713          | rBV      | 664151         | 1128751       | 30.30%          | 6.266%        |
| 9         | 7.608       | 761           | 769         | 778          | rBV      | 816538         | 1397558       | 37.51%          | 7.758%        |
| 10        | 8.078       | 842           | 849         | 859          | rBV      | 138698         | 241770        | 6.49%           | 1.342%        |
| 11        | 8.401       | 897           | 904         | 913          | rBV      | 631075         | 1059023       | 28.43%          | 5.879%        |
| 12        | 9.259       | 1042          | 1050        | 1062         | rBV      | 541139         | 988634        | 26.54%          | 5.488%        |
| 13        | 10.898      | 1323          | 1329        | 1339         | rBV      | 165190         | 309576        | 8.31%           | 1.718%        |
| 14        | 13.336      | 1737          | 1744        | 1758         | rBV      | 1504933        | 2265378       | 60.81%          | 12.575%       |
| 15        | 14.711      | 1971          | 1978        | 1993         | rVB2     | 288512         | 478734        | 12.85%          | 2.657%        |
| 16        | 15.510      | 2109          | 2114        | 2120         | rVB      | 36785          | 52852         | 1.42%           | 0.293%        |
| 17        | 16.204      | 2224          | 2232        | 2250         | rBV      | 1162422        | 1866552       | 50.10%          | 10.361%       |
| 18        | 17.461      | 2437          | 2446        | 2456         | rBV2     | 403159         | 616968        | 16.56%          | 3.425%        |
| 19        | 20.058      | 2882          | 2888        | 2897         | rBV      | 2900287        | 3725594       | 100.00%         | 20.681%       |
| 20        | 21.732      | 3166          | 3173        | 3181         | rBV2     | 414284         | 711889        | 19.11%          | 3.952%        |
| 21        | 25.046      | 3728          | 3737        | 3747         | rVB2     | 222434         | 632494        | 16.98%          | 3.511%        |


Sum of corrected areas: 18014533

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061819\  
Data File : BG041318.D  
Acq On : 19 Jun 2019 5:29  
Operator : HP/JU  
Sample : K3157-06  
Misc :  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
CL-01-061719-C

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061719.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L  
TIC Integration Parameters: LSCINT.P

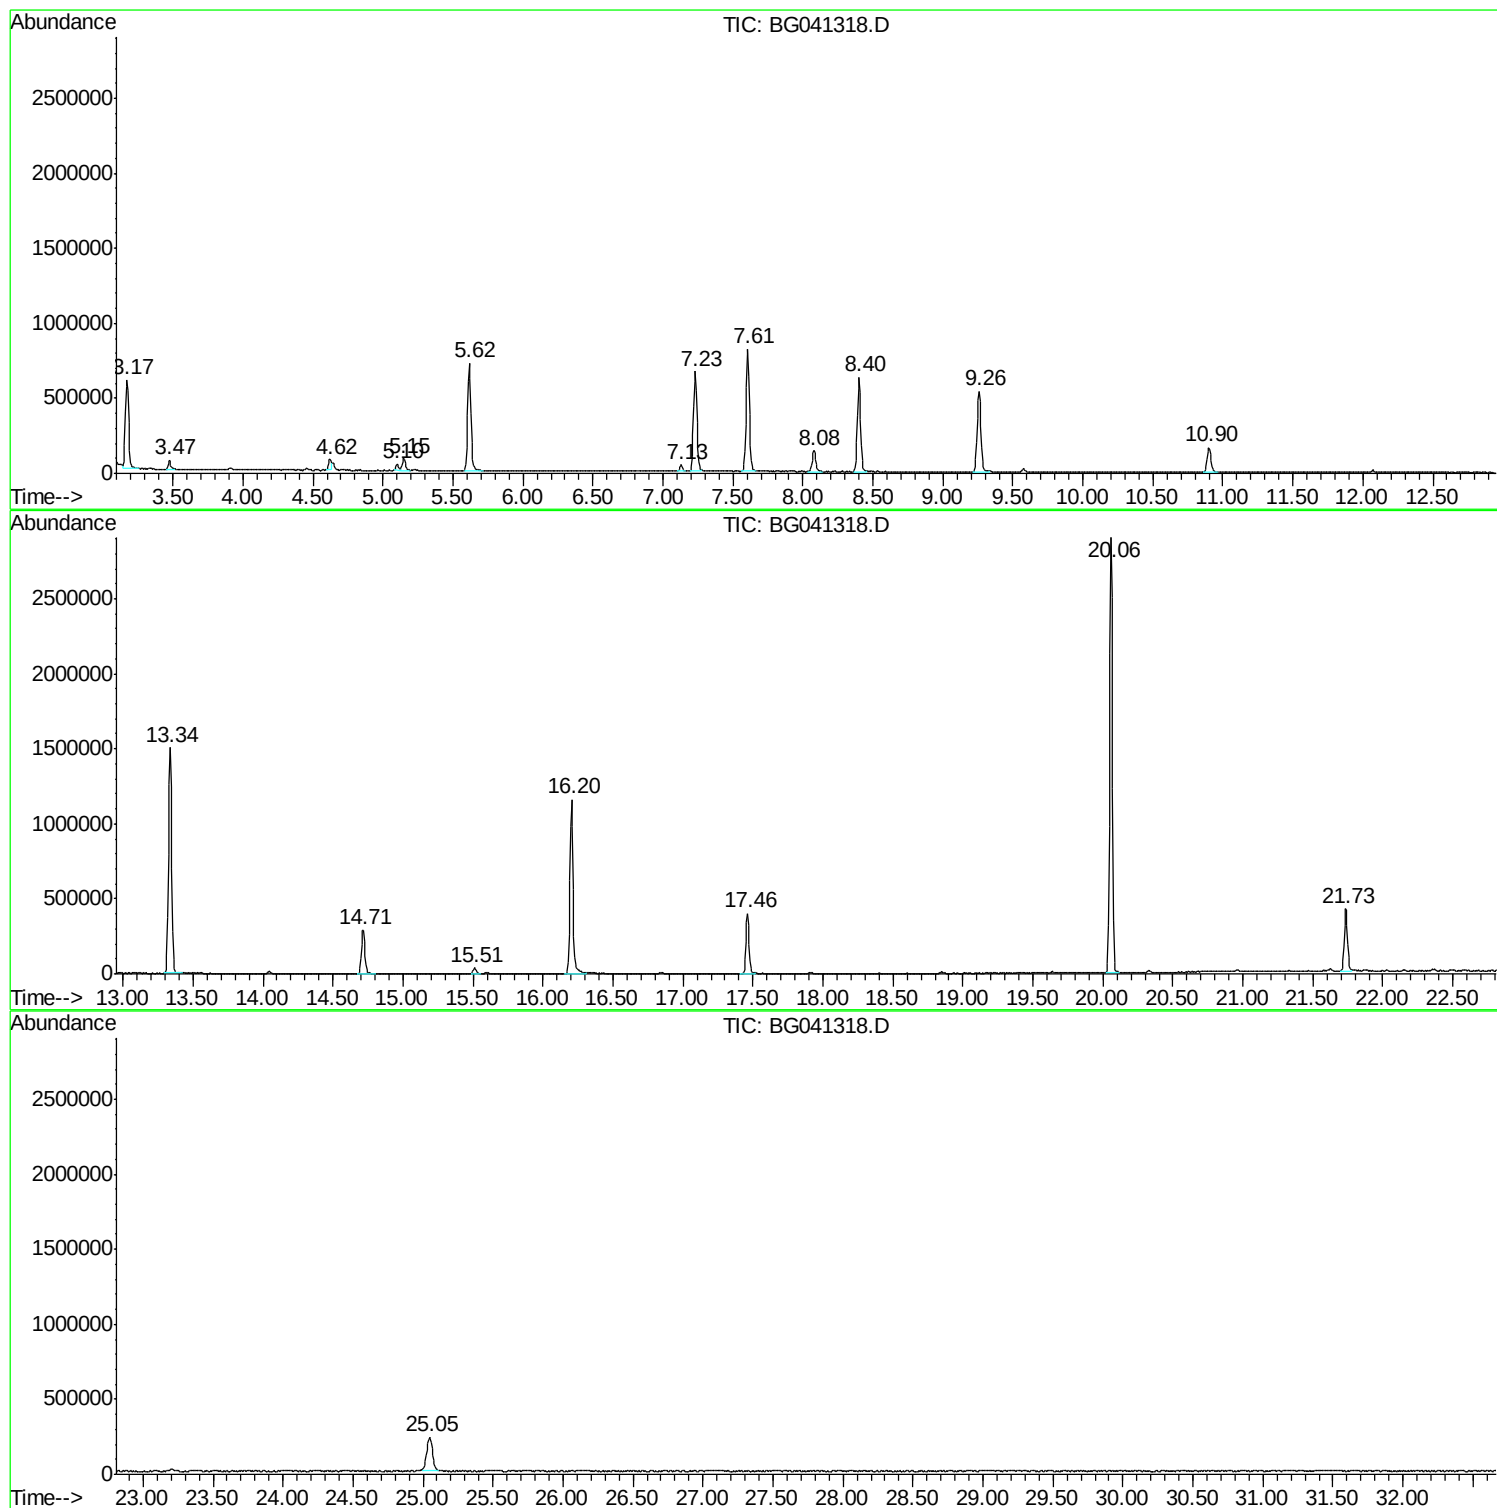

Data\_Path : Z:\SVOASRV\HPCHEM1\BNA\_G\DATA\BG061819\  
Data\_File : BG041318.D  
Acq\_On : 19 Jun 2019 5:299  
Operator : HP/JUU  
Sample : K3157-066  
Misc :  
ALS\_Vial : 22 Sample\_Multiplier: 11

Instrument :  
BNA\_G  
ClientSampleId :  
CL-01-061719-C

Quant\_Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG061719.MM  
Quant\_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC\_Library : C:\Database\NIST11.LL  
TIC\_Integration Parameters: LSCINT.PP

| TIC Top Hit name | RT | EstConc | Units | Response | Internal Standard |
|------------------|----|---------|-------|----------|-------------------|
|                  |    |         |       | #        | RT Resp Conc      |

No Library Search Compounds Detected

\*\*\*\*\*