

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061819\
 Data File : BG041319.D
 Acq On : 19 Jun 2019 6:07
 Operator : HP/JU
 Sample : K3417-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CONTROL-HOUSE-BRICKS

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.152	7	11	21	rVB	178307	257963	1.62%	0.536%
2	5.614	424	430	443	rBV	627805	1030854	6.48%	2.142%
3	7.229	697	705	719	rBV	709923	1224630	7.70%	2.545%
4	7.606	762	769	781	rBV	666215	1144362	7.19%	2.378%
5	8.076	843	849	861	rVB	145014	258672	1.63%	0.538%
6	8.399	897	904	912	rBV	475723	836062	5.25%	1.737%
7	9.257	1042	1050	1062	rBV	407012	765182	4.81%	1.590%
8	10.232	1205	1216	1224	rBV2	106586	272271	1.71%	0.566%
9	10.902	1323	1330	1339	rVB	186380	340840	2.14%	0.708%
10	11.701	1456	1466	1475	rBV	138213	311677	1.96%	0.648%
11	12.676	1626	1632	1647	rBV	61499	168304	1.06%	0.350%
12	13.334	1736	1744	1756	rBV	1139951	1727971	10.86%	3.591%
13	14.157	1879	1884	1892	rVB	110021	160974	1.01%	0.335%
14	14.715	1972	1979	1989	rBV2	319682	528681	3.32%	1.099%
15	16.201	2223	2232	2245	rBV	1022753	1528882	9.61%	3.177%
16	16.830	2333	2339	2355	rBV	225203	355632	2.23%	0.739%
17	17.100	2380	2385	2393	rBV	189048	311813	1.96%	0.648%
18	17.459	2440	2446	2451	rBV2	438782	671134	4.22%	1.395%
19	18.375	2587	2602	2624	rBV	5739237	15912796	100.00%	33.069%
20	18.986	2702	2706	2712	rBV2	145190	207765	1.31%	0.432%
21	19.480	2785	2790	2801	rBV2	913006	1965527	12.35%	4.085%
22	19.627	2803	2815	2825	rBV	5476664	11047119	69.42%	22.958%
23	19.815	2843	2847	2853	rBV	196361	250758	1.58%	0.521%
24	20.061	2883	2889	2900	rVB	2055727	2662488	16.73%	5.533%
25	20.584	2974	2978	2986	rVB2	188025	279922	1.76%	0.582%
26	20.661	2987	2991	2997	rBV	454114	668738	4.20%	1.390%
27	21.336	3102	3106	3123	rVB3	190054	422031	2.65%	0.877%
28	21.477	3126	3130	3140	rVB8	109891	255847	1.61%	0.532%
29	21.736	3166	3174	3181	rBV2	486497	957011	6.01%	1.989%
30	22.141	3239	3243	3251	rVB	148124	254248	1.60%	0.528%
31	23.516	3471	3477	3483	rVB6	87520	174677	1.10%	0.363%
32	25.050	3730	3738	3752	rVB3	249900	787771	4.95%	1.637%
33	26.953	4053	4062	4079	rVB	105070	376707	2.37%	0.783%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061819\
Data File : BG041319.D
Acq On : 19 Jun 2019 6:07
Operator : HP/JU
Sample : K3417-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CONTROL-HOUSE-BRICKS

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061719.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION


Sum of corrected areas: 48119309

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061819\
Data File : BG041319.D
Acq On : 19 Jun 2019 6:07
Operator : HP/JU
Sample : K3417-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CONTROL-HOUSE-BRICKS

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

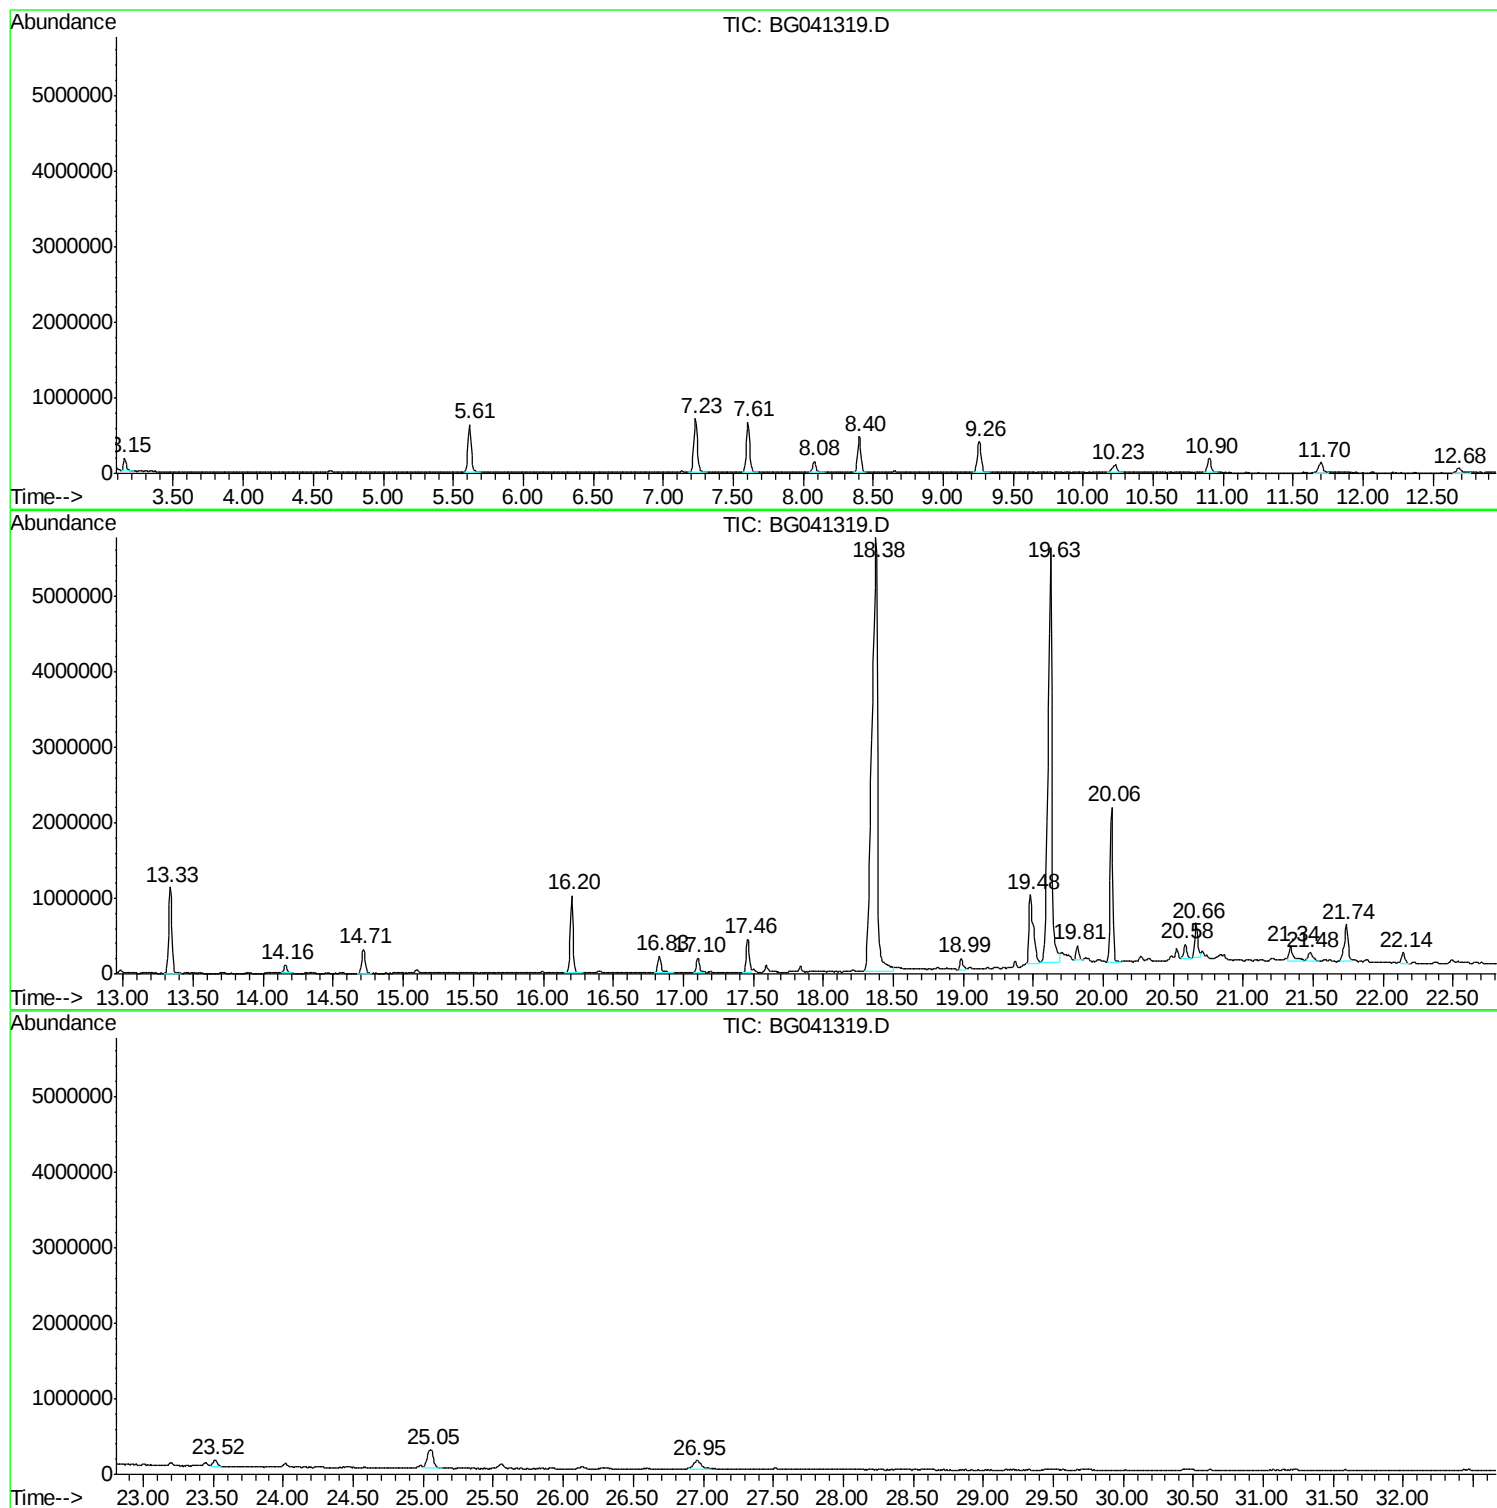

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG061819\
Data_File : BG041319.D
Acq_On : 19 Jun 2019 6:077
Operator : HP/JUU
Sample : K3417-011
Misc :
ALS_Vial : 23 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
CONTROL-HOUSE-BRICKS

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061719.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\Database\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
