


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG061819\
 Data File : BG041295.D
 Acq On : 18 Jun 2019 13:03
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 17 14:58:02 2019

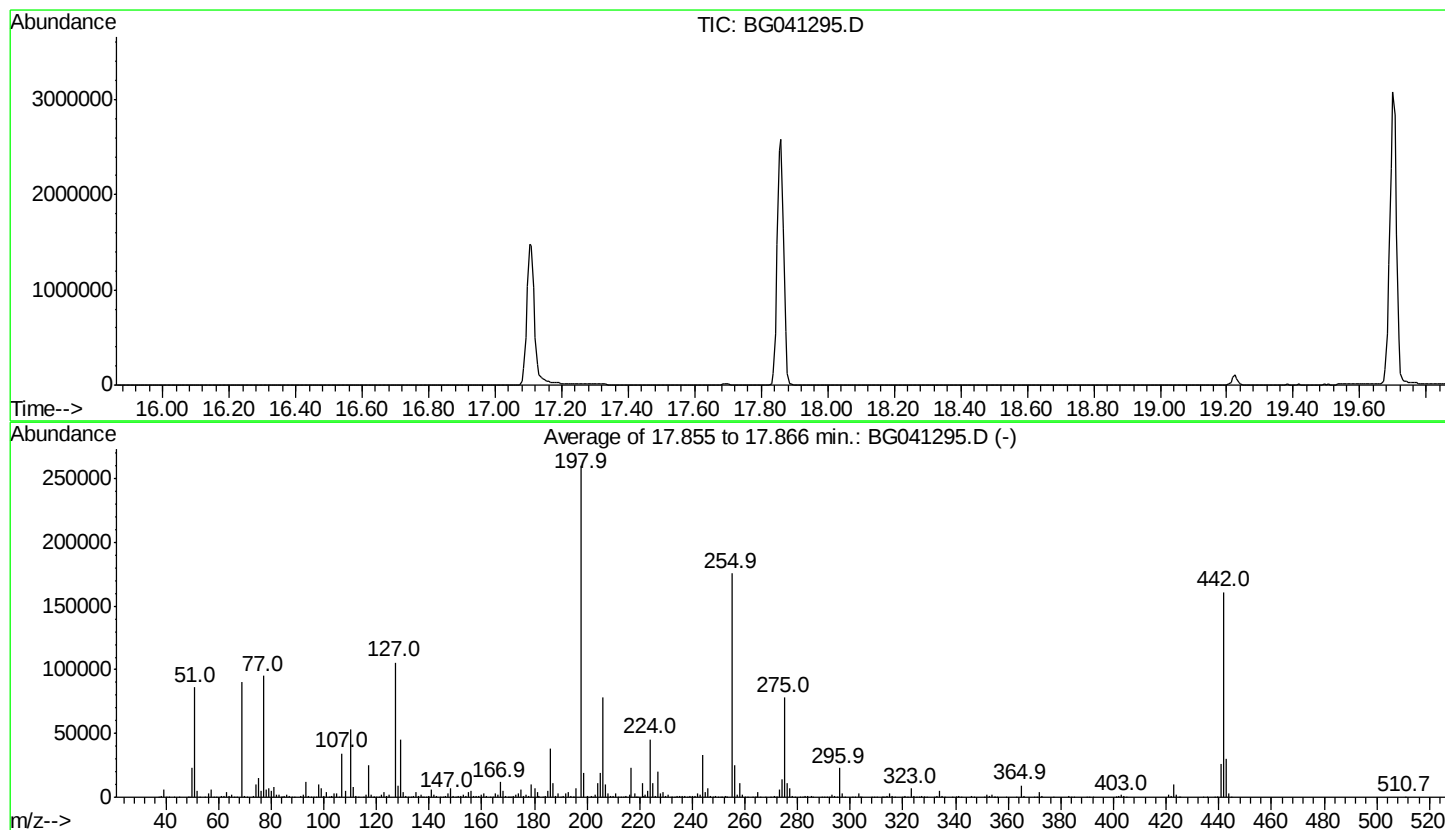

AutoFind: Scans 2513, 2514, 2515; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.1	86093	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.6	90138	PASS
70	69	0.00	2	0.7	663	PASS
127	198	10	80	40.6	105552	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	260181	PASS
199	198	5	9	7.3	18896	PASS
275	198	10	60	29.9	77909	PASS
365	198	1	100	3.6	9427	PASS
441	198	0.01	100	10.1	26234	PASS
442	198	50	100	61.9	161045	PASS
443	442	15	24	18.7	30053	PASS