
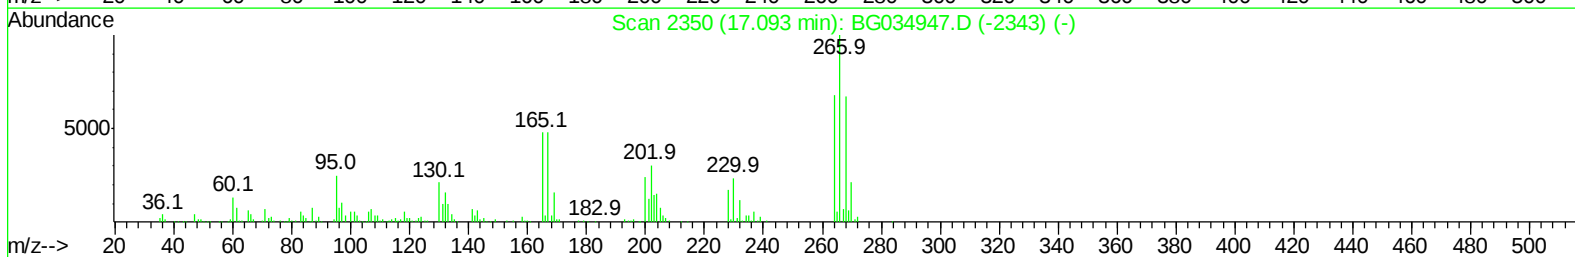
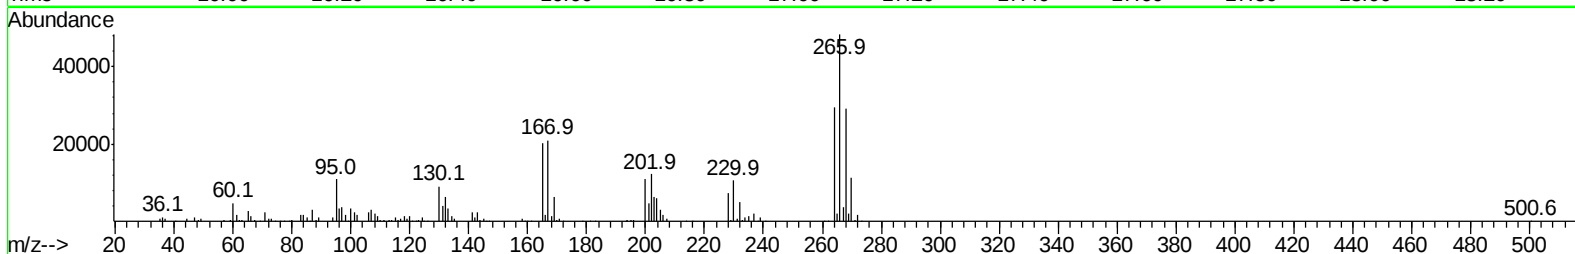


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG061918\
Data File : BG035249.D
Acq On : 19 Jun 2018 15:05
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 20 08:16:22 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

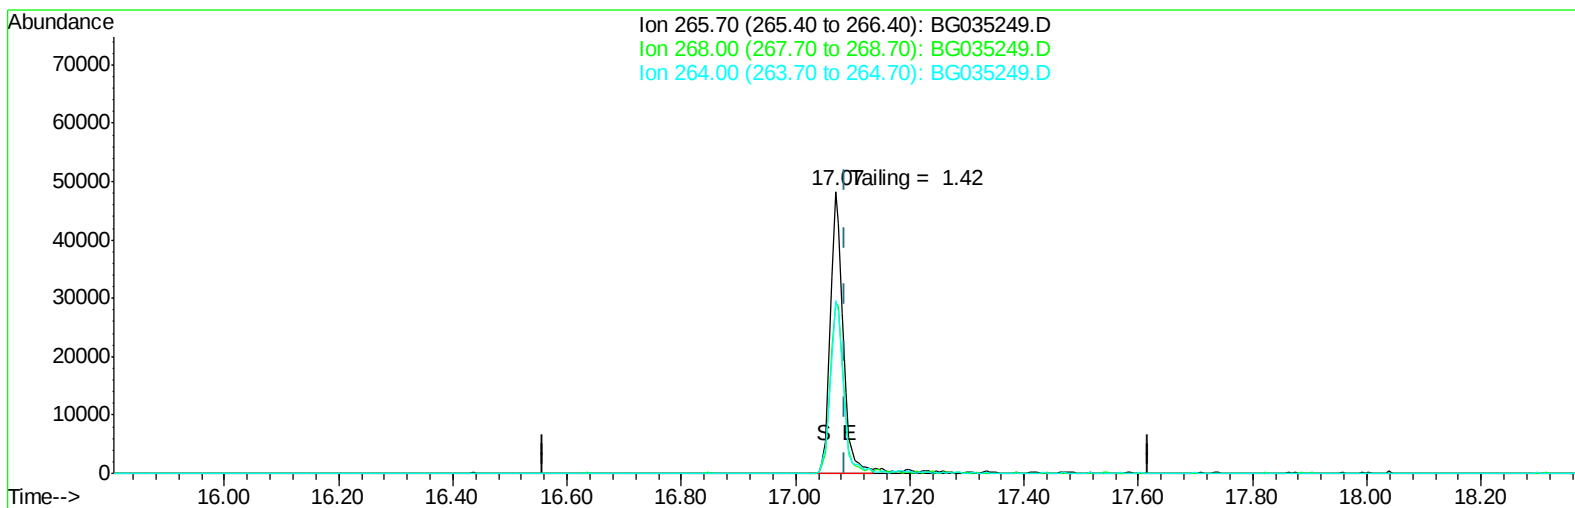

TIC: BG035249.D

(69) Pentachlorophenol (C)




17.069min (-0.018) 141301.49ng

response 73371

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.54
264.00	62.00	61.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG061918\
 Data File : BG035249.D
 Acq On : 19 Jun 2018 15:05
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 20 08:16:22 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 08 17:16:28 2018
 Response via : Initial Calibration

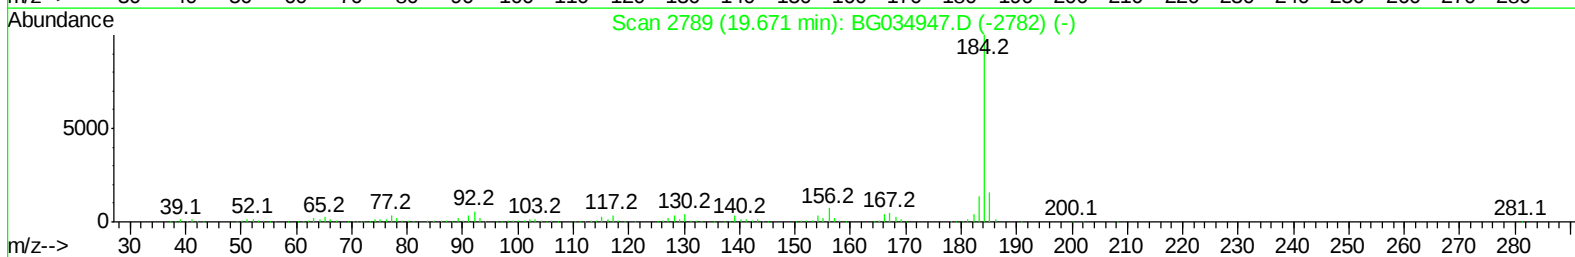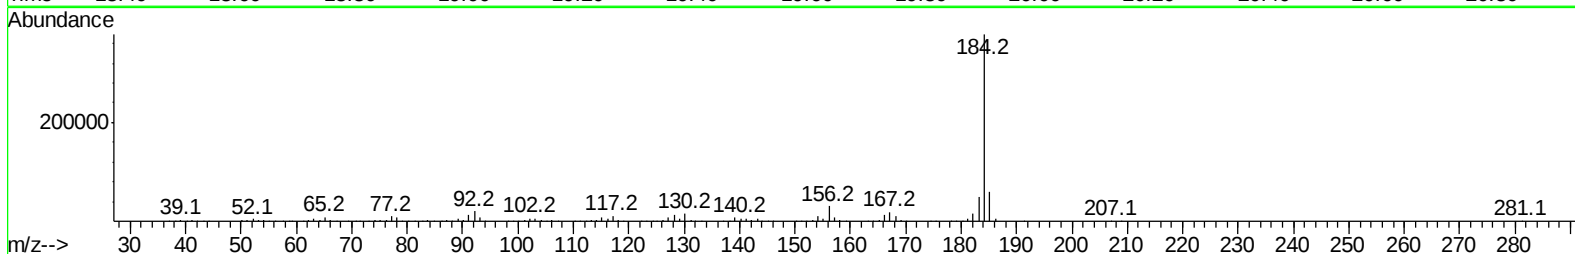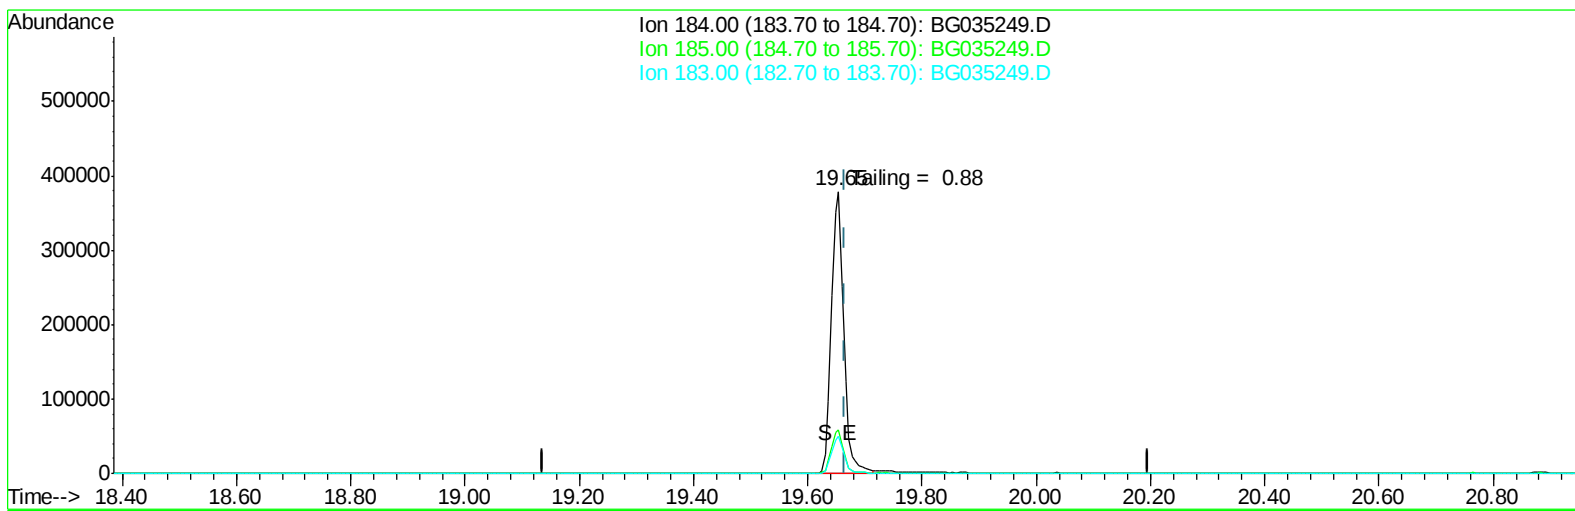

TIC: BG035249.D

(76) Benzidine

19.654min (-0.012) 58650.80ng

response 573872

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.54
183.00	13.30	13.06
0.00	0.00	0.00