

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061918\
 Data File : BG035259.D
 Acq On : 19 Jun 2018 22:15
 Operator : SJ/JU
 Sample : PB110338BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB110338BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG060718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.632	393	399	411	rBV	337901	582888	10.73%	4.361%
2	7.212	661	668	678	rBV	383176	680021	12.51%	5.088%
3	7.594	725	733	744	rBV	341270	614263	11.30%	4.596%
4	8.058	806	812	819	rBV	50931	91245	1.68%	0.683%
5	8.381	859	867	876	rBV2	249776	445693	8.20%	3.334%
6	9.221	1002	1010	1020	rBV	206913	385010	7.09%	2.880%
7	10.866	1284	1290	1298	rBV	71986	121083	2.23%	0.906%
8	13.304	1697	1705	1716	rBV	647873	1023962	18.84%	7.661%
9	14.684	1932	1940	1947	rBV2	125655	212419	3.91%	1.589%
10	16.165	2184	2192	2209	rBV	875944	1335182	24.57%	9.989%
11	17.428	2398	2407	2414	rBV	289221	455566	8.38%	3.408%
12	20.030	2844	2850	2862	rBV	3919960	5433942	100.00%	40.654%
13	21.692	3126	3133	3145	rVB2	656290	1088882	20.04%	8.147%
14	24.917	3670	3682	3694	rBV2	305737	896065	16.49%	6.704%


Sum of corrected areas: 13366221

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061918\
Data File : BG035259.D
Acq On : 19 Jun 2018 22:15
Operator : SJ/JU
Sample : PB110338BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB110338BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

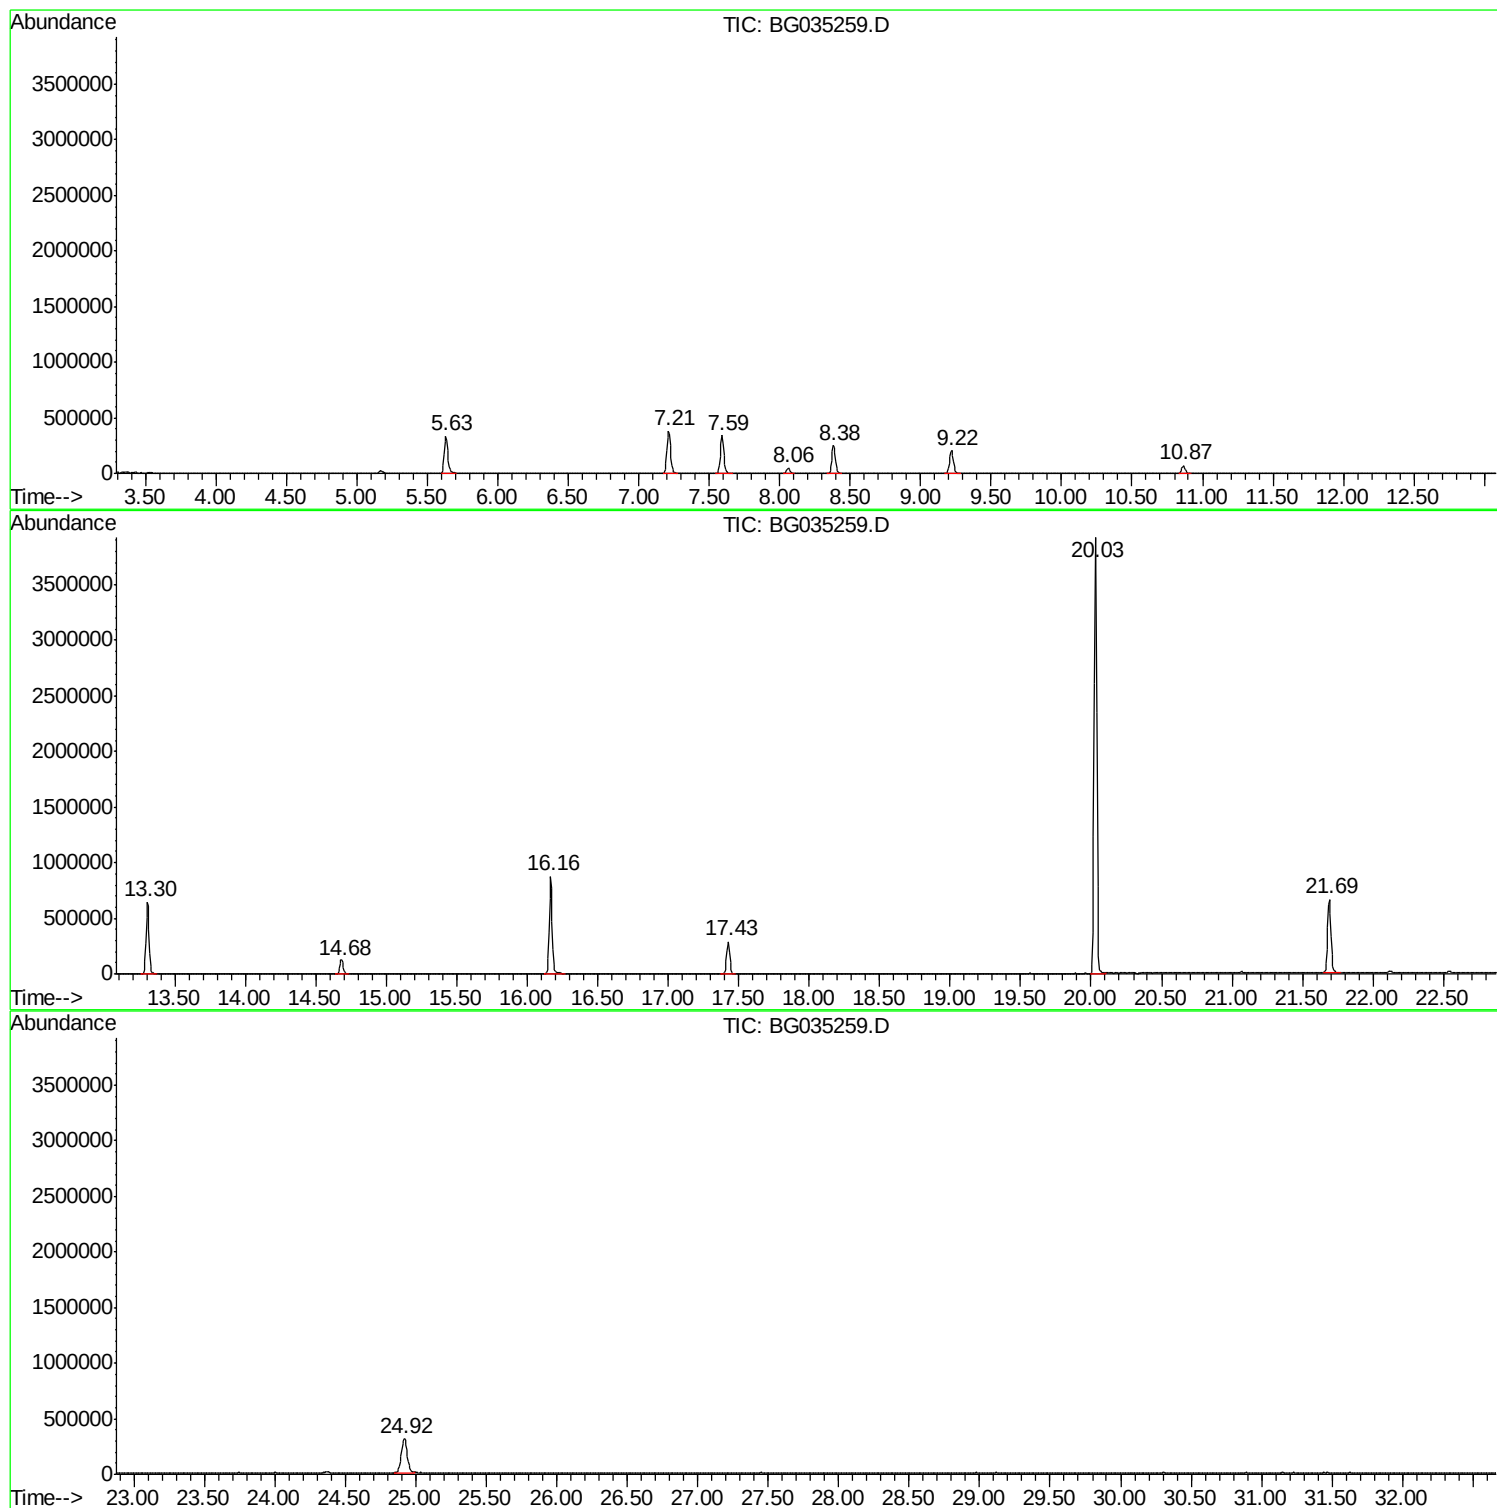

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061918\
Data File : BG035259.D
Acq On : 19 Jun 2018 22:15
Operator : SJ/JU
Sample : PB110338BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB110338BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.59 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.59	134.64 ng	614263	1,4-Dichlorobenzene-d4	8.06

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	27
3		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	25
4		5-Aminoindole	132	C8H8N2	005192-03-0	22
5		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22

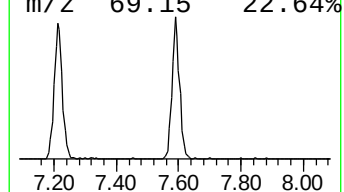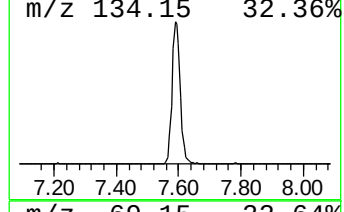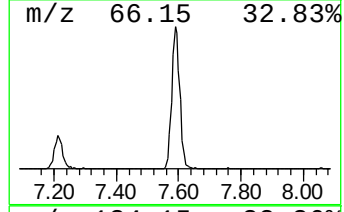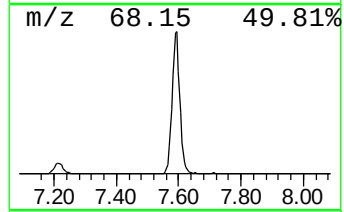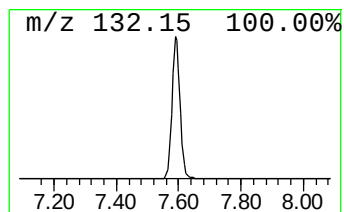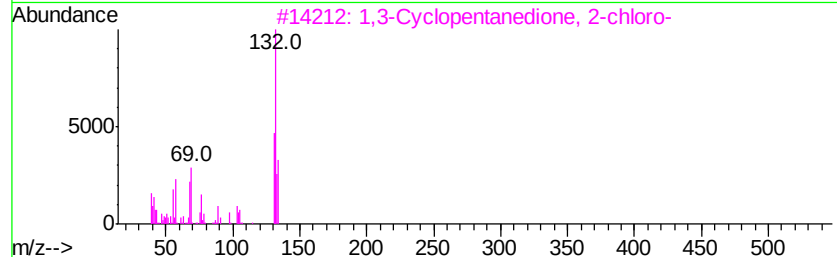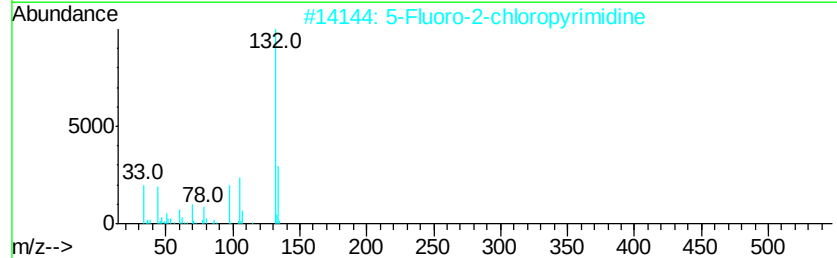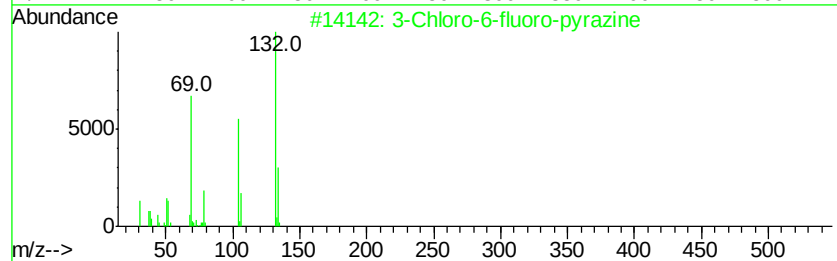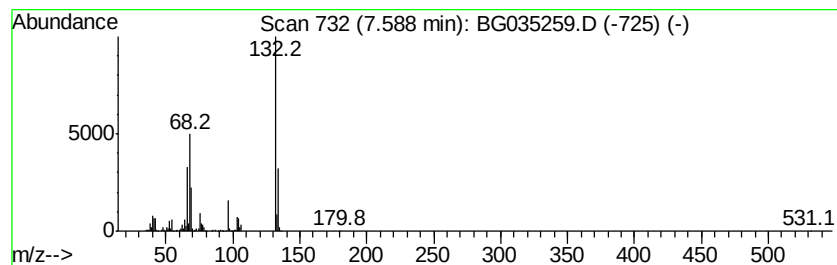

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG061918\
Data File : BG035259.D
Acq On : 19 Jun 2018 22:15
Operator : SJ/JU
Sample : PB110338BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB110338BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.59	7.59	134.6	ng	614263	1	8.06	91245	20.0