


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG061918\
 Data File : BG035249.D
 Acq On : 19 Jun 2018 15:05
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG060718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 08 17:16:28 2018

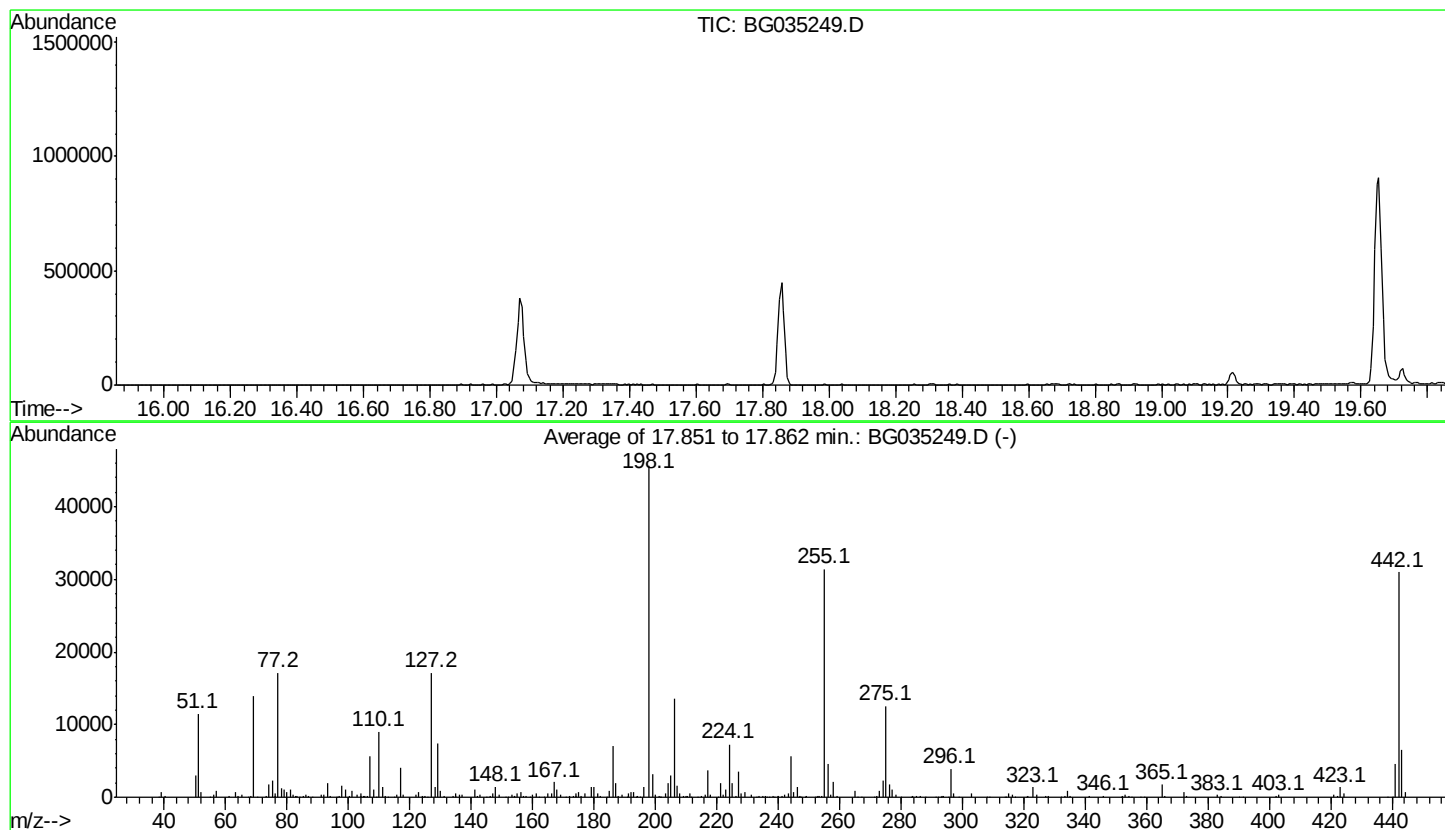

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.2	11488	PASS
68	69	0.00	2	1.3	185	PASS
69	198	0.00	100	30.4	13895	PASS
70	69	0.00	2	0.5	69	PASS
127	198	10	80	37.5	17116	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	45640	PASS
199	198	5	9	7.1	3228	PASS
275	198	10	60	27.4	12527	PASS
365	198	1	100	3.9	1760	PASS
441	443	0.01	100	69.6	4535	PASS
442	198	50	100	67.9	30981	PASS
443	442	15	24	21.0	6520	PASS