

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061919\
 Data File : BG041328.D
 Acq On : 19 Jun 2019 15:04
 Operator : HP/JU
 Sample : K3154-01 2X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Jun 19 16:32:30 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 14:58:02 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.08	152	38700	20.00	ng	0.00
21) Naphthalene-d8	10.90	136	156655	20.00	ng	0.00
39) Acenaphthene-d10	14.71	164	106393	20.00	ng	0.00
64) Phenanthrene-d10	17.46	188	249968	20.00	ng	0.00
76) Chrysene-d12	21.74	240	256635	20.00	ng	0.00
87) Perylene-d12	25.05	264	283718	20.00	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.61	112	104310	49.52	ng	0.00
7) Phenol-d6	7.23	99	149748	49.05	ng	0.00
23) Nitrobenzene-d5	9.26	82	106890	28.70	ng	0.00
42) 2,4,6-Tribromophenol	16.20	330	69862	42.77	ng	0.00
45) 2-Fluorobiphenyl	13.33	172	230595	29.46	ng	0.00
79) Terphenyl-d14	20.06	244	372151	28.74	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
19) n-Nitroso-di-n-propylamine	9.26	70	15376	6.227	ng	# 81
51) 2,6-Dinitrotoluene	14.71	165	14199	7.114	ng	# 16
56) 4-Nitrophenol	15.00	139	63	3.256	ng	85
57) 2,4-Dinitrotoluene	14.71	165	14199	4.866	ng	# 19
71) Phenanthrene	17.51	178	31339	2.351	ng	98
72) Anthracene	17.51	178	31339	2.384	ng	99
75) Fluoranthene	19.51	202	89620	5.060	ng	99
78) Pyrene	19.87	202	86799	5.015	ng	97
81) Benzo(a)anthracene	21.72	228	51979	2.991	ng	96
83) Chrysene	21.78	228	51994	3.111	ng	96
88) Benzo(b)fluoranthene	23.99	252	59108	3.362	ng	# 89
89) Benzo(k)fluoranthene	23.99	252	59108	3.393	ng	# 91
90) Benzo(a)pyrene	24.89	252	46529	2.802	ng	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061919\
Data File : BG041328.D
Acq On : 19 Jun 2019 15:04
Operator : HP/JU
Sample : K3154-01 2X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Jun 19 16:32:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 14:58:02 2019
Response via : Initial Calibration

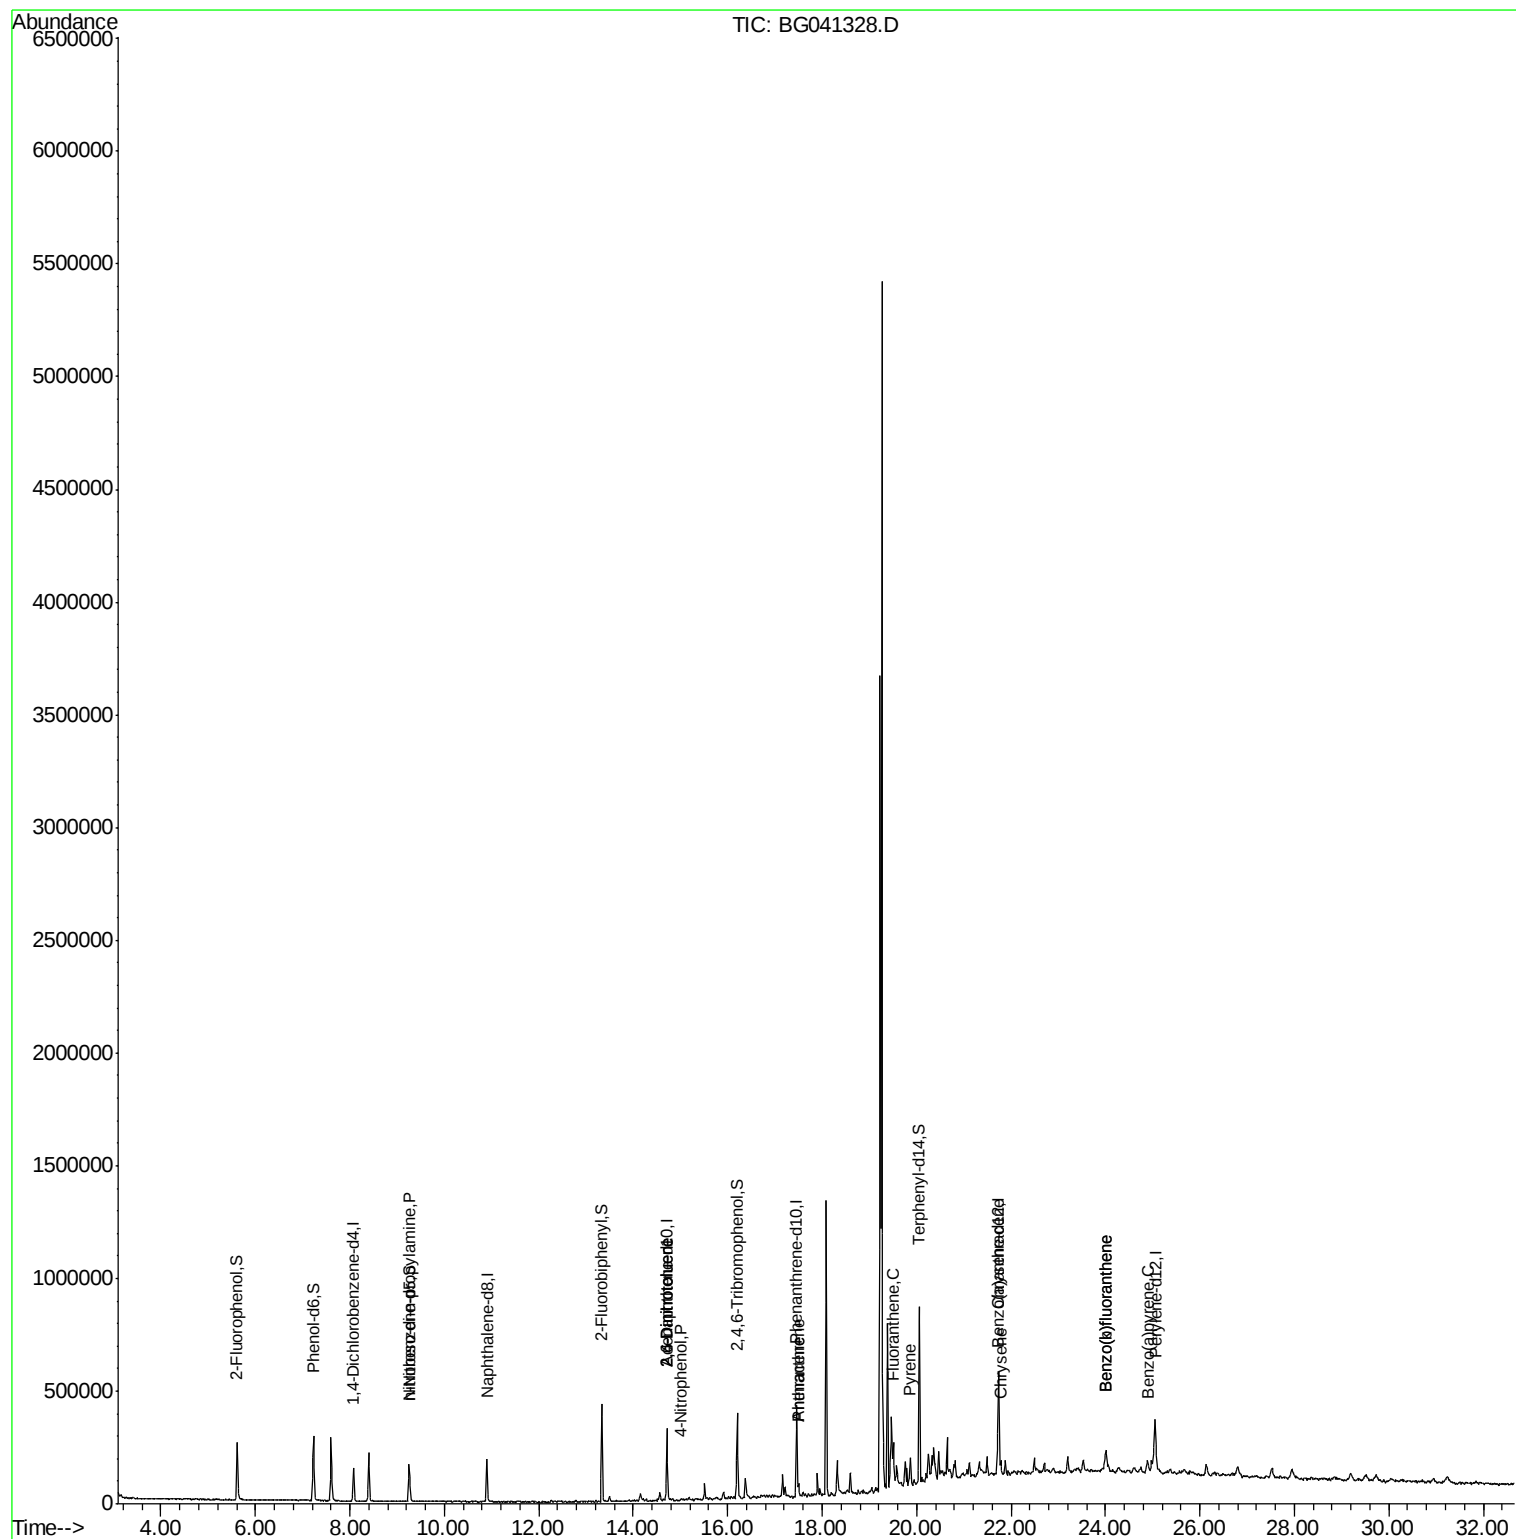

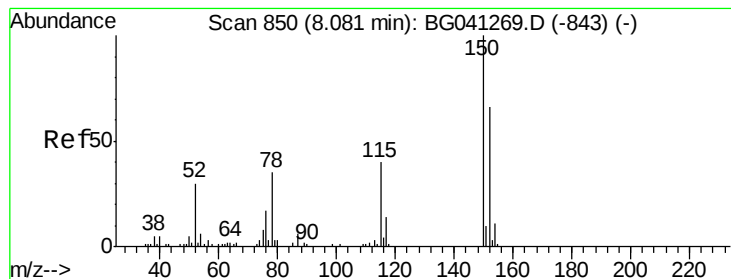


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.08 min Scan# 849
Delta R.T. -0.01 min
Lab File: BG041328.D
Acq: 19 Jun 2019 15:04

Instrument :
BNA_G
ClientSampleId :

Tot Ion:152 Resp: 38700
Ion Ratio Lower Upper
152 100
150 167.6 120.6 181.0
115 61.2 47.9 71.9




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

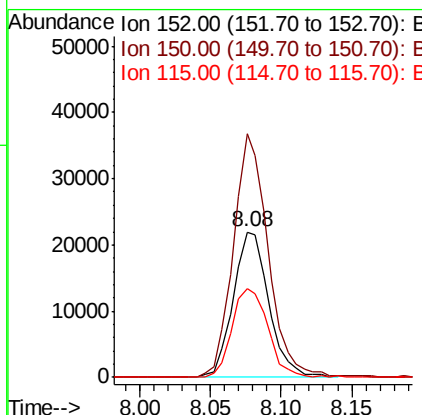



#5


2-Fluorophenol
Concen: 49.525 ng
RT: 5.61 min Scan# 430
Delta R.T. -0.01 min
Lab File: BG041328.D
Acq: 19 Jun 2019 15:04

Tgt Ion:112 Resp: 104310
Ion Ratio Lower Upper
112 100
64 71.6 55.9 83.9
63 42.0 34.6 51.8



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

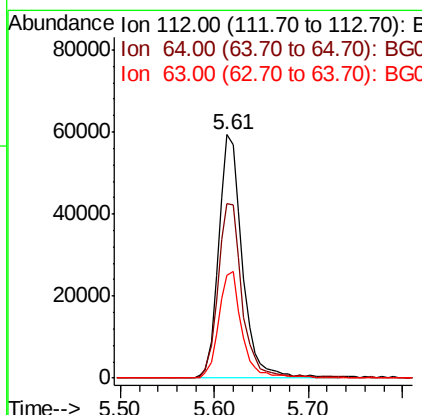

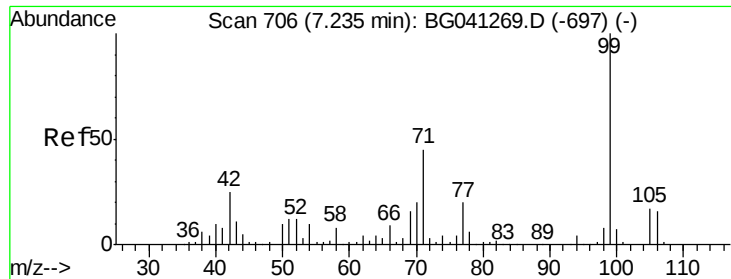

#7

Phenol-d6

Concen: 49.050 ng

RT: 7.23 min Scan# 705

Delta R.T. -0.01 min

Lab File: BG041328.D

Acq: 19 Jun 2019 15:04

Instrument :

BNA_G

ClientSampled :


Tot Ion: 99 Resp: 149748

Ion Ratio Lower Upper




99 100

42 25.4 19.9 29.9

71 49.4 36.4 54.6



Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

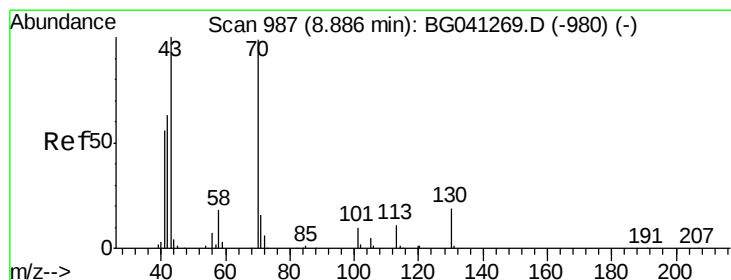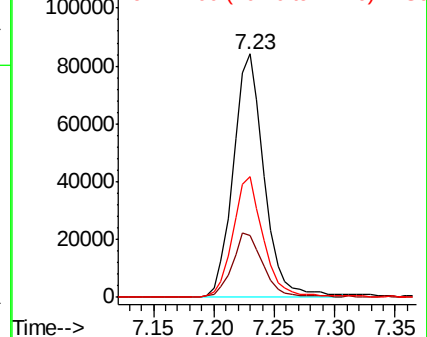

#19

n-Nitroso-di-n-propylamine

Concen: 6.227 ng

RT: 9.26 min Scan# 1050

Delta R.T. 0.37 min

Lab File: BG041328.D

Acq: 19 Jun 2019 15:04

Tgt Ion: 70 Resp: 15376


Ion Ratio Lower Upper

70 100



42 55.6 51.4 77.2


101 0.0 8.2 12.2#

130 0.0 15.2 22.8#



Abundance Ion 70.00 (69.70 to 70.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 101.00 (100.70 to 101.70): BGC
Ion 130.00 (129.70 to 130.70): BGC




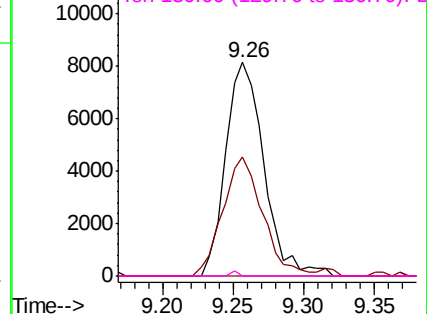


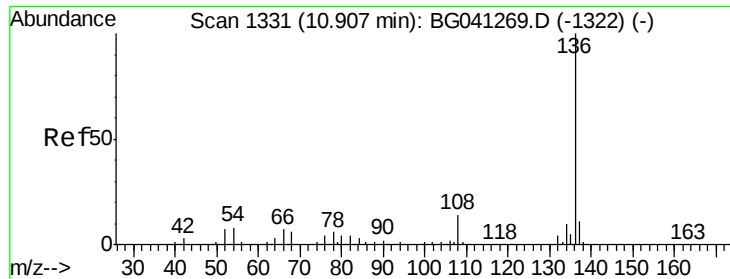

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.90 min Scan# 1330
Delta R.T. -0.01 min
Lab File: BG041328.D
Acq: 19 Jun 2019 15:04




Instrument :
BNA_G
ClientSampleId :


Tot Ion:136	Resp:	156655
Ion Ratio	Lower	Upper
136	100	
137	11.8	8.8 13.2
54	8.9	6.4 9.6
68	3.9	4.8 7.2#

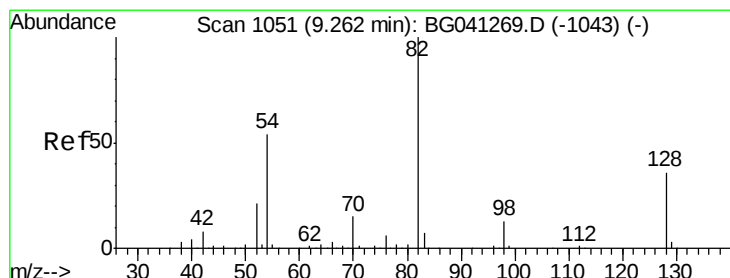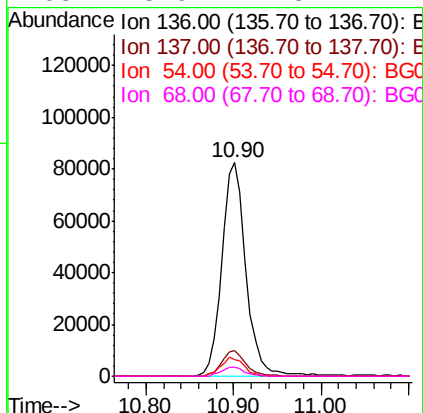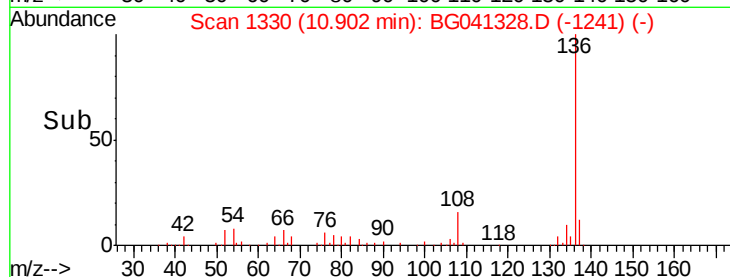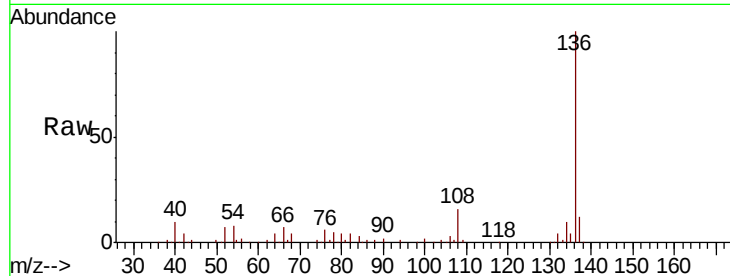

#23
Nitrobenzene-d5
Concen: 28.696 ng
RT: 9.26 min Scan# 1050
Delta R.T. -0.01 min
Lab File: BG041328.D
Acq: 19 Jun 2019 15:04

Tgt Ion: 82	Resp:	106890
Ion Ratio	Lower	Upper
82	100	
128	34.1	29.2 43.8
54	58.5	43.4 65.0

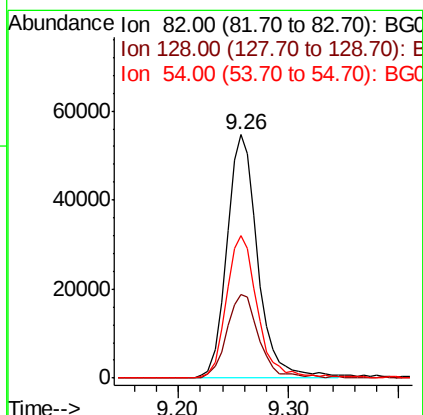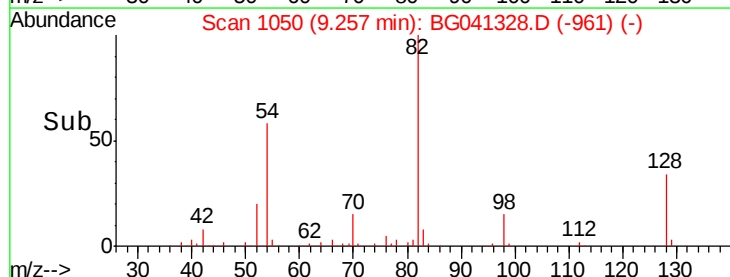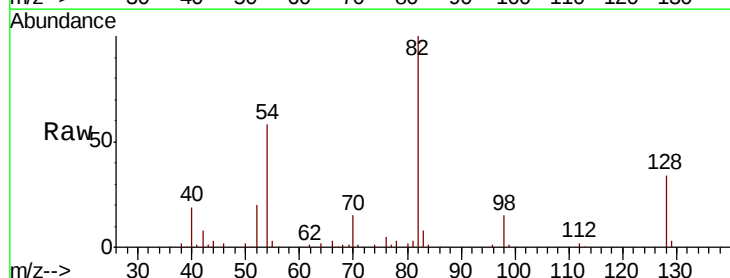

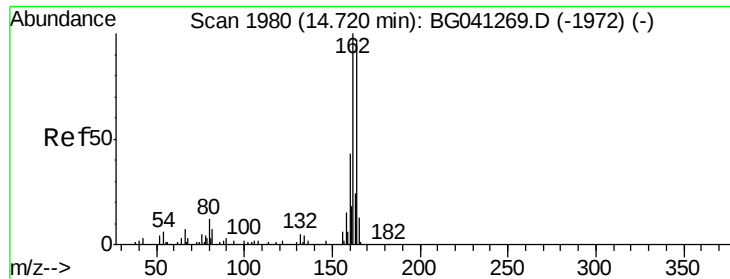

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.71 min Scan# 1979

Delta R.T. -0.01 min

Lab File: BG041328.D

Acq: 19 Jun 2019 15:04

Instrument :

BNA_G

ClientSampled :





Tot Ion:164 Resp: 106393

Ion Ratio Lower Upper

164 100

162 102.9 82.8 124.2

160 46.1 35.8 53.8

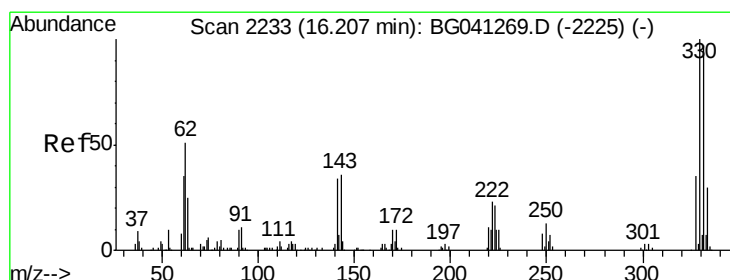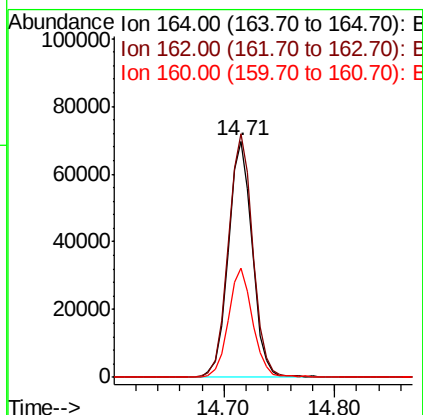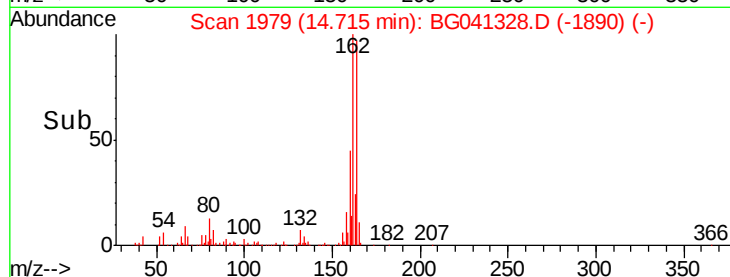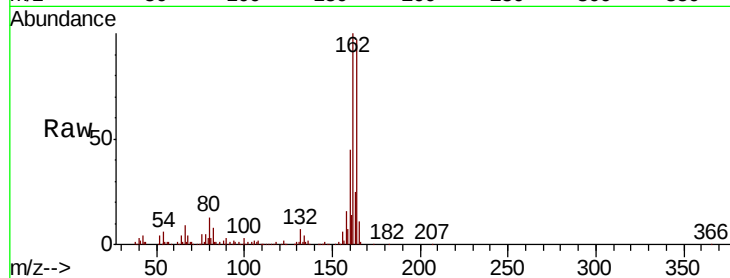

#42

2,4,6-Tribromophenol

Concen: 42.772 ng

RT: 16.20 min Scan# 2232

Delta R.T. -0.01 min

Lab File: BG041328.D

Acq: 19 Jun 2019 15:04




Tgt Ion:330 Resp: 69862


Ion Ratio Lower Upper

330 100

332 92.6 75.5 113.3

141 37.1 29.0 43.4


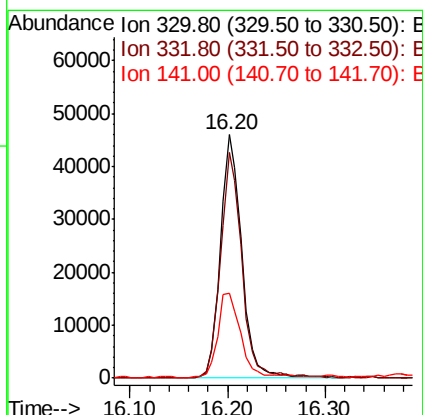
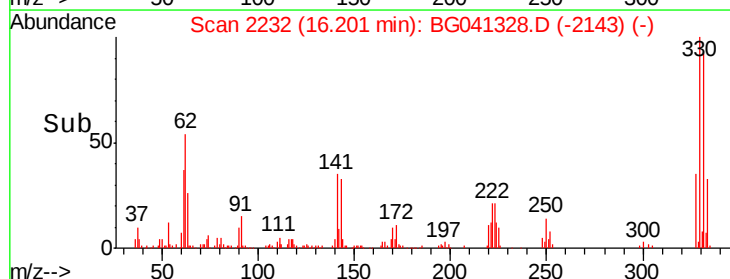
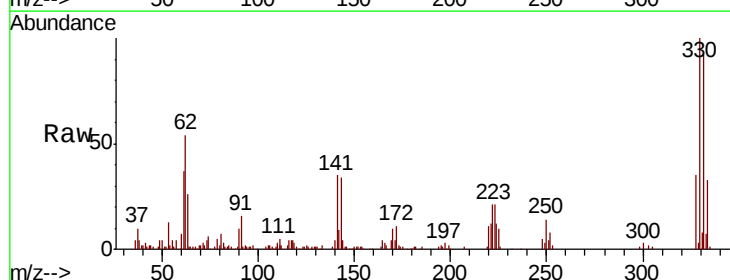




#45
2-Fluorobiphenyl
Concen: 29.458 ng
RT: 13.33 min Scan# 1744
Delta R.T. -0.01 min
Lab File: BG041328.D
Acq: 19 Jun 2019 15:04




Instrument :
BNA_G
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
172	100		
171	36.7	30.0	45.0
170	25.0	19.8	29.6

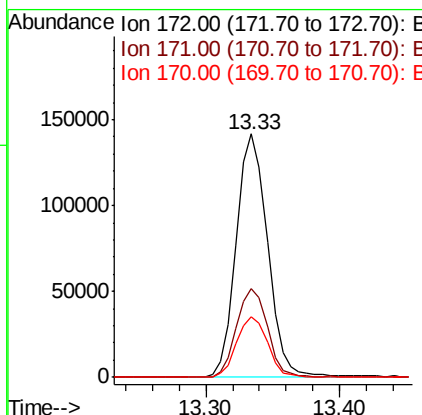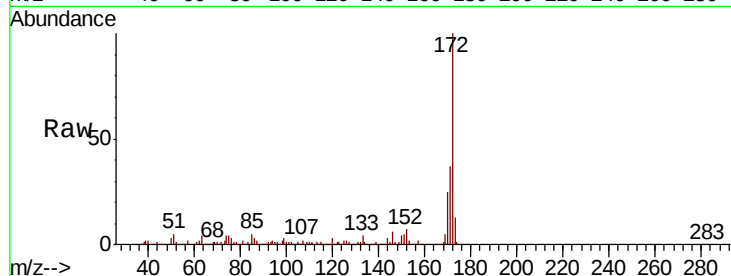

#51
2,6-Dinitrotoluene
Concen: 7.114 ng
RT: 14.71 min Scan# 1978
Delta R.T. 0.41 min
Lab File: BG041328.D
Acq: 19 Jun 2019 15:04

Tgt Ion	Ratio	Lower	Upper
165	100		
63	2.3	55.4	83.0#
89	0.0	56.5	84.7#


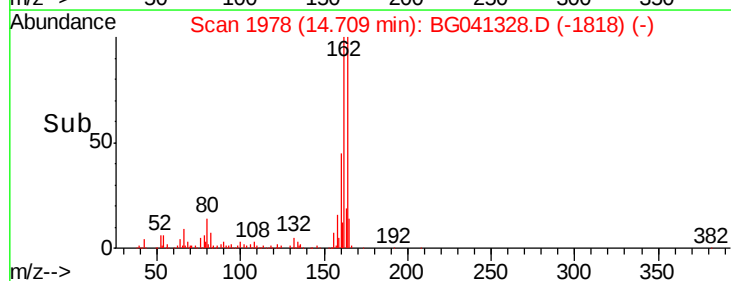
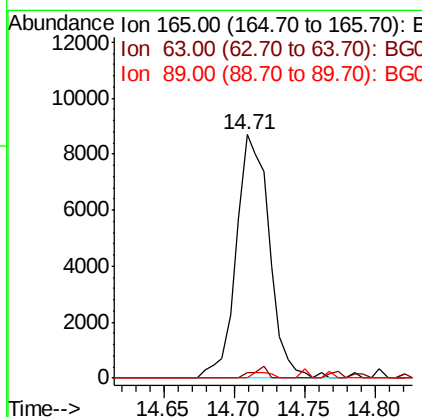



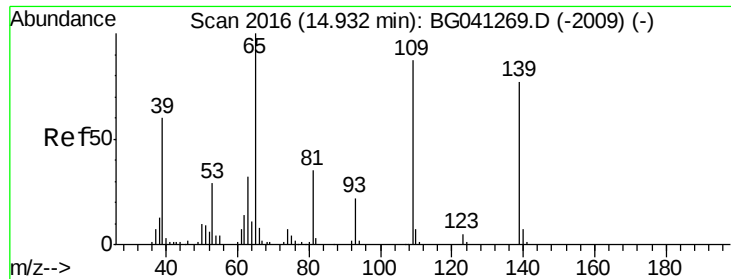

#56
4-Nitrophenol
Concen: 3.256 ng
RT: 15.00 min Scan# 2027
Delta R.T. 0.07 min
Lab File: BG041328.D
Acq: 19 Jun 2019 15:04




Instrument :
BNA_G
ClientSampled :


Tot Ion:139 Resp: 63
Ion Ratio Lower Upper
139 100
109 132.0 93.2 133.2
65 116.3 110.2 150.2

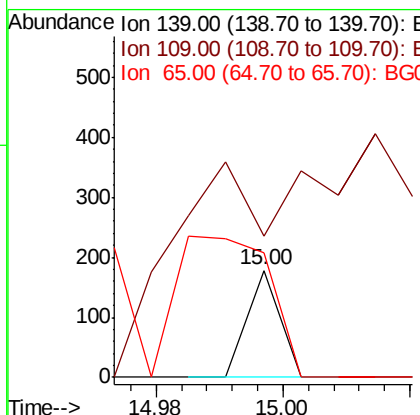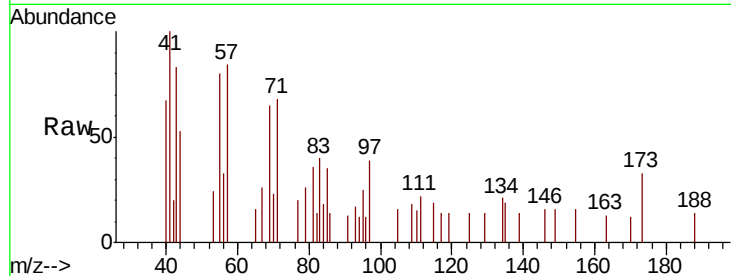

#57
2,4-Dinitrotoluene
Concen: 4.866 ng
RT: 14.71 min Scan# 1978
Delta R.T. -0.38 min
Lab File: BG041328.D
Acq: 19 Jun 2019 15:04

Tgt Ion:165 Resp: 14199
Ion Ratio Lower Upper
165 100
63 2.3 40.0 60.0#
89 0.0 64.6 96.8#
182 0.0 2.9 4.3#


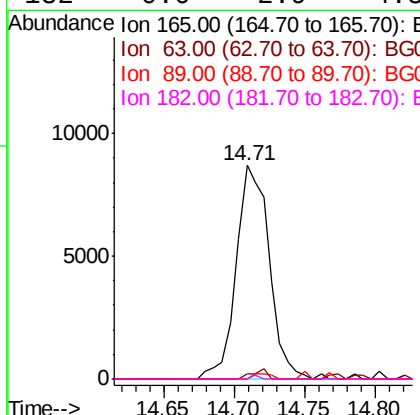




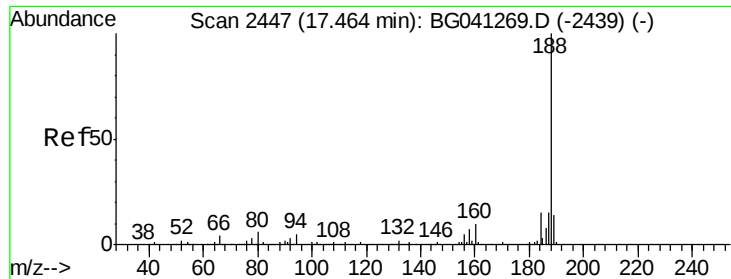

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.46 min Scan# 2446
Delta R.T. -0.01 min
Lab File: BG041328.D
Acq: 19 Jun 2019 15:04




Instrument :
BNA_G
ClientSampleId :


Tot Ion:188 Resp: 249968
Ion Ratio Lower Upper
188 100
94 5.2 3.6 5.4
80 6.5 4.8 7.2

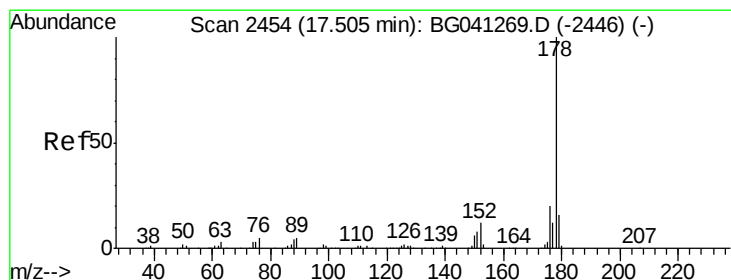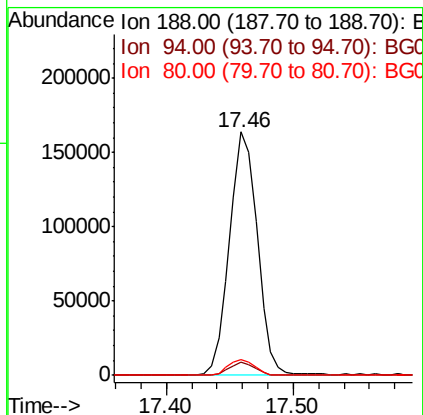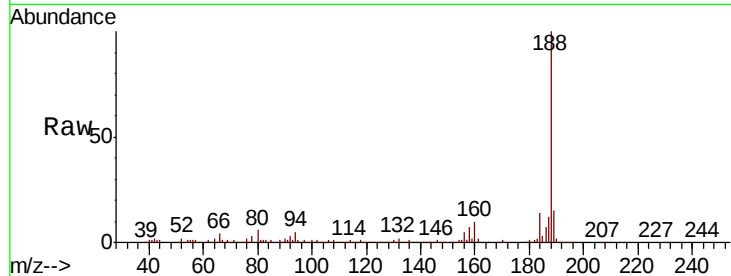

#71
Phenanthrene
Concen: 2.351 ng
RT: 17.51 min Scan# 2454
Delta R.T. 0.00 min
Lab File: BG041328.D
Acq: 19 Jun 2019 15:04

Tgt Ion:178 Resp: 31339
Ion Ratio Lower Upper
178 100
176 19.1 16.1 24.1
179 16.9 12.9 19.3

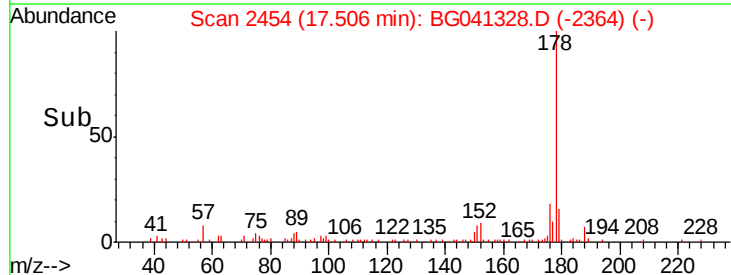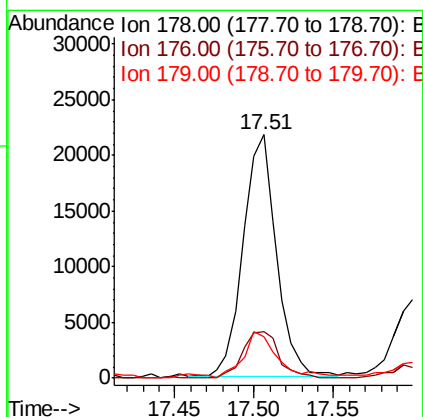



#72

Anthracene

Concen: 2.384 ng

RT: 17.51 min Scan# 2454

Delta R.T. -0.09 min

Lab File: BG041328.D

Acq: 19 Jun 2019 15:04

Instrument :

BNA_G

ClientSampleId :


Tot Ion:178 Resp: 31339

Ion	Ratio	Lower	Upper
178	100		
176	19.1	15.4	23.2
179	16.9	13.0	19.4

178 100

176 19.1 15.4 23.2

179 16.9 13.0 19.4



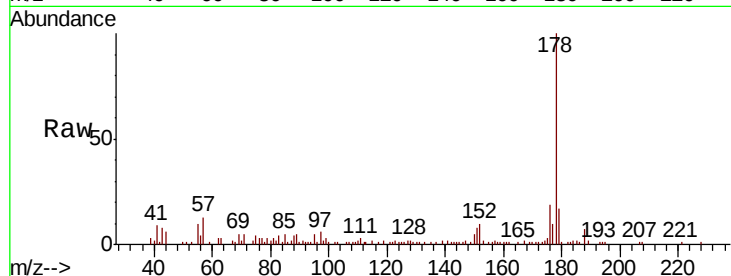


Abundance

Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

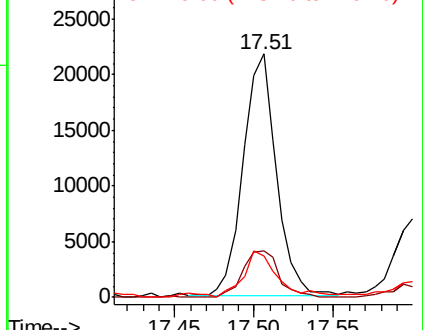

#75

Fluoranthene

Concen: 5.060 ng

RT: 19.51 min Scan# 2795

Delta R.T. 0.00 min

Lab File: BG041328.D

Acq: 19 Jun 2019 15:04


Tgt Ion:202 Resp: 89620

Ion	Ratio	Lower	Upper
202	100		
101	5.7	0.0	26.0
203	17.2	0.0	37.7

202 100

101 5.7 0.0 26.0

203 17.2 0.0 37.7






Abundance

Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E




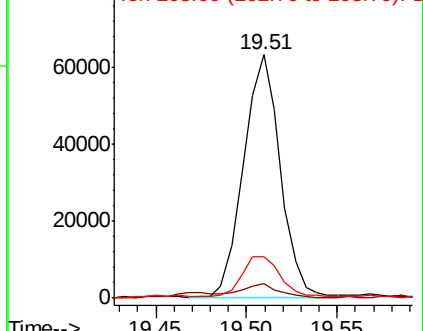


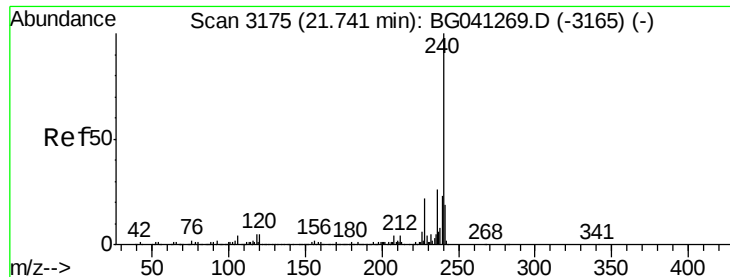

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.74 min Scan# 3174
Delta R.T. -0.01 min
Lab File: BG041328.D
Acq: 19 Jun 2019 15:04




Instrument :
BNA_G
ClientSampleId :


Tot Ion:240 Resp: 256635
Ion Ratio Lower Upper
240 100
120 4.5 3.7 5.5
236 25.7 21.1 31.7

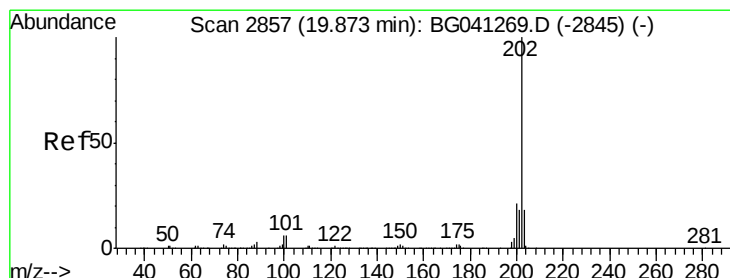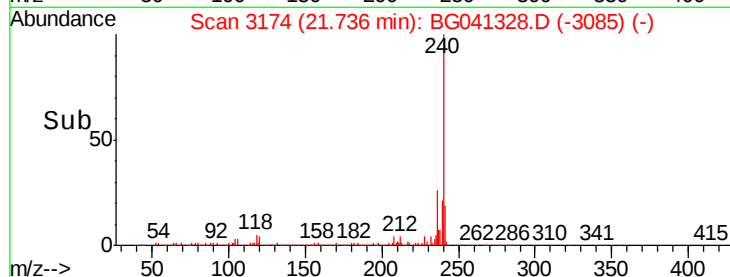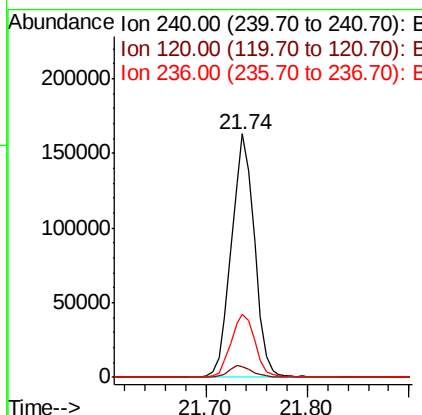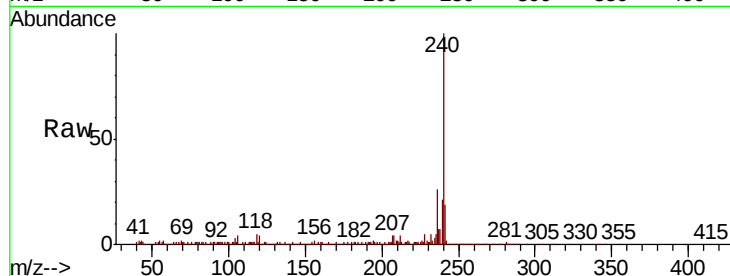

#78
Pyrene
Concen: 5.015 ng
RT: 19.87 min Scan# 2857
Delta R.T. 0.00 min
Lab File: BG041328.D
Acq: 19 Jun 2019 15:04

Tgt Ion:202 Resp: 86799
Ion Ratio Lower Upper
202 100
200 19.0 16.8 25.2
203 17.9 14.6 21.8

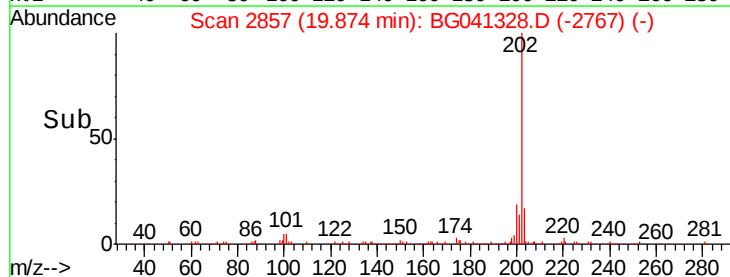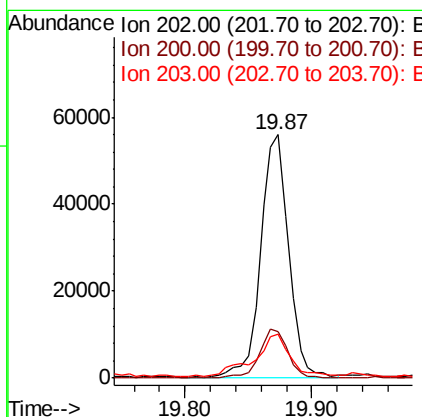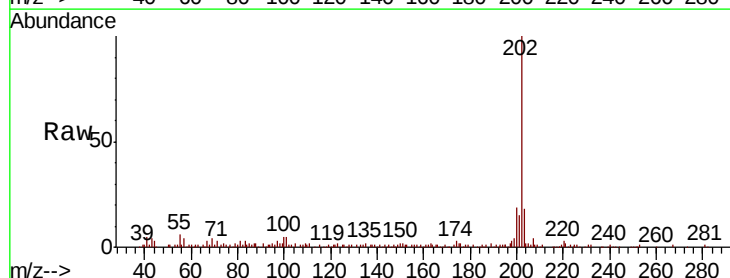



#79

Terphenyl-d14

Concen: 28.738 ng

RT: 20.06 min Scan# 2888

Delta R.T. -0.01 min

Lab File: BG041328.D

Acq: 19 Jun 2019 15:04

Instrument :

BNA_G

ClientSampleId :


Tot Ion:244 Resp: 372151

Ion Ratio Lower Upper

244 100

212 7.9 6.6 10.0




122 6.0 5.0 7.4



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

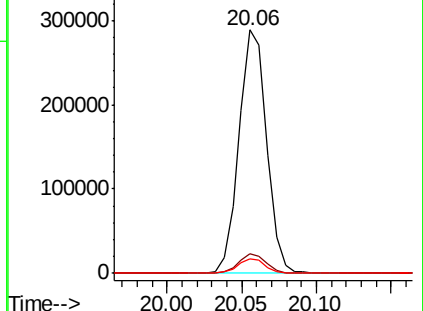

#81

Benzo(a)anthracene

Concen: 2.991 ng

RT: 21.72 min Scan# 3171

Delta R.T. 0.00 min

Lab File: BG041328.D

Acq: 19 Jun 2019 15:04


Tgt Ion:228 Resp: 51979

Ion Ratio Lower Upper

228 100

226 31.5 23.2 34.8



229 22.4 16.8 25.2




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

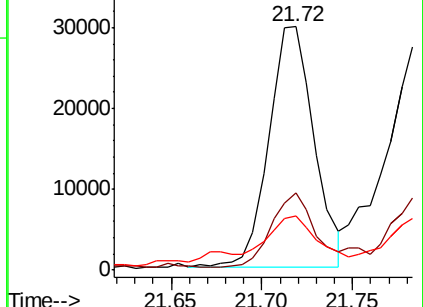



#83

Chrysene

Concen: 3.111 ng

RT: 21.78 min Scan# 3182

Delta R.T. -0.01 min

Lab File: BG041328.D

Acq: 19 Jun 2019 15:04

Instrument :

BNA_G

ClientSampleId :


Tot Ion:228 Resp: 51994

Ion Ratio Lower Upper




228 100

226 32.6 25.4 38.0

229 23.3 16.2 24.2

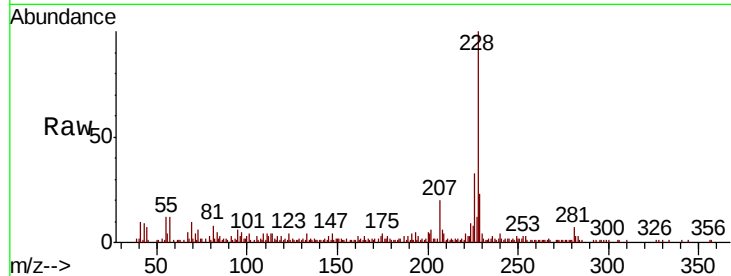

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

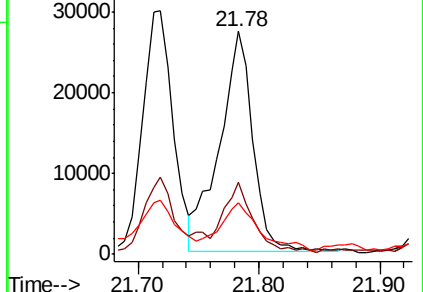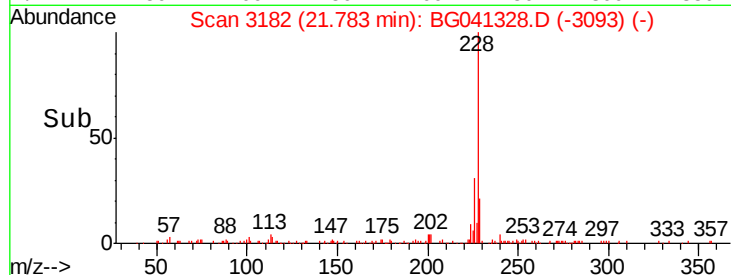

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.05 min Scan# 3738

Delta R.T. 0.01 min

Lab File: BG041328.D

Acq: 19 Jun 2019 15:04


Tgt Ion:264 Resp: 283718

Ion Ratio Lower Upper



264 100


260 24.1 17.4 26.2

265 22.9 17.2 25.8



Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

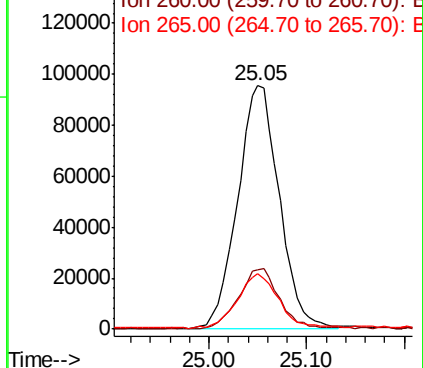

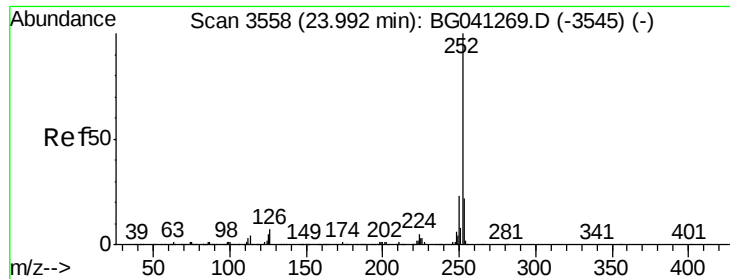

#88

Benzo(b)fluoranthene

Concen: 3.362 ng

RT: 23.99 min Scan# 3558

Delta R.T. 0.00 min

Lab File: BG041328.D

Acq: 19 Jun 2019 15:04

Instrument :

BNA_G

ClientSampled :


Tot Ion:252 Resp: 59108

Ion Ratio Lower Upper




252 100

253 27.0 17.4 26.0#

125 8.1 3.9 5.9#

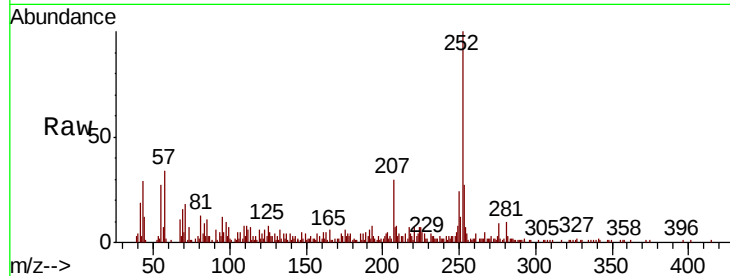

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

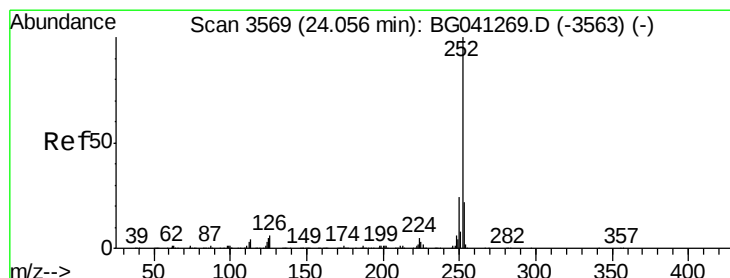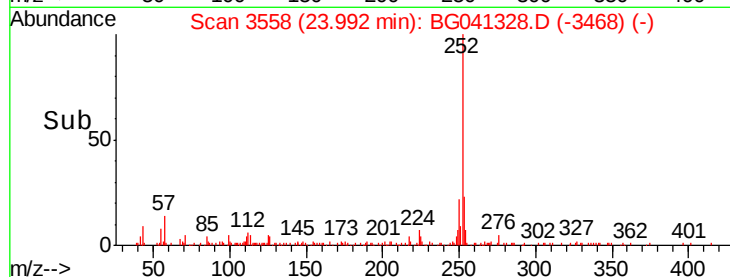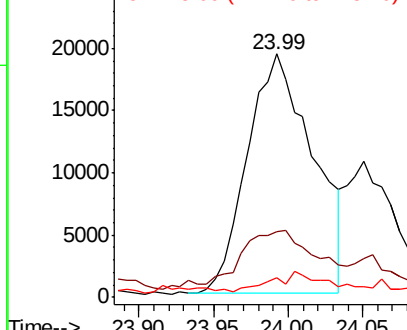

#89

Benzo(k)fluoranthene

Concen: 3.393 ng

RT: 23.99 min Scan# 3558

Delta R.T. -0.06 min

Lab File: BG041328.D

Acq: 19 Jun 2019 15:04


Tgt Ion:252 Resp: 59108

Ion Ratio Lower Upper



252 100


253 27.0 18.0 27.0

125 8.1 4.3 6.5#

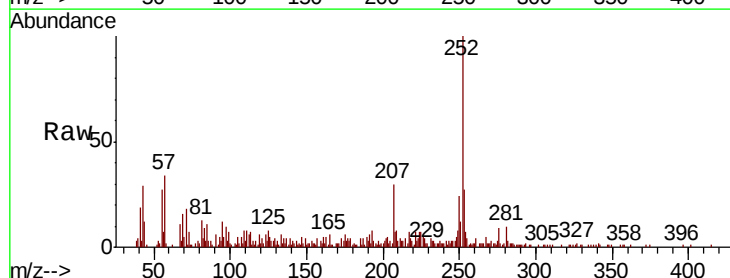

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

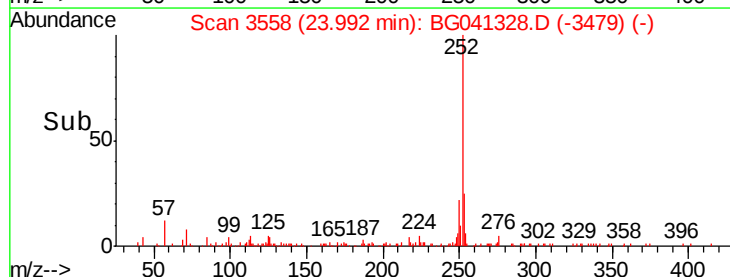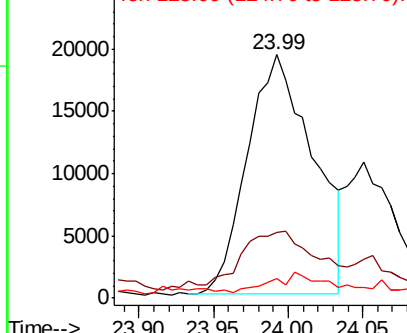


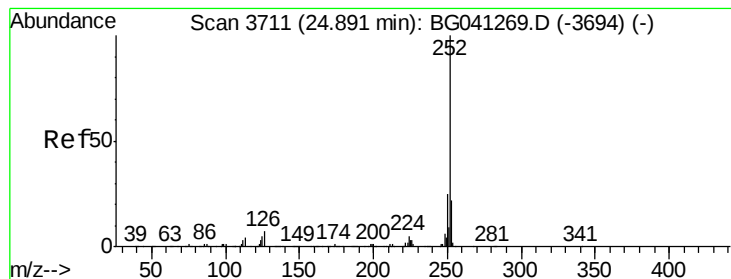

#90
 Benzo(a)pyrene
 Concen: 2.802 ng
 RT: 24.89 min Scan# 3711
 Delta R.T. 0.00 min
 Lab File: BG041328.D
 Acq: 19 Jun 2019 15:04

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
252	100		
253	26.5	17.8	26.6
125	6.3	4.2	6.4



Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

