
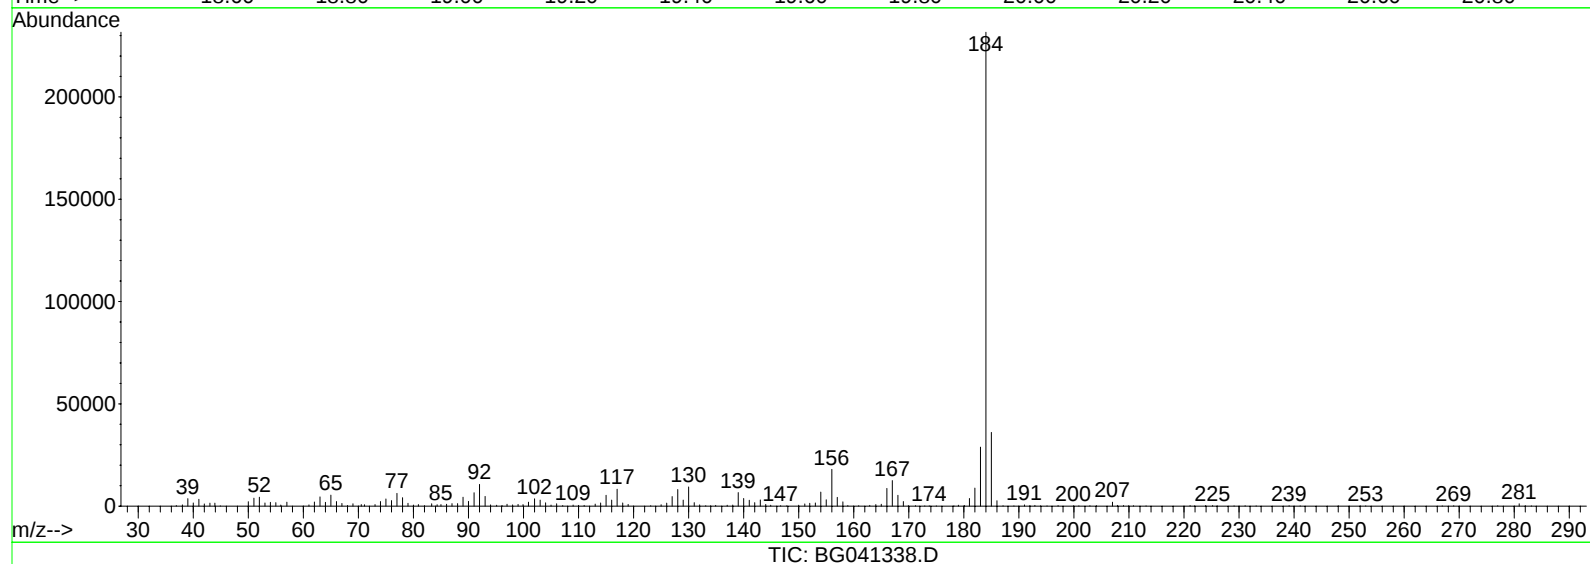


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG061919\
Data File : BG041338.D
Acq On : 19 Jun 2019 23:18
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 05:54:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 14:58:02 2019
Response via : Initial Calibration

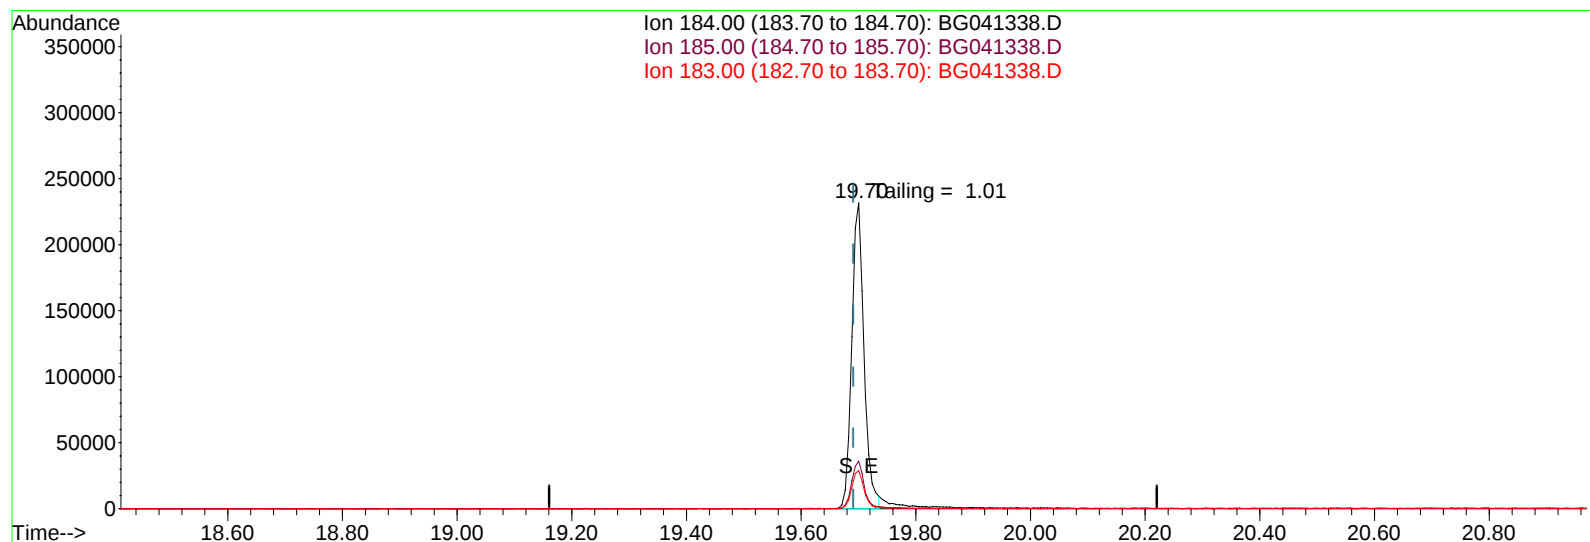

(77) Benzidine



19.700min (+0.010) 70644.86ng

response 360543

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.57
183.00	12.00	12.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG061919\
Data File : BG041338.D
Acq On : 19 Jun 2019 23:18
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 05:54:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 14:58:02 2019
Response via : Initial Calibration

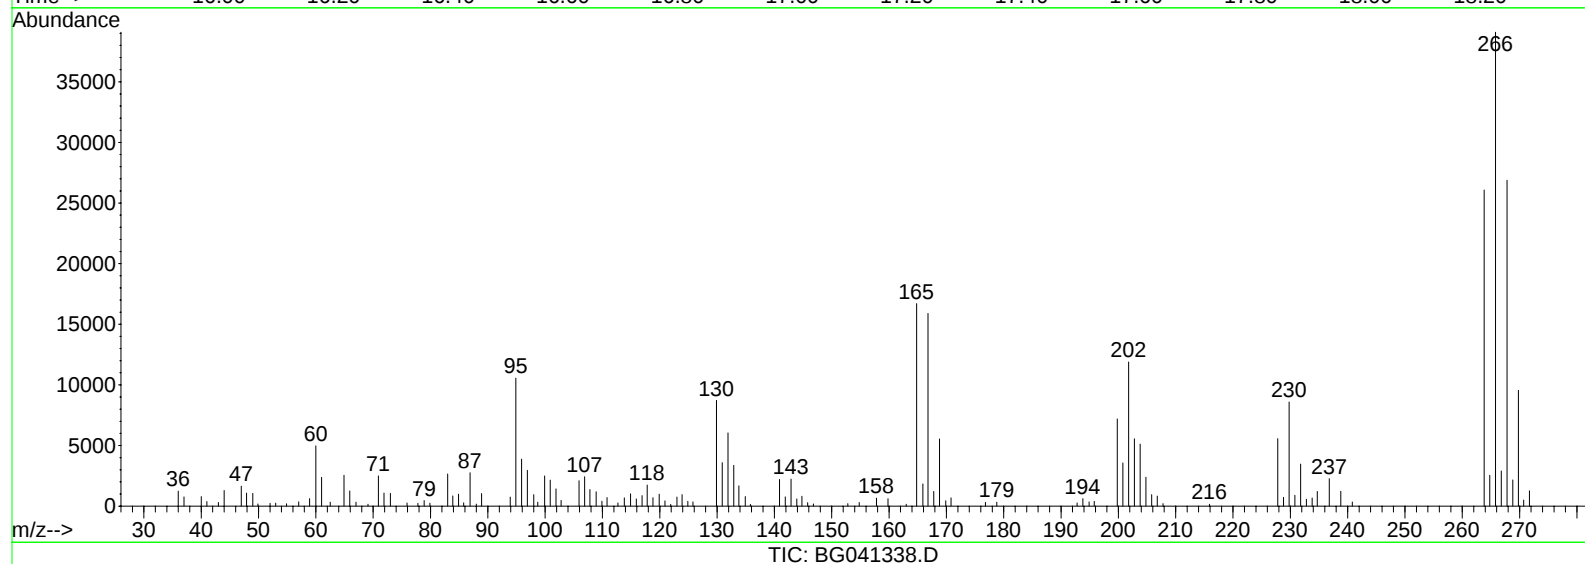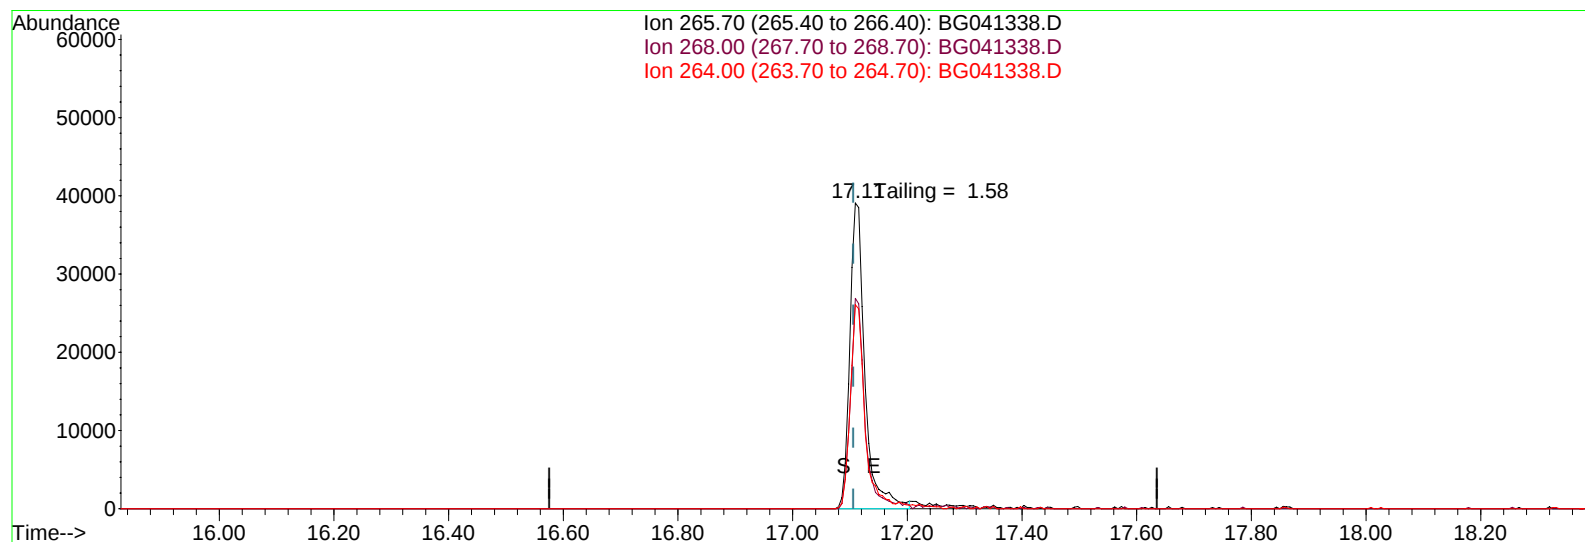

(70) Pentachlorophenol (C)

17.109min (+0.004) 38605.12ng

response 71439

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	68.79
264.00	64.00	66.72
0.00	0.00	0.00