


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061919\
 Data File : BG041320.D
 Acq On : 19 Jun 2019 9:59
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 17 14:58:02 2019

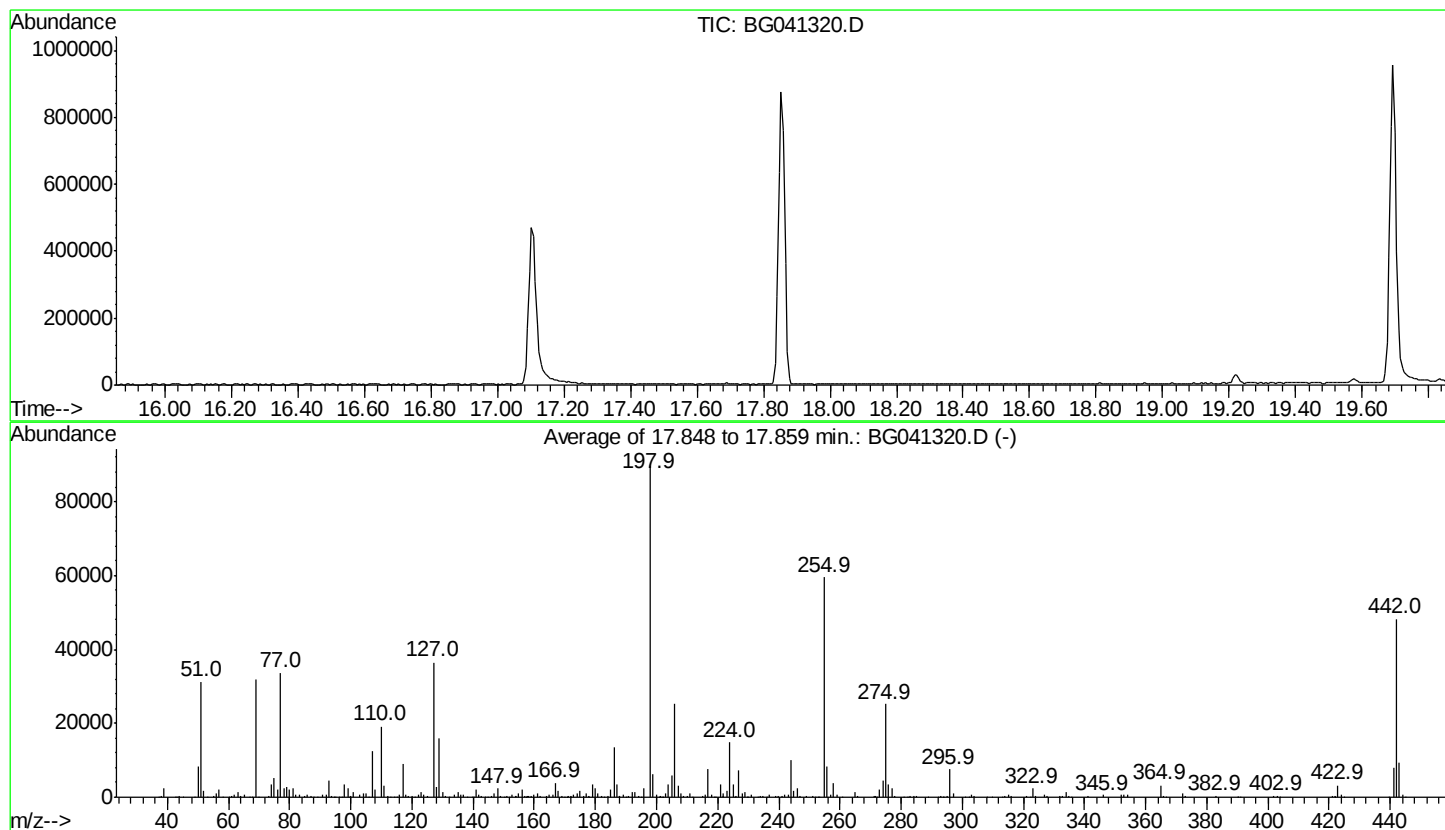

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	31202	PASS
68	69	0.00	2	0.6	187	PASS
69	198	0.00	100	35.6	31989	PASS
70	69	0.00	2	0.5	174	PASS
127	198	10	80	40.7	36520	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	89744	PASS
199	198	5	9	7.1	6334	PASS
275	198	10	60	28.1	25248	PASS
365	198	1	100	3.5	3178	PASS
441	198	0.01	100	8.8	7857	PASS
442	198	50	100	53.7	48232	PASS
443	442	15	24	19.7	9519	PASS