
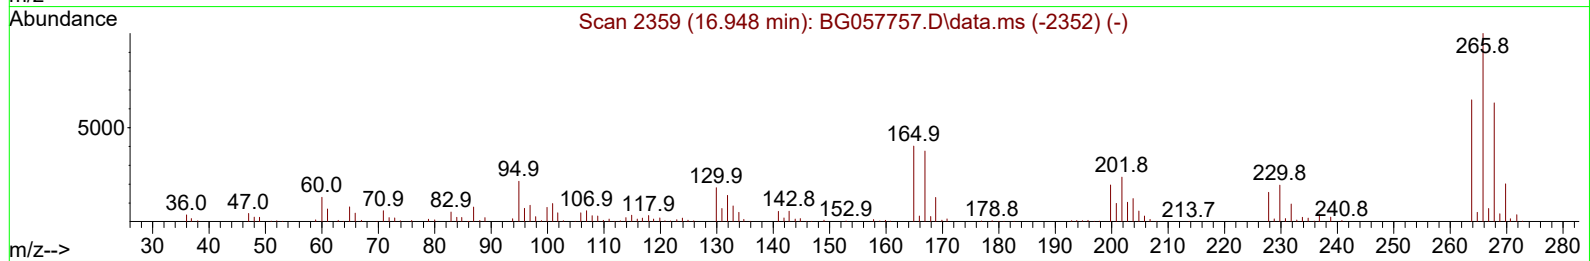
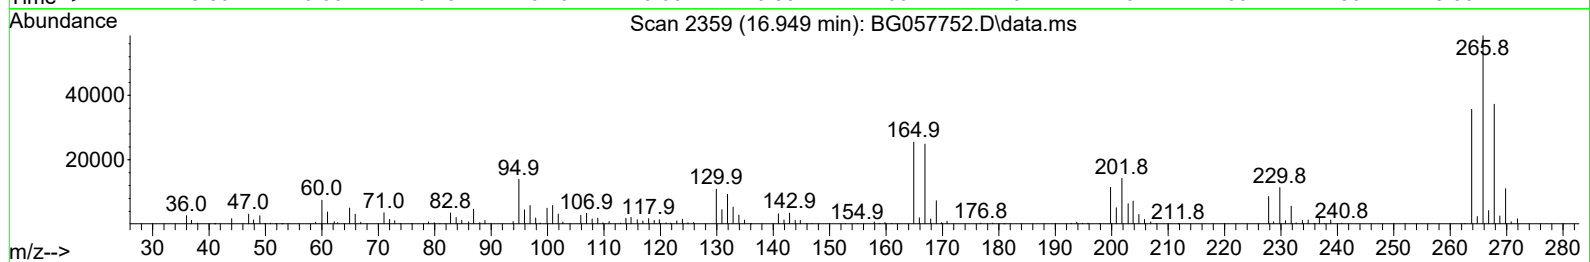


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG061923\  
Data File : BG057752.D  
Acq On : 19 Jun 2023 12:39  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 20 05:06:21 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG061923.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jun 20 03:40:38 2023  
Response via : Initial Calibration

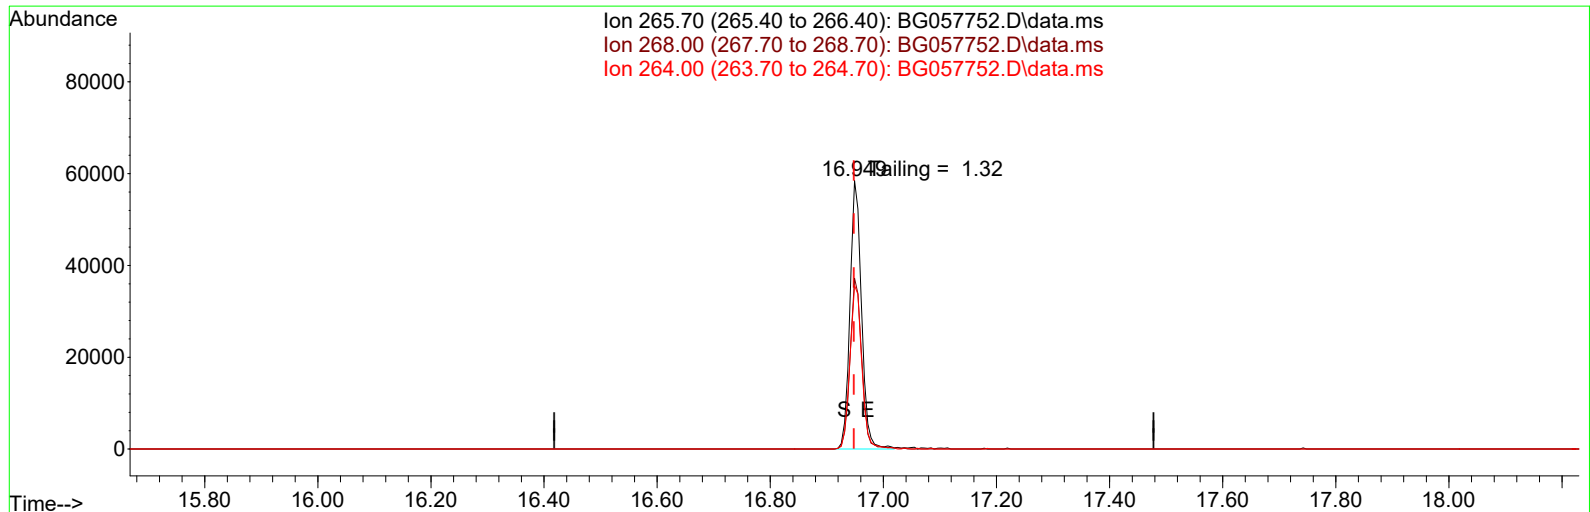

TIC: BG057752.D\data.ms

**(70) Pentachlorophenol (C)**




16.949min (+ 0.001) 0.00 ng

response 83237

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.10  | 63.64  |
| 264.00 | 64.70  | 60.92  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG061923\  
Data File : BG057752.D  
Acq On : 19 Jun 2023 12:39  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 20 05:06:21 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG061923.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jun 20 03:40:38 2023  
Response via : Initial Calibration

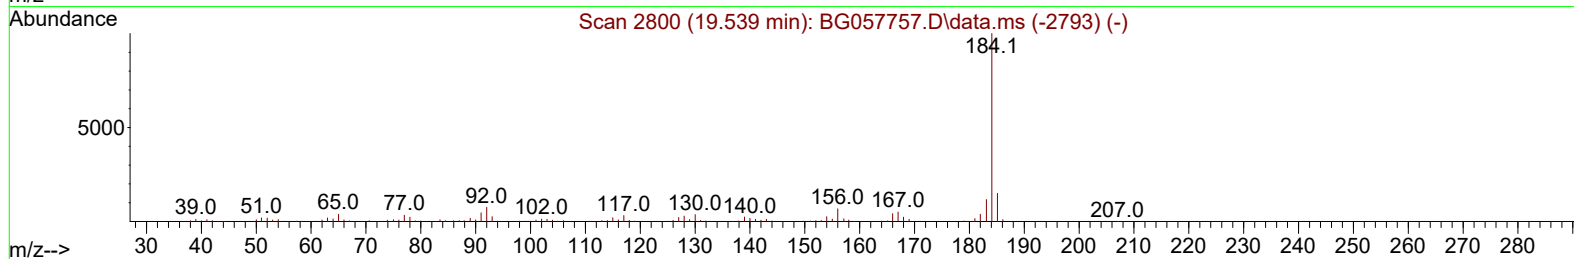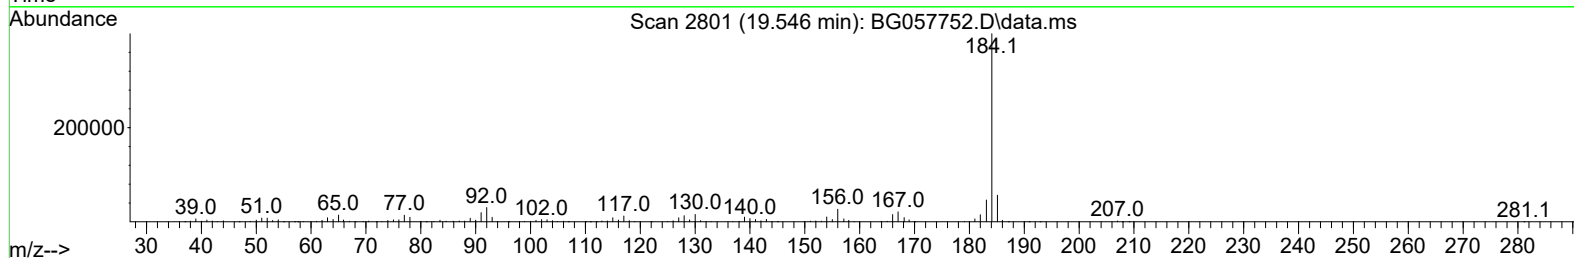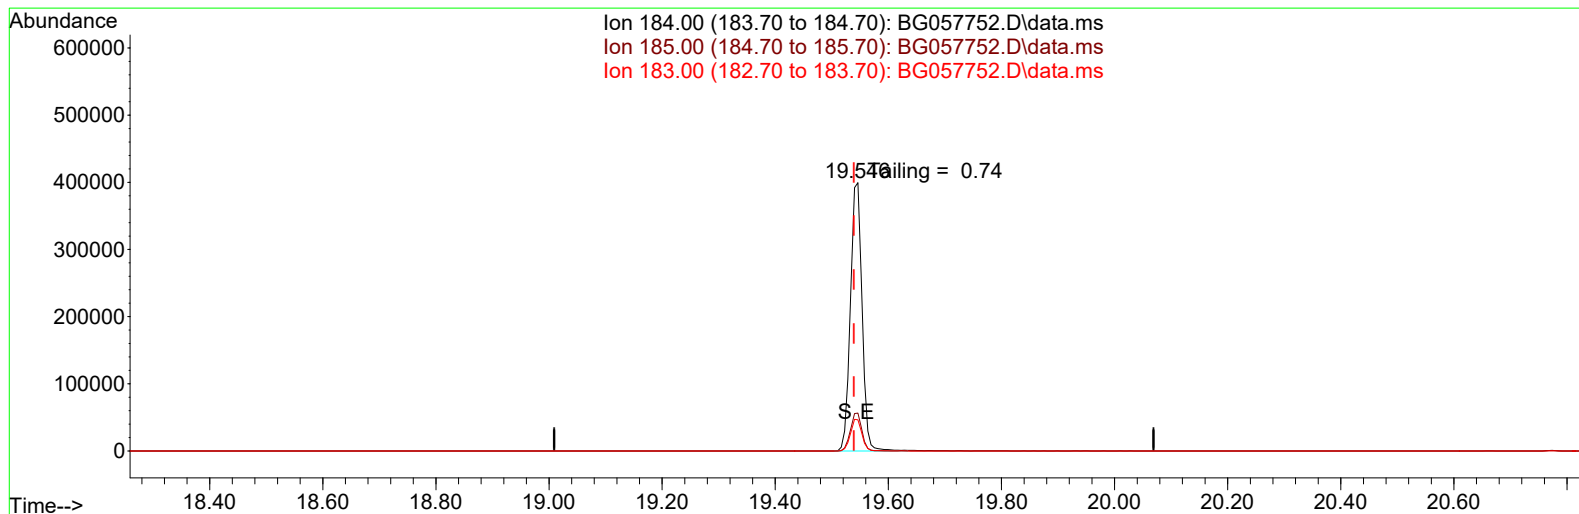

TIC: BG057752.D\data.ms

**(77) Benzidine****19.546min (+ 0.007) 0.00 ng****response 575884**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.00  | 14.17  |
| 183.00 | 11.70  | 11.65  |
| 0.00   | 0.00   | 0.00   |