


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061923\
 Data File : BG057752.D
 Acq On : 19 Jun 2023 12:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061923.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 20 03:40:38 2023

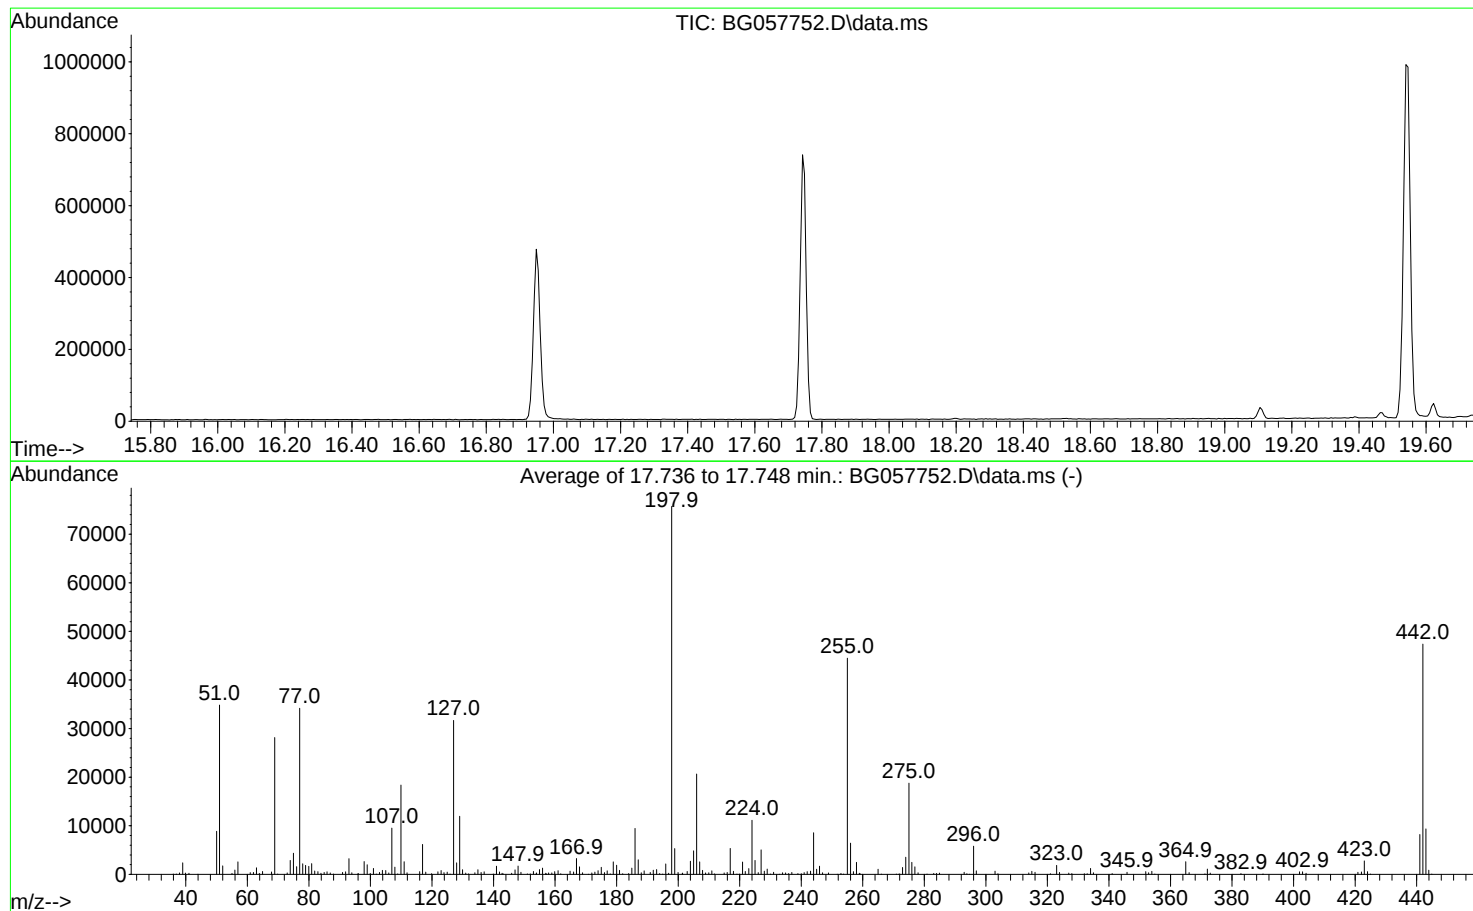

AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.0	34834	PASS
68	69	0.00	2	1.8	494	PASS
69	198	0.00	100	37.2	28157	PASS
70	69	0.00	2	0.2	69	PASS
127	198	10	80	41.9	31691	PASS
197	198	0.00	2	0.3	225	PASS
198	198	100	100	100.0	75691	PASS
199	198	5	9	7.0	5313	PASS
275	198	10	60	24.8	18775	PASS
365	198	1	100	3.4	2599	PASS
441	198	0.01	100	10.8	8206	PASS
442	442	50	100	100.0	47368	PASS
443	442	15	24	19.7	9354	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/19/2023	BNA_G	<u>BG057752.D</u>
Compound Name	Response	Retention Time
DDT	228804	20.774
DDD	2237	20.386
DDE	0	20.162
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2237	231041	0.97

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061923\
Data File : BG057752.D
Acq On : 19 Jun 2023 12:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 20 05:06:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 03:40:38 2023
Response via : Initial Calibration

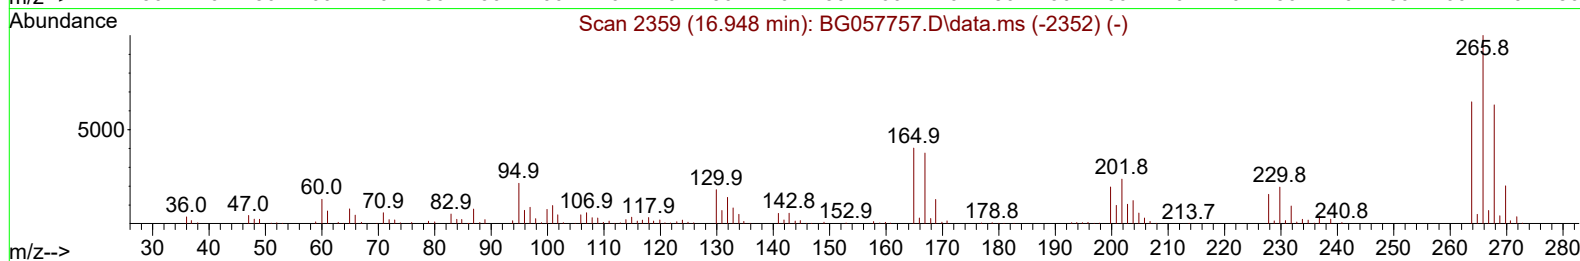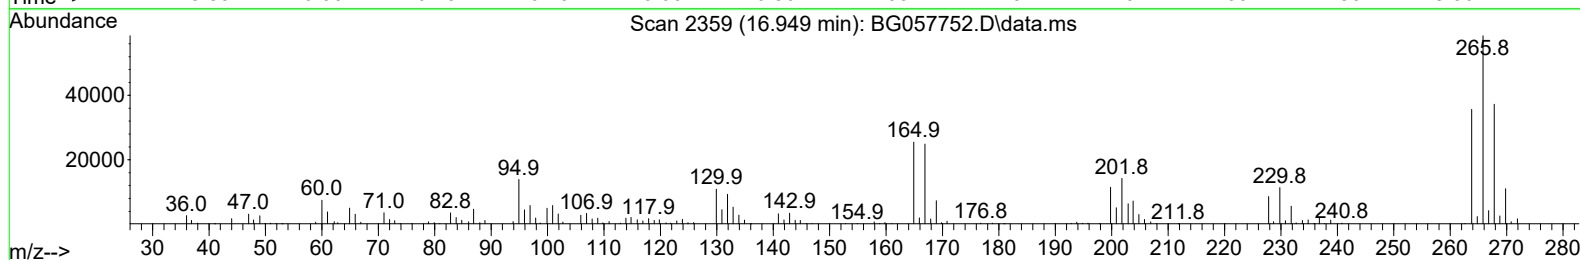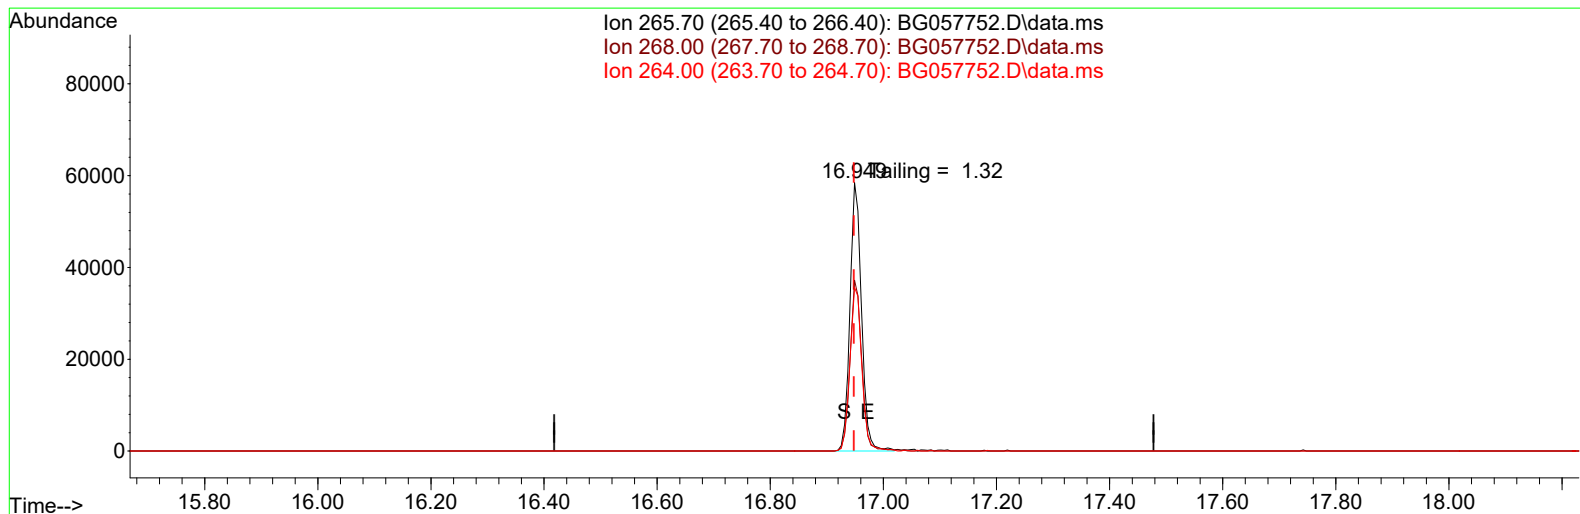

TIC: BG057752.D\data.ms

(70) Pentachlorophenol (C)

16.949min (+ 0.001) 0.00 ng




response 83237

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.64
264.00	64.70	60.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061923\
Data File : BG057752.D
Acq On : 19 Jun 2023 12:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 20 05:06:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 03:40:38 2023
Response via : Initial Calibration

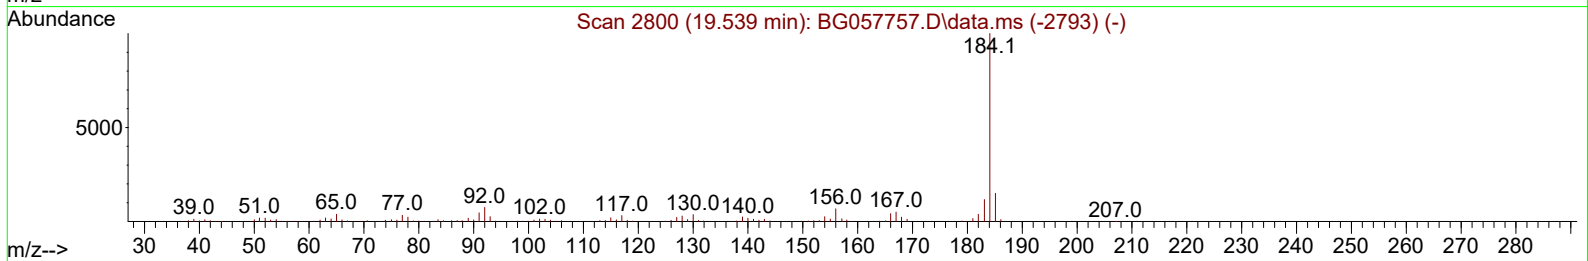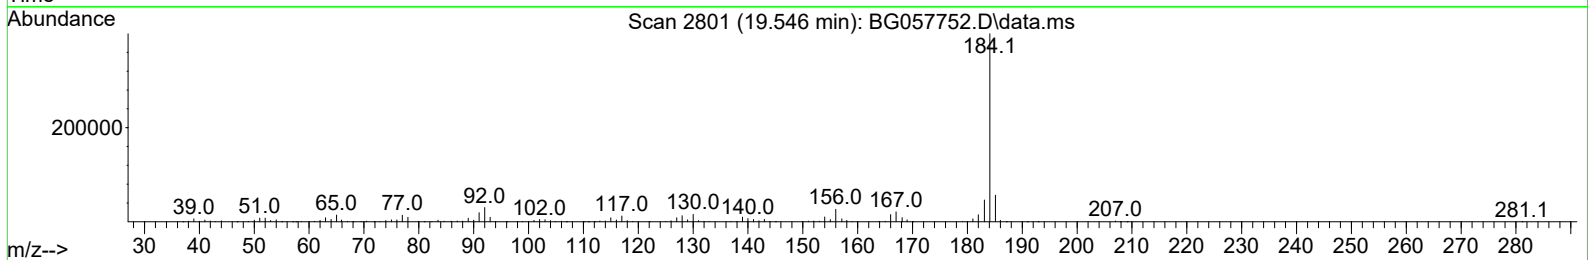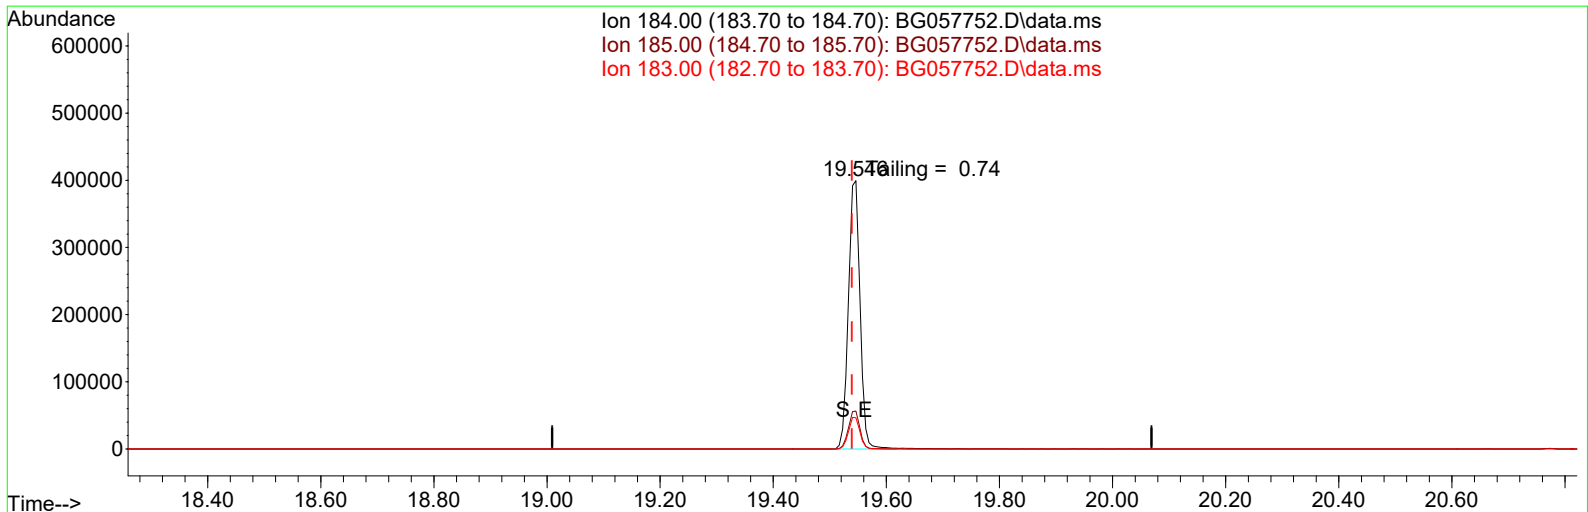

TIC: BG057752.D\data.ms

(77) Benzidine

19.546min (+ 0.007) 0.00 ng

response 575884

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.17
183.00	11.70	11.65
0.00	0.00	0.00