

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062018\
 Data File : BG035282.D
 Acq On : 21 Jun 2018 2:42
 Operator : SJ/JU
 Sample : J3245-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Jun 21 03:59:55 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 08 17:16:28 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	60428	20.00	ng	-0.02
21) Naphthalene-d8	10.86	136	207125	20.00	ng	-0.02
38) Acenaphthene-d10	14.68	164	139209	20.00	ng	-0.02
63) Phenanthrene-d10	17.42	188	388290	20.00	ng	-0.02
75) Chrysene-d12	21.69	240	425284	20.00	ng	-0.03
86) Perylene-d12	24.91	264	400098	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	474093	132.40	ng	0.00
7) Phenol-d6	7.22	99	602450	113.99	ng	0.00
23) Nitrobenzene-d5	9.22	82	477728	109.64	ng	-0.02
41) 2,4,6-Tribromophenol	16.16	330	335119	188.05	ng	-0.02
44) 2-Fluorobiphenyl	13.30	172	1071892	100.10	ng	-0.02
78) Terphenyl-d14	20.03	244	1957701	96.42	ng	-0.02
Target Compounds						
19) n-Nitroso-di-n-propylamine	9.22	70	63375	14.115	ng	# 69
50) 2,6-Dinitrotoluene	14.67	165	19389	8.755	ng	# 18
56) 2,4-Dinitrotoluene	14.67	165	19389	6.591	ng	# 16
66) 4-Bromophenyl-phenylether	16.16	248	26312	5.627	ng	# 1
76) Benzidine	20.03	184	33963	2.147	ng	# 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062018\
Data File : BG035282.D
Acq On : 21 Jun 2018 2:42
Operator : SJ/JU
Sample : J3245-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Jun 21 03:59:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

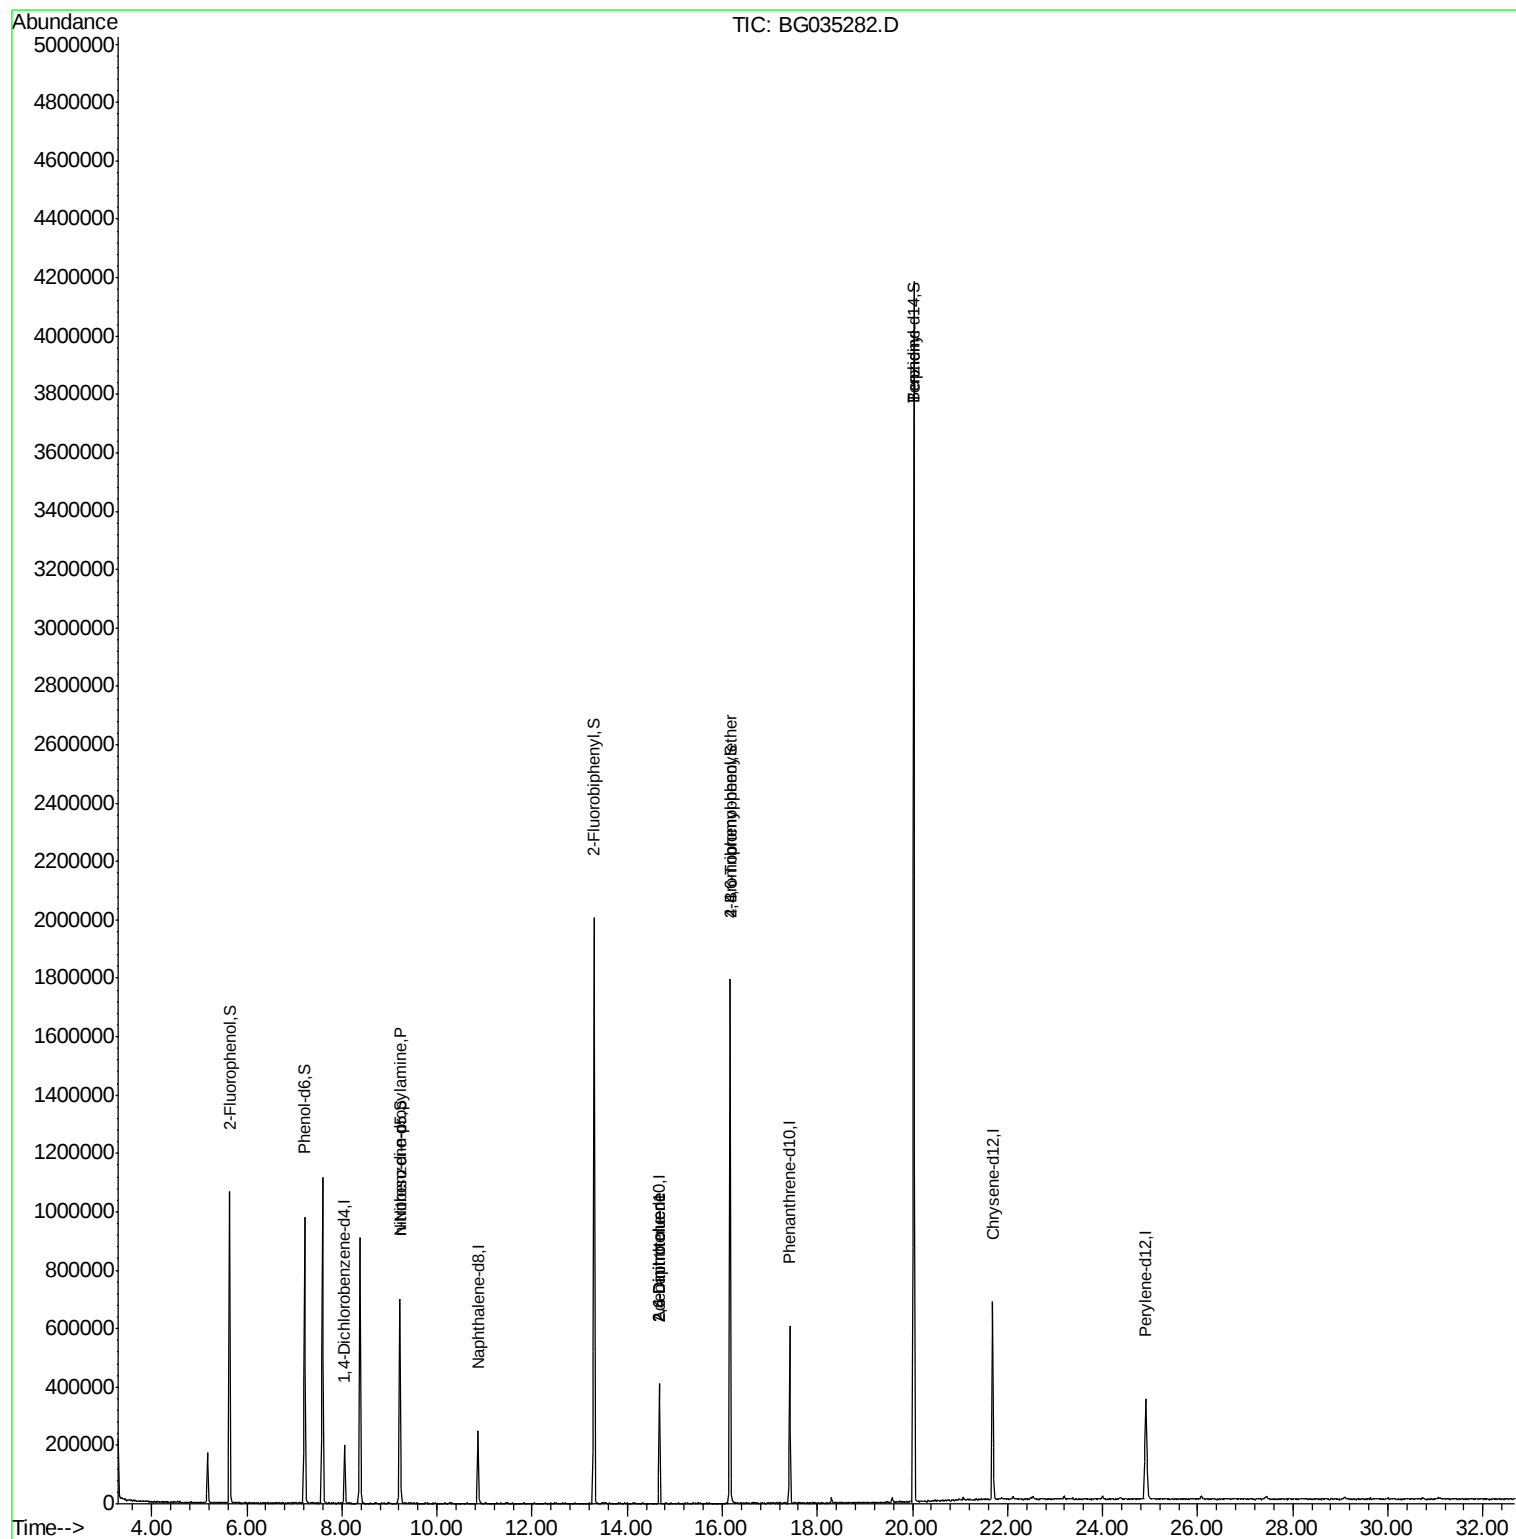






#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.06 min Scan# 812
Delta R.T. -0.02 min
Lab File: BG035282.D
Acq: 21 Jun 2018 2:42

Instrument :
BNA_G
ClientSampled :




Tot Ion:152 Resp: 60428
Ion Ratio Lower Upper
152 100
150 146.3 126.6 189.8
115 62.0 53.0 79.4

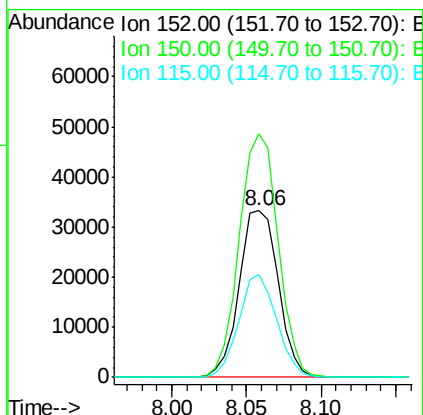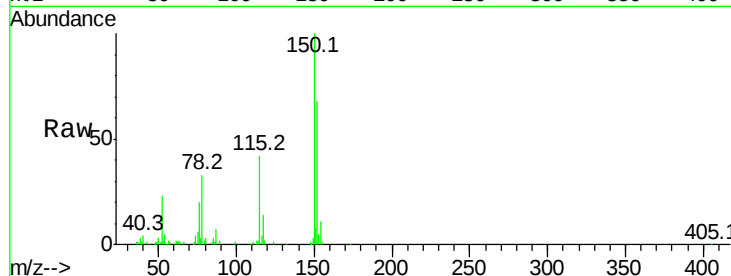


#5

2-Fluorophenol
Concen: 132.403 ng
RT: 5.64 min Scan# 400
Delta R.T. -0.01 min
Lab File: BG035282.D
Acq: 21 Jun 2018 2:42

Tgt Ion:112 Resp: 474093
Ion Ratio Lower Upper
112 100
64 61.7 56.3 84.5
63 35.5 30.1 45.1

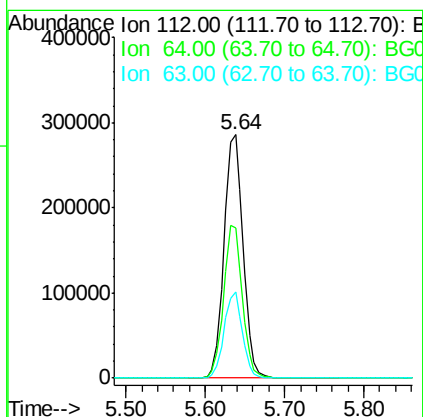

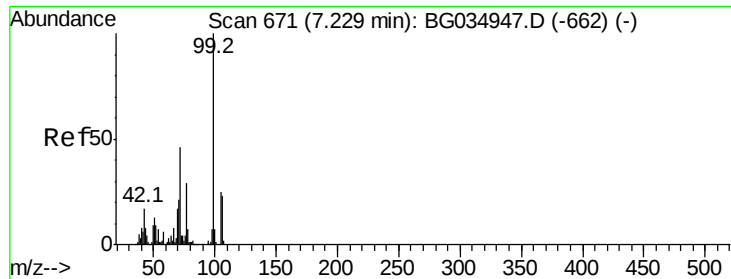

#7

Phenol-d6

Concen: 113.995 ng

RT: 7.22 min Scan# 669

Delta R.T. -0.01 min

Lab File: BG035282.D

Acq: 21 Jun 2018 2:42

Instrument :

BNA_G

ClientSampleId :





Tot Ion: 99 Resp: 602450

Ion Ratio Lower Upper

99 100

42 14.7 14.1 21.1

71 42.5 26.1 39.1#

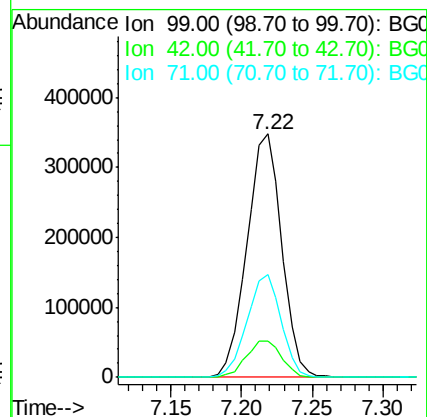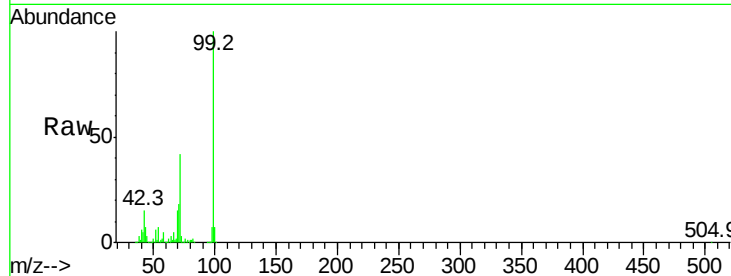

#19

n-Nitroso-di-n-propylamine

Concen: 14.115 ng

RT: 9.22 min Scan# 1009

Delta R.T. 0.33 min

Lab File: BG035282.D

Acq: 21 Jun 2018 2:42

Tgt Ion: 70 Resp: 63375




Ion Ratio Lower Upper


70 100

42 38.4 49.1 73.7#

101 0.0 8.5 12.7#

130 1.8 13.4 20.0#

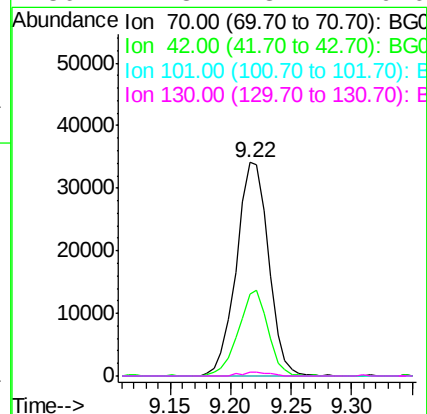


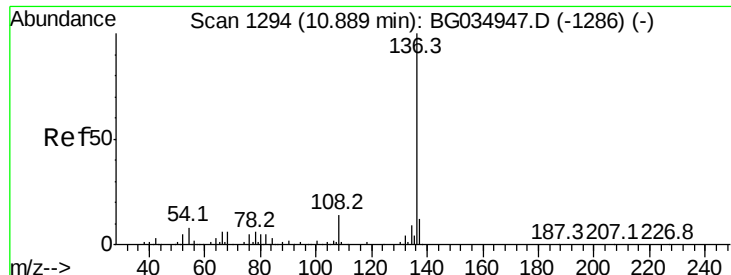




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.86 min Scan# 1289
Delta R.T. -0.02 min
Lab File: BG035282.D
Acq: 21 Jun 2018 2:42

Instrument :
BNA_G
ClientSampleId :

Tot Ion:	136	Resp:	207125
Ion	Ratio	Lower	Upper
136	100		
137	10.1	9.2	13.8
54	6.3	10.3	15.5#
68	4.6	4.5	6.7

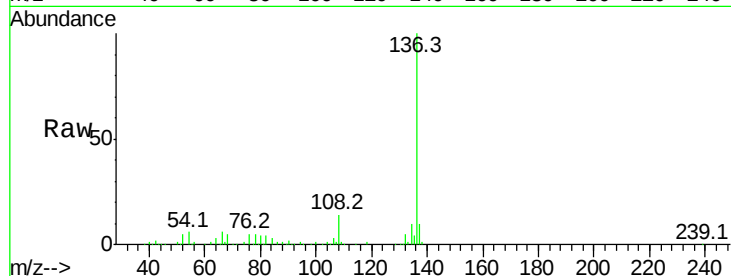


Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

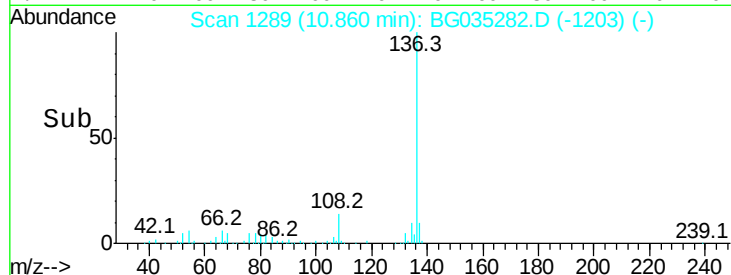
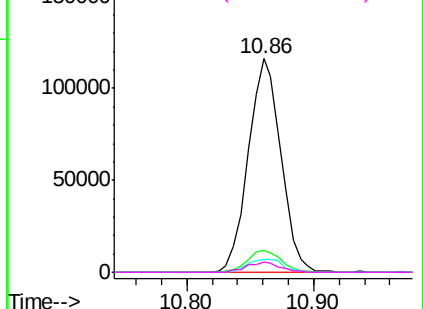



#23
Nitrobenzene-d5
Concen: 109.637 ng
RT: 9.22 min Scan# 1009
Delta R.T. -0.02 min
Lab File: BG035282.D
Acq: 21 Jun 2018 2:42

Tgt Ion:	82	Resp:	477728
Ion	Ratio	Lower	Upper
82	100		
128	31.9	29.7	44.5
54	41.4	43.1	64.7#

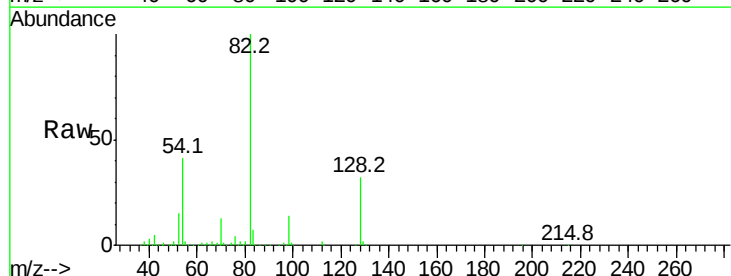

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

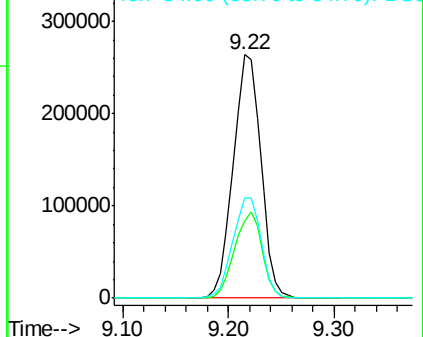



#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.68 min Scan# 1939

Delta R.T. -0.02 min

Lab File: BG035282.D

Acq: 21 Jun 2018 2:42

Instrument :

BNA_G

ClientSampleId :


Tot Ion:164 Resp: 139209

Ion Ratio Lower Upper

164 100

162 104.8 78.8 118.2




160 45.3 35.4 53.0



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

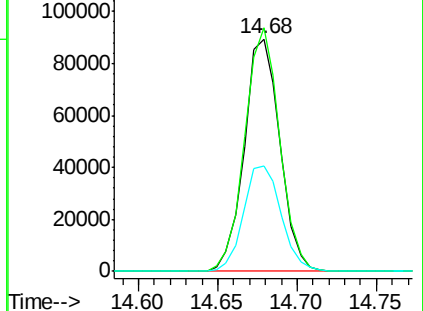

#41

2,4,6-Tribromophenol

Concen: 188.052 ng

RT: 16.16 min Scan# 2192

Delta R.T. -0.02 min

Lab File: BG035282.D

Acq: 21 Jun 2018 2:42


Tgt Ion:330 Resp: 335119

Ion Ratio Lower Upper

330 100

332 96.0 77.0 115.6



141 36.9 25.2 37.8




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

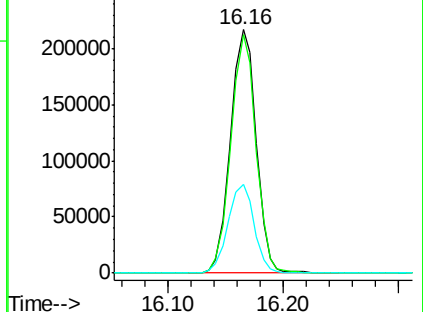




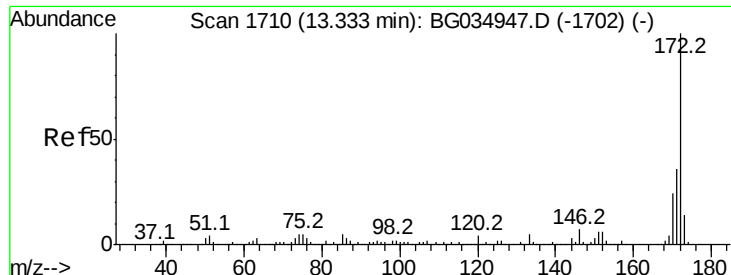


#44
 2-Fluorobiphenyl
 Concen: 100.098 ng
 RT: 13.30 min Scan# 1705
 Delta R.T. -0.02 min
 Lab File: BG035282.D
 Acq: 21 Jun 2018 2:42

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion:172 Resp: 1071892




Ion	Ratio	Lower	Upper
172	100		
171	35.8	30.0	45.0
170	23.9	19.5	29.3

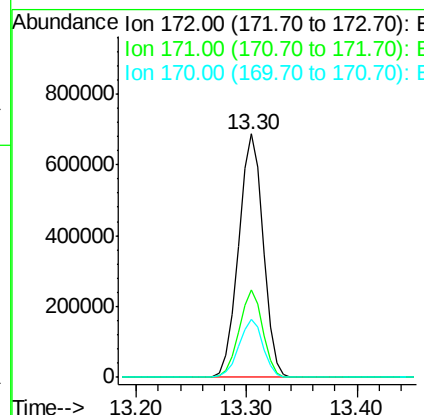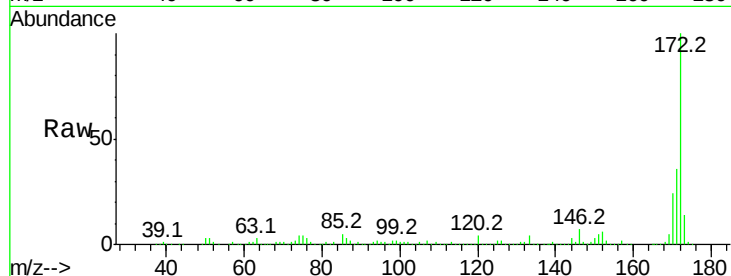


#50
 2,6-Dinitrotoluene
 Concen: 8.755 ng
 RT: 14.67 min Scan# 1938
 Delta R.T. 0.41 min
 Lab File: BG035282.D
 Acq: 21 Jun 2018 2:42

Tgt Ion:165 Resp: 19389

Ion	Ratio	Lower	Upper
165	100		
63	0.0	52.7	79.1#
89	0.0	49.2	73.8#

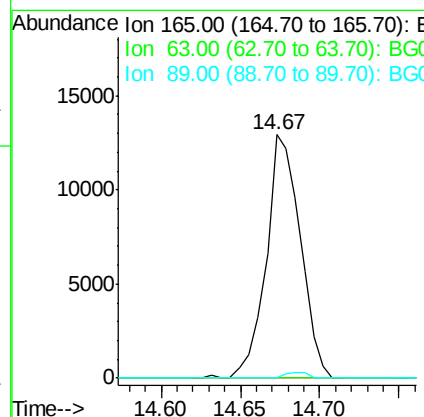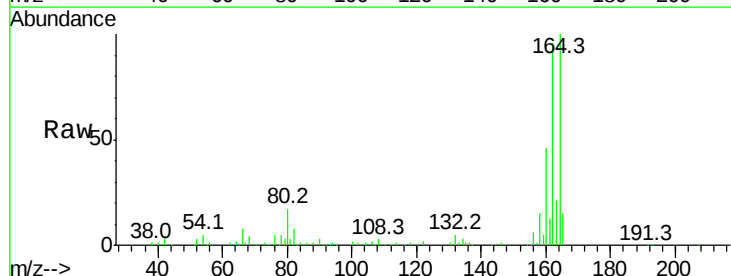


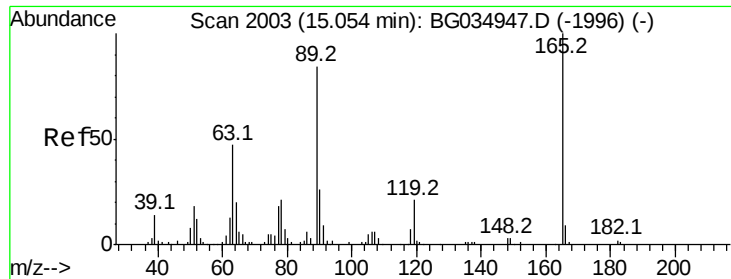

#56
 2,4-Dinitrotoluene
 Concen: 6.591 ng
 RT: 14.67 min Scan# 1938
 Delta R.T. -0.38 min
 Lab File: BG035282.D
 Acq: 21 Jun 2018 2:42

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion:	165	Resp:	19389
Ion	Ratio	Lower	Upper
165	100		
63	0.0	42.0	63.0#
89	0.0	66.9	100.3#
182	0.0	2.6	3.8#






Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BGC


Ion 89.00 (88.70 to 89.70): BGC

Ion 182.00 (181.70 to 182.70): E

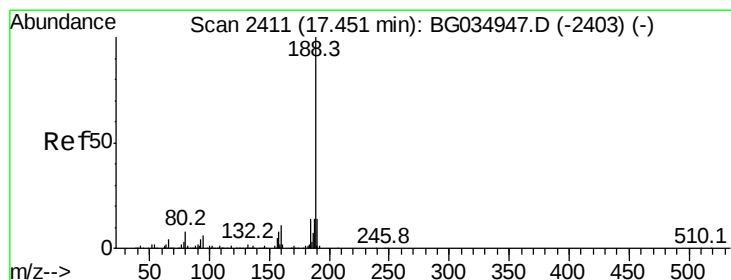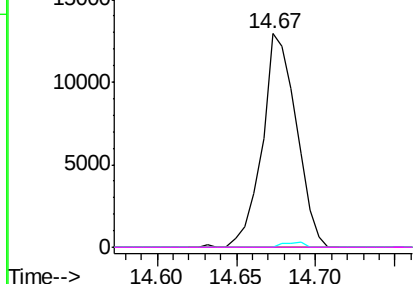

#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.42 min Scan# 2406
 Delta R.T. -0.02 min
 Lab File: BG035282.D
 Acq: 21 Jun 2018 2:42



Tgt Ion:	188	Resp:	388290
Ion	Ratio	Lower	Upper
188	100		
94	5.4	6.9	10.3#
80	7.1	7.7	11.5#



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC



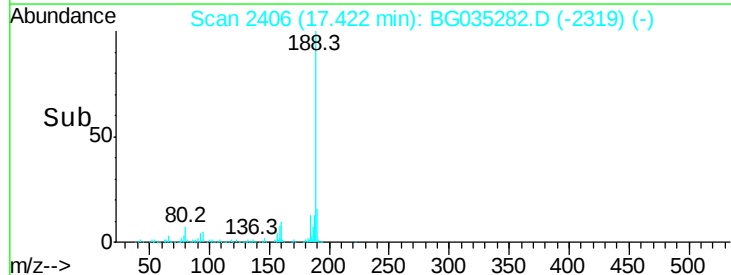
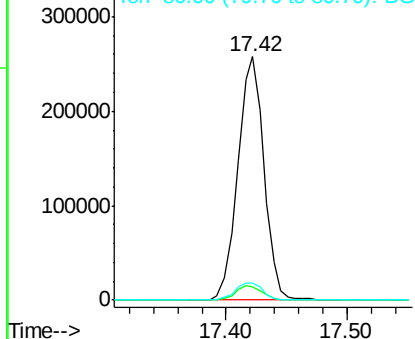




#66
4-Bromophenyl-phenylether
Concen: 5.627 ng
RT: 16.16 min Scan# 2192
Delta R.T. -0.47 min
Lab File: BG035282.D
Acq: 21 Jun 2018 2:42




Instrument :
BNA_G
ClientSampled :


Tot Ion:248 Resp: 26312
Ion Ratio Lower Upper
248 100
250 185.2 77.1 115.7#
141 427.3 50.8 76.2#

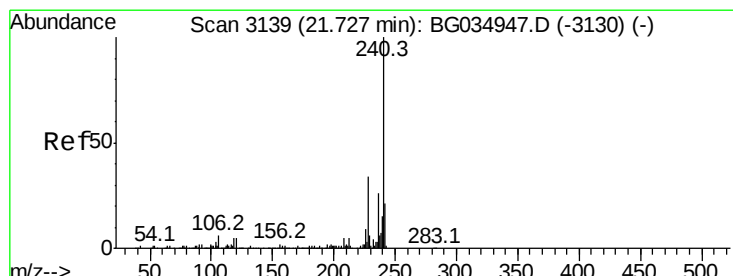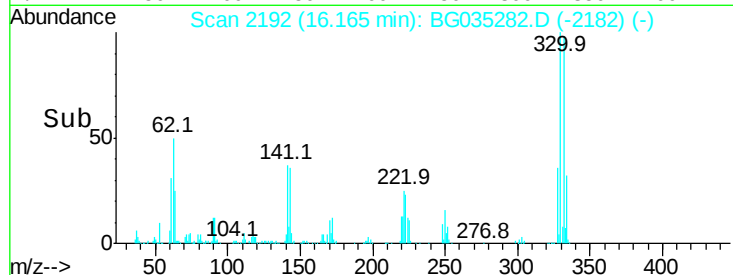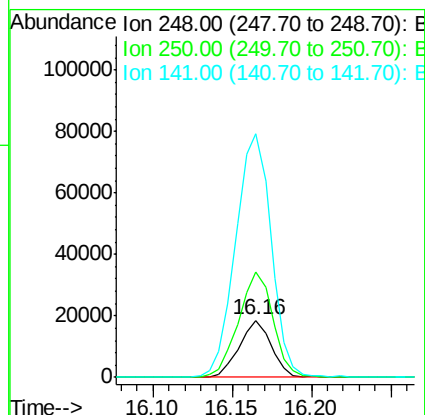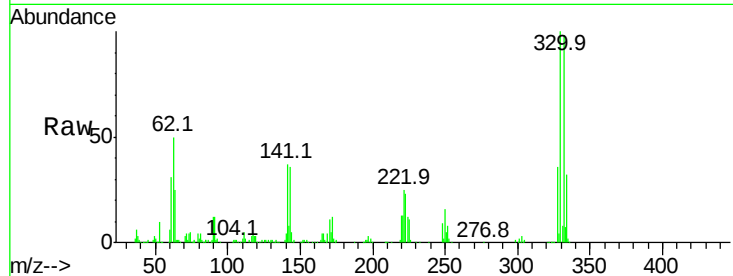

#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.69 min Scan# 3132
Delta R.T. -0.03 min
Lab File: BG035282.D
Acq: 21 Jun 2018 2:42

Tgt Ion:240 Resp: 425284
Ion Ratio Lower Upper
240 100
120 5.0 6.8 10.2#
236 26.7 20.9 31.3

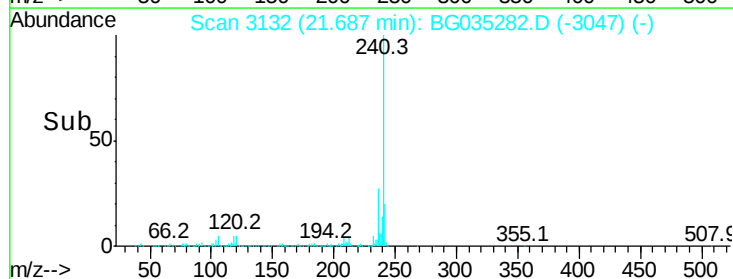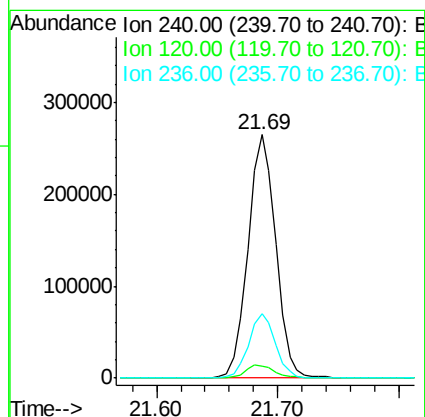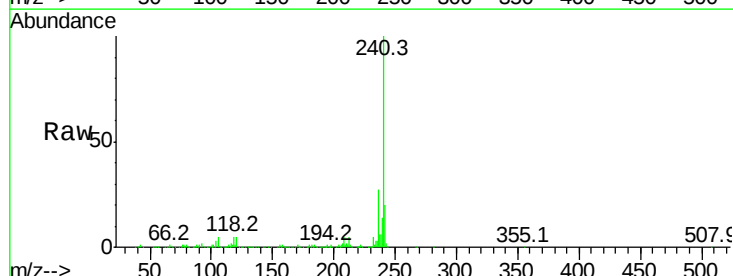



#76

Benzidine

Concen: 2.147 ng

RT: 20.03 min Scan# 2850

Delta R.T. 0.36 min

Lab File: BG035282.D

Acq: 21 Jun 2018 2:42

Instrument :

BNA_G

ClientSampleId :


Tot Ion:184 Resp: 33963

Ion Ratio Lower Upper

184 100

185 19.0 11.1 16.7#




183 9.3 10.6 16.0#

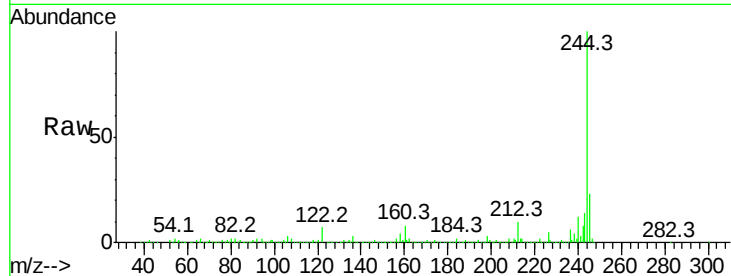

Abundance Ion 184.00 (183.70 to 184.70): E

Ion 185.00 (184.70 to 185.70): E

Ion 183.00 (182.70 to 183.70): E

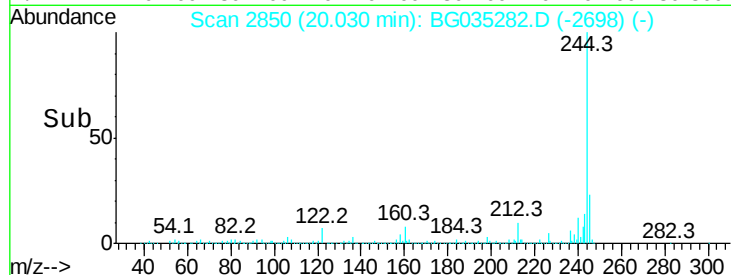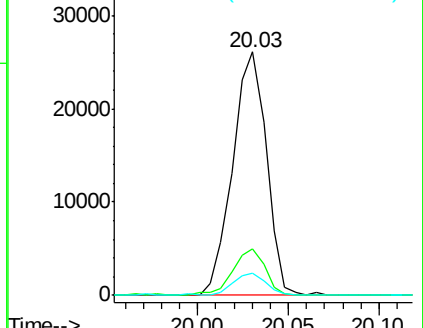

#78

Terphenyl-d14

Concen: 96.424 ng

RT: 20.03 min Scan# 2850

Delta R.T. -0.02 min

Lab File: BG035282.D

Acq: 21 Jun 2018 2:42


Tgt Ion:244 Resp: 1957701

Ion Ratio Lower Upper

244 100

212 9.8 5.8 8.8#



122 6.8 7.0 10.4#




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

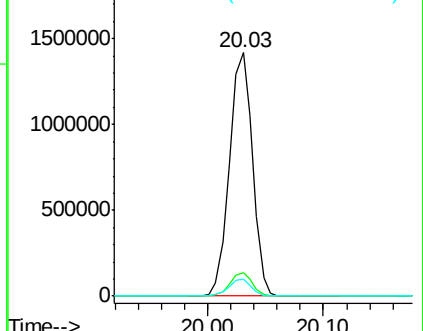


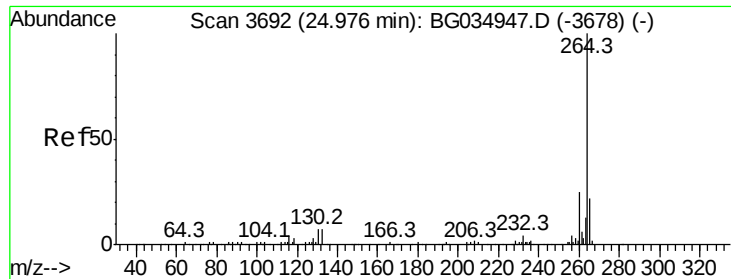

#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 24.91 min Scan# 3680
 Delta R.T. -0.05 min
 Lab File: BG035282.D
 Acq: 21 Jun 2018 2:42

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.0	17.4	26.0
265	20.7	17.7	26.5

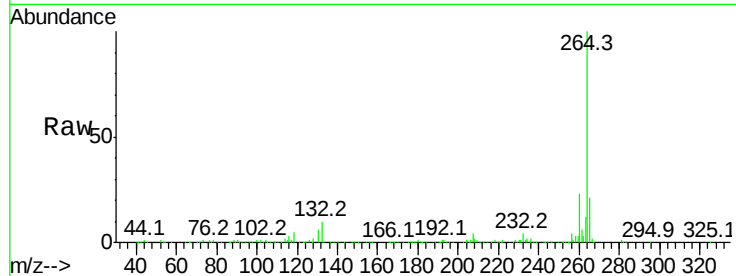

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

