

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG062018\
Quantitation Report (QT/LSC Reviewed)

Data File : BG035268.D
Acq On : 20 Jun 2018 16:18
Operator : SJ/JU
Sample : J3249-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PL-01-061818-A

Quant Time: Jun 20 17:10:48 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	50208	20.00	ng	-0.02
21) Naphthalene-d8	10.86	136	169561	20.00	ng	-0.02
38) Acenaphthene-d10	14.68	164	118699	20.00	ng	-0.02
63) Phenanthrene-d10	17.42	188	351297	20.00	ng	-0.02
75) Chrysene-d12	21.69	240	419408	20.00	ng	-0.03
86) Perylene-d12	24.91	264	407473	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.63	112	389301	130.85	ng	-0.01
7) Phenol-d6	7.21	99	502014	114.33	ng	-0.01
23) Nitrobenzene-d5	9.22	82	388179	108.82	ng	-0.02
41) 2,4,6-Tribromophenol	16.17	330	294924	194.09	ng	-0.02
44) 2-Fluorobiphenyl	13.31	172	898292	98.38	ng	-0.02
78) Terphenyl-d14	20.03	244	1897697	94.78	ng	-0.02


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BG035268.D
Acq On : 20 Jun 2018 16:18
Operator : SJ/JU
Sample : J3249-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PL-01-061818-A

Quant Time: Jun 20 17:10:48 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

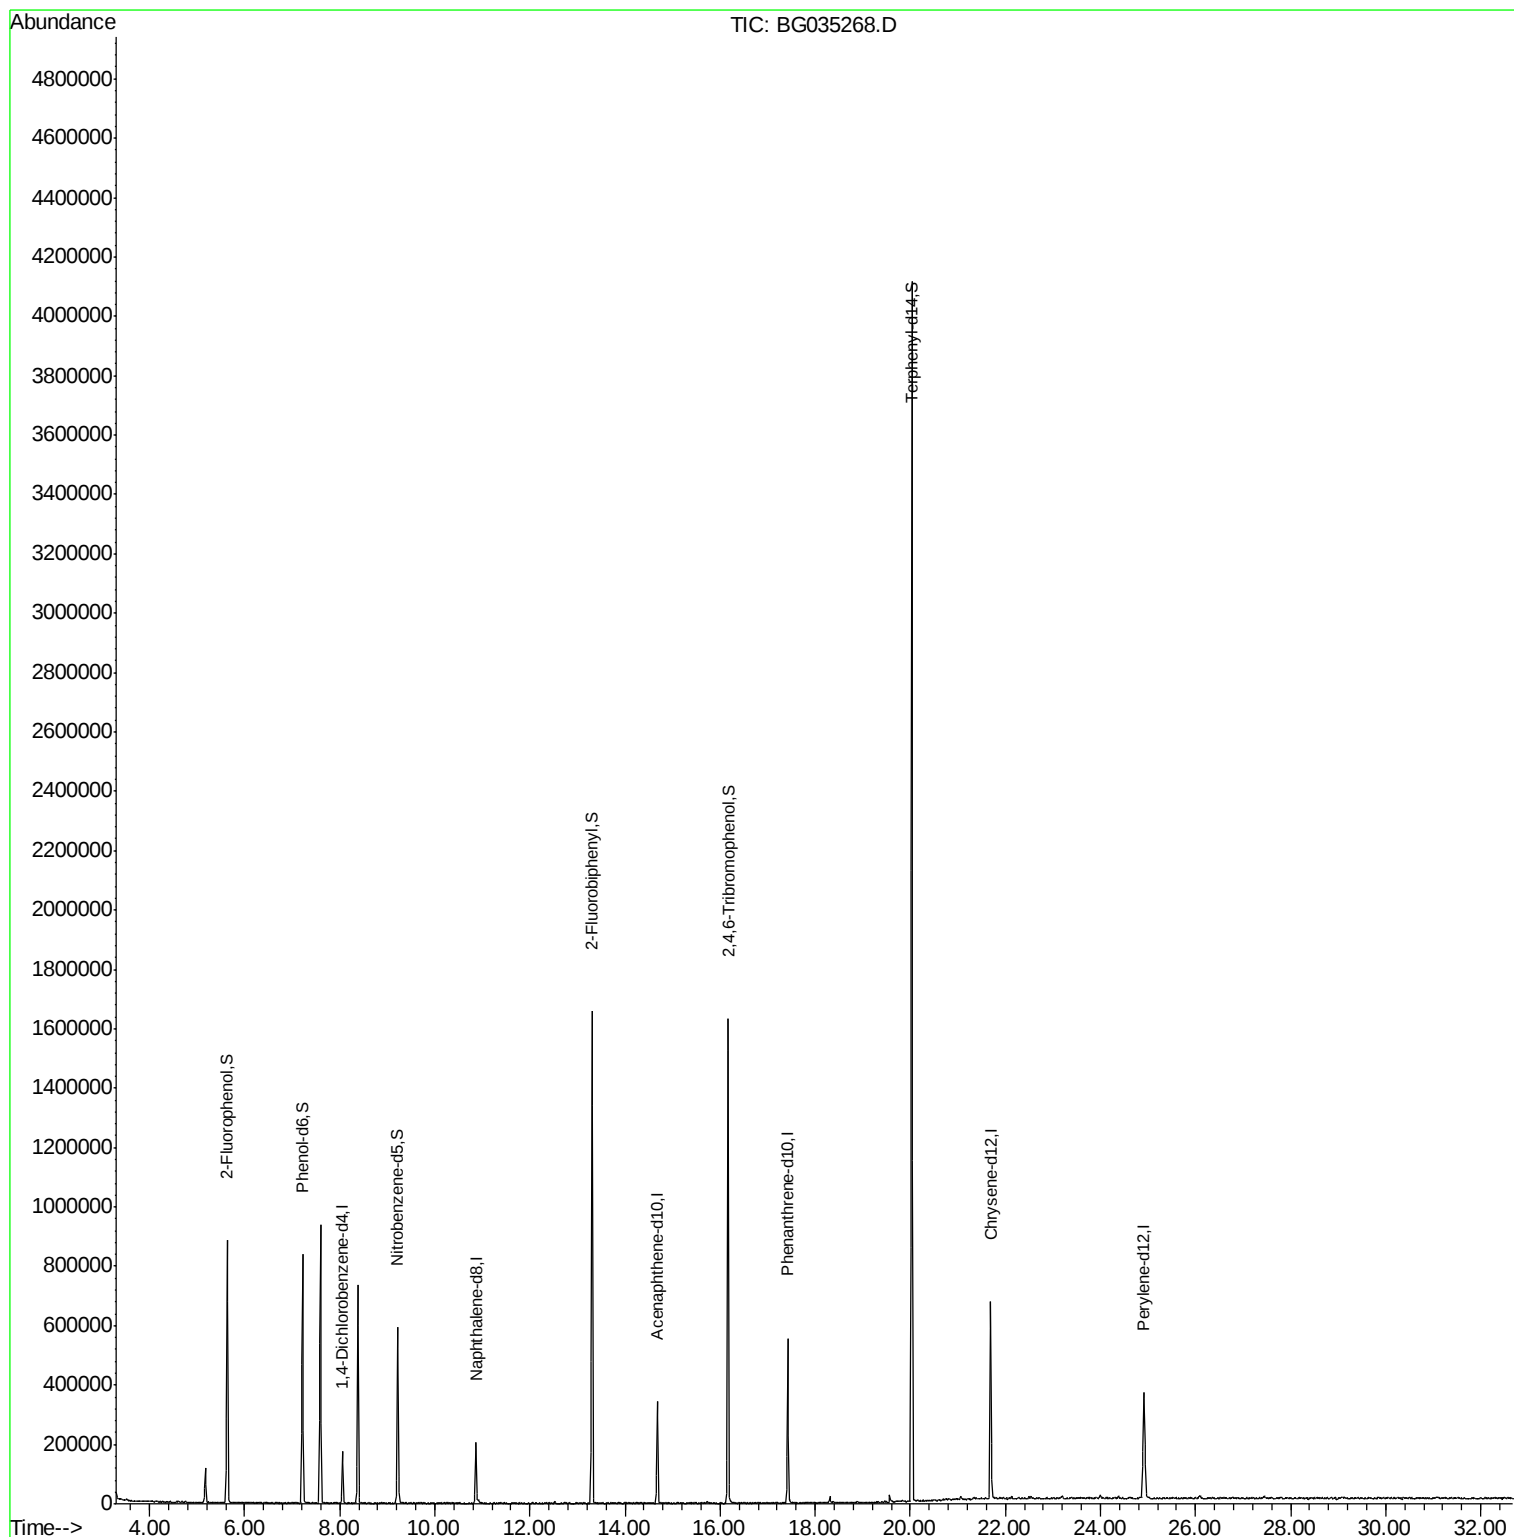

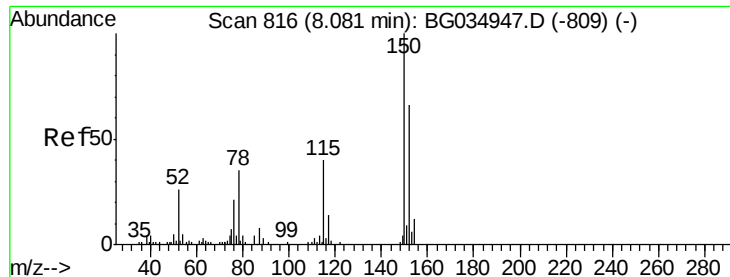


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.05 min Scan# 811
Delta R.T. -0.02 min
Lab File: BG035268.D
Acq: 20 Jun 2018 16:18

Instrument :
BNA_G
ClientSampleId :
PL-01-061818-A

Tgt Ion:152 Resp: 50208
Ion Ratio Lower Upper
152 100
150 131.8 126.6 189.8
115 55.7 53.0 79.4

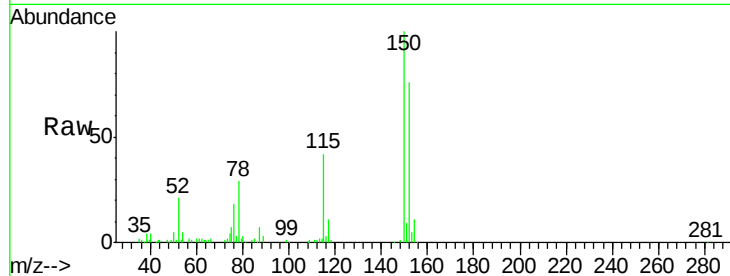


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

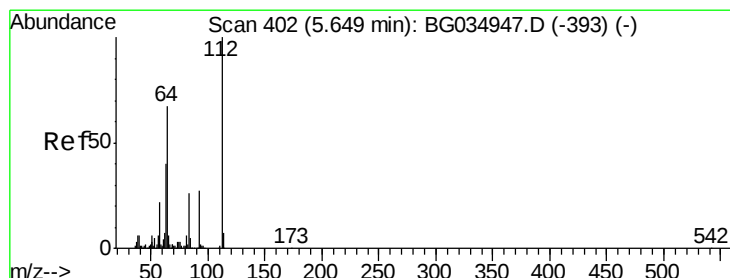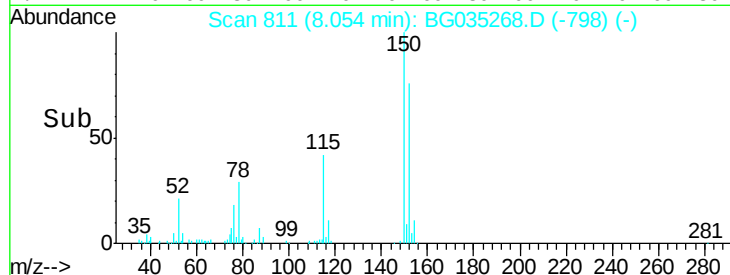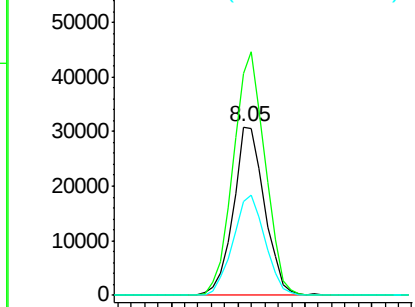



#5


2-Fluorophenol
Concen: 130.853 ng
RT: 5.63 min Scan# 399
Delta R.T. -0.01 min
Lab File: BG035268.D
Acq: 20 Jun 2018 16:18

Tgt Ion:112 Resp: 389301
Ion Ratio Lower Upper
112 100
64 63.5 56.3 84.5
63 35.1 30.1 45.1

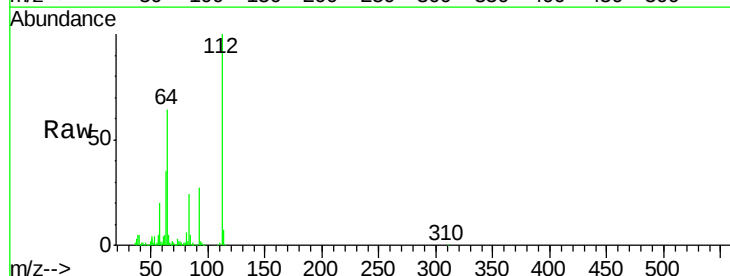

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

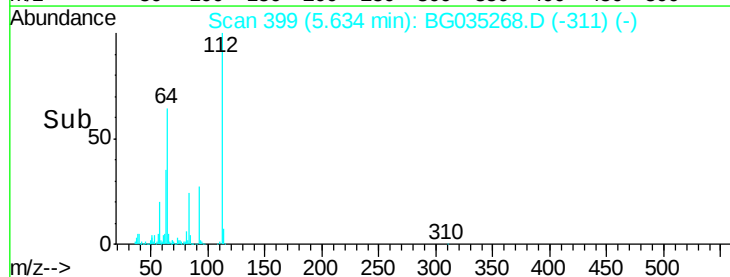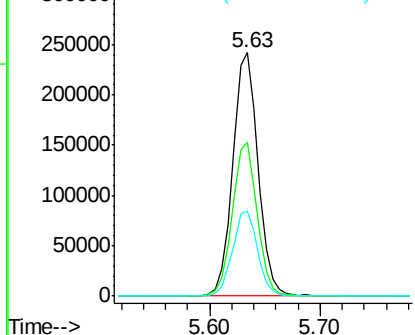

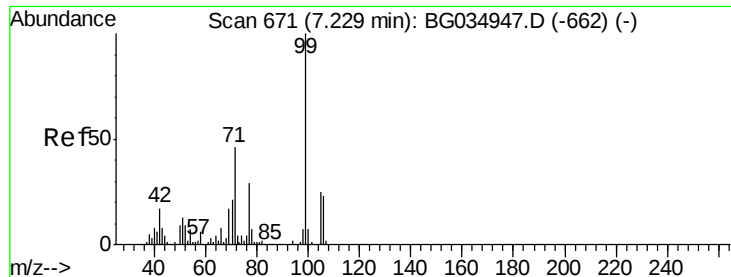

#7

Phenol-d6

Concen: 114.326 ng

RT: 7.21 min Scan# 668

Delta R.T. -0.01 min

Lab File: BG035268.D

Acq: 20 Jun 2018 16:18

Instrument :

BNA_G

ClientSampleId :

PL-01-061818-A


Tgt Ion: 99 Resp: 502014

Ion Ratio Lower Upper




99 100

42 17.3 14.1 21.1

71 41.8 26.1 39.1#

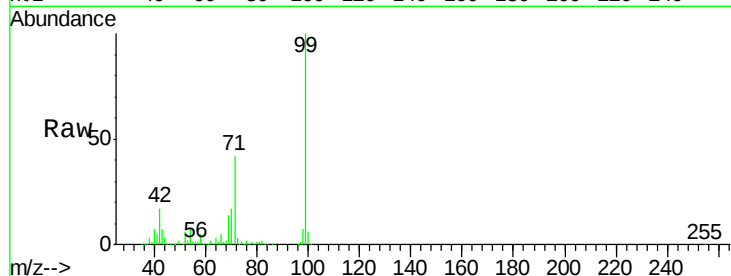

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

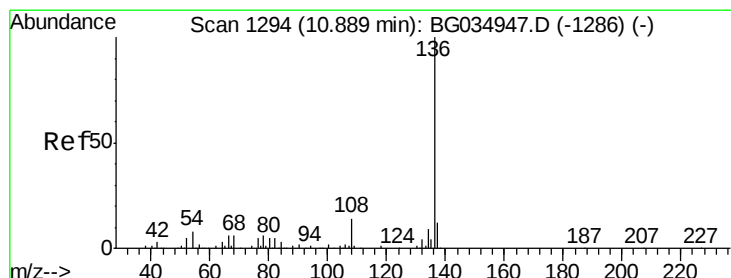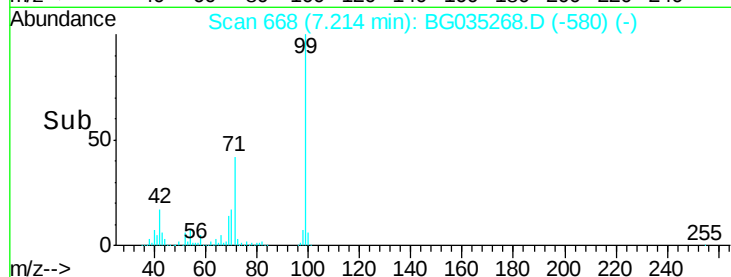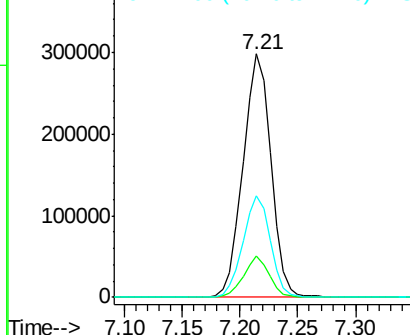

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.86 min Scan# 1289

Delta R.T. -0.02 min

Lab File: BG035268.D

Acq: 20 Jun 2018 16:18

Tgt Ion: 136 Resp: 169561


Ion Ratio Lower Upper

136 100



137 11.8 9.2 13.8


54 5.3 10.3 15.5#

68 4.6 4.5 6.7

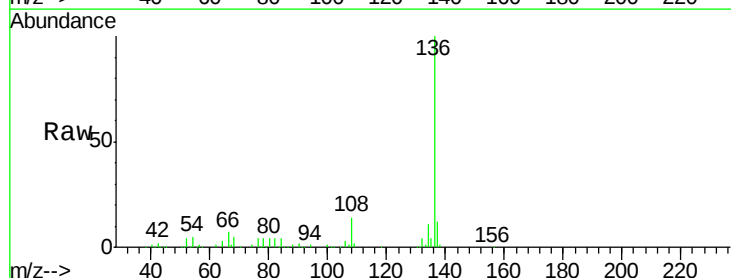

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



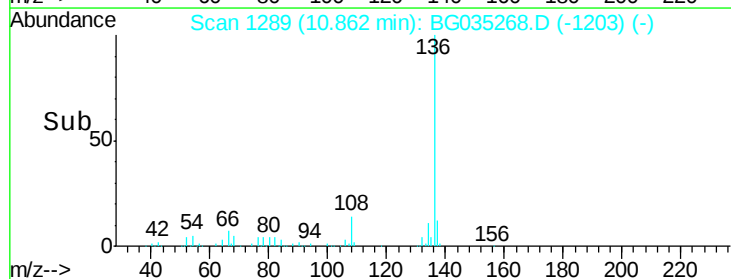
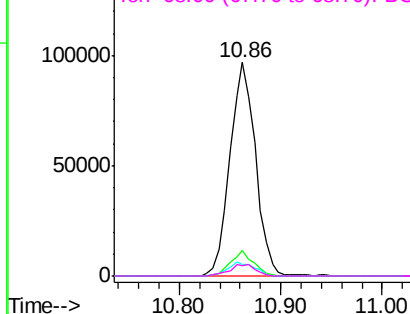


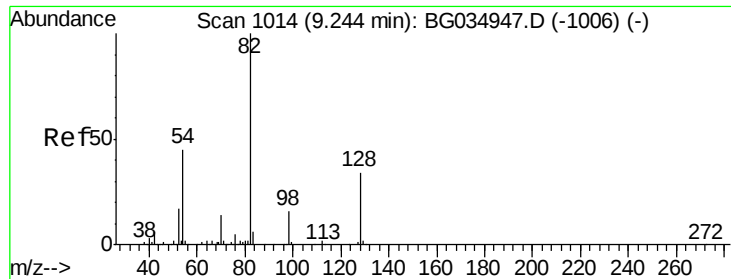

#23
 Nitrobenzene-d5
 Concen: 108.821 ng
 RT: 9.22 min Scan# 1009
 Delta R.T. -0.02 min
 Lab File: BG035268.D
 Acq: 20 Jun 2018 16:18




Instrument :
 BNA_G
 ClientSampleId :
 PL-01-061818-A


Tgt Ion	Ratio	Lower	Upper
82	100		
128	34.5	29.7	44.5
54	42.4	43.1	64.7

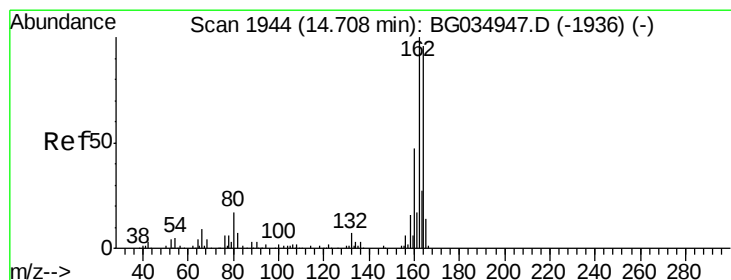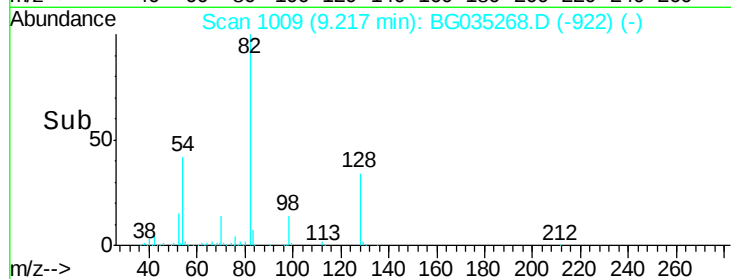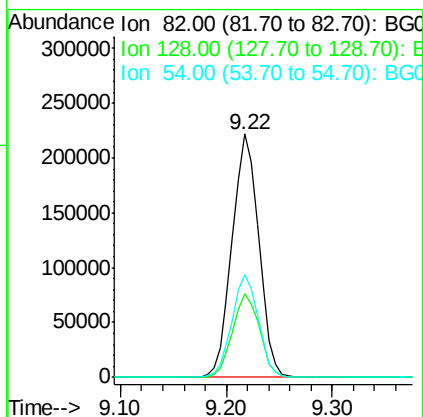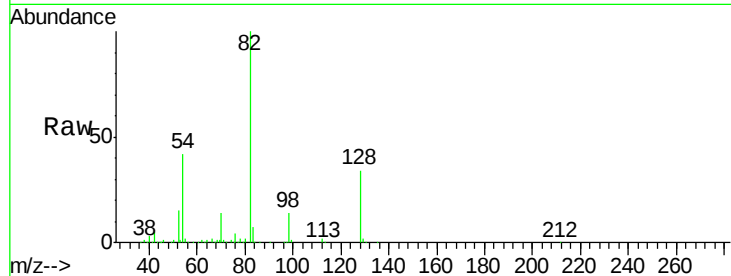

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.68 min Scan# 1939
 Delta R.T. -0.02 min
 Lab File: BG035268.D
 Acq: 20 Jun 2018 16:18

Tgt Ion	Ratio	Lower	Upper
164	100		
162	114.3	78.8	118.2
160	47.8	35.4	53.0

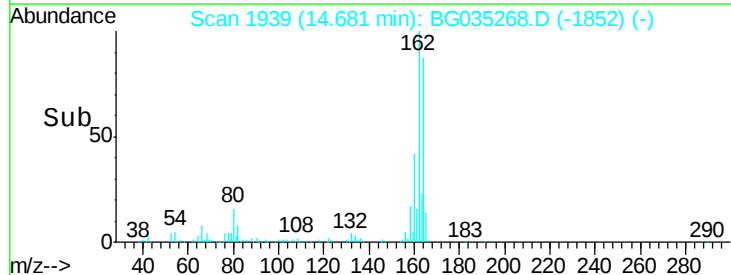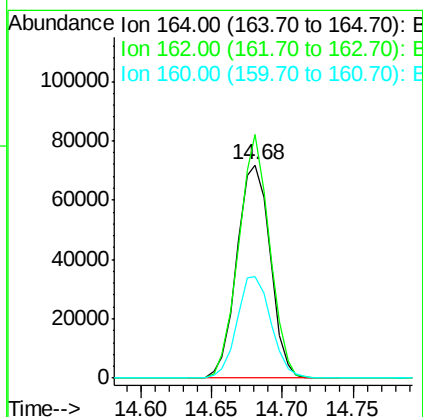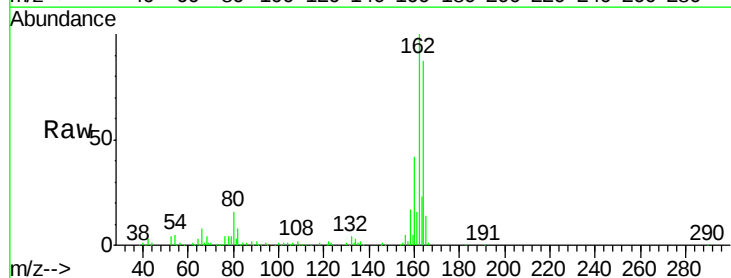


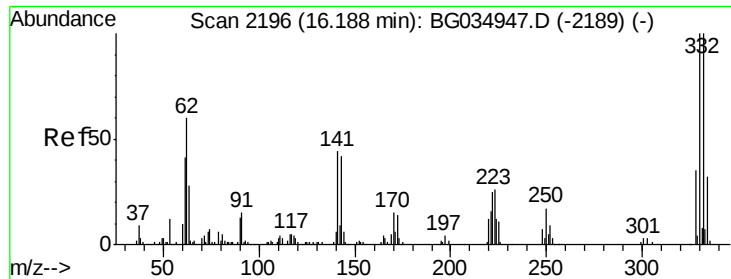




#41
 2,4,6-Tribromophenol
 Concen: 194.093 ng
 RT: 16.17 min Scan# 2192
 Delta R.T. -0.02 min
 Lab File: BG035268.D
 Acq: 20 Jun 2018 16:18

Instrument :
 BNA_G
 ClientSampleId :
 PL-01-061818-A

Tgt Ion:330 Resp: 294924
 Ion Ratio Lower Upper
 330 100
 332 97.3 77.0 115.6
 141 37.4 25.2 37.8

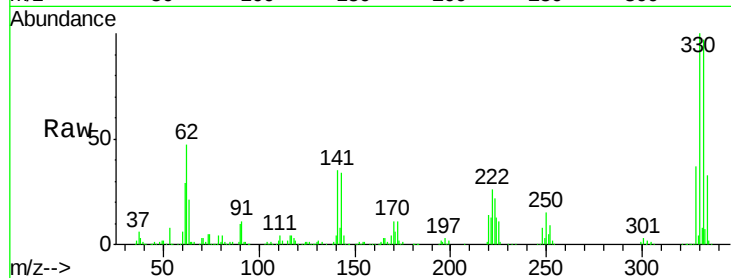


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

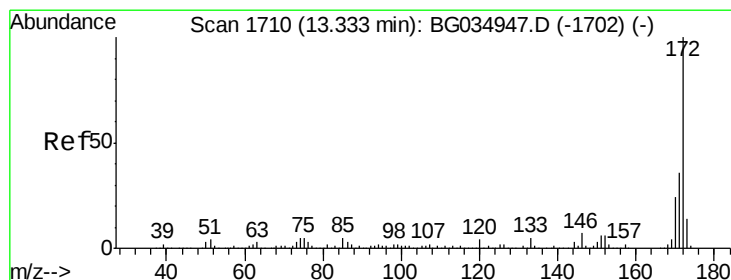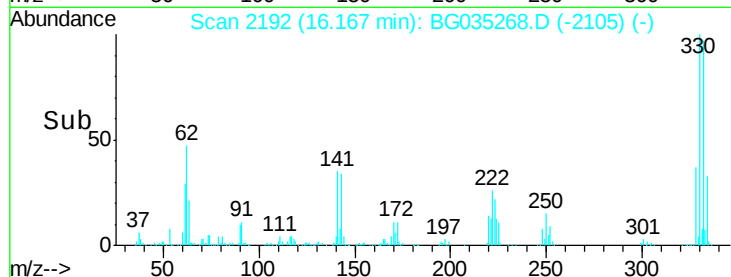
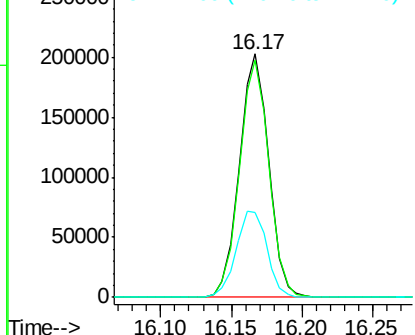



#44
 2-Fluorobiphenyl
 Concen: 98.381 ng
 RT: 13.31 min Scan# 1705
 Delta R.T. -0.02 min
 Lab File: BG035268.D
 Acq: 20 Jun 2018 16:18

Tgt Ion:172 Resp: 898292
 Ion Ratio Lower Upper
 172 100
 171 34.8 30.0 45.0
 170 23.1 19.5 29.3

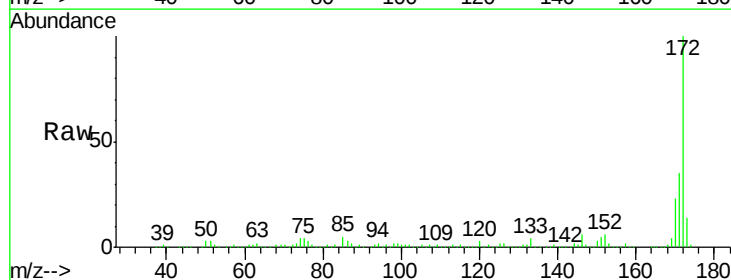

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

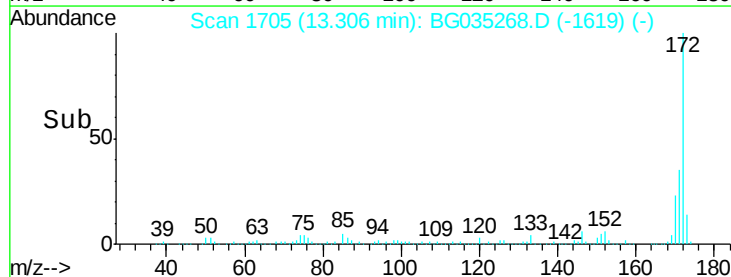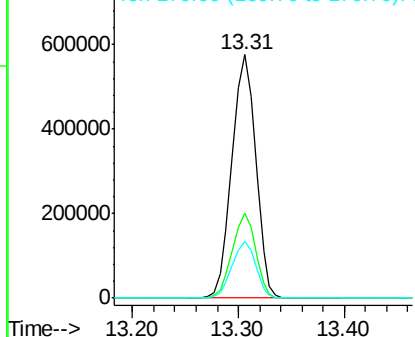

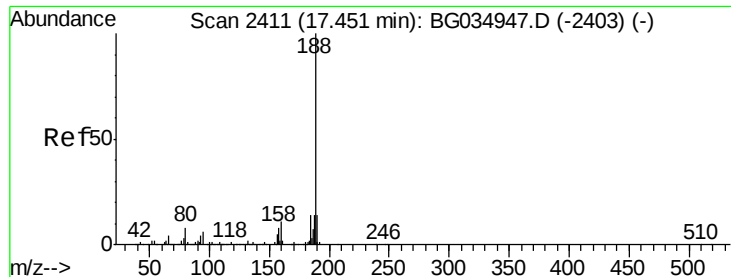

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.42 min Scan# 2406

Delta R.T. -0.02 min

Lab File: BG035268.D

Acq: 20 Jun 2018 16:18

Instrument :

BNA_G

ClientSampleId :

PL-01-061818-A


Tgt Ion:188 Resp: 351297

Ion Ratio Lower Upper

188 100

94 6.3 6.9 10.3#


80 7.1 7.7 11.5#

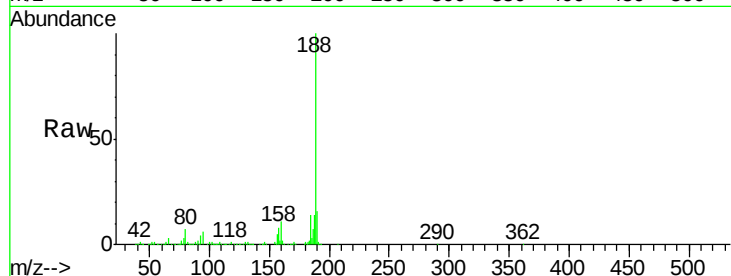



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

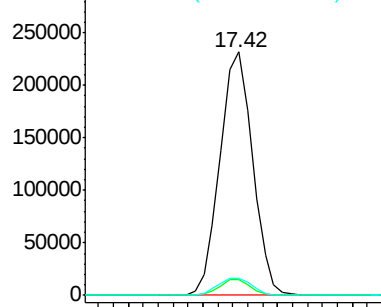

Time-->

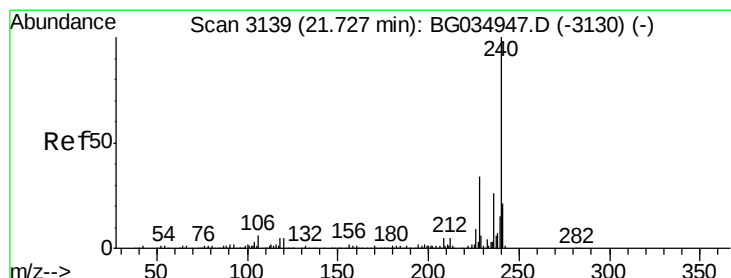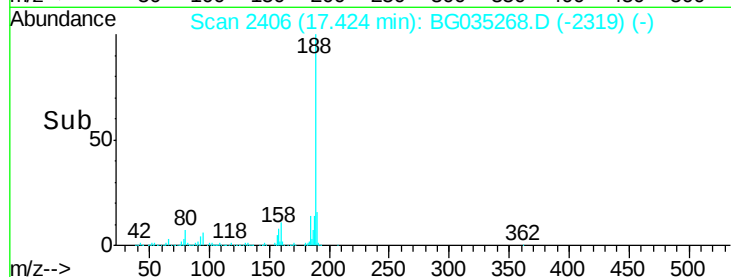

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.69 min Scan# 3132

Delta R.T. -0.03 min

Lab File: BG035268.D

Acq: 20 Jun 2018 16:18


Tgt Ion:240 Resp: 419408

Ion Ratio Lower Upper

240 100

120 6.3 6.8 10.2#


236 25.6 20.9 31.3

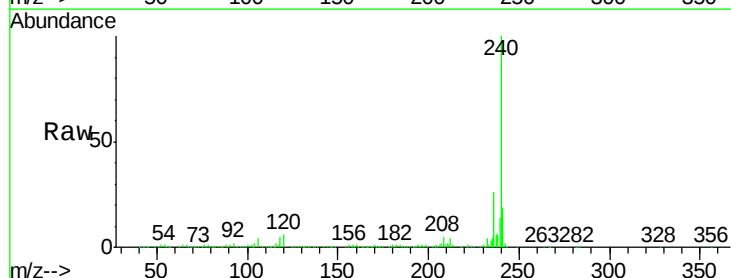


Abundance Ion 240.00 (239.70 to 240.70): E


Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

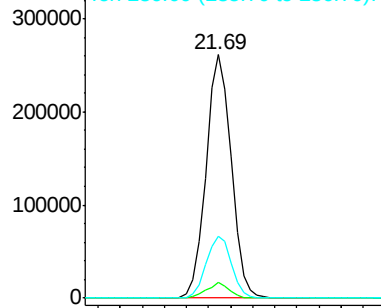

Time-->

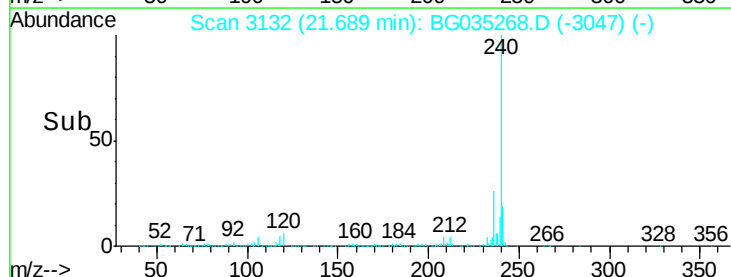

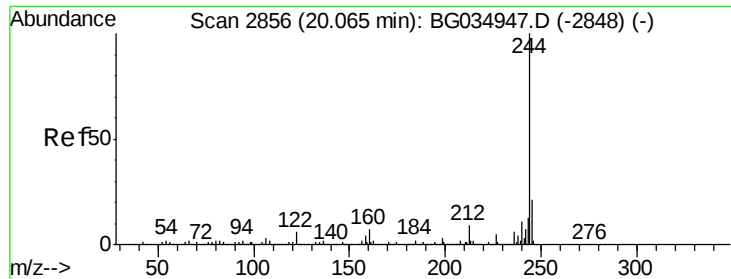

#78

Terphenyl-d14

Concen: 94.778 ng

RT: 20.03 min Scan# 2850

Delta R.T. -0.02 min

Lab File: BG035268.D

Acq: 20 Jun 2018 16:18

Instrument :

BNA_G

ClientSampleId :

PL-01-061818-A


Tgt Ion:244 Resp: 1897697

Ion Ratio Lower Upper

244 100

212 10.0 5.8 8.8#




122 7.1 7.0 10.4

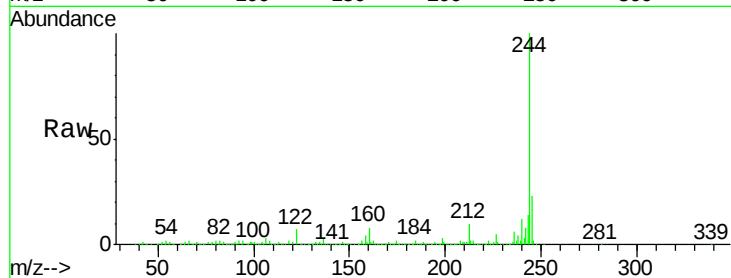

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

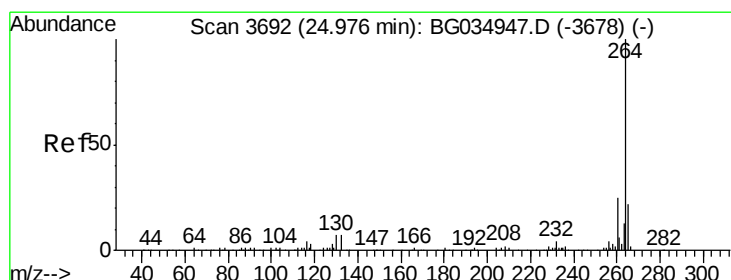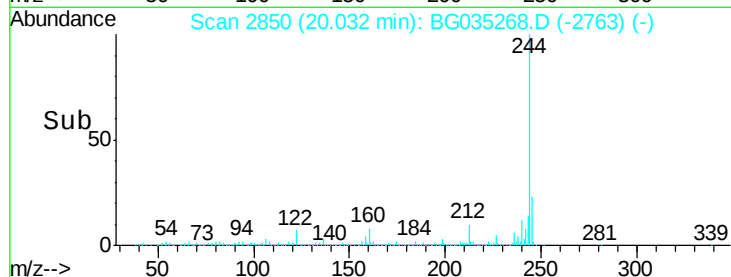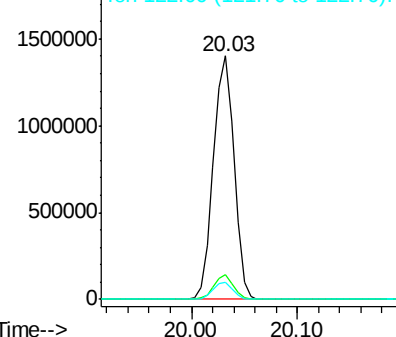

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.91 min Scan# 3681

Delta R.T. -0.04 min

Lab File: BG035268.D

Acq: 20 Jun 2018 16:18


Tgt Ion:264 Resp: 407473

Ion Ratio Lower Upper

264 100

260 22.6 17.4 26.0

265 20.3 17.7 26.5

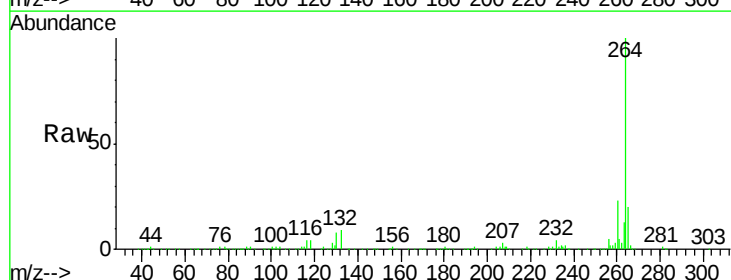

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

