

Data File : BG035285.D
Acq On : 21 Jun 2018 4:38
Operator : SJ/JU
Sample : J3245-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CL-02-061918-D

Quant Time: Jun 21 06:58:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	62627	20.00	ng	-0.02
21) Naphthalene-d8	10.86	136	209933	20.00	ng	-0.02
38) Acenaphthene-d10	14.68	164	144459	20.00	ng	-0.02
63) Phenanthrene-d10	17.42	188	395553	20.00	ng	-0.02
75) Chrysene-d12	21.69	240	431947	20.00	ng	-0.03
86) Perylene-d12	24.91	264	415427	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	495105	133.42	ng	0.00
7) Phenol-d6	7.22	99	632984	115.57	ng	0.00
23) Nitrobenzene-d5	9.22	82	493668	111.78	ng	-0.02
41) 2,4,6-Tribromophenol	16.16	330	332665	179.89	ng	-0.02
44) 2-Fluorobiphenyl	13.30	172	1070783	96.36	ng	-0.02
78) Terphenyl-d14	20.03	244	1946427	94.39	ng	-0.02


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BG035285.D
Acq On : 21 Jun 2018 4:38
Operator : SJ/JU
Sample : J3245-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CL-02-061918-D

Quant Time: Jun 21 06:58:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

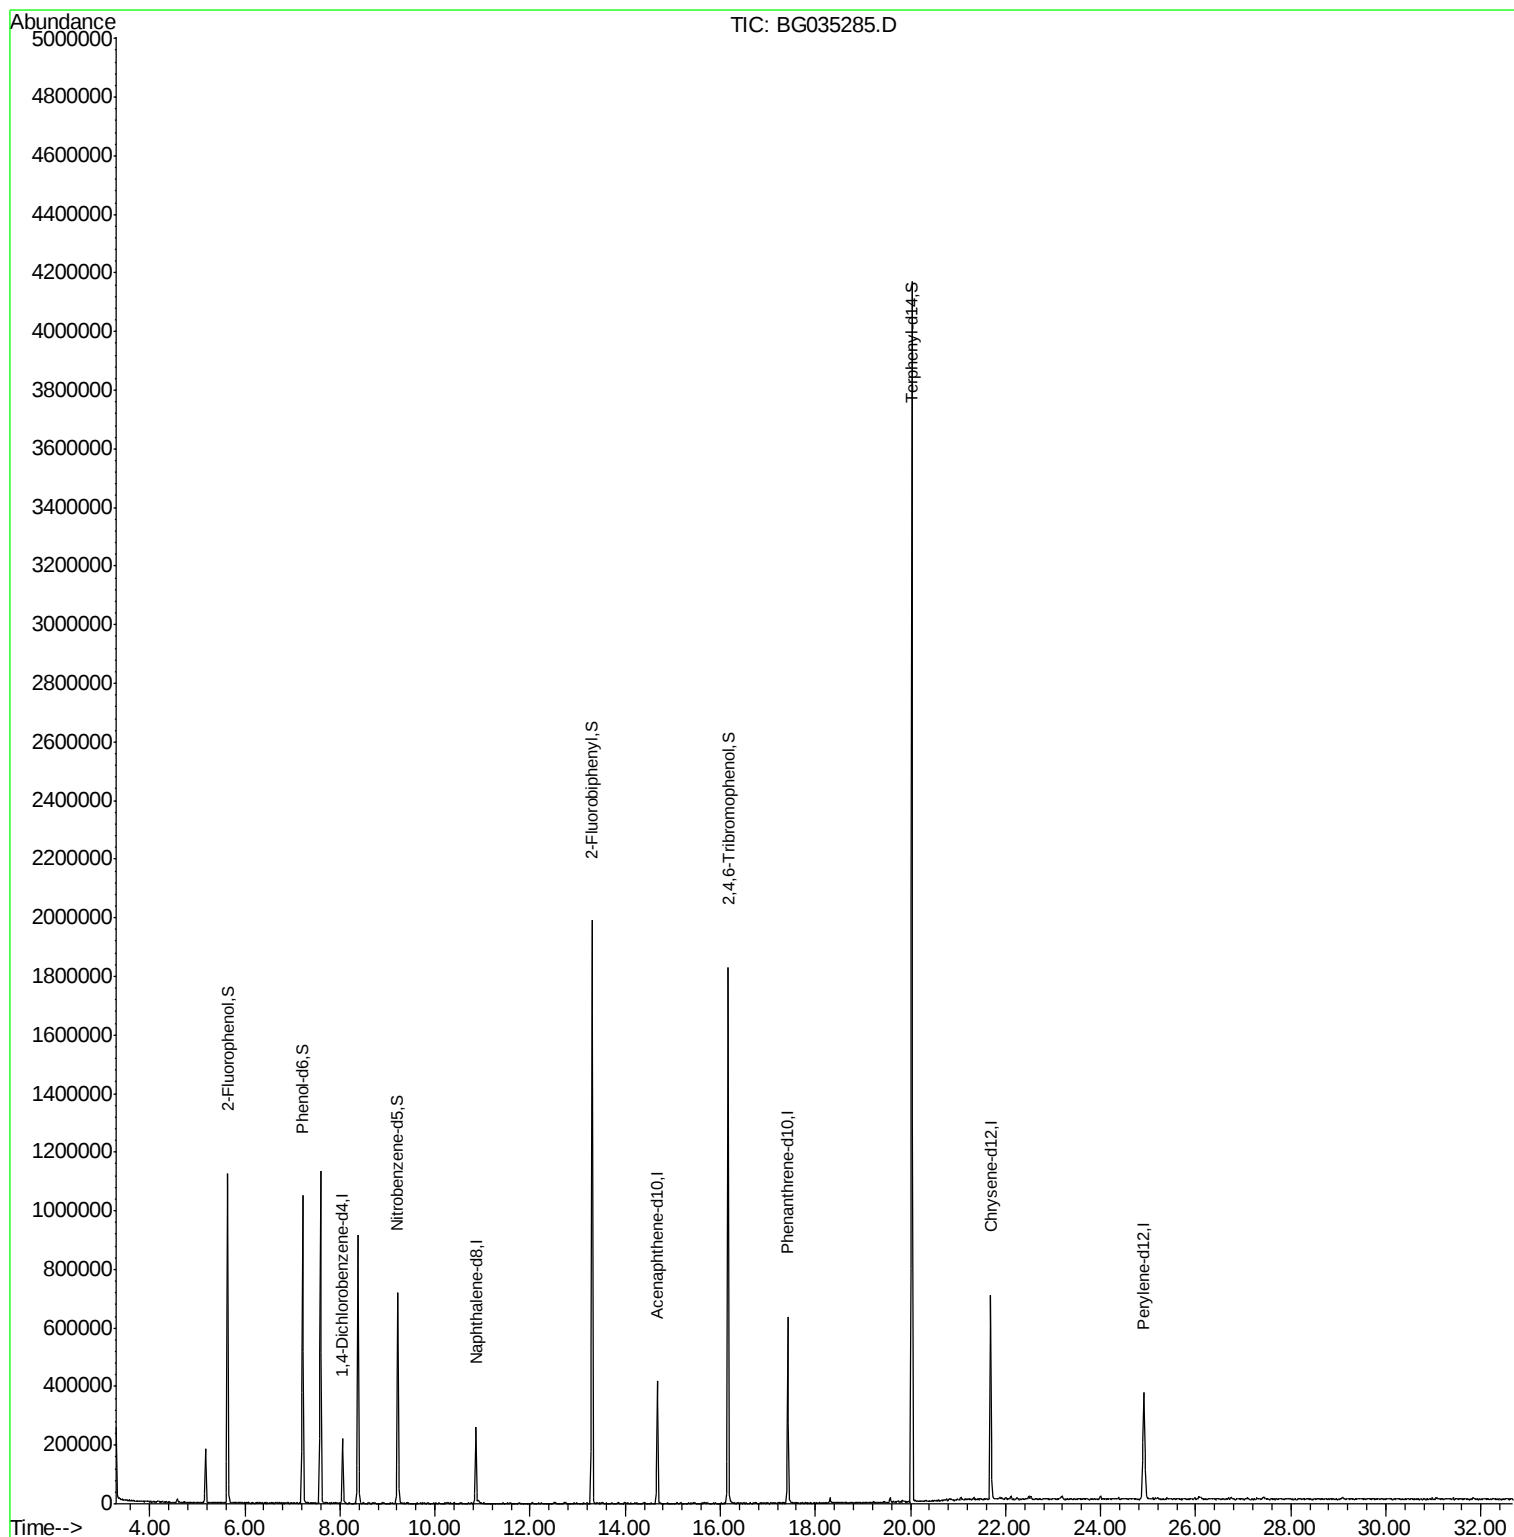

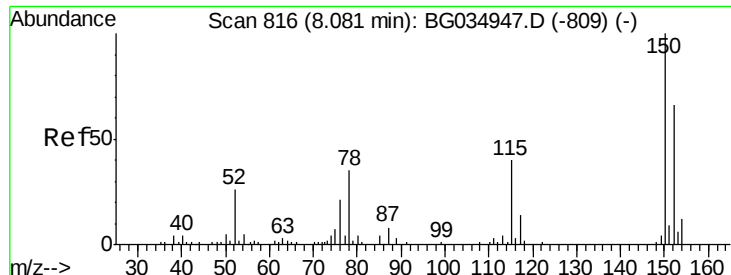


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.06 min Scan# 812
Delta R.T. -0.02 min
Lab File: BG035285.D
Acq: 21 Jun 2018 4:38

Instrument :
BNA_G
ClientSampleId :
CL-02-061918-D

Tgt Ion:152 Resp: 62627
Ion Ratio Lower Upper
152 100
150 133.6 126.6 189.8
115 58.7 53.0 79.4

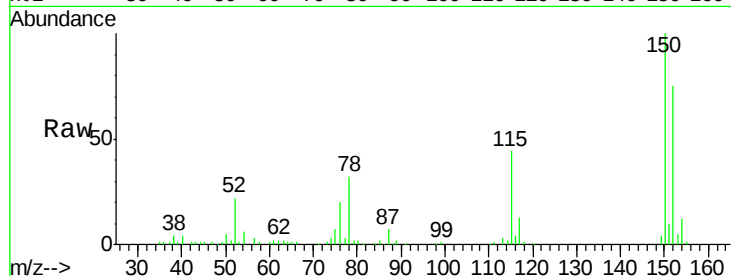


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

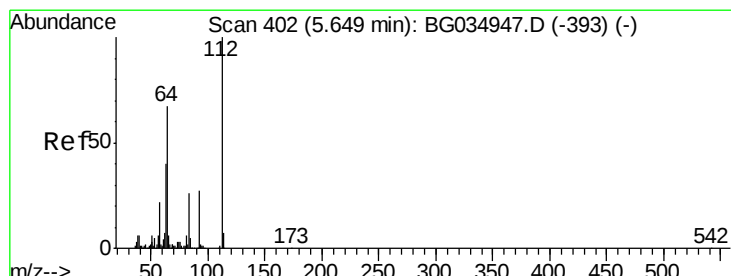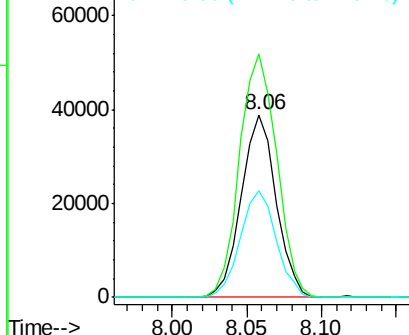



#5


2-Fluorophenol
Concen: 133.416 ng
RT: 5.64 min Scan# 400
Delta R.T. -0.01 min
Lab File: BG035285.D
Acq: 21 Jun 2018 4:38

Tgt Ion:112 Resp: 495105
Ion Ratio Lower Upper
112 100
64 61.0 56.3 84.5
63 34.5 30.1 45.1

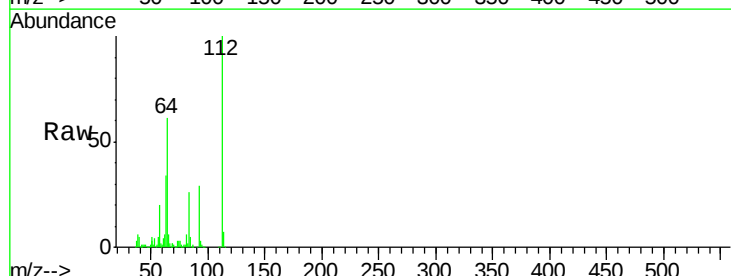

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

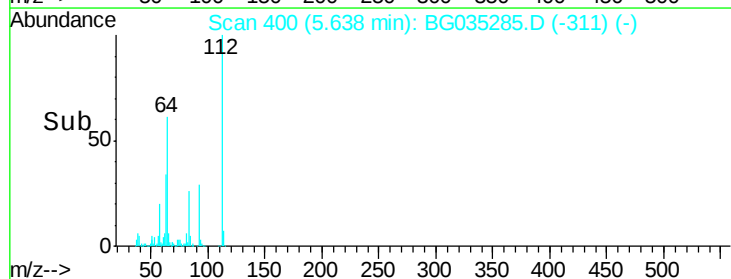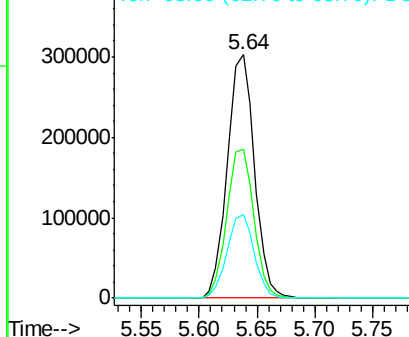

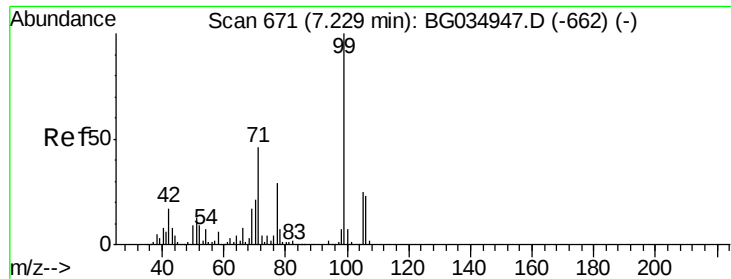

#7

Phenol-d6

Concen: 115.567 ng

RT: 7.22 min Scan# 669

Delta R.T. -0.01 min

Lab File: BG035285.D

Acq: 21 Jun 2018 4:38

Instrument :

BNA_G

ClientSampleId :

CL-02-061918-D


Tgt Ion: 99 Resp: 632984

Ion Ratio Lower Upper




99 100

42 15.3 14.1 21.1

71 40.6 26.1 39.1#

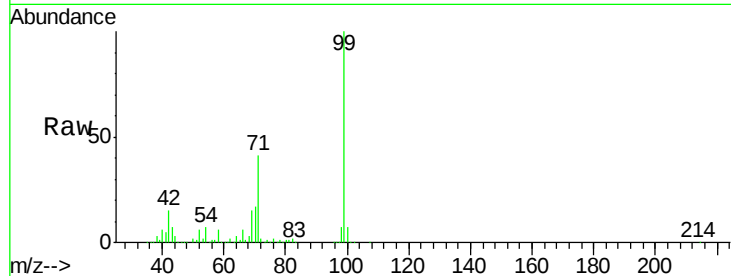

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

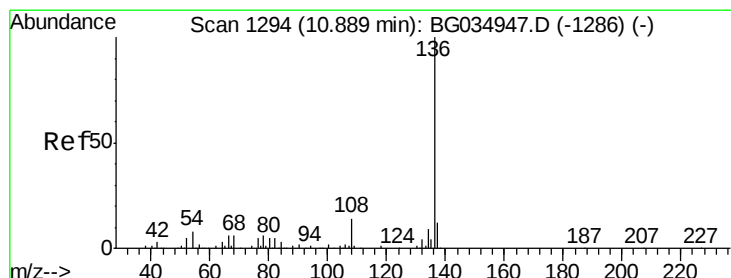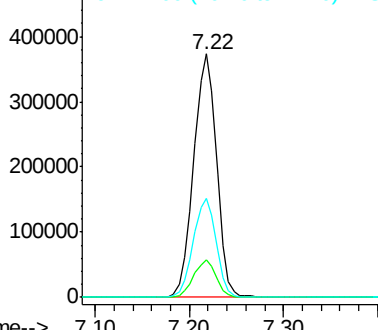

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.86 min Scan# 1289

Delta R.T. -0.02 min

Lab File: BG035285.D

Acq: 21 Jun 2018 4:38

Tgt Ion: 136 Resp: 209933


Ion Ratio Lower Upper

136 100



137 11.2 9.2 13.8


54 6.6 10.3 15.5#

68 4.1 4.5 6.7#

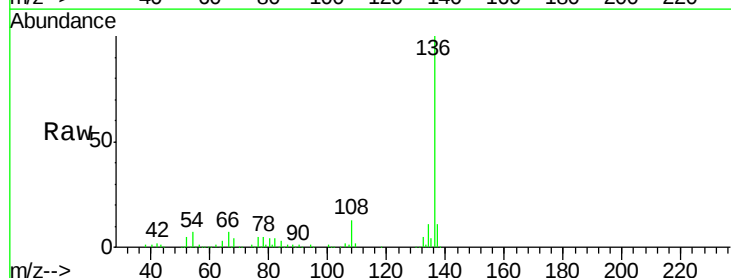

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

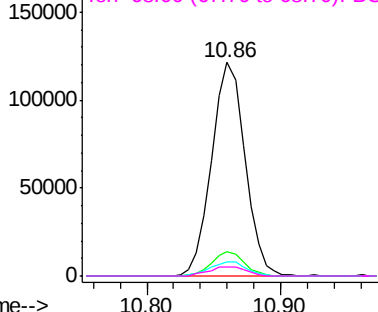







#23
 Nitrobenzene-d5
 Concen: 111.779 ng
 RT: 9.22 min Scan# 1010
 Delta R.T. -0.02 min
 Lab File: BG035285.D
 Acq: 21 Jun 2018 4:38

Instrument :
 BNA_G
 ClientSampleId :
 CL-02-061918-D

Tgt Ion: 82 Resp: 493668
 Ion Ratio Lower Upper
 82 100
 128 34.5 29.7 44.5
 54 40.1 43.1 64.7#

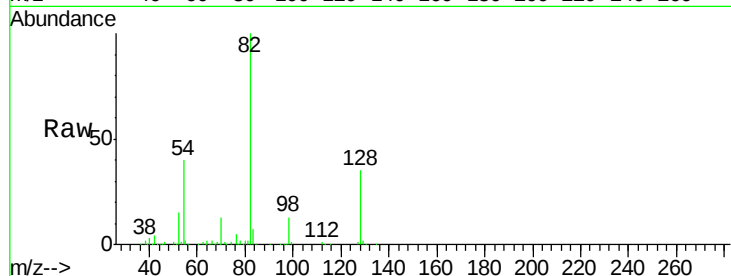


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC

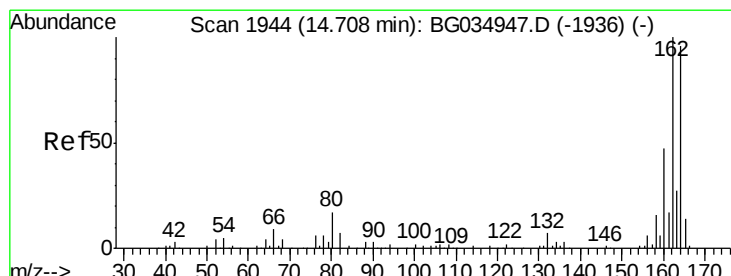
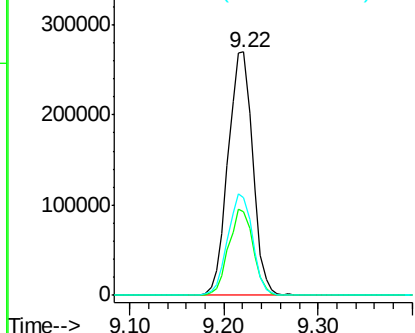



#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.68 min Scan# 1939
 Delta R.T. -0.02 min
 Lab File: BG035285.D
 Acq: 21 Jun 2018 4:38

Tgt Ion: 164 Resp: 144459
 Ion Ratio Lower Upper
 164 100
 162 101.7 78.8 118.2
 160 45.8 35.4 53.0

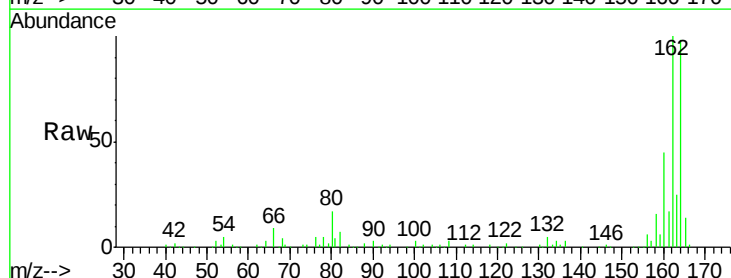

Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC

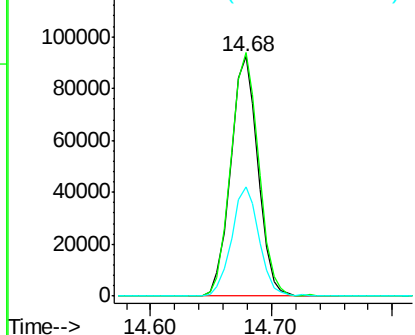


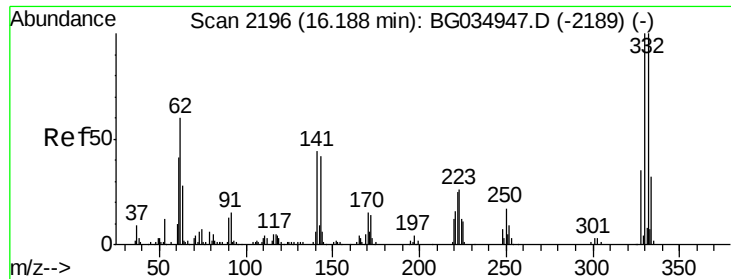




#41
 2,4,6-Tribromophenol
 Concen: 179.891 ng
 RT: 16.16 min Scan# 2192
 Delta R.T. -0.02 min
 Lab File: BG035285.D
 Acq: 21 Jun 2018 4:38

Instrument :
 BNA_G
 ClientSampleId :
 CL-02-061918-D

Tgt Ion	Ratio	Lower	Upper
330	100		
332	95.9	77.0	115.6
141	37.5	25.2	37.8

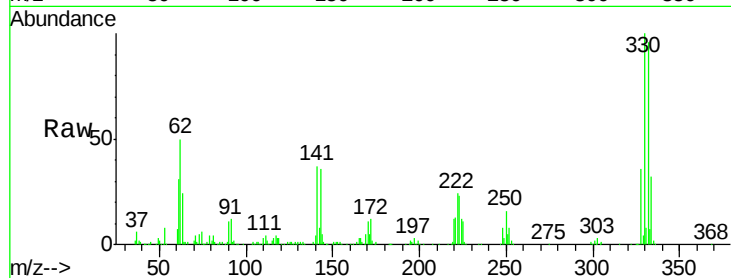


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

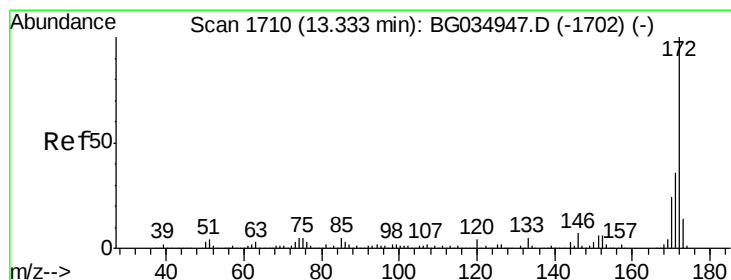
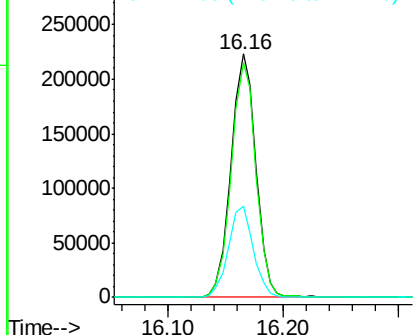



#44
 2-Fluorobiphenyl
 Concen: 96.361 ng
 RT: 13.30 min Scan# 1705
 Delta R.T. -0.02 min
 Lab File: BG035285.D
 Acq: 21 Jun 2018 4:38

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.8	30.0	45.0
170	23.9	19.5	29.3

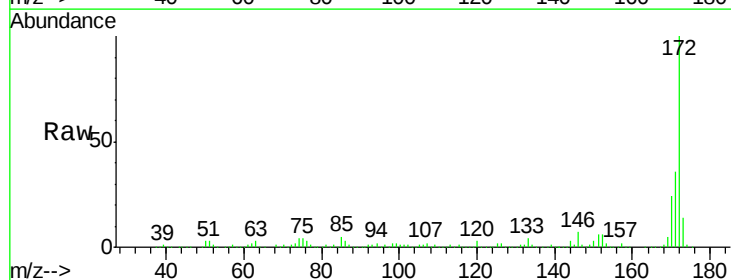

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

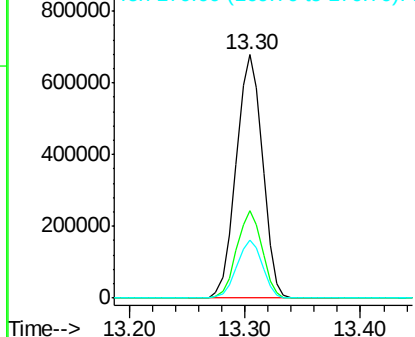



#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.42 min Scan# 2406

Delta R.T. -0.02 min

Lab File: BG035285.D

Acq: 21 Jun 2018 4:38

Instrument :

BNA_G

ClientSampleId :

CL-02-061918-D


Tgt Ion:188 Resp: 395553

Ion Ratio Lower Upper

188 100

94 5.4 6.9 10.3#




80 7.5 7.7 11.5#

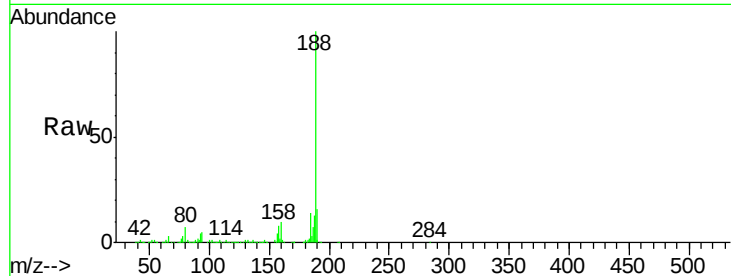

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

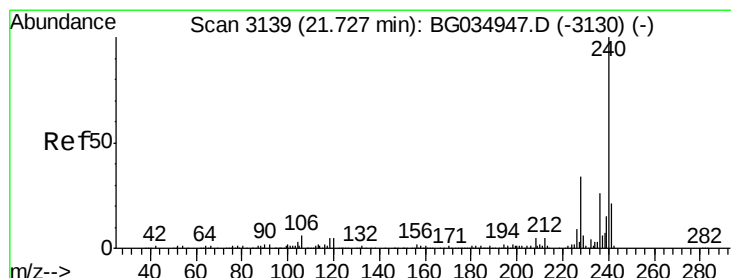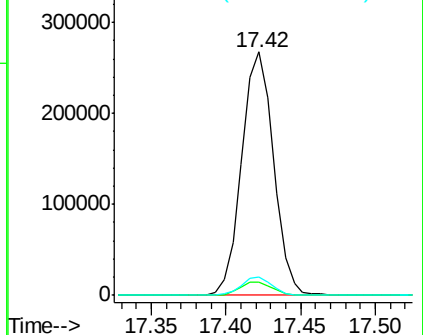

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.69 min Scan# 3132

Delta R.T. -0.03 min

Lab File: BG035285.D

Acq: 21 Jun 2018 4:38


Tgt Ion:240 Resp: 431947

Ion Ratio Lower Upper

240 100

120 5.5 6.8 10.2#



236 25.5 20.9 31.3

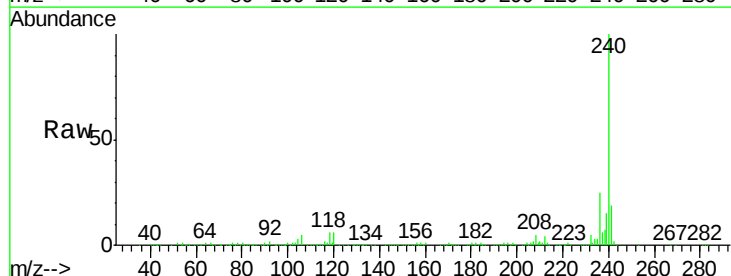


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

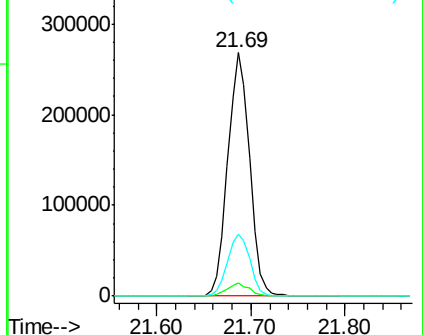

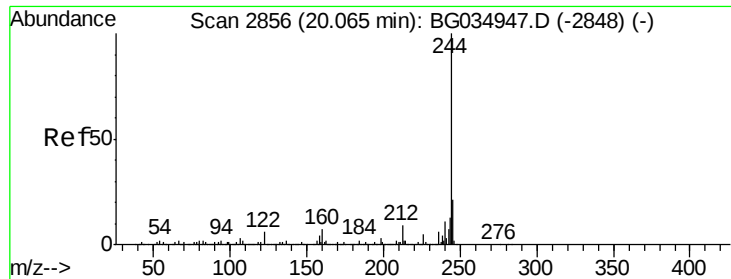

#78

Terphenyl-d14

Concen: 94.390 ng

RT: 20.03 min Scan# 2850

Delta R.T. -0.02 min

Lab File: BG035285.D

Acq: 21 Jun 2018 4:38

Instrument :

BNA_G

ClientSampleId :

CL-02-061918-D


Tgt Ion:244 Resp: 1946427

Ion Ratio Lower Upper




244 100

212 9.8 5.8 8.8#

122 6.6 7.0 10.4#

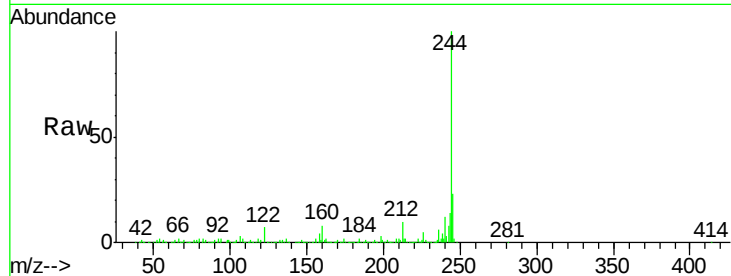

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

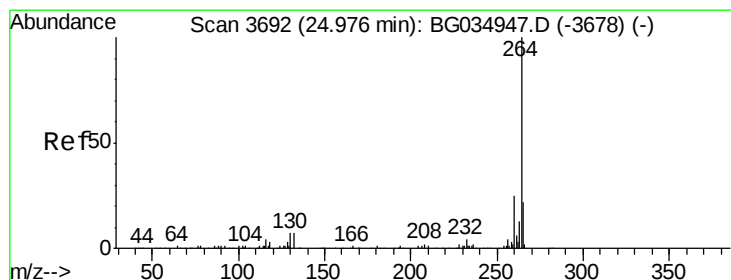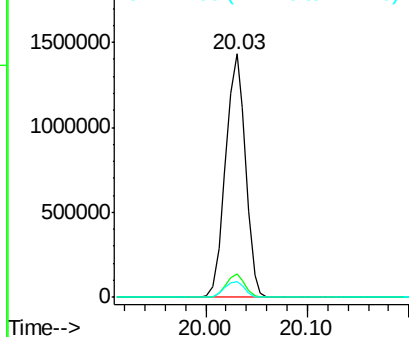

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.91 min Scan# 3681

Delta R.T. -0.04 min

Lab File: BG035285.D

Acq: 21 Jun 2018 4:38


Tgt Ion:264 Resp: 415427

Ion Ratio Lower Upper

264 100

260 24.6 17.4 26.0

265 23.3 17.7 26.5

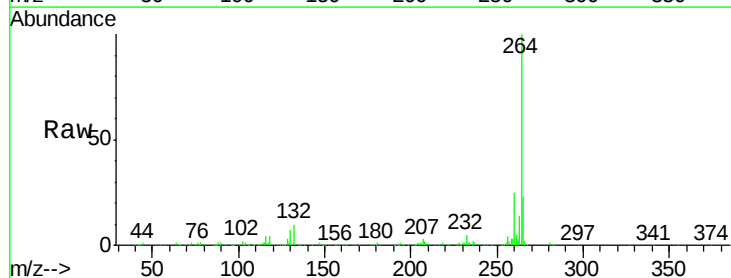

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

